

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
 Data File : PL076076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 09:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 22:25:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.632	15343420	37357979	20.287	19.697
28)	SA Decachlor...	11.634	10.372	14058160	31014791	22.341	20.193
Target Compounds							
4)	MA Heptachlor	0.000	6.140f	0	84223	N.D.	0.037 #
6)	B beta-BHC	0.000	6.140	0	84223	N.D.	0.081 #
7)	B delta-BHC	0.000	6.394	0	381467	N.D.	0.169 #
10)	B gamma-Chl...	0.000	7.333	0	322051	N.D.	0.168 #
14)	MA Endrin	0.000	8.058f	0	831209	N.D.	0.547 #
15)	B Endosulfa...	9.302	0.000	208520	0	0.329	N.D. #
17)	MA 4,4'-DDT	0.000	8.455	0	31582	N.D.	0.021 #
21)	B Endrin ke...	10.181	0.000	255094	0	0.354	N.D. #
25)	Chlordane-3	0.000	7.333	0	322051	N.D.	1.826 #
27)	Chlordane-5	9.378	0.000	61143	0	2.866	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
Data File : PL076076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 09:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 22:25:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

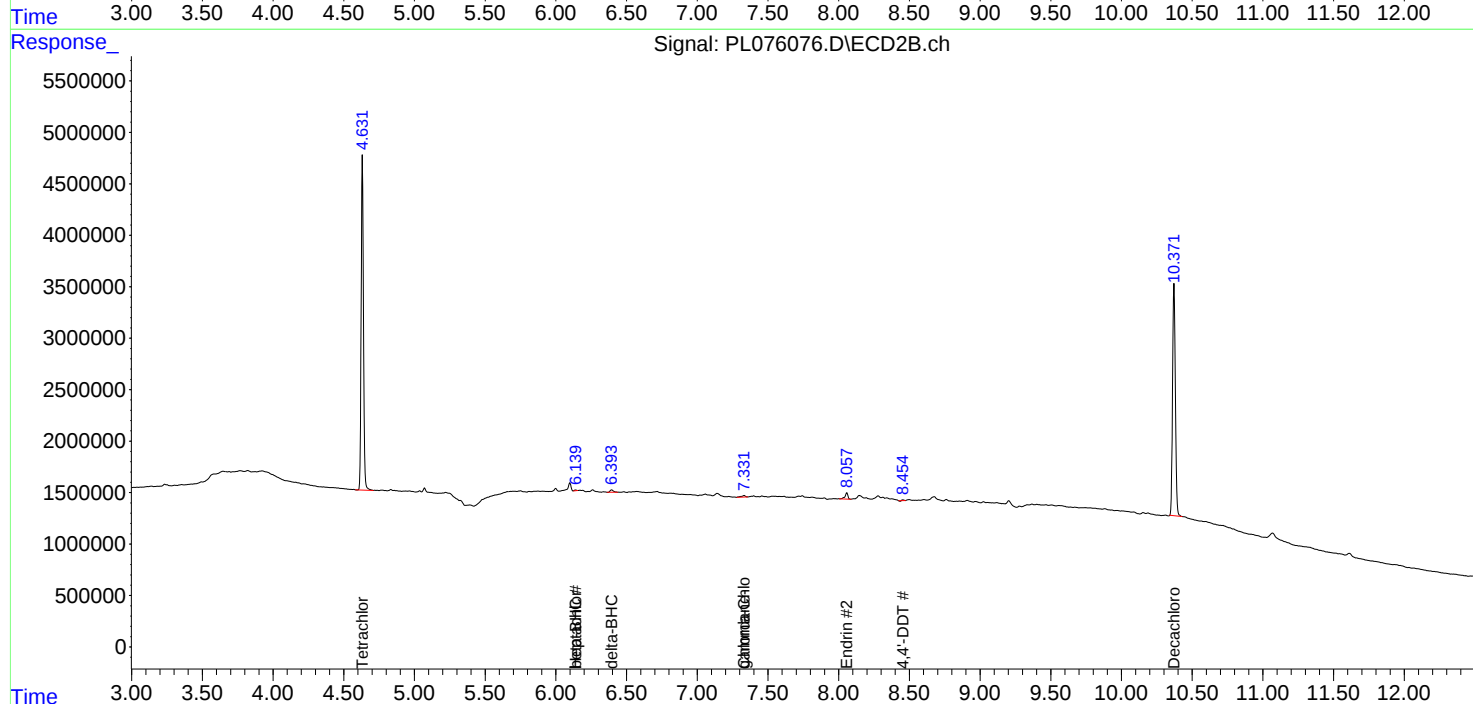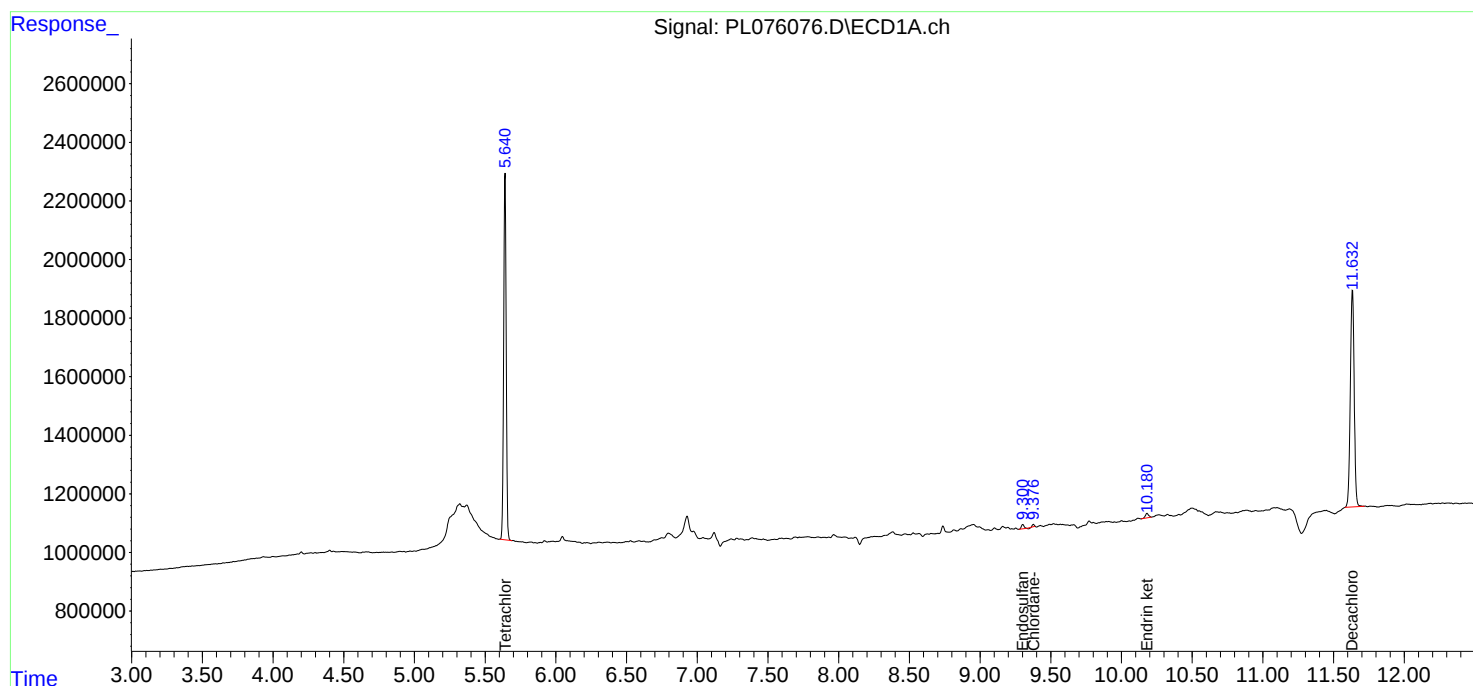


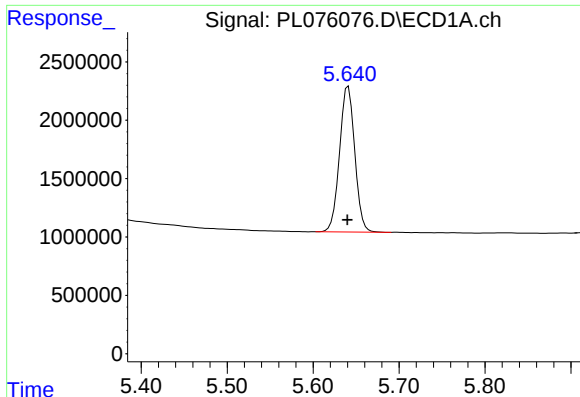

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 15343420
Conc: 20.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

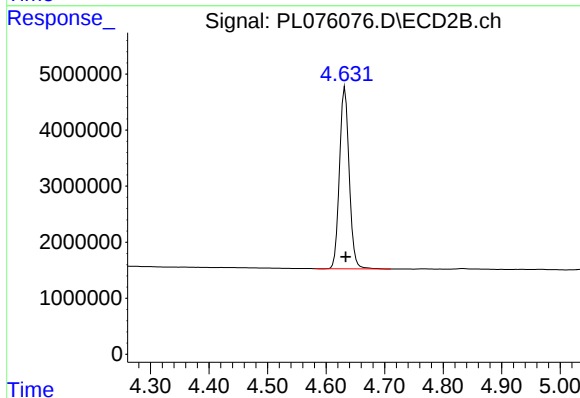


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 37357979
Conc: 19.70 ng/ml

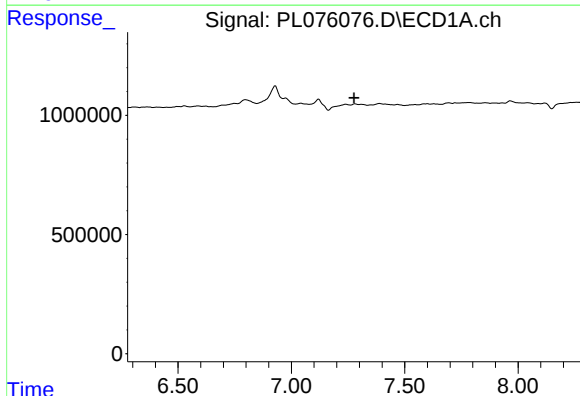


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.277 min
Response: 0
Conc: N.D.

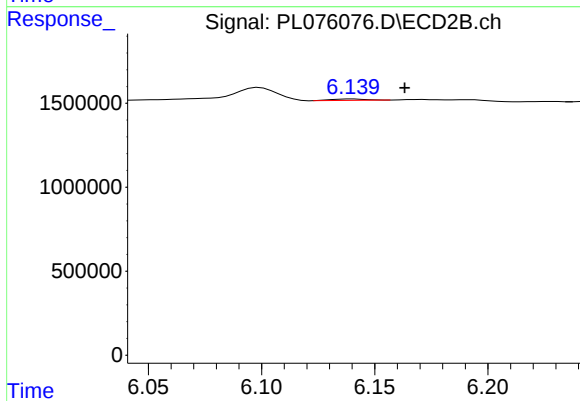

#4 Heptachlor


R.T.: 6.140 min
Delta R.T.: -0.023 min
Response: 84223
Conc: 0.04 ng/ml

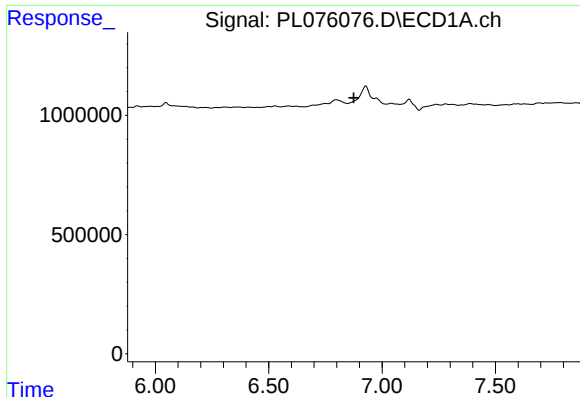

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.875 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

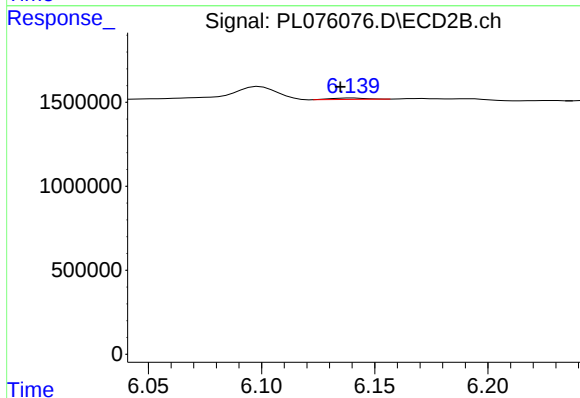


#6 beta-BHC

R.T.: 6.140 min
Delta R.T.: 0.005 min
Response: 84223
Conc: 0.08 ng/ml

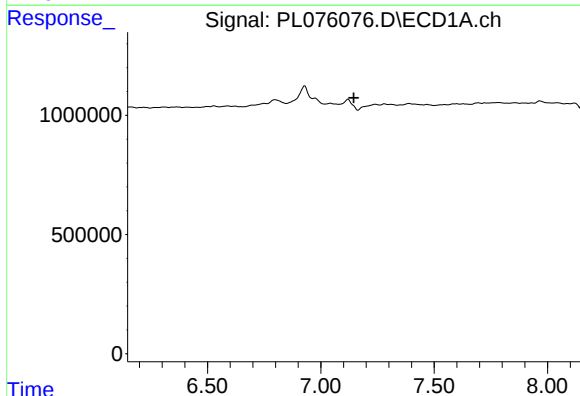


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

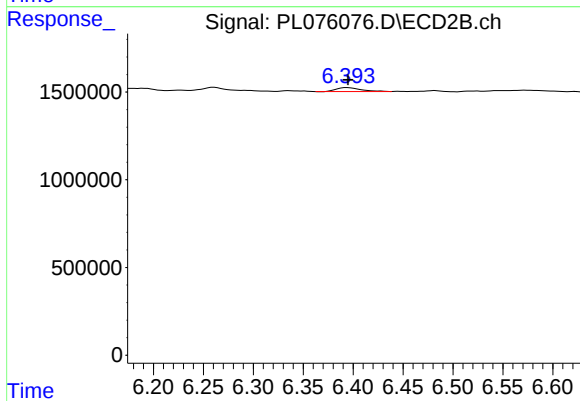

#7 delta-BHC


R.T.: 6.394 min
Delta R.T.: 0.000 min
Response: 381467
Conc: 0.17 ng/ml

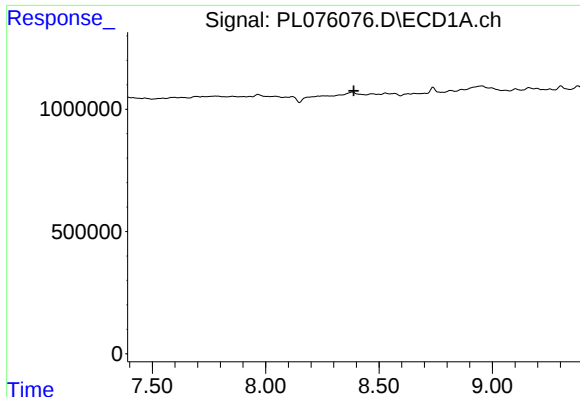

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

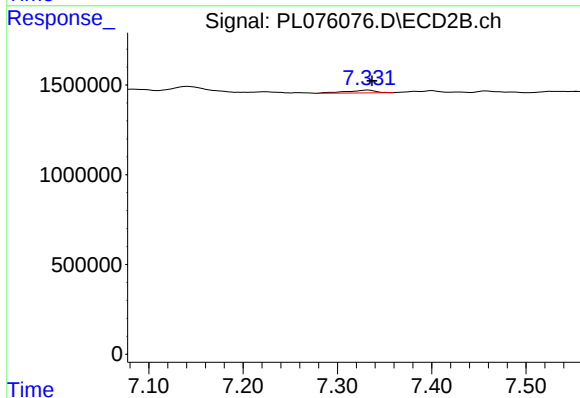


#10 gamma-Chlordane

R.T.: 7.333 min
Delta R.T.: -0.004 min
Response: 322051
Conc: 0.17 ng/ml

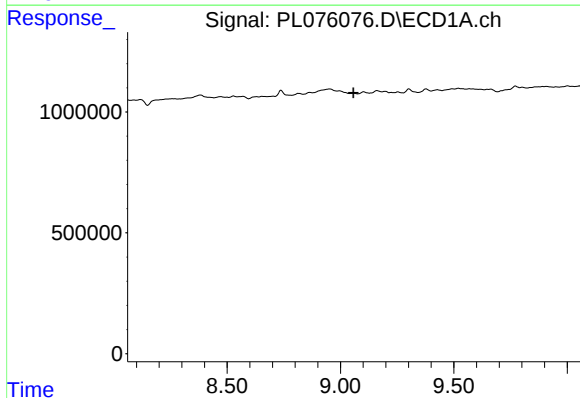


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.058 min
Response: 0
Conc: N.D.

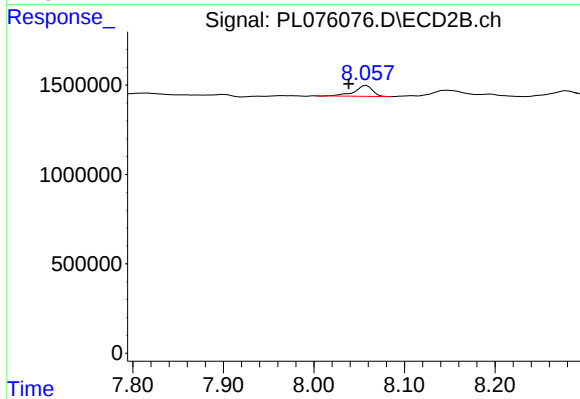

#14 Endrin


R.T.: 8.058 min
Delta R.T.: 0.019 min
Response: 831209
Conc: 0.55 ng/ml

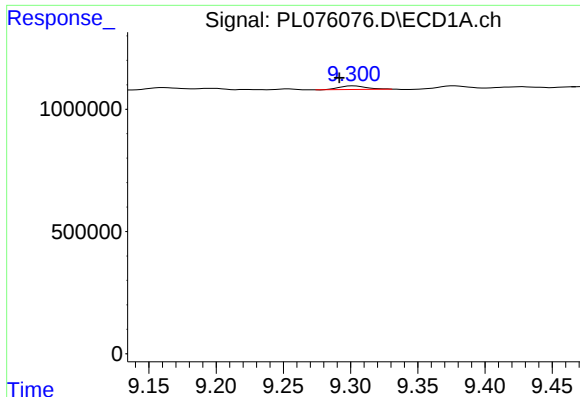

#15 Endosulfan II


R.T.: 9.302 min
Delta R.T.: 0.010 min
Response: 208520
Conc: 0.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

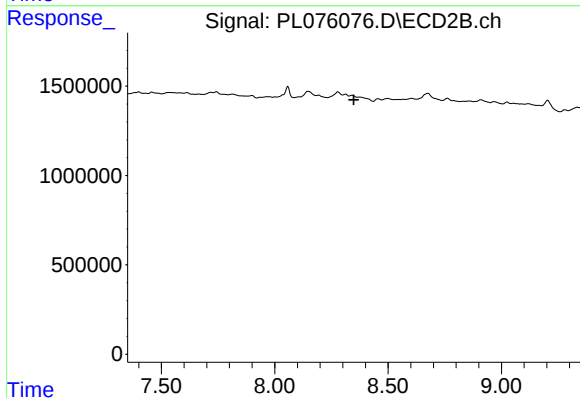


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

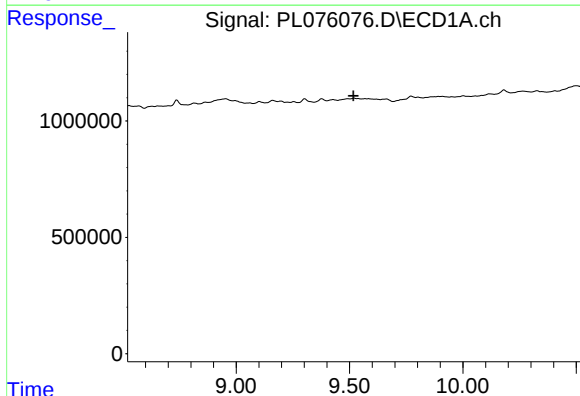


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 9.518 min
Response: 0
Conc: N.D.

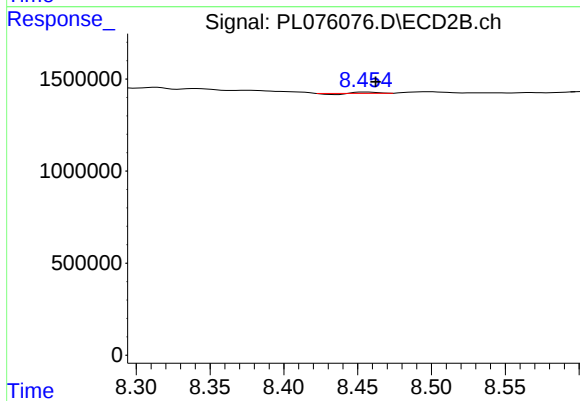

#17 4,4'-DDT


R.T.: 8.455 min
Delta R.T.: -0.007 min
Response: 31582
Conc: 0.02 ng/ml

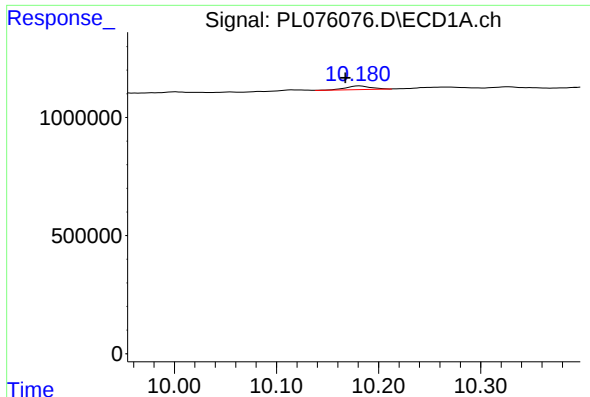

#21 Endrin ketone


R.T.: 10.181 min
Delta R.T.: 0.014 min
Response: 255094
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

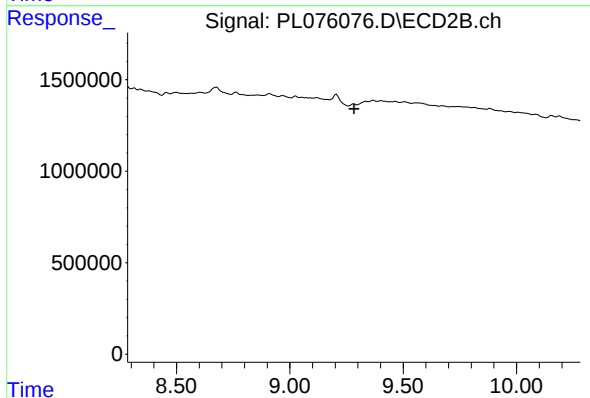


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.284 min
Response: 0
Conc: N.D.

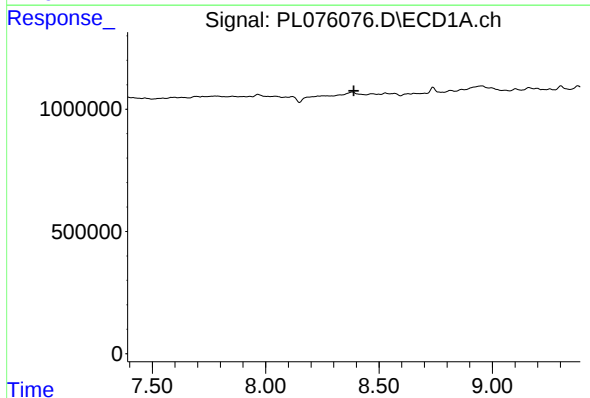


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

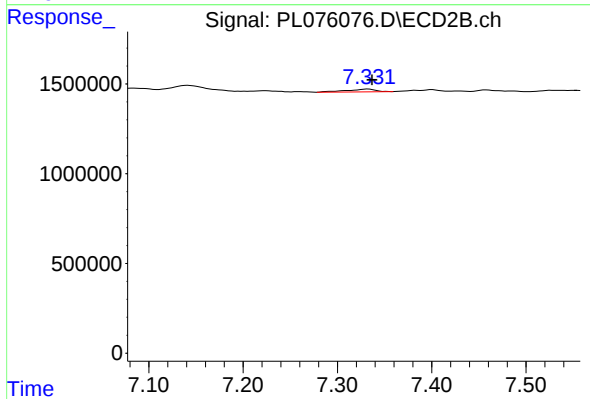

#25 Chlordane-3


R.T.: 7.333 min
Delta R.T.: -0.004 min
Response: 322051
Conc: 1.83 ng/ml

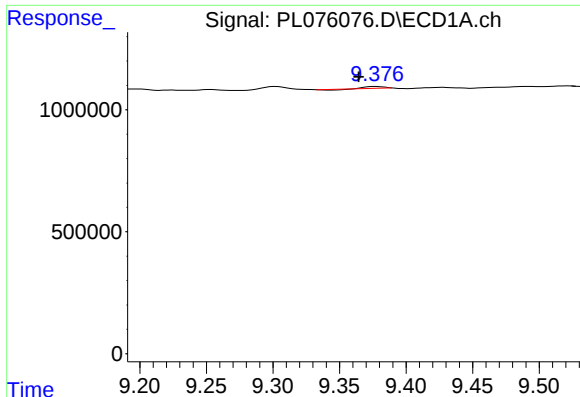

#27 Chlordane-5


R.T.: 9.378 min
Delta R.T.: 0.013 min
Response: 61143
Conc: 2.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

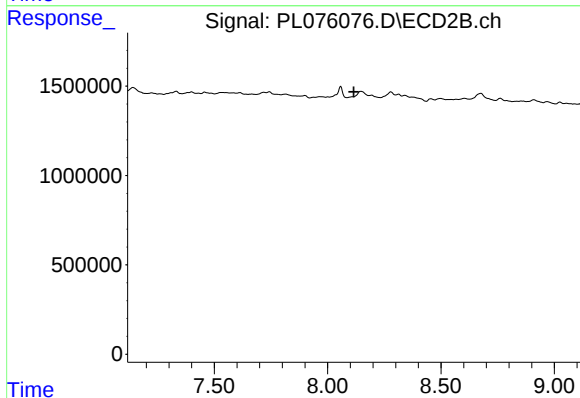


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

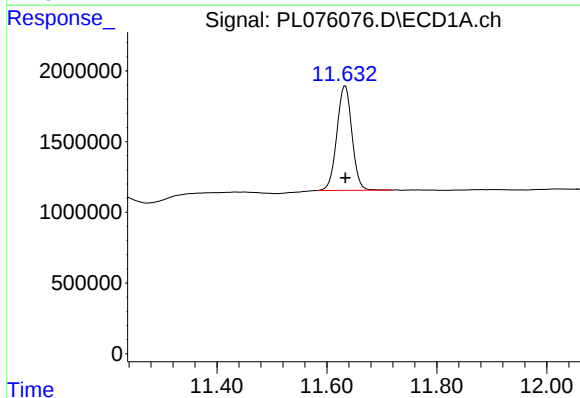

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: 0.000 min
Response: 14058160
Conc: 22.34 ng/ml

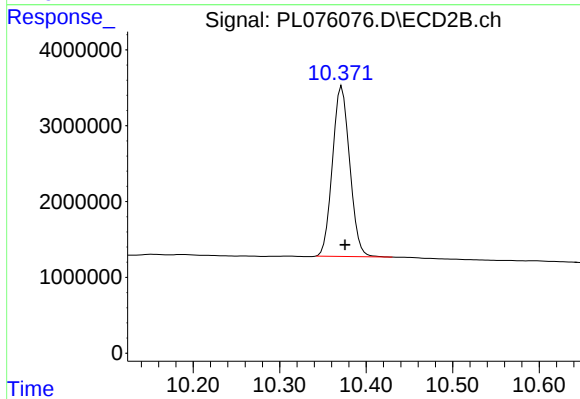

#28 Decachlorobiphenyl

R.T.: 10.372 min
Delta R.T.: -0.003 min
Response: 31014791
Conc: 20.19 ng/ml