

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
 Data File : PL076079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 12:59
 Operator : AR\AJ
 Sample : N3494-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-EXC-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 22:27:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.646	4.634	13197450	30394087	17.450	16.025
28) SA Decachlor...	11.637	10.374	12923256	25644789	20.537	16.697
Target Compounds						
6) B beta-BHC	6.875	6.146	24386137	26353399	55.680m	25.264 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
Data File : PL076079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 12:59
Operator : AR\AJ
Sample : N3494-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-EXC-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 22:27:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

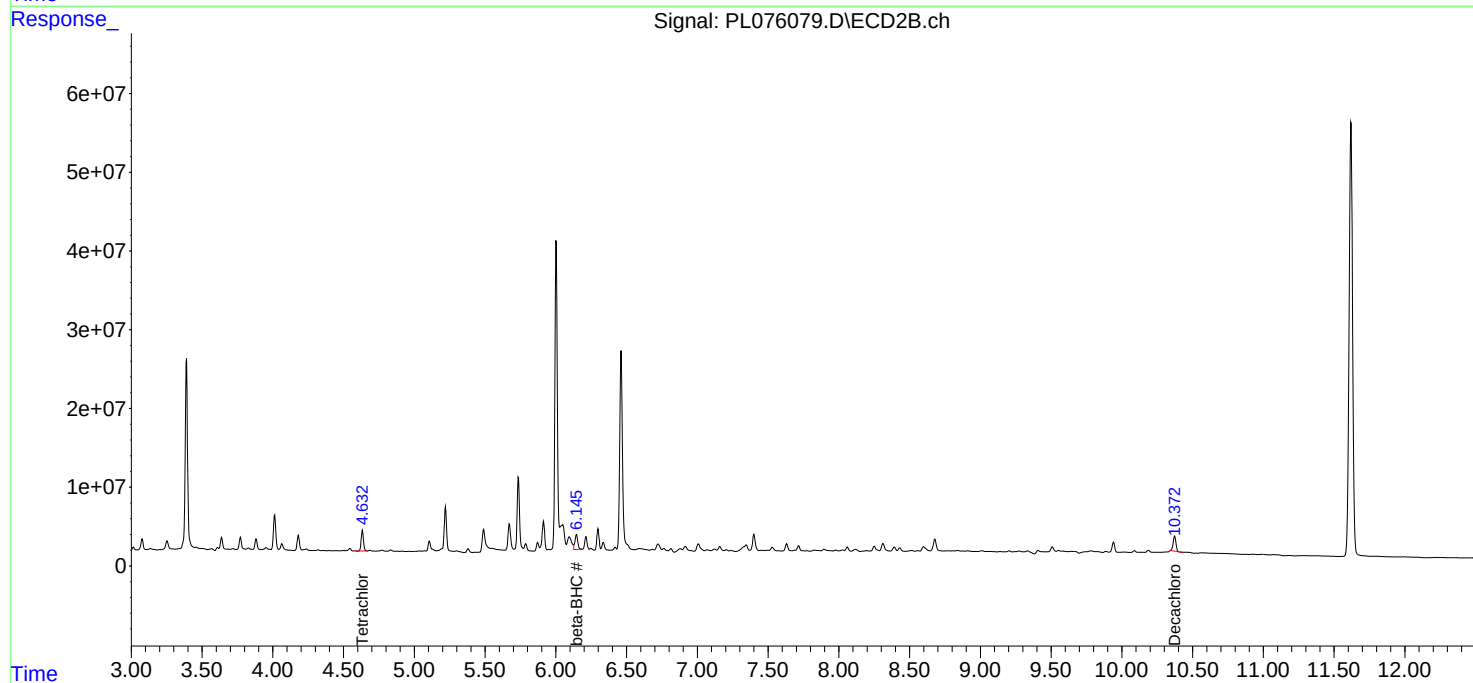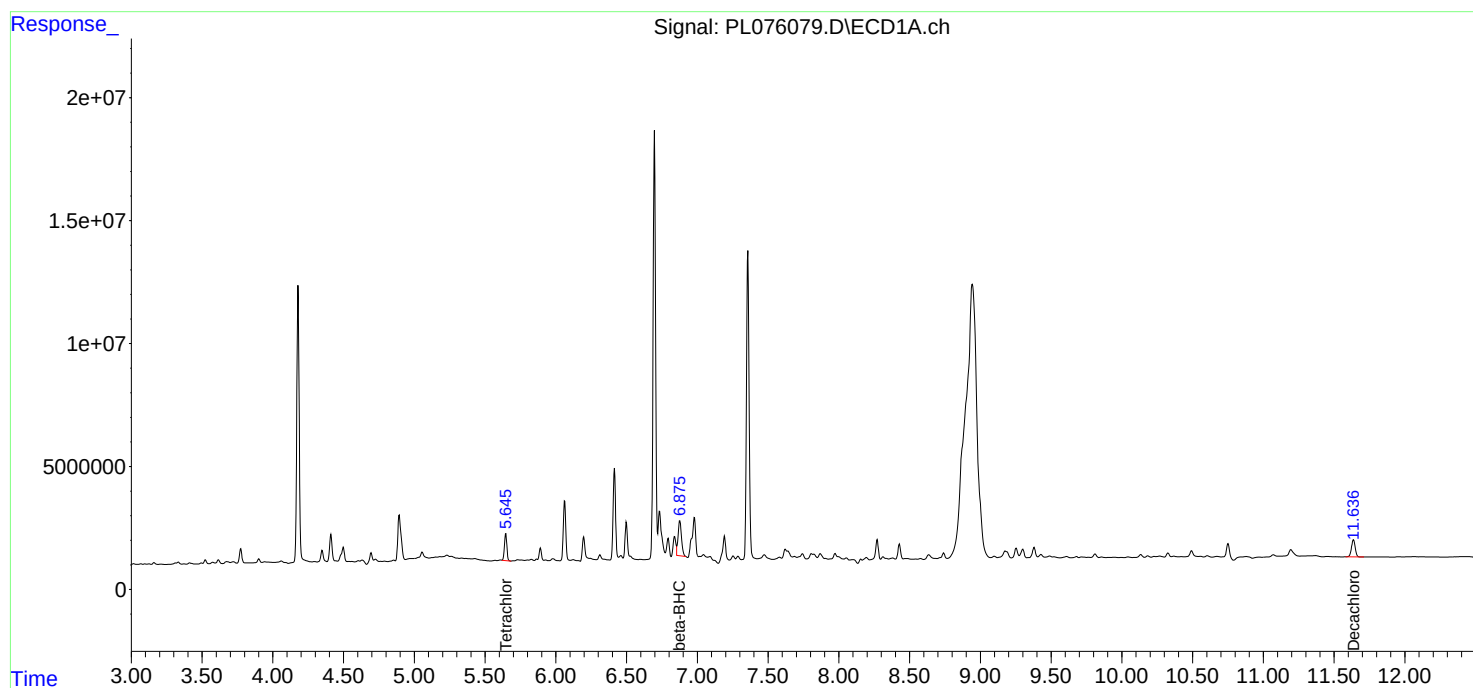


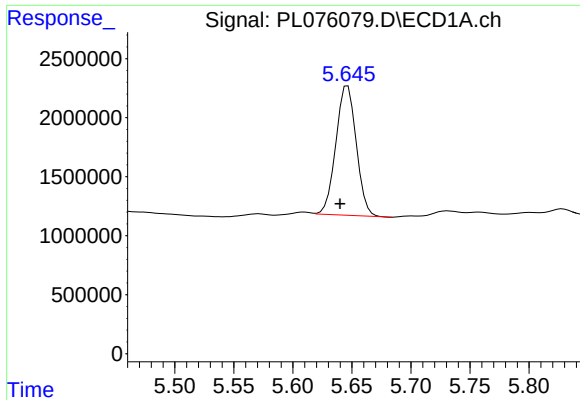

#1 Tetrachloro-m-xylene


R.T.: 5.646 min
Delta R.T.: 0.006 min
Response: 13197450
Conc: 17.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-EXC-3

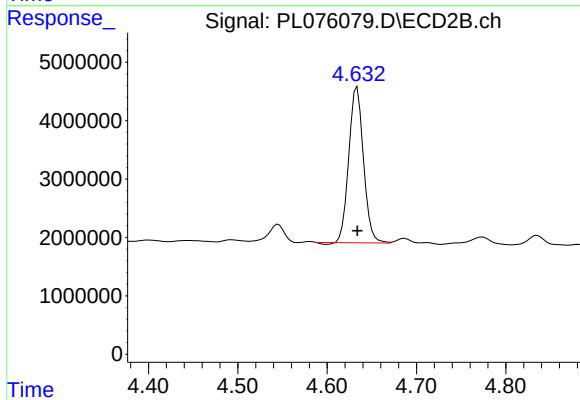


#1 Tetrachloro-m-xylene

R.T.: 4.634 min
Delta R.T.: 0.000 min
Response: 30394087
Conc: 16.03 ng/ml

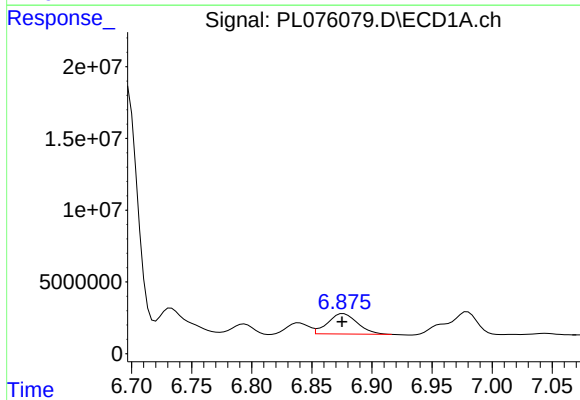


#6 beta-BHC

R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 24386137
Conc: 55.68 ng/ml m

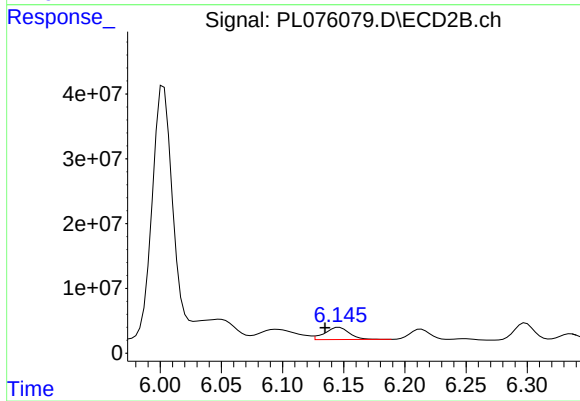

#6 beta-BHC


R.T.: 6.146 min
Delta R.T.: 0.012 min
Response: 26353399
Conc: 25.26 ng/ml

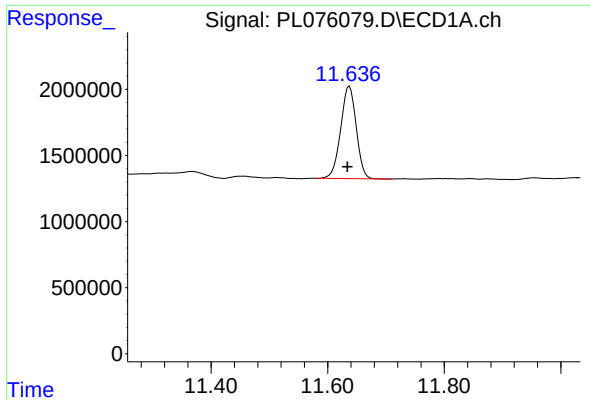

#28 Decachlorobiphenyl

R.T.: 11.637 min
Delta R.T.: 0.004 min
Response: 12923256
Conc: 20.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-EXC-3

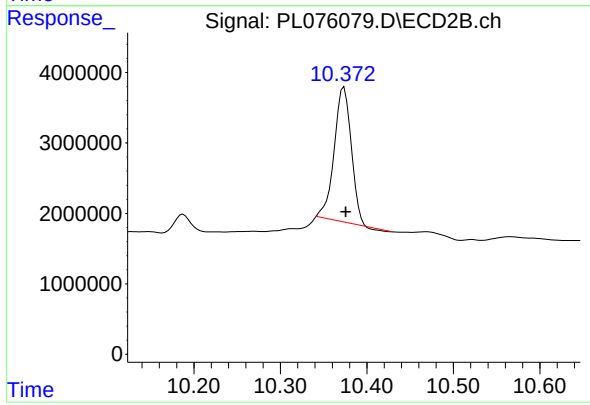

#28 Decachlorobiphenyl

R.T.: 10.374 min
Delta R.T.: -0.002 min
Response: 25644789
Conc: 16.70 ng/ml