

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
 Data File : PL076092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2022 17:25
 Operator : AR\AJ
 Sample : N3442-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 28 22:35:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.632	9494971	23923158	12.554m	12.614m
28)	SA Decachlor...	11.633	10.369	5030268	16322208	7.994	10.627 #
Target Compounds							
12)	B 4,4'-DDE	8.658	7.613	3643229	11347489	5.390m	6.685m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062822\
Data File : PL076092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2022 17:25
Operator : AR\AJ
Sample : N3442-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 28 22:35:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

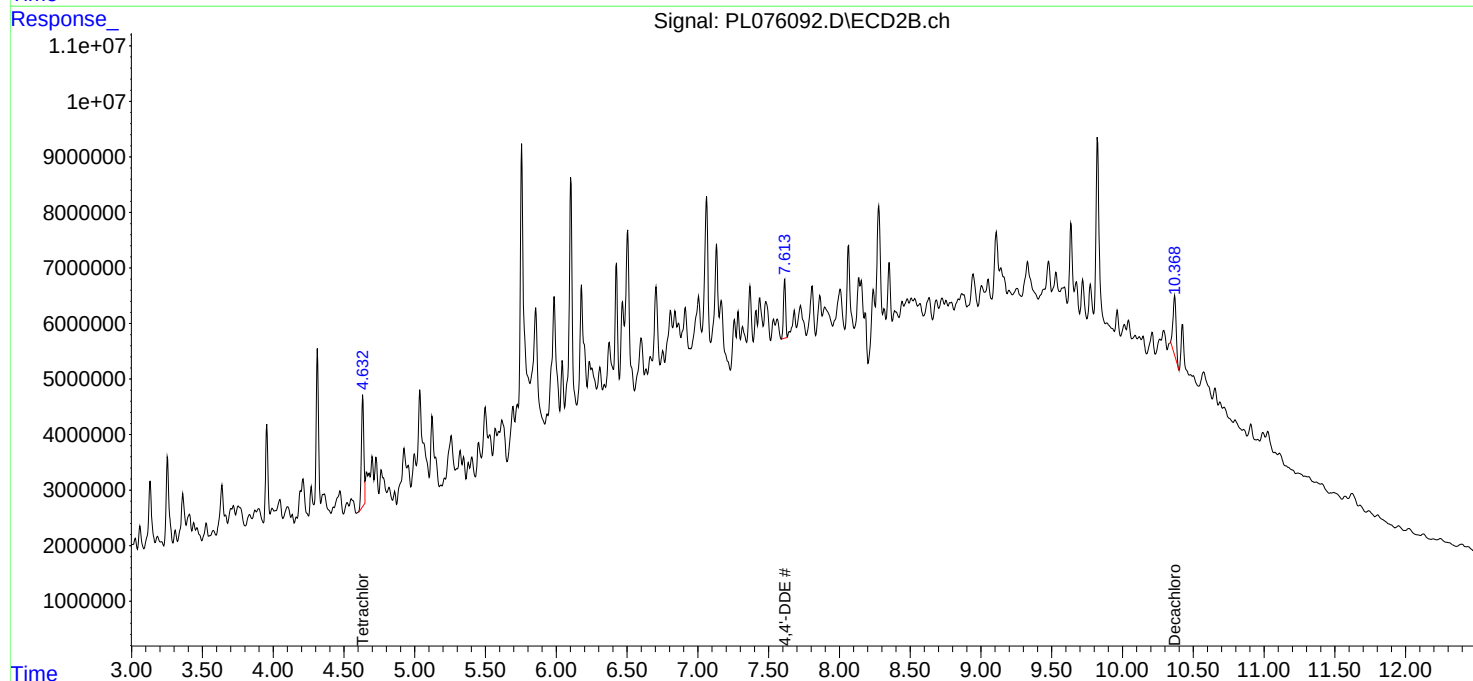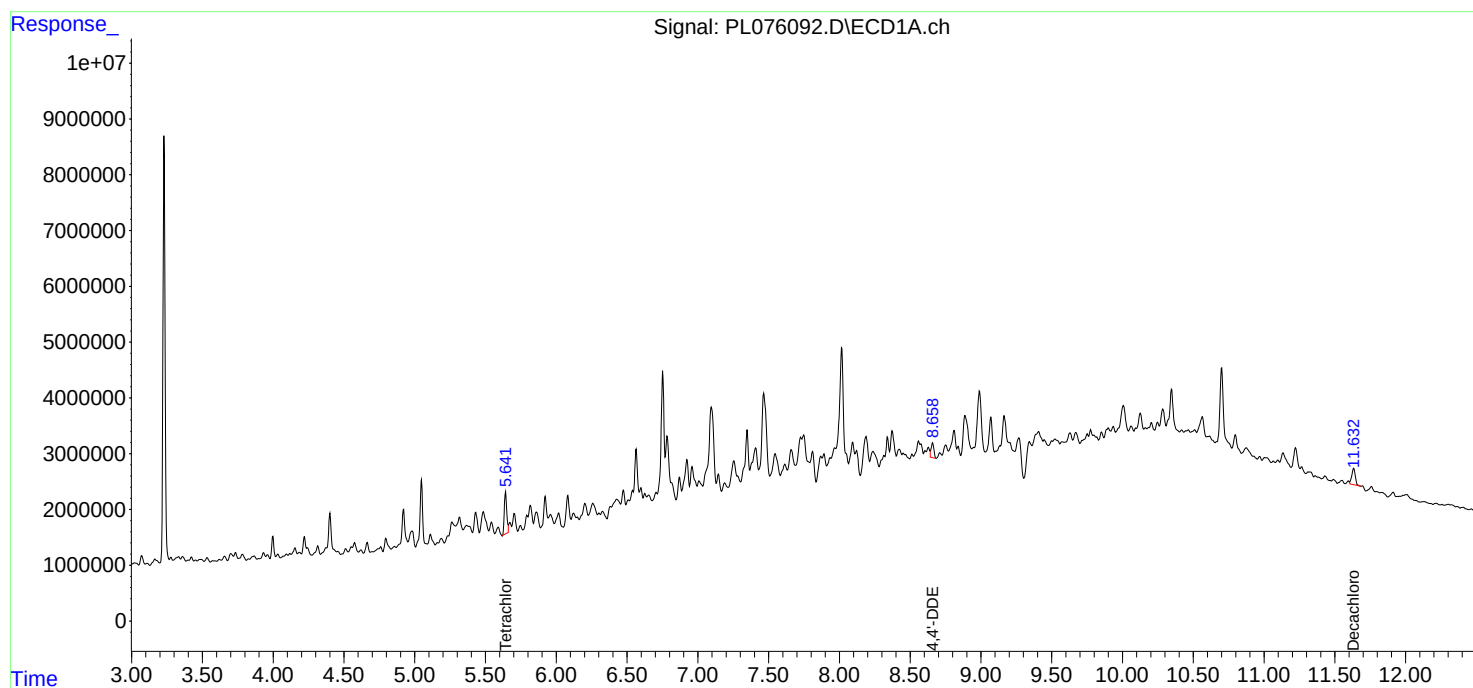


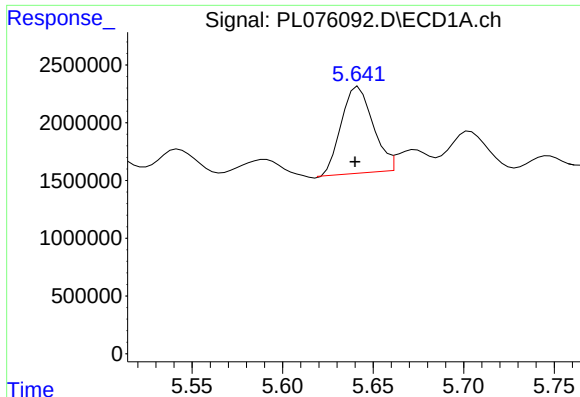

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 9494971
Conc: 12.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

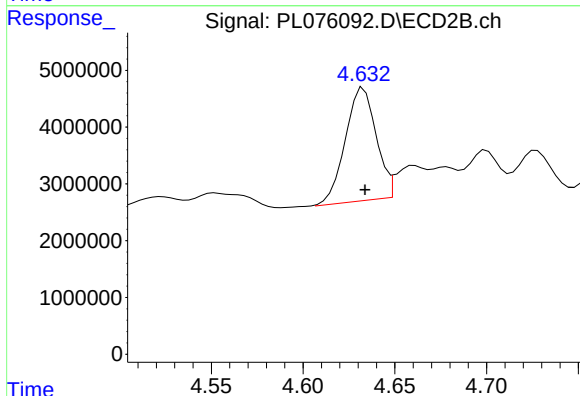


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 23923158
Conc: 12.61 ng/ml m

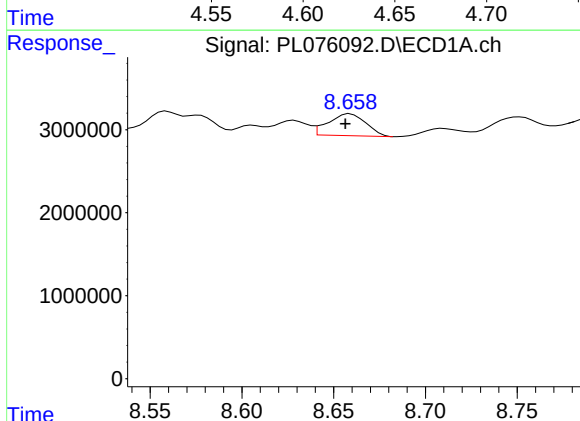


#12 4,4'-DDE

R.T.: 8.658 min
Delta R.T.: 0.001 min
Response: 3643229
Conc: 5.39 ng/ml m

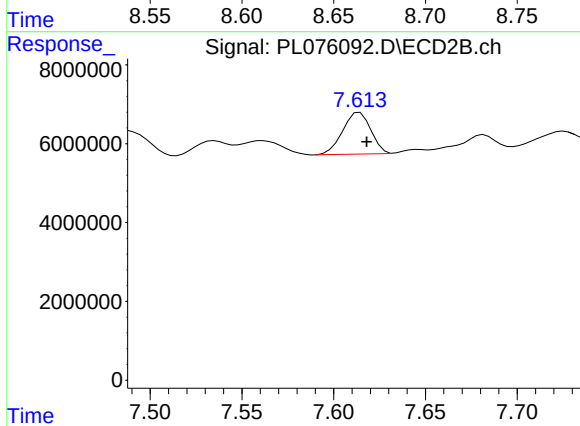

#12 4,4'-DDE


R.T.: 7.613 min
Delta R.T.: -0.005 min
Response: 11347489
Conc: 6.69 ng/ml m

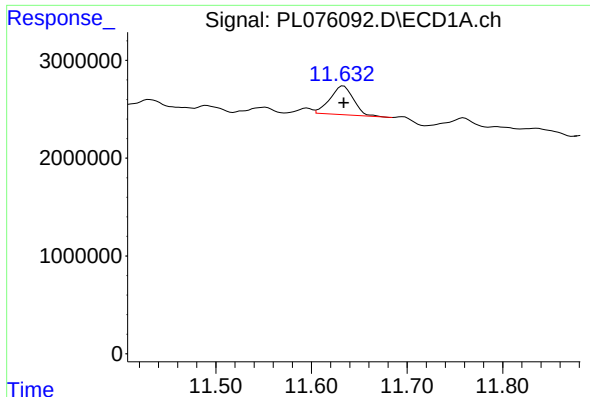

#28 Decachlorobiphenyl

R.T.: 11.633 min
Delta R.T.: 0.000 min
Response: 5030268
Conc: 7.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

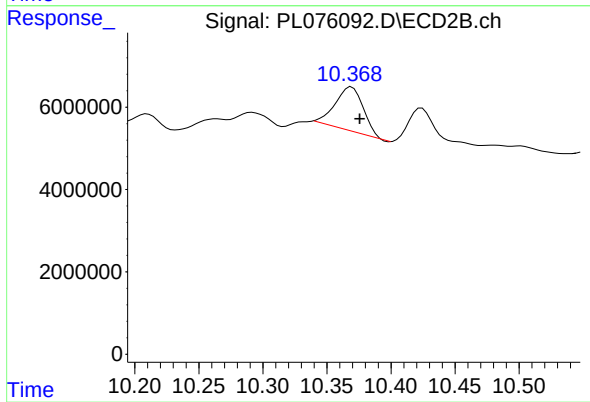

#28 Decachlorobiphenyl

R.T.: 10.369 min
Delta R.T.: -0.006 min
Response: 16322208
Conc: 10.63 ng/ml