

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062823\
 Data File : PL083763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2023 14:08
 Operator : AR\AJ
 Sample : 03428-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PNNL-APM-0621-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 02:23:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 26 10:45:09 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.431	2.693	26887463	31163505	10.821	10.733
28)	SA Decachlor...	8.973	7.881	22324963	30850409	13.072	12.477

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062823\
Data File : PL083763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2023 14:08
Operator : AR\AJ
Sample : 03428-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PNNL-APM-0621-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 02:23:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062523.M
Quant Title : GC Extractables
QLast Update : Mon Jun 26 10:45:09 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

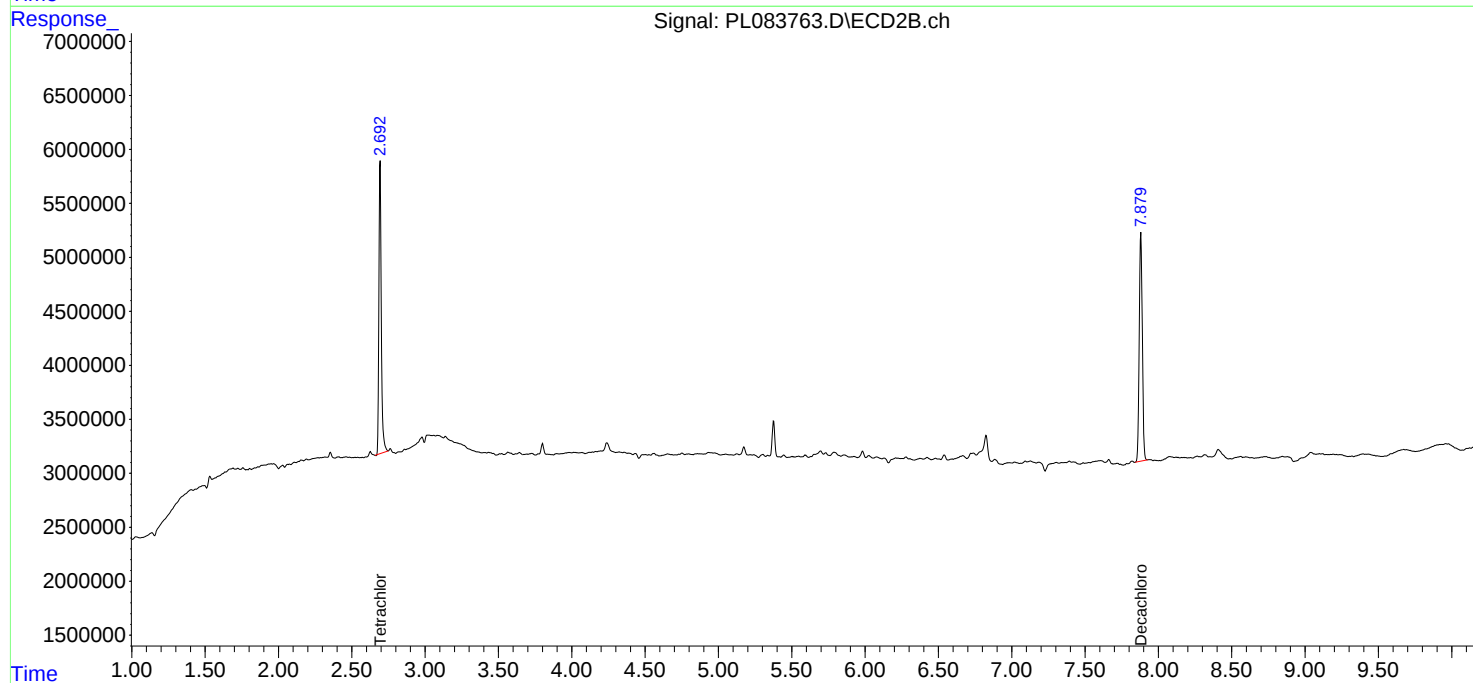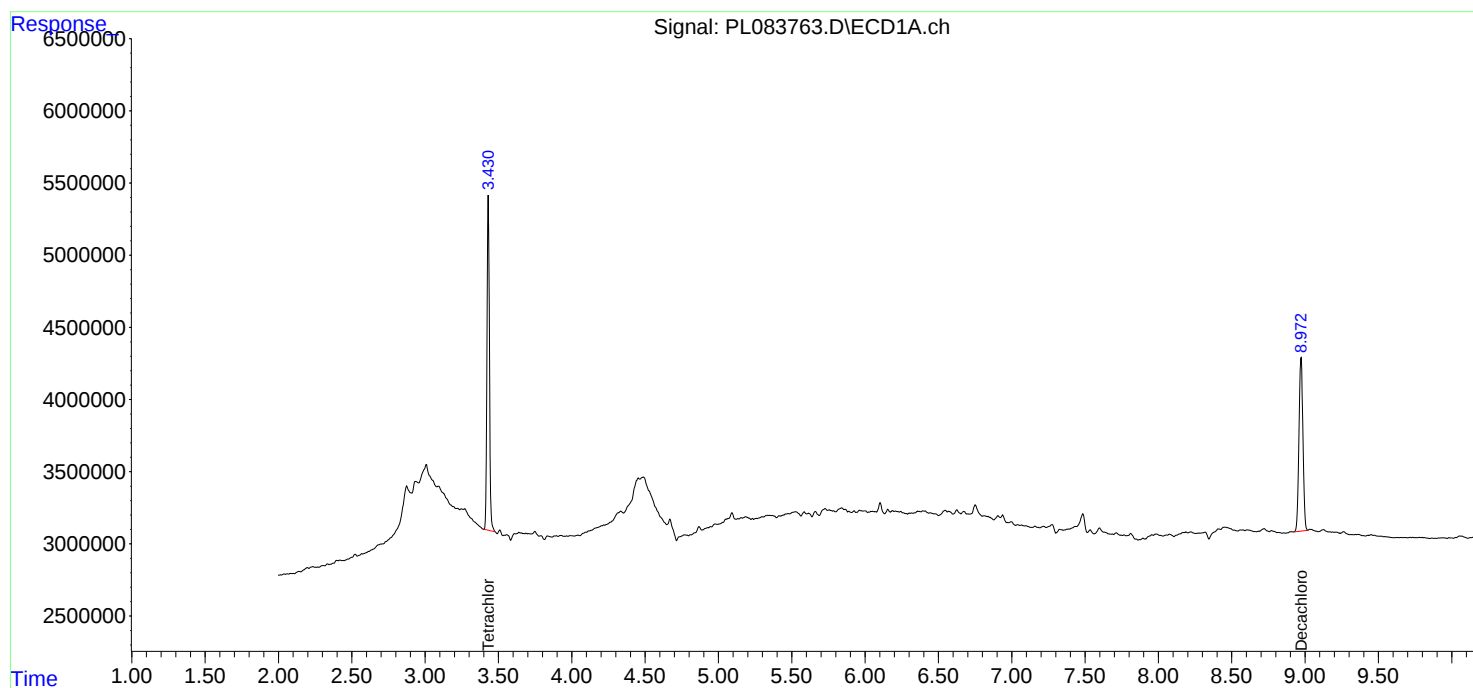


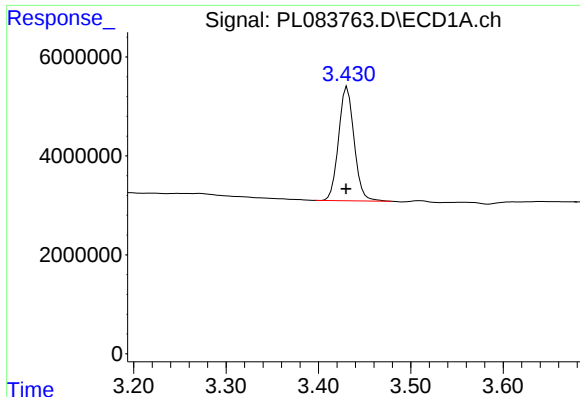

#1 Tetrachloro-m-xylene


R.T.: 3.431 min
Delta R.T.: 0.001 min
Response: 26887463
Conc: 10.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PNNL-APM-0621-2

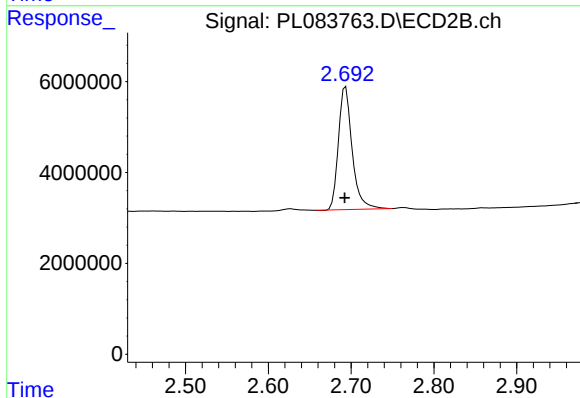


#1 Tetrachloro-m-xylene

R.T.: 2.693 min
Delta R.T.: 0.001 min
Response: 31163505
Conc: 10.73 ng/ml

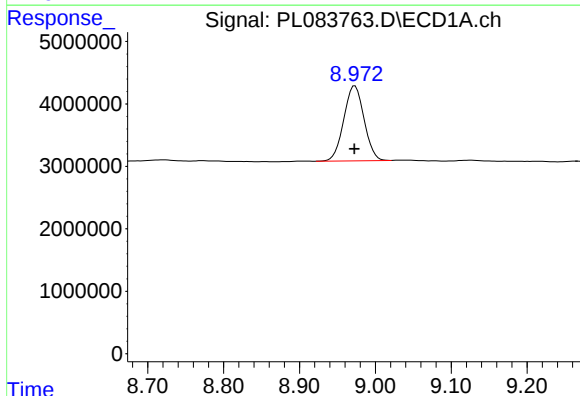

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: 0.000 min
Response: 22324963
Conc: 13.07 ng/ml

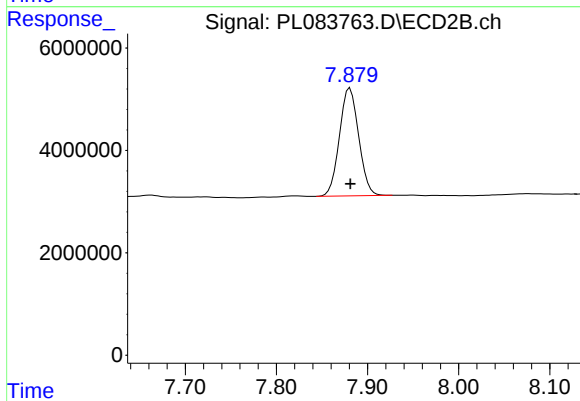

#28 Decachlorobiphenyl

R.T.: 7.881 min
Delta R.T.: 0.000 min
Response: 30850409
Conc: 12.48 ng/ml