

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
 Data File : PL090384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 16:14
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:55:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 29 04:54:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.790	10135754	6861493	5.185	4.982
27)	SA Decachlor...	9.057	7.934	14912188	14302594	9.574	9.760
Target Compounds							
2)	A alpha-BHC	4.001	3.293	14333285	8305184	5.162	4.371
3)	MA gamma-BHC...	4.334	3.624	13366625	8147469	5.030	4.443
4)	MA Heptachlor	4.923	3.965	13943535	8699481	5.373	4.639
9)	A Endosulfan I	6.075	5.118	11748337	7713988	5.420	4.900
13)	MA Dieldrin	6.349	5.382	23192997	15877659	10.630	9.123
14)	MA Endrin	6.579	5.657	19595429	14003561	10.492	9.007
16)	A 4,4'-DDD	6.712	5.805	15715963	10983336	10.373	8.712
17)	MA 4,4'-DDT	7.027	6.056	16864064	12432189	10.471	8.877
20)	A Methoxychlor	7.502	6.631	42313208	37401084	53.792	48.558


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
Data File : PL090384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 16:14
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:55:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 29 04:54:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

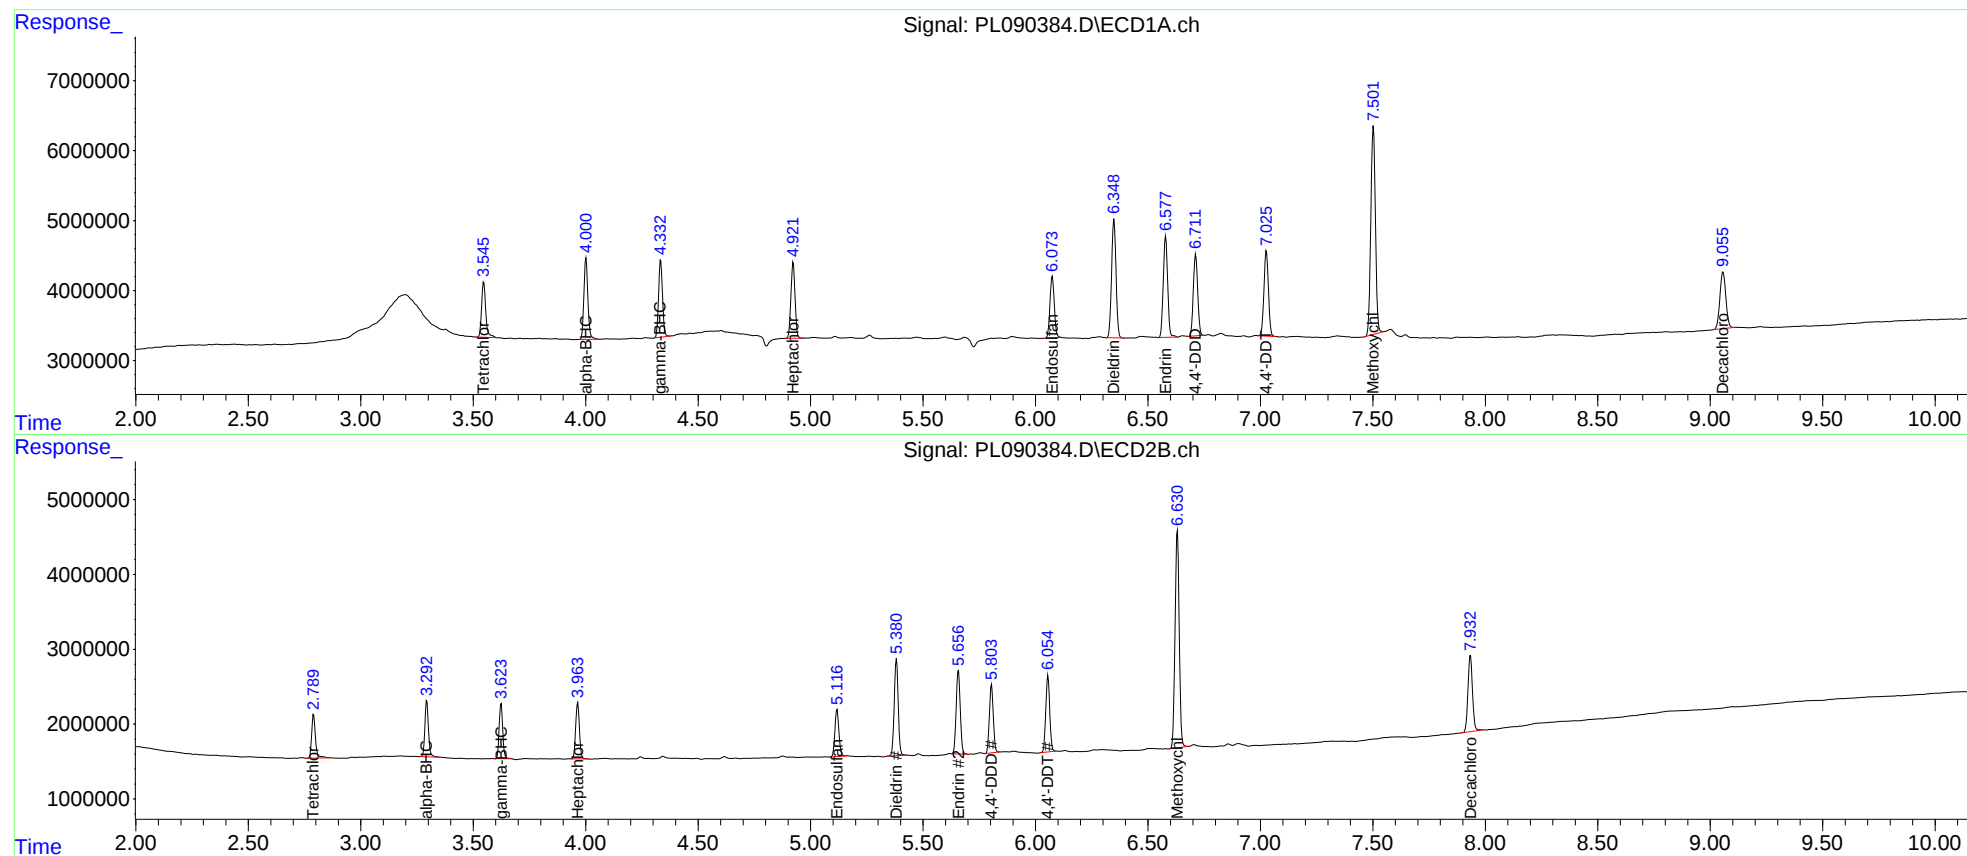

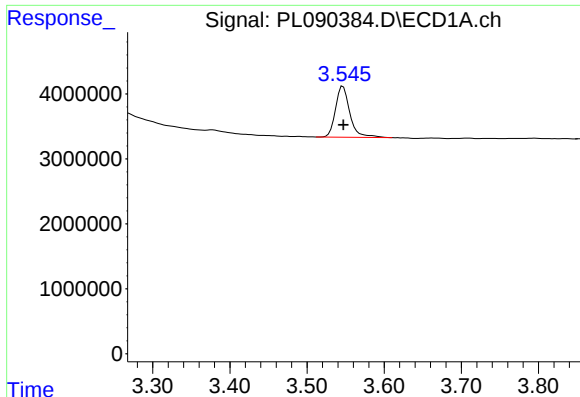


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 10135754
Conc: 5.18 ng/ml

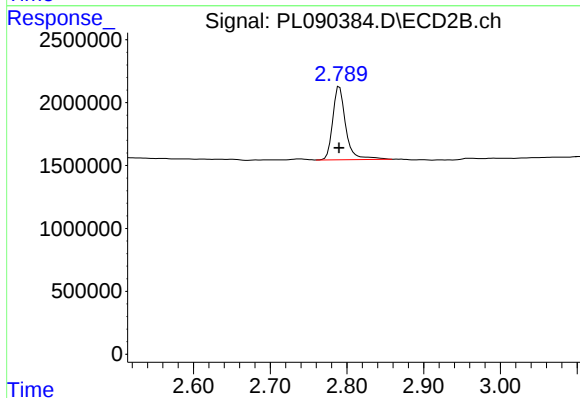


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 6861493
Conc: 4.98 ng/ml

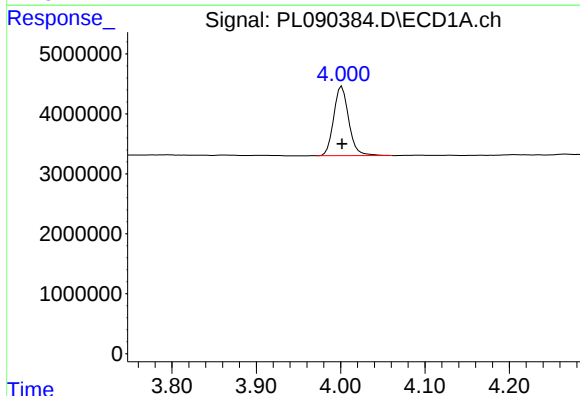


#2 alpha-BHC

R.T.: 4.001 min
Delta R.T.: 0.000 min
Response: 14333285
Conc: 5.16 ng/ml

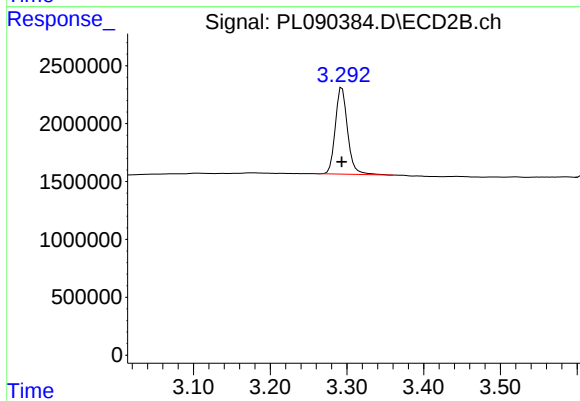


#2 alpha-BHC

R.T.: 3.293 min
Delta R.T.: 0.000 min
Response: 8305184
Conc: 4.37 ng/ml

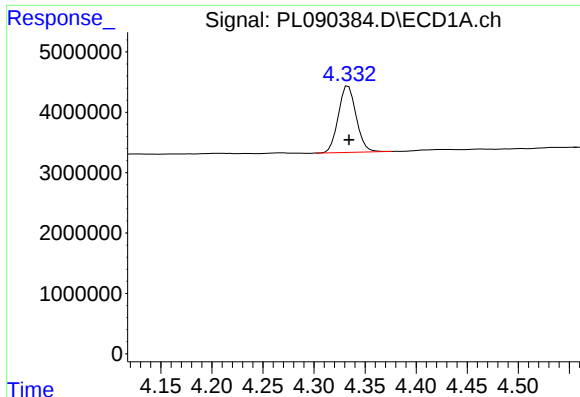


#3 gamma-BHC (Lindane)

R.T.: 4.334 min
Delta R.T.: 0.000 min
Response: 13366625
Conc: 5.03 ng/ml

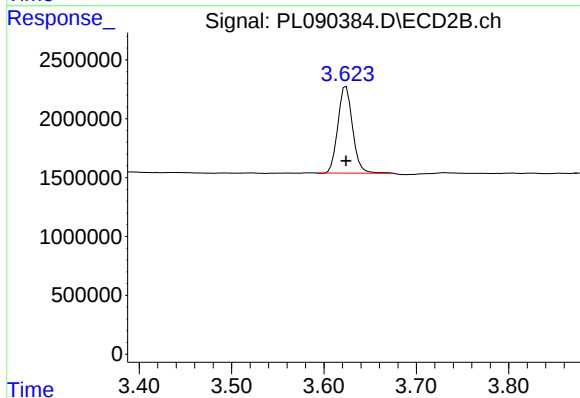


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 8147469
Conc: 4.44 ng/ml

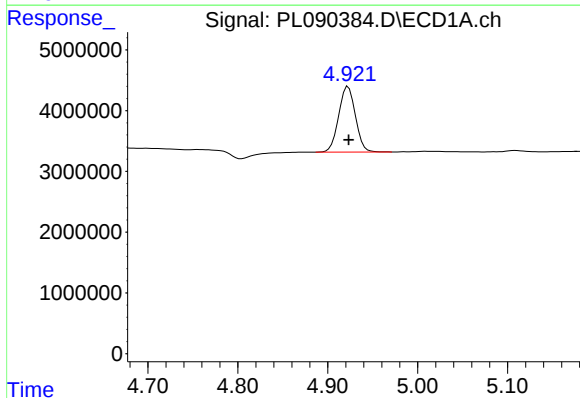


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 13943535
Conc: 5.37 ng/ml

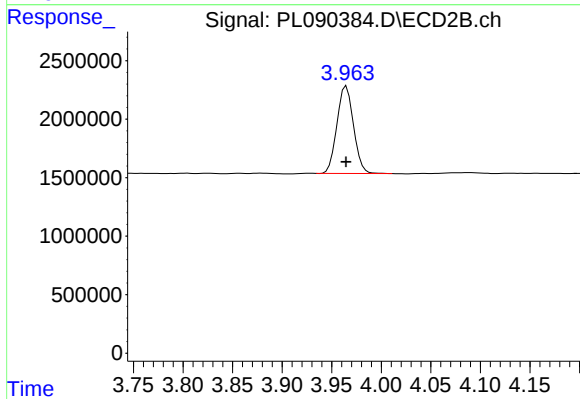


#4 Heptachlor

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 8699481
Conc: 4.64 ng/ml

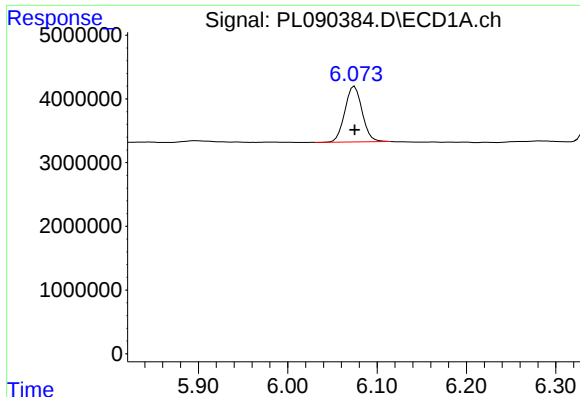


#9 Endosulfan I

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 11748337
Conc: 5.42 ng/ml

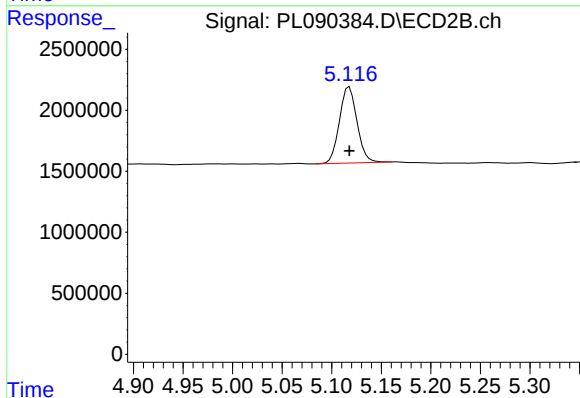


#9 Endosulfan I

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 7713988
Conc: 4.90 ng/ml

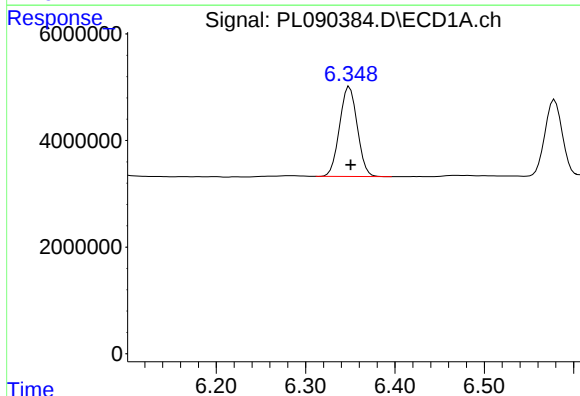


#13 Dieldrin

R.T.: 6.349 min
Delta R.T.: -0.001 min
Response: 23192997
Conc: 10.63 ng/ml

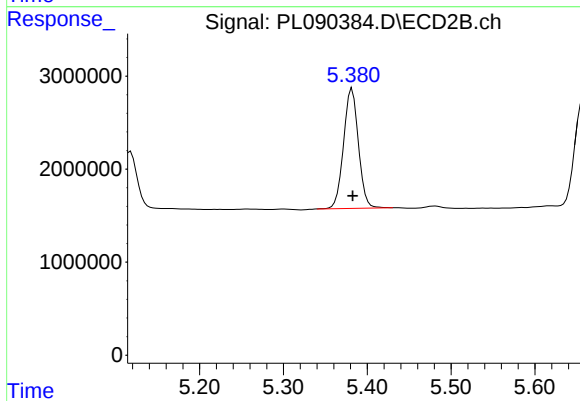


#13 Dieldrin

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 15877659
Conc: 9.12 ng/ml

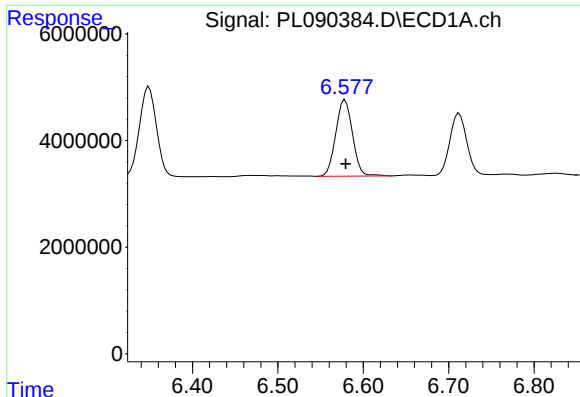


#14 Endrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 19595429
Conc: 10.49 ng/ml

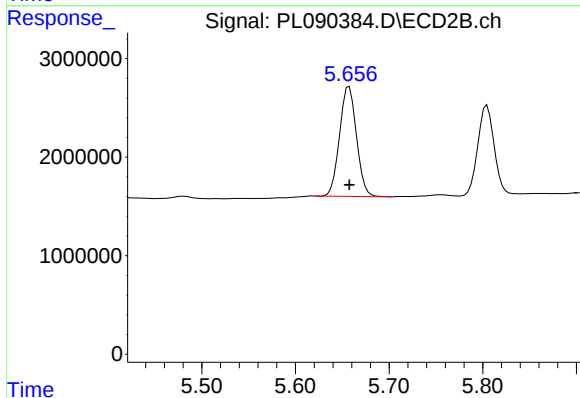


#14 Endrin

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 14003561
Conc: 9.01 ng/ml

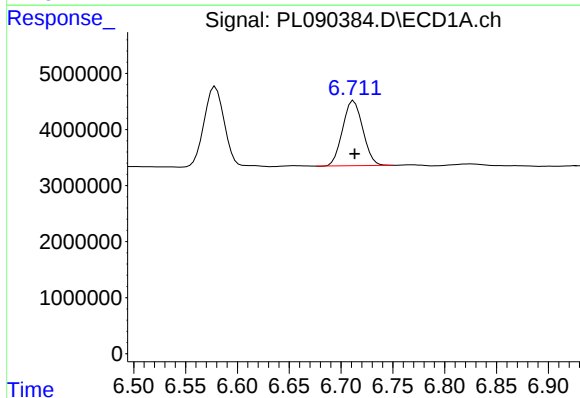


#16 4,4'-DDD

R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 15715963
Conc: 10.37 ng/ml

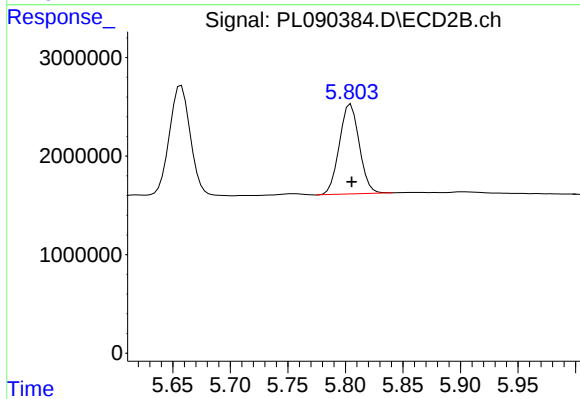


#16 4,4'-DDD

R.T.: 5.805 min
Delta R.T.: 0.000 min
Response: 10983336
Conc: 8.71 ng/ml

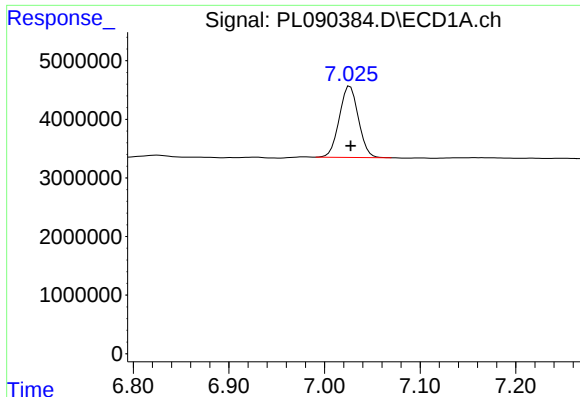


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 16864064
Conc: 10.47 ng/ml

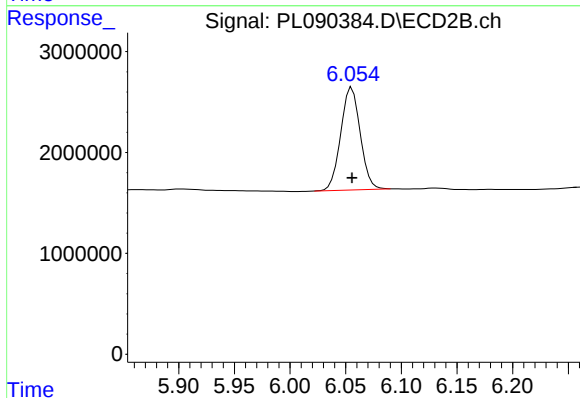


#17 4,4'-DDT

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 12432189
Conc: 8.88 ng/ml

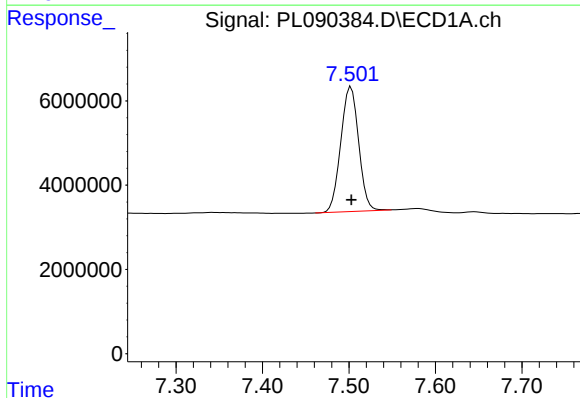


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 42313208
Conc: 53.79 ng/ml

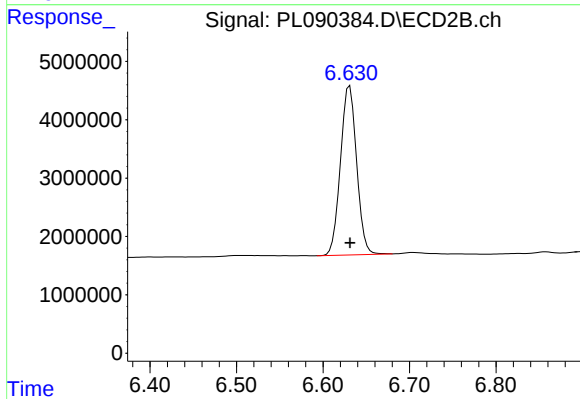


#20 Methoxychlor

R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 37401084
Conc: 48.56 ng/ml

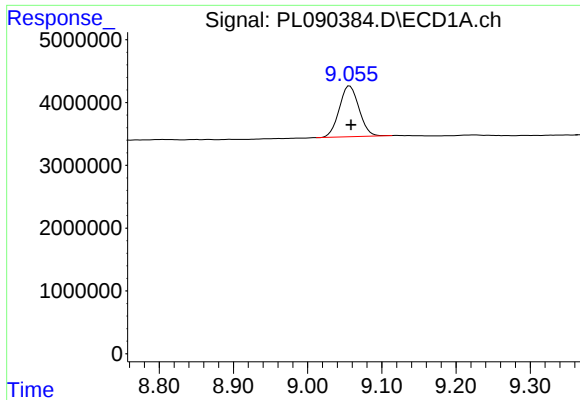

#27 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.002 min
Response: 14912188
Conc: 9.57 ng/ml

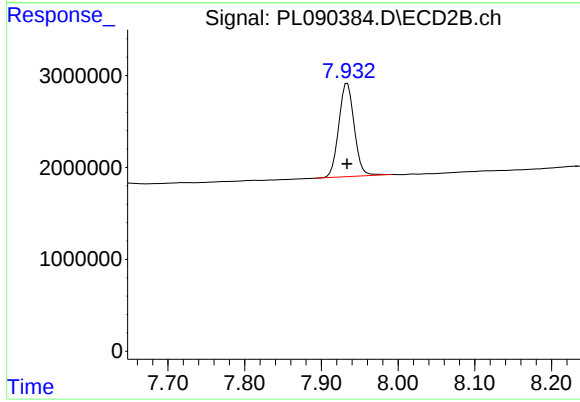

#27 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 14302594
Conc: 9.76 ng/ml