

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
 Data File : PL090386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 16:42
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:56:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 29 04:54:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.790	22599716	15046153	11.560	10.925
27)	SA Decachlor...	9.058	7.933	33279116	32654876	21.366	22.285
Target Compounds							
2)	A alpha-BHC	4.002	3.293	31554975	20042758	11.365	10.548
3)	MA gamma-BHC...	4.334	3.624	30317070	19595849	11.410	10.686
4)	MA Heptachlor	4.923	3.965	30290430	20232992	11.673	10.788
9)	A Endosulfan I	6.075	5.117	25357589	17289760	11.698	10.984
13)	MA Dieldrin	6.350	5.382	50632125	37378325	23.206	21.477
14)	MA Endrin	6.579	5.657	44345695	33819111	23.745	21.752
16)	A 4,4'-DDD	6.713	5.805	35312072	27175718	23.308	21.555
17)	MA 4,4'-DDT	7.027	6.056	37443458	30066192	23.248	21.469
20)	A Methoxychlor	7.503	6.631	92106979	86908279	117.094	112.834


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
Data File : PL090386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 16:42
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:56:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 29 04:54:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

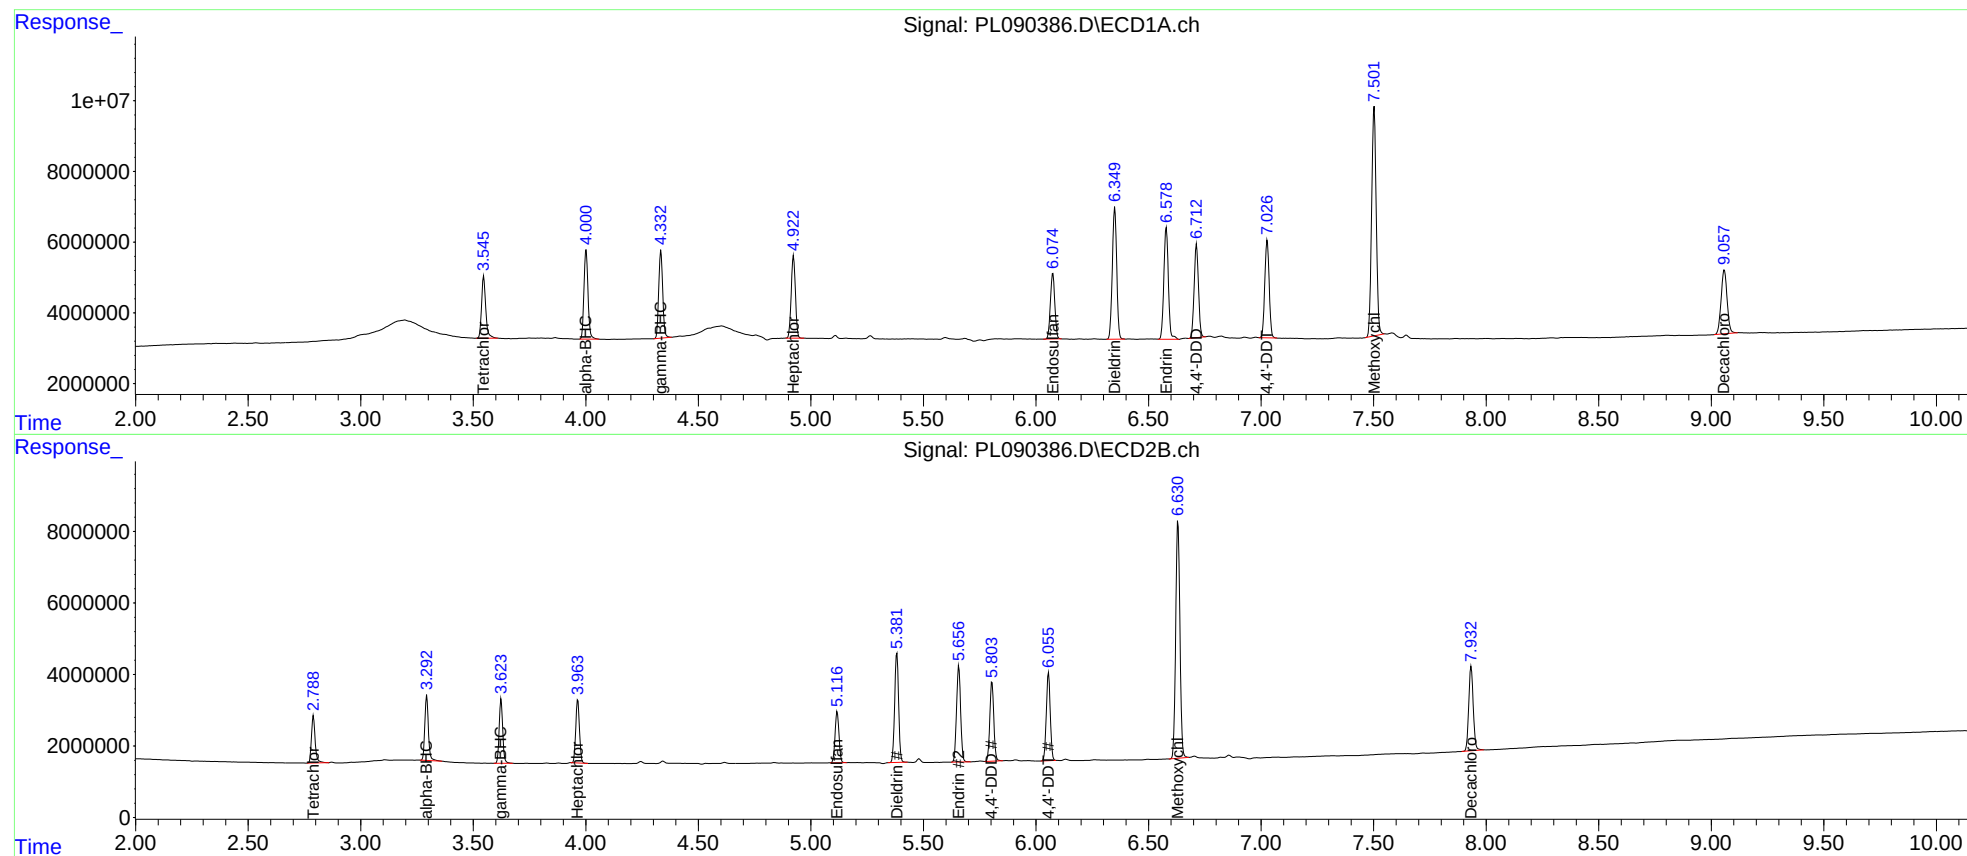

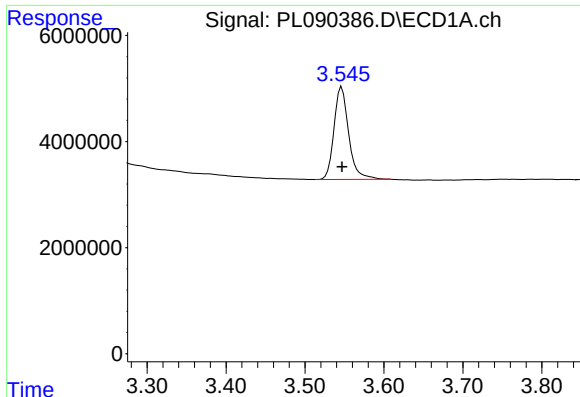


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 22599716
Conc: 11.56 ng/ml

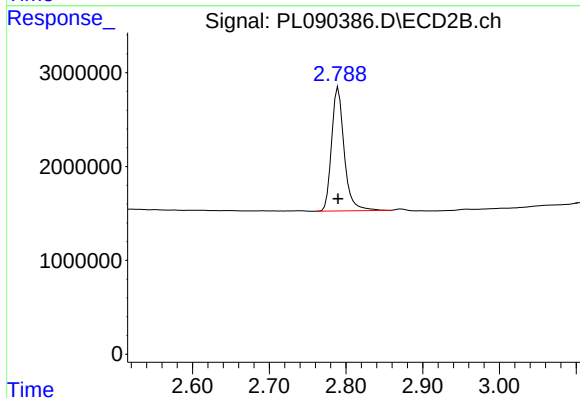


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 15046153
Conc: 10.92 ng/ml

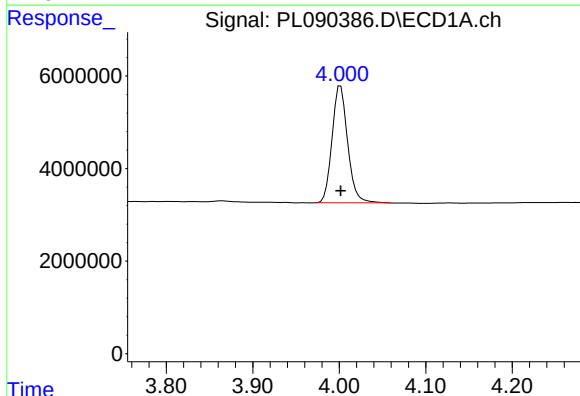


#2 alpha-BHC

R.T.: 4.002 min
Delta R.T.: 0.000 min
Response: 31554975
Conc: 11.36 ng/ml

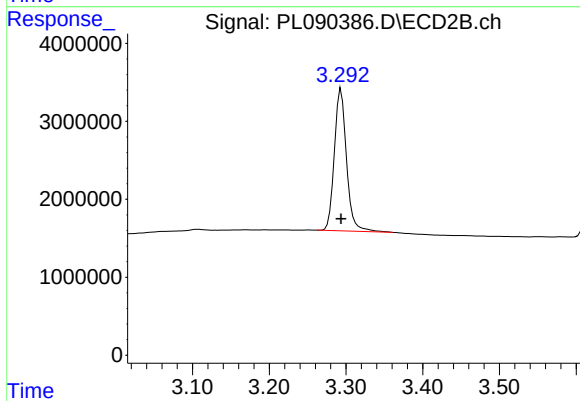


#2 alpha-BHC

R.T.: 3.293 min
Delta R.T.: 0.000 min
Response: 20042758
Conc: 10.55 ng/ml

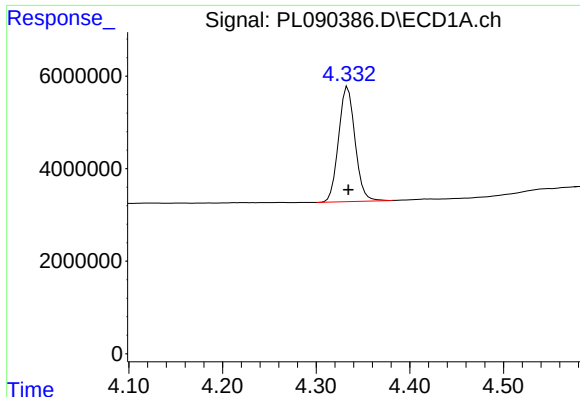


#3 gamma-BHC (Lindane)

R.T.: 4.334 min
Delta R.T.: 0.000 min
Response: 30317070
Conc: 11.41 ng/ml

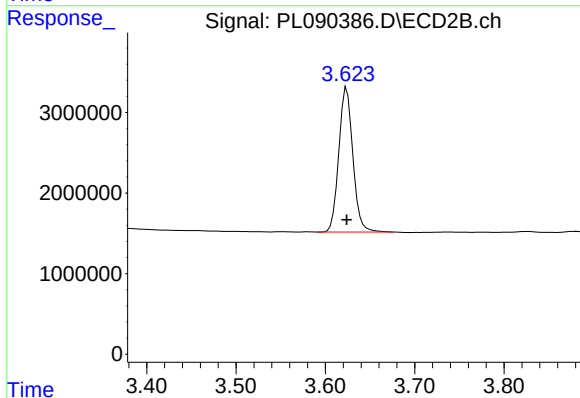


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 19595849
Conc: 10.69 ng/ml

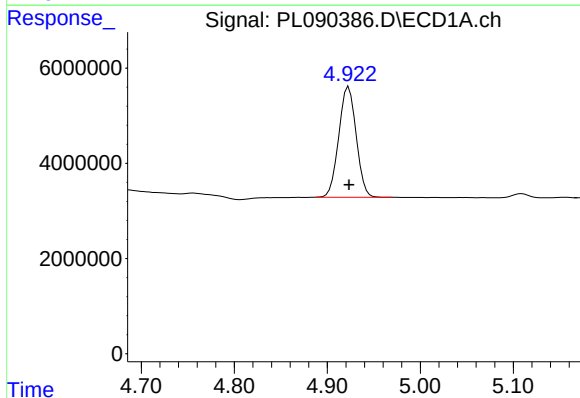


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 30290430
Conc: 11.67 ng/ml

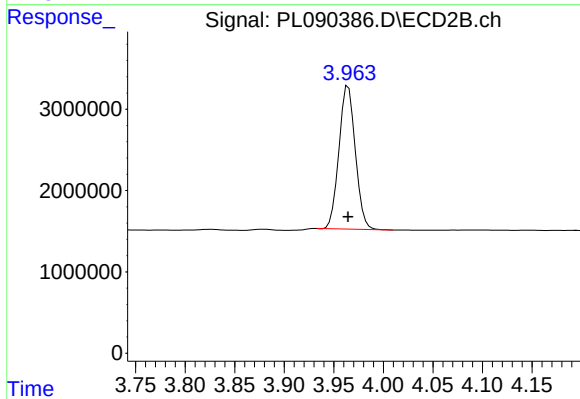


#4 Heptachlor

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 20232992
Conc: 10.79 ng/ml

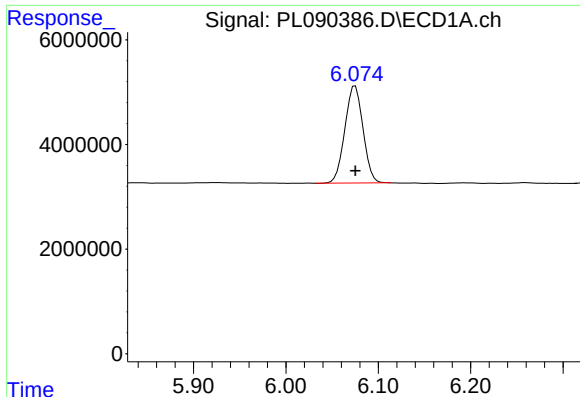


#9 Endosulfan I

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 25357589
Conc: 11.70 ng/ml

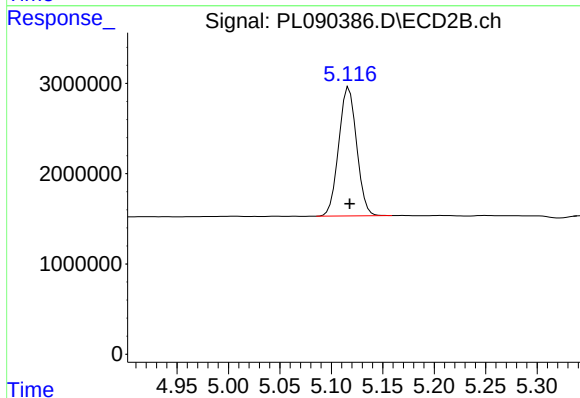


#9 Endosulfan I

R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 17289760
Conc: 10.98 ng/ml

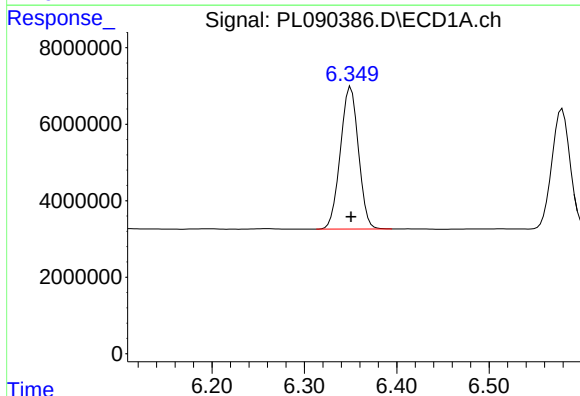


#13 Dieldrin

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 50632125
Conc: 23.21 ng/ml

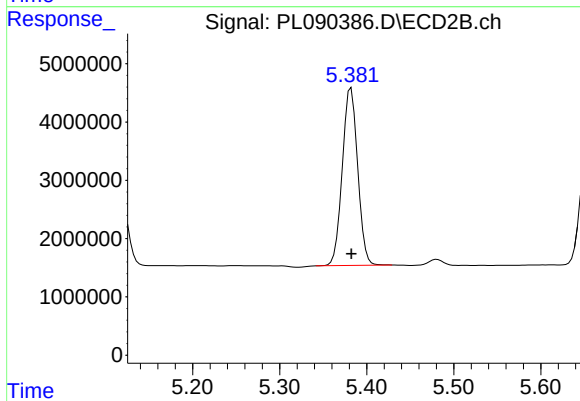


#13 Dieldrin

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 37378325
Conc: 21.48 ng/ml

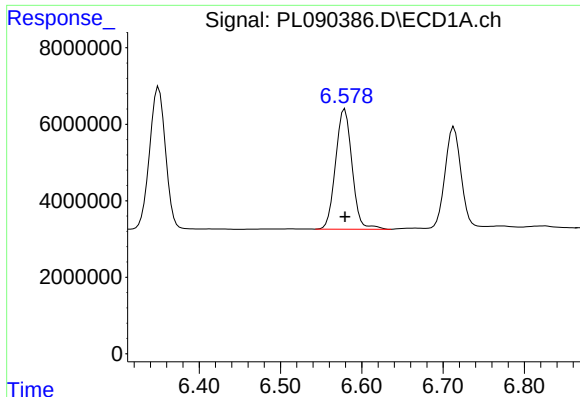


#14 Endrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 44345695
Conc: 23.75 ng/ml

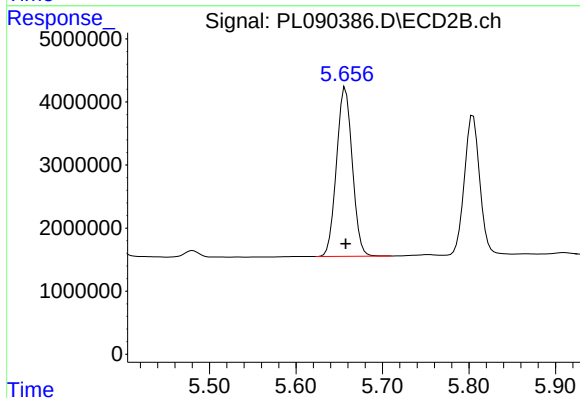


#14 Endrin

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 33819111
Conc: 21.75 ng/ml

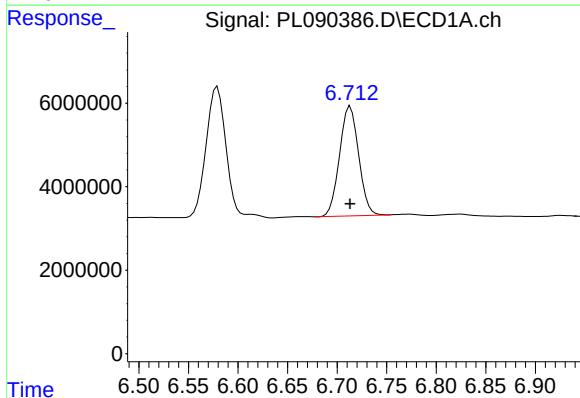


#16 4,4'-DDD

R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 35312072
Conc: 23.31 ng/ml

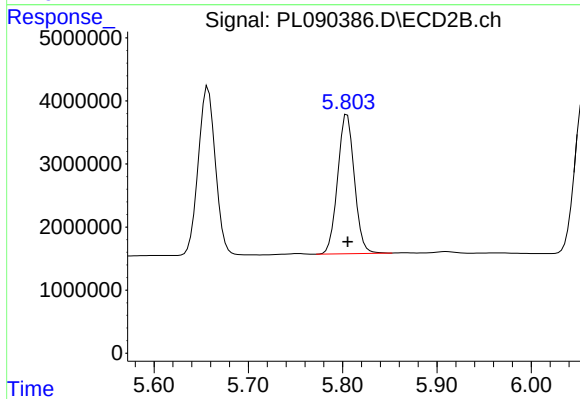


#16 4,4'-DDD

R.T.: 5.805 min
Delta R.T.: 0.000 min
Response: 27175718
Conc: 21.55 ng/ml

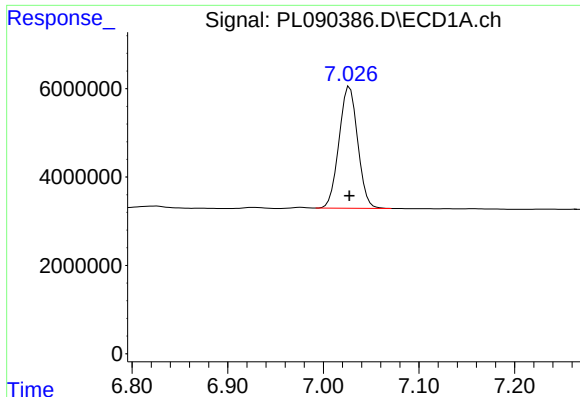


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 37443458
Conc: 23.25 ng/ml

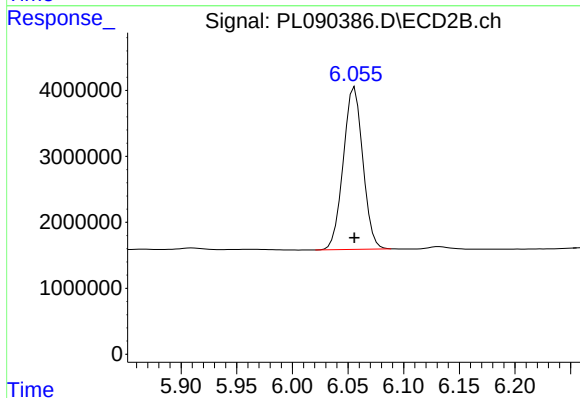


#17 4,4'-DDT

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 30066192
Conc: 21.47 ng/ml

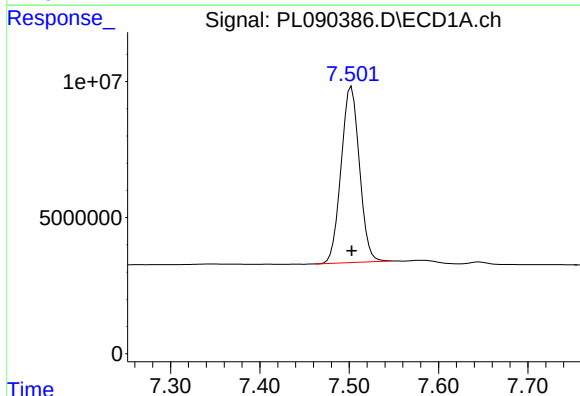


#20 Methoxychlor

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 92106979
Conc: 117.09 ng/ml

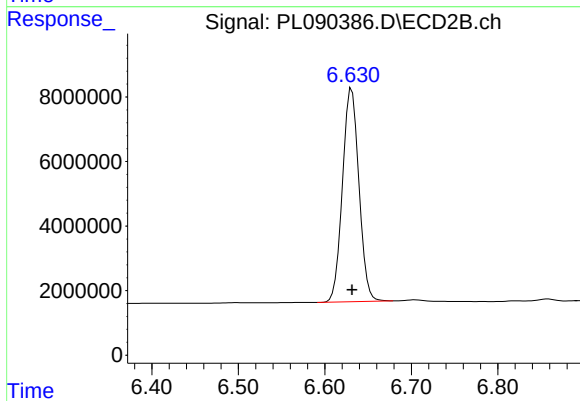


#20 Methoxychlor

R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 86908279
Conc: 112.83 ng/ml

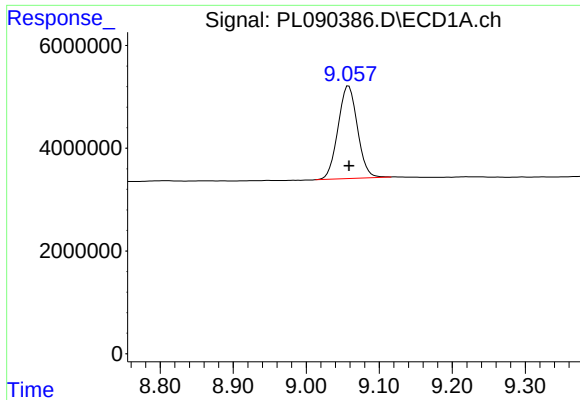

#27 Decachlorobiphenyl

R.T.: 9.058 min
Delta R.T.: 0.000 min
Response: 33279116
Conc: 21.37 ng/ml

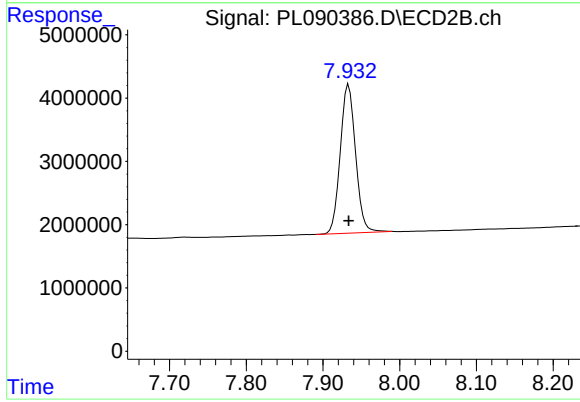

#27 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 32654876
Conc: 22.28 ng/ml