

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
 Data File : PL090388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 17:09
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:56:36 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 29 04:54:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.790	39098336	27545017	20.000	20.000
27)	SA Decachlor...	9.059	7.934	62303635	58614206	40.000	40.000
Target Compounds							
2)	A alpha-BHC	4.002	3.293	55532220	38003909	20.000	20.000
3)	MA gamma-BHC...	4.334	3.624	53142711	36675635	20.000	20.000
4)	MA Heptachlor	4.923	3.965	51898083	37508941	20.000	20.000
9)	A Endosulfan I	6.075	5.118	43355193	31482708	20.000	20.000
13)	MA Dieldrin	6.350	5.382	87275250	69614507	40.000	40.000
14)	MA Endrin	6.579	5.657	74703136	62191488	40.000	40.000
16)	A 4,4'-DDD	6.713	5.805	60601973	50431009	40.000	40.000
17)	MA 4,4'-DDT	7.027	6.056	64423183	56017375	40.000	40.000
20)	A Methoxychlor	7.503	6.631	157.3E6	154.0E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
Data File : PL090388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 17:09
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:56:36 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 29 04:54:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

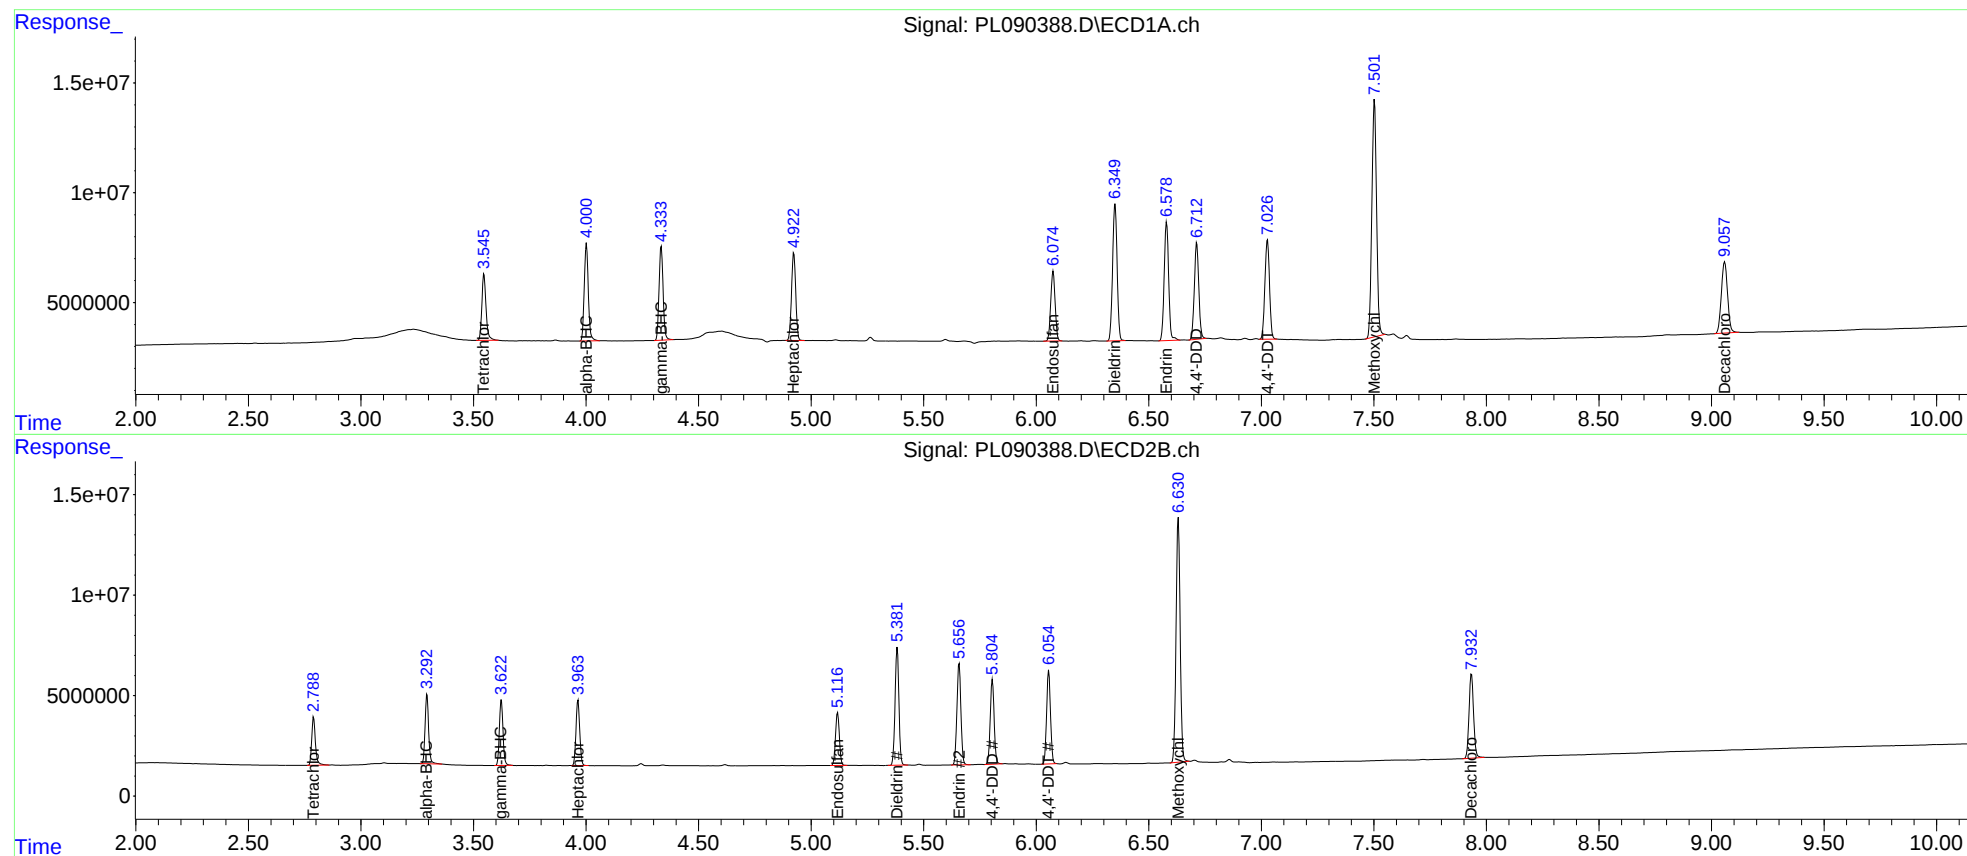

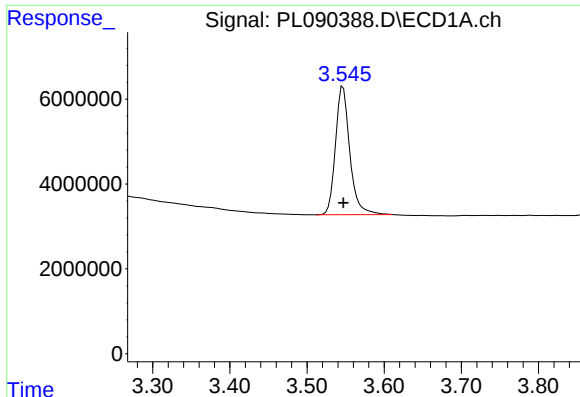


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 39098336
Conc: 20.00 ng/ml

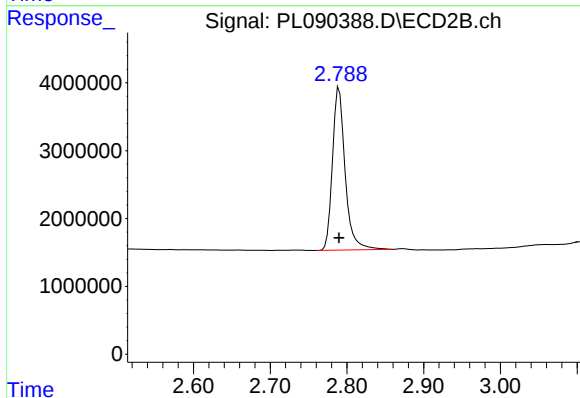


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 27545017
Conc: 20.00 ng/ml

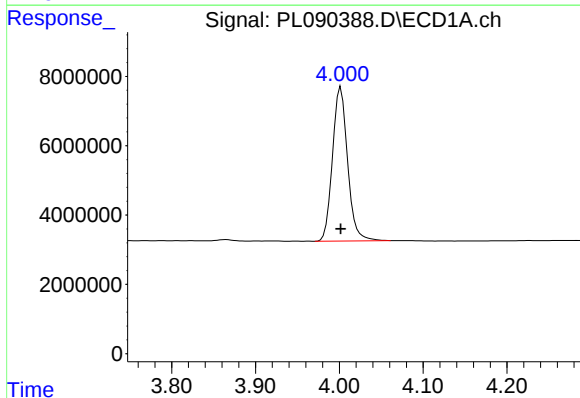


#2 alpha-BHC

R.T.: 4.002 min
Delta R.T.: 0.000 min
Response: 55532220
Conc: 20.00 ng/ml

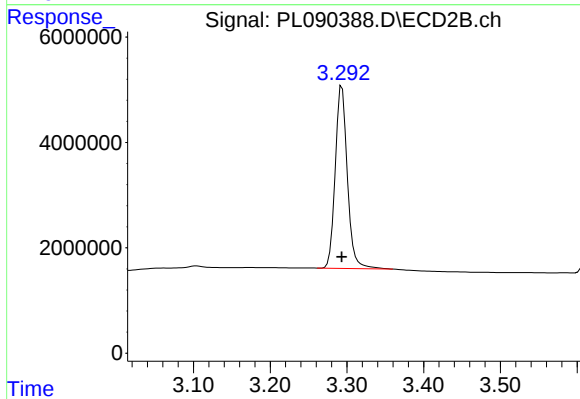


#2 alpha-BHC

R.T.: 3.293 min
Delta R.T.: 0.000 min
Response: 38003909
Conc: 20.00 ng/ml

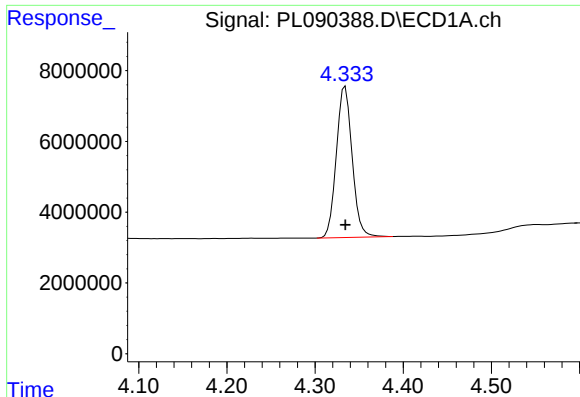


#3 gamma-BHC (Lindane)

R.T.: 4.334 min
Delta R.T.: 0.000 min
Response: 53142711
Conc: 20.00 ng/ml

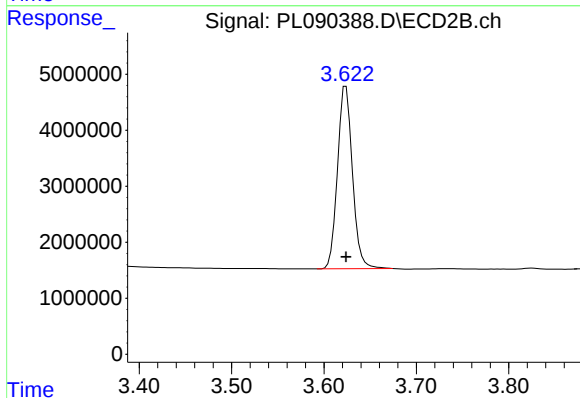


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 36675635
Conc: 20.00 ng/ml

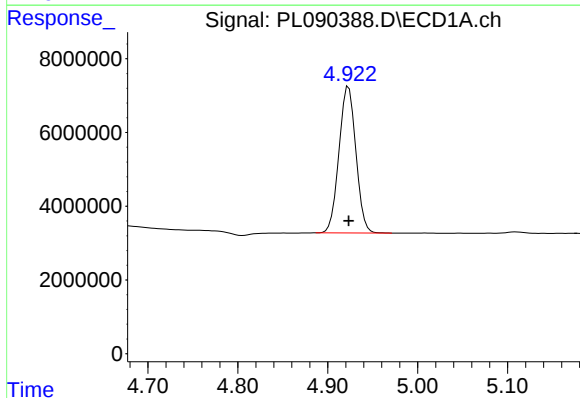


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 51898083
Conc: 20.00 ng/ml

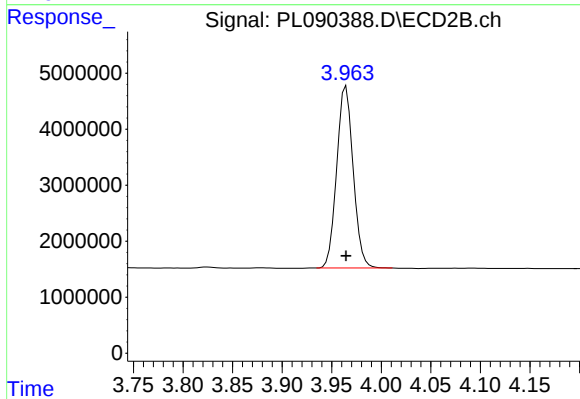


#4 Heptachlor

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 37508941
Conc: 20.00 ng/ml

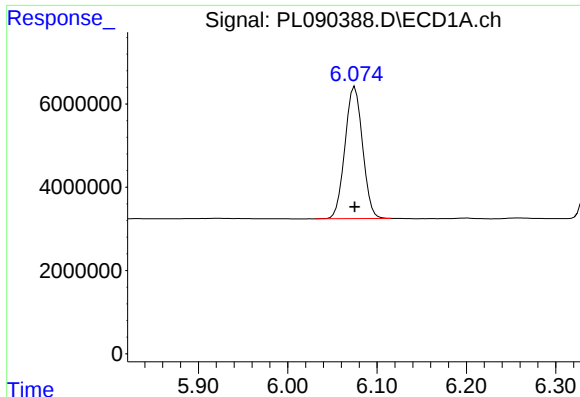


#9 Endosulfan I

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 43355193
Conc: 20.00 ng/ml

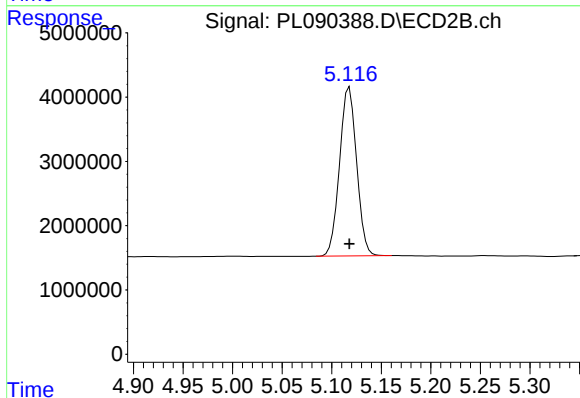


#9 Endosulfan I

R.T.: 5.118 min
Delta R.T.: 0.000 min
Response: 31482708
Conc: 20.00 ng/ml

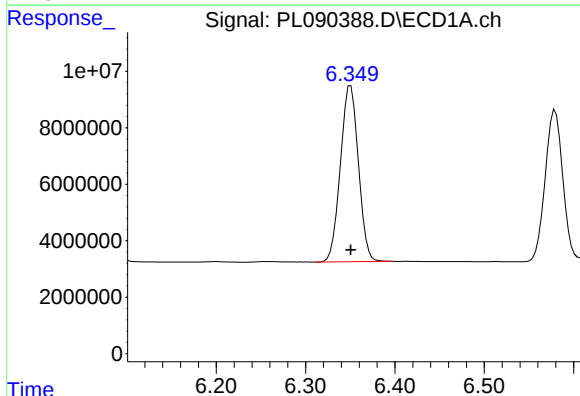


#13 Dieldrin

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 87275250
Conc: 40.00 ng/ml

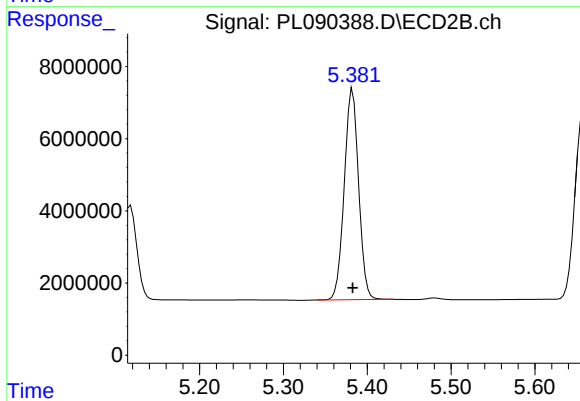


#13 Dieldrin

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 69614507
Conc: 40.00 ng/ml

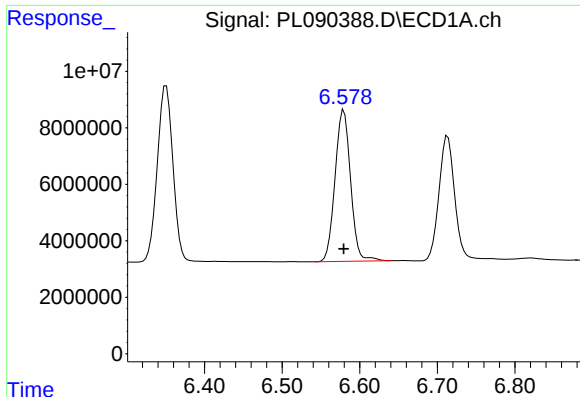


#14 Endrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 74703136
Conc: 40.00 ng/ml

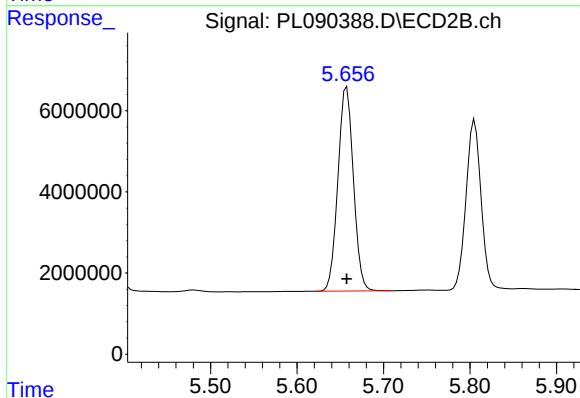


#14 Endrin

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 62191488
Conc: 40.00 ng/ml

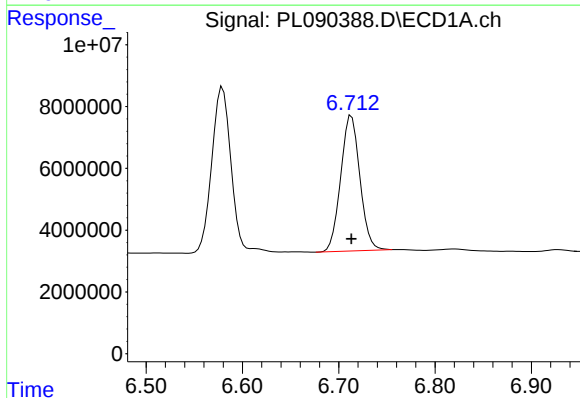


#16 4,4'-DDD

R.T.: 6.713 min
Delta R.T.: 0.000 min
Response: 60601973
Conc: 40.00 ng/ml

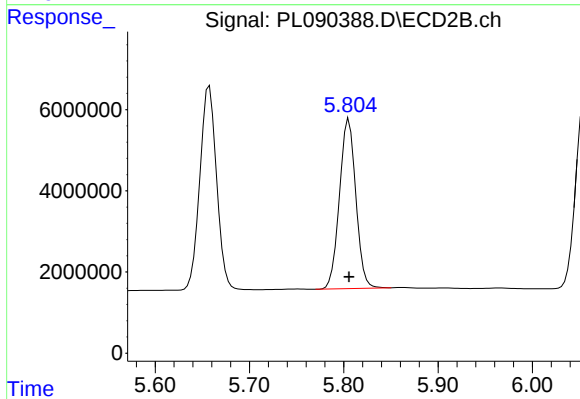


#16 4,4'-DDD

R.T.: 5.805 min
Delta R.T.: 0.000 min
Response: 50431009
Conc: 40.00 ng/ml

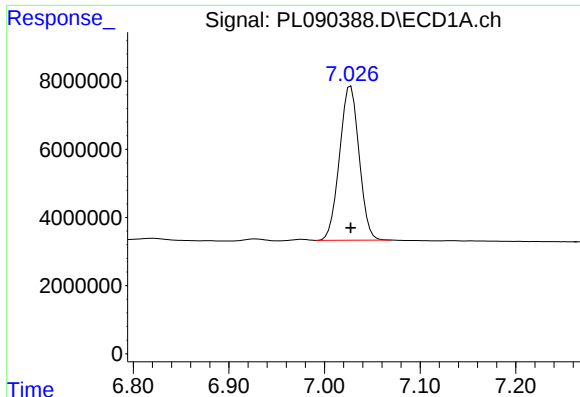


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 64423183
Conc: 40.00 ng/ml

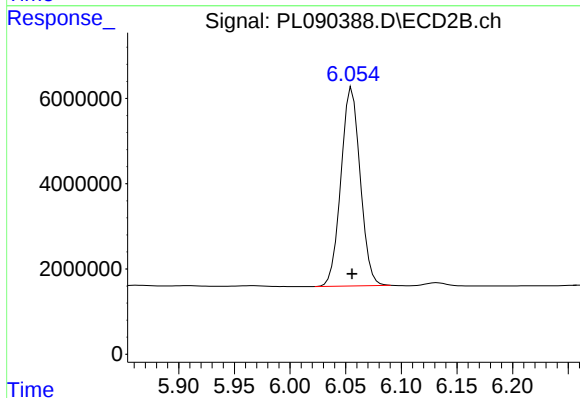


#17 4,4'-DDT

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 56017375
Conc: 40.00 ng/ml

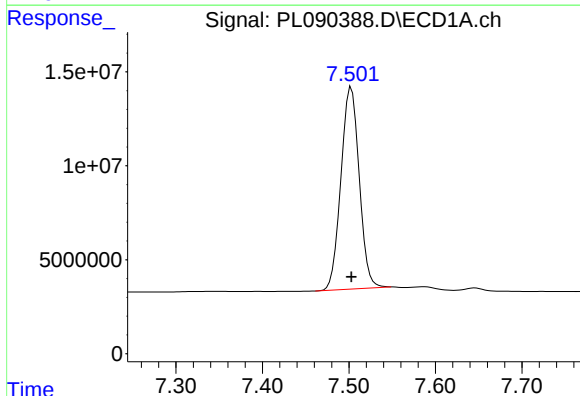


#20 Methoxychlor

R.T.: 7.503 min
Delta R.T.: 0.000 min
Response: 157322039
Conc: 200.00 ng/ml

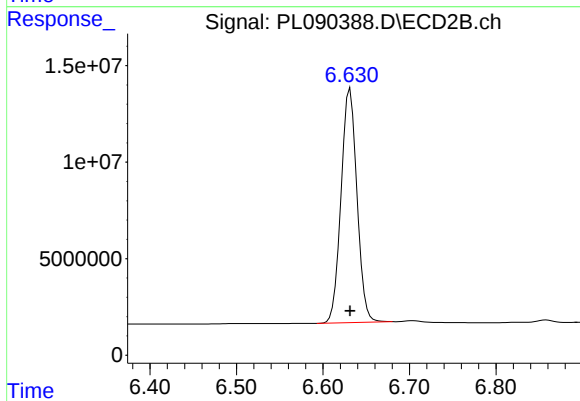


#20 Methoxychlor

R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 154045801
Conc: 200.00 ng/ml

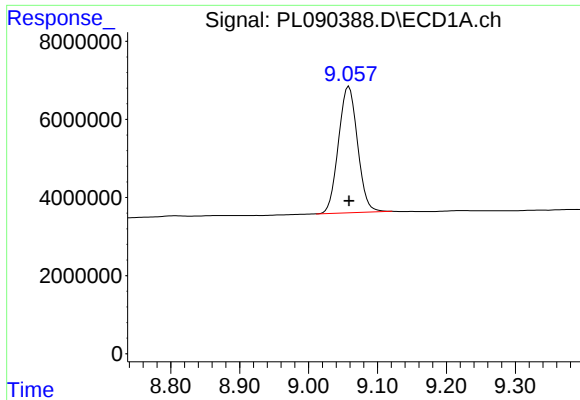

#27 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.000 min
Response: 62303635
Conc: 40.00 ng/ml

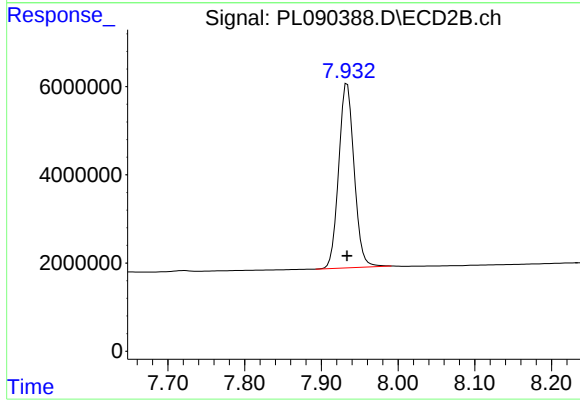

#27 Decachlorobiphenyl

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 58614206
Conc: 40.00 ng/ml