

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
 Data File : PL090390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 17:37
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:56:54 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 29 04:54:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.790	75891355	55383428	38.821	40.213
27)	SA Decachlor...	9.057	7.933	108.0E6	112.4E6	69.366	76.695
Target Compounds							
2)	A alpha-BHC	4.001	3.294	110.9E6	81931768	39.943	43.118
3)	MA gamma-BHC...	4.333	3.624	105.3E6	78254405	39.624	42.674
4)	MA Heptachlor	4.922	3.964	99893523	77267736	38.496	41.200
9)	A Endosulfan I	6.074	5.117	81705245	61990921	37.691	39.381
13)	MA Dieldrin	6.349	5.382	169.7E6	145.8E6	77.784	83.764
14)	MA Endrin	6.579	5.657	149.6E6	129.4E6	80.118	83.241
16)	A 4,4'-DDD	6.712	5.804	118.9E6	107.1E6	78.468	84.932
17)	MA 4,4'-DDT	7.027	6.055	125.2E6	117.5E6	77.715	83.905
20)	A Methoxychlor	7.502	6.630	307.5E6	304.7E6	390.869	395.548


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
Data File : PL090390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 17:37
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:56:54 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 29 04:54:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

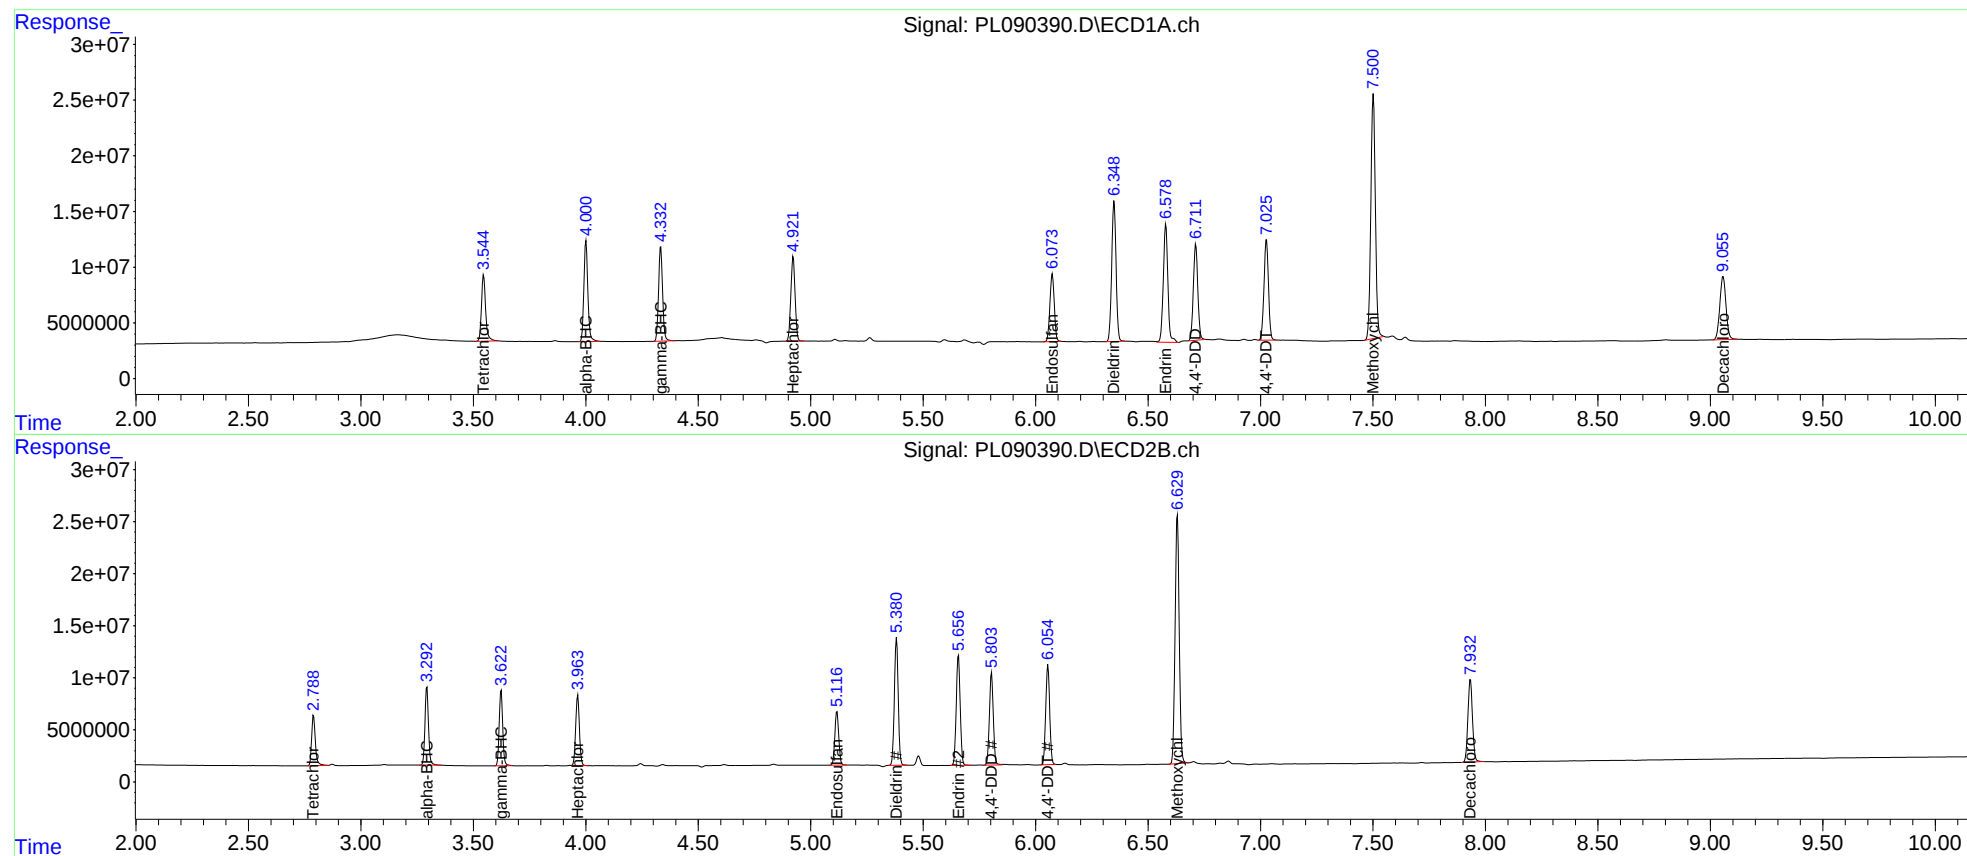

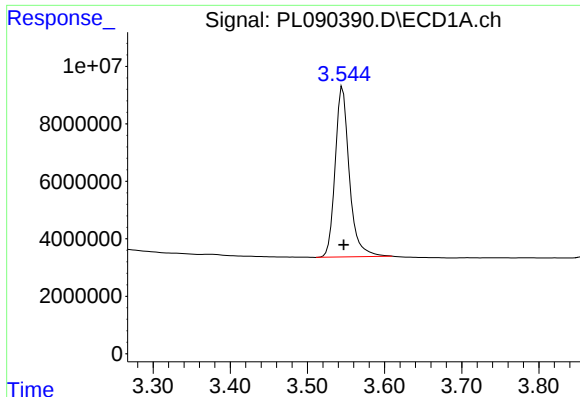


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.001 min
Response: 75891355
Conc: 38.82 ng/ml

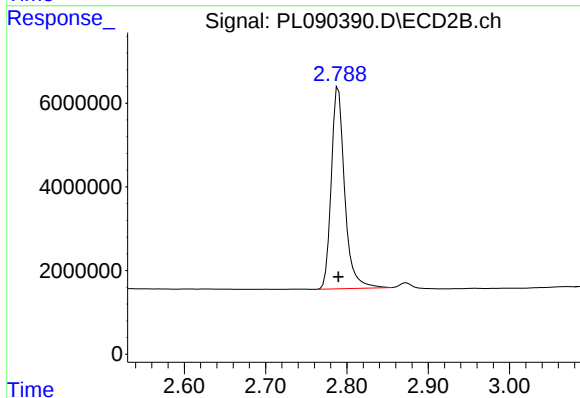


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 55383428
Conc: 40.21 ng/ml

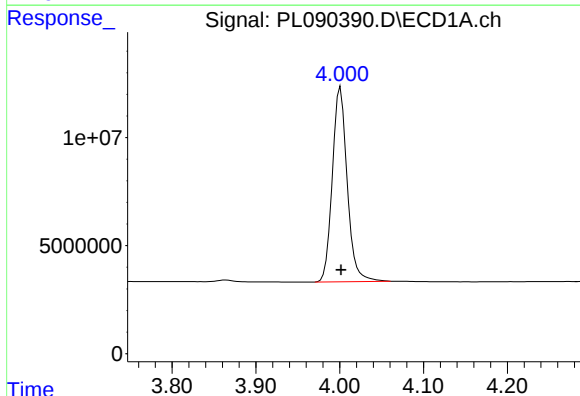


#2 alpha-BHC

R.T.: 4.001 min
Delta R.T.: 0.000 min
Response: 110905678
Conc: 39.94 ng/ml

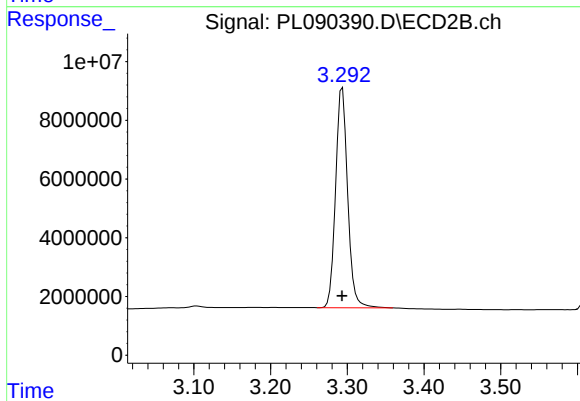


#2 alpha-BHC

R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 81931768
Conc: 43.12 ng/ml

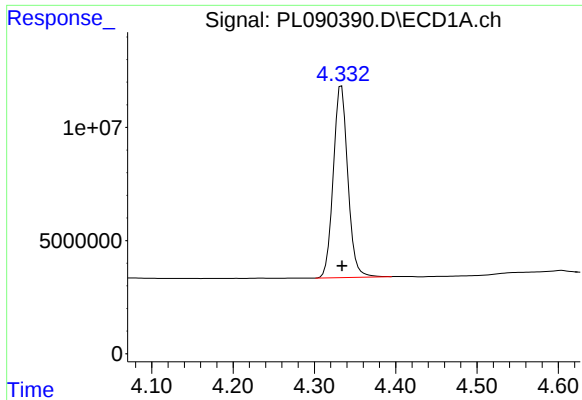


#3 gamma-BHC (Lindane)

R.T.: 4.333 min
Delta R.T.: 0.000 min
Response: 105287307
Conc: 39.62 ng/ml

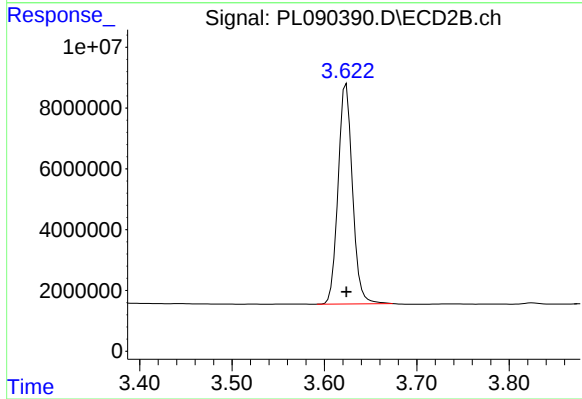


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 78254405
Conc: 42.67 ng/ml

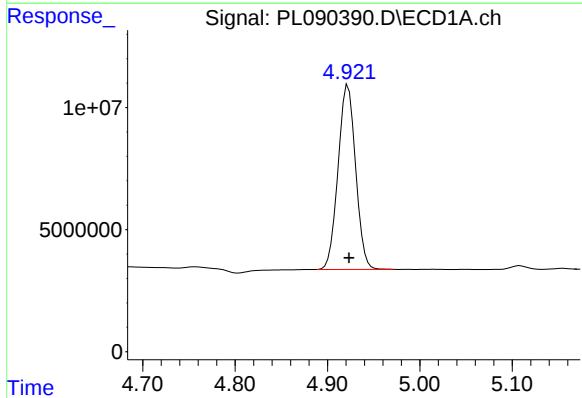


#4 Heptachlor

R.T.: 4.922 min
Delta R.T.: 0.000 min
Response: 99893523
Conc: 38.50 ng/ml

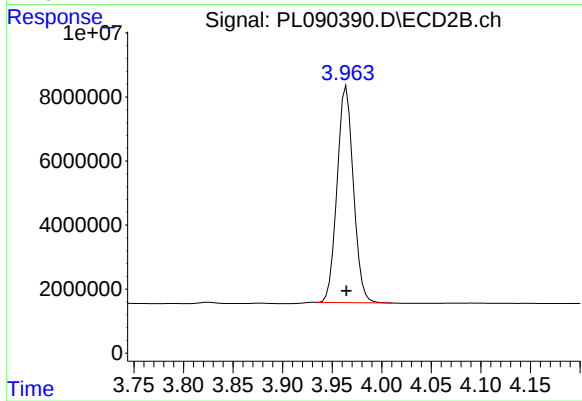


#4 Heptachlor

R.T.: 3.964 min
Delta R.T.: 0.000 min
Response: 77267736
Conc: 41.20 ng/ml

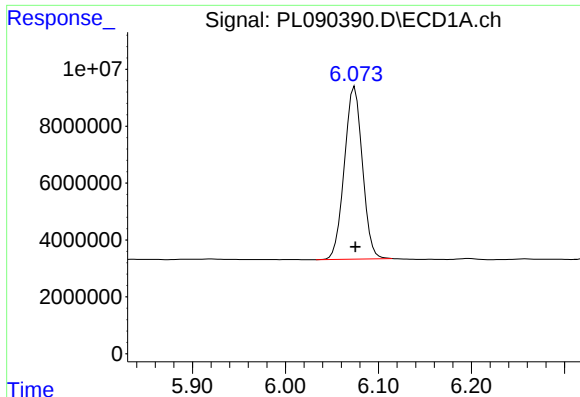


#9 Endosulfan I

R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 81705245
Conc: 37.69 ng/ml

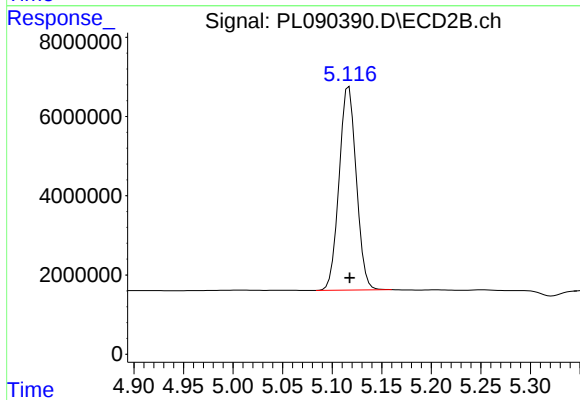


#9 Endosulfan I

R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 61990921
Conc: 39.38 ng/ml

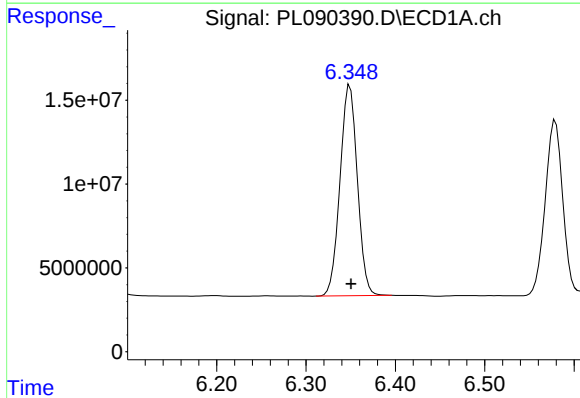


#13 Dieldrin

R.T.: 6.349 min
Delta R.T.: -0.001 min
Response: 169715610
Conc: 77.78 ng/ml

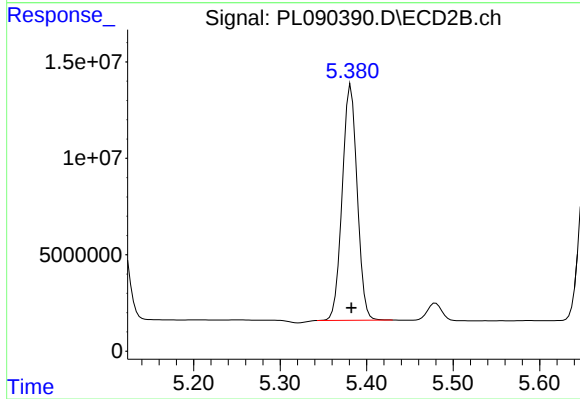


#13 Dieldrin

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 145779175
Conc: 83.76 ng/ml

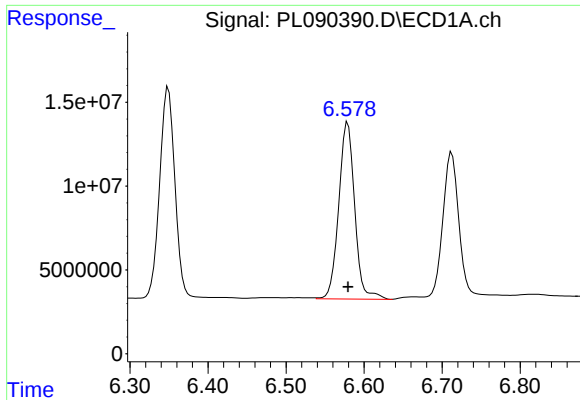


#14 Endrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 149627175
Conc: 80.12 ng/ml

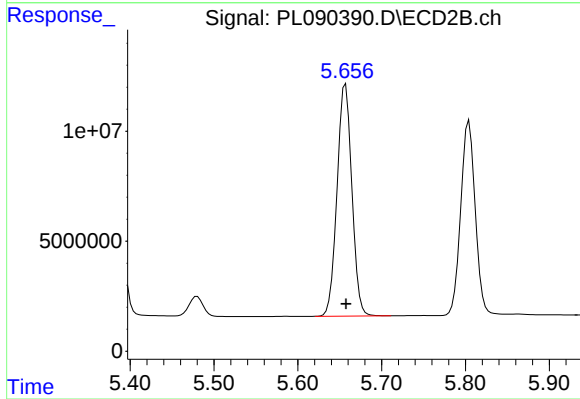


#14 Endrin

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 129421504
Conc: 83.24 ng/ml

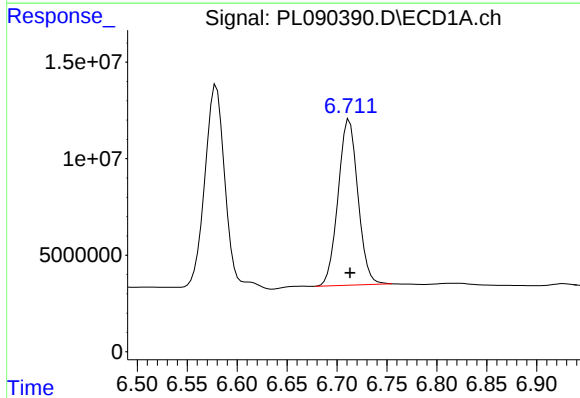


#16 4,4'-DDD

R.T.: 6.712 min
Delta R.T.: 0.000 min
Response: 118882624
Conc: 78.47 ng/ml

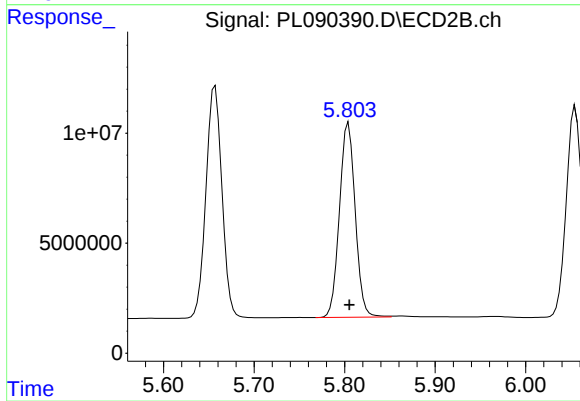


#16 4,4'-DDD

R.T.: 5.804 min
Delta R.T.: -0.001 min
Response: 107080470
Conc: 84.93 ng/ml

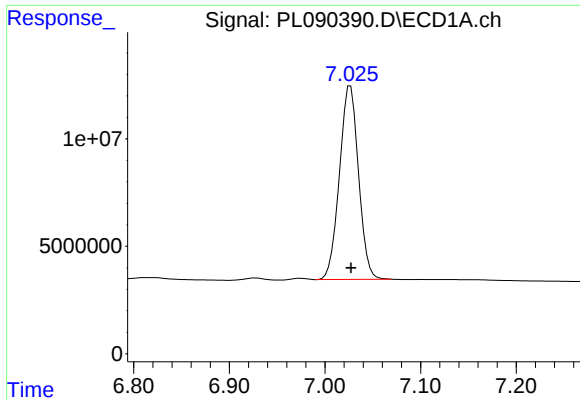


#17 4,4'-DDT

R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 125166724
Conc: 77.72 ng/ml

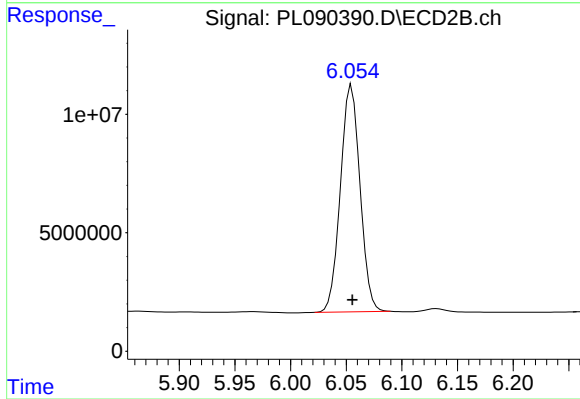


#17 4,4'-DDT

R.T.: 6.055 min
Delta R.T.: 0.000 min
Response: 117503209
Conc: 83.90 ng/ml

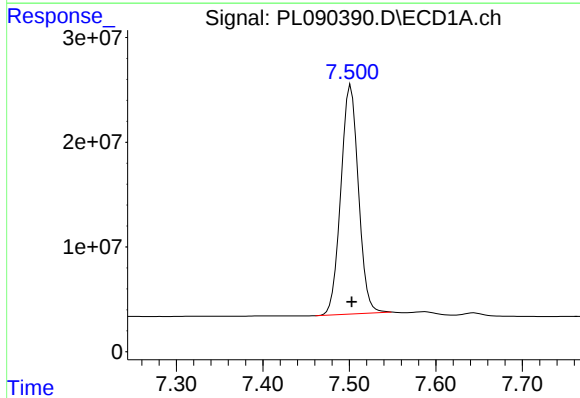


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: -0.001 min
Response: 307461477
Conc: 390.87 ng/ml

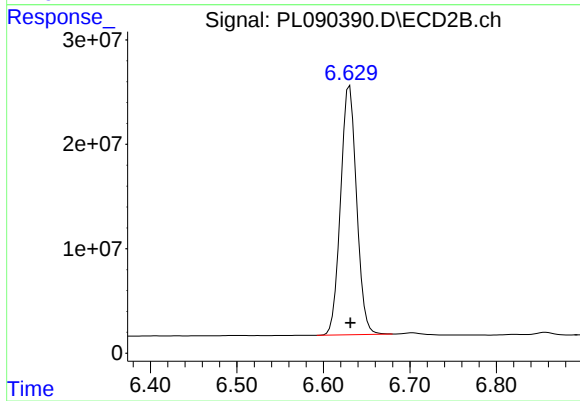


#20 Methoxychlor

R.T.: 6.630 min
Delta R.T.: 0.000 min
Response: 304662668
Conc: 395.55 ng/ml

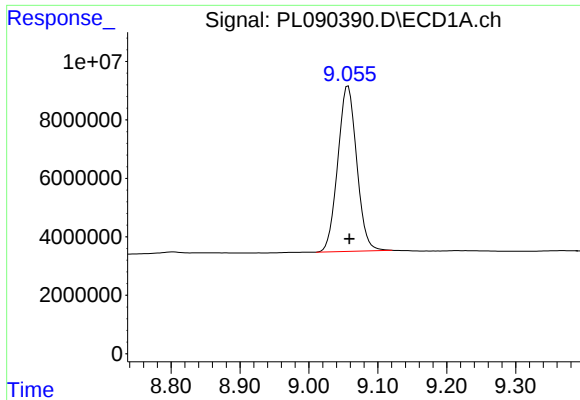

#27 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.002 min
Response: 108043268
Conc: 69.37 ng/ml

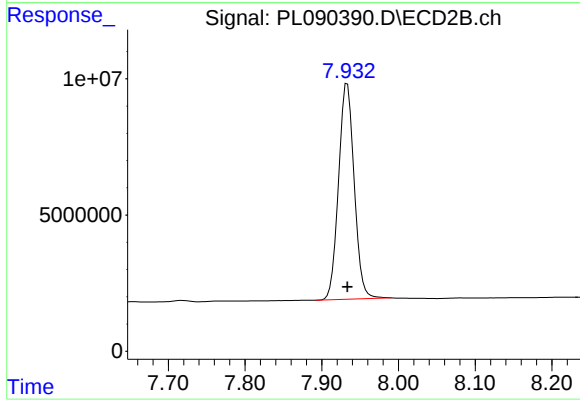

#27 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 112385554
Conc: 76.70 ng/ml