

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
 Data File : PL090392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jun 2024 18:04
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 04:57:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 29 04:54:33 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.790	155.0E6	118.8E6	79.291	86.243
27)	SA Decachlor...	9.057	7.933	215.5E6	231.6E6	138.327	158.072
Target Compounds							
2)	A alpha-BHC	4.002	3.294	235.1E6	188.0E6	84.669	98.930
3)	MA gamma-BHC...	4.334	3.624	223.0E6	176.0E6	83.927	95.998
4)	MA Heptachlor	4.924	3.965	204.3E6	172.0E6	78.733	91.710
9)	A Endosulfan I	6.075	5.117	163.9E6	128.6E6	75.596	81.694
13)	MA Dieldrin	6.350	5.382	355.0E6	323.6E6	162.681	185.923
14)	MA Endrin	6.579	5.658	316.5E6	287.7E6	169.494	185.058
16)	A 4,4'-DDD	6.714	5.805	250.6E6	242.1E6	165.430	192.039
17)	MA 4,4'-DDT	7.028	6.056	265.2E6	265.0E6	164.683	189.250
20)	A Methoxychlor	7.502	6.631	625.9E6	629.3E6	795.663	816.968


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062824\
Data File : PL090392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jun 2024 18:04
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 04:57:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062824CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 29 04:54:33 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

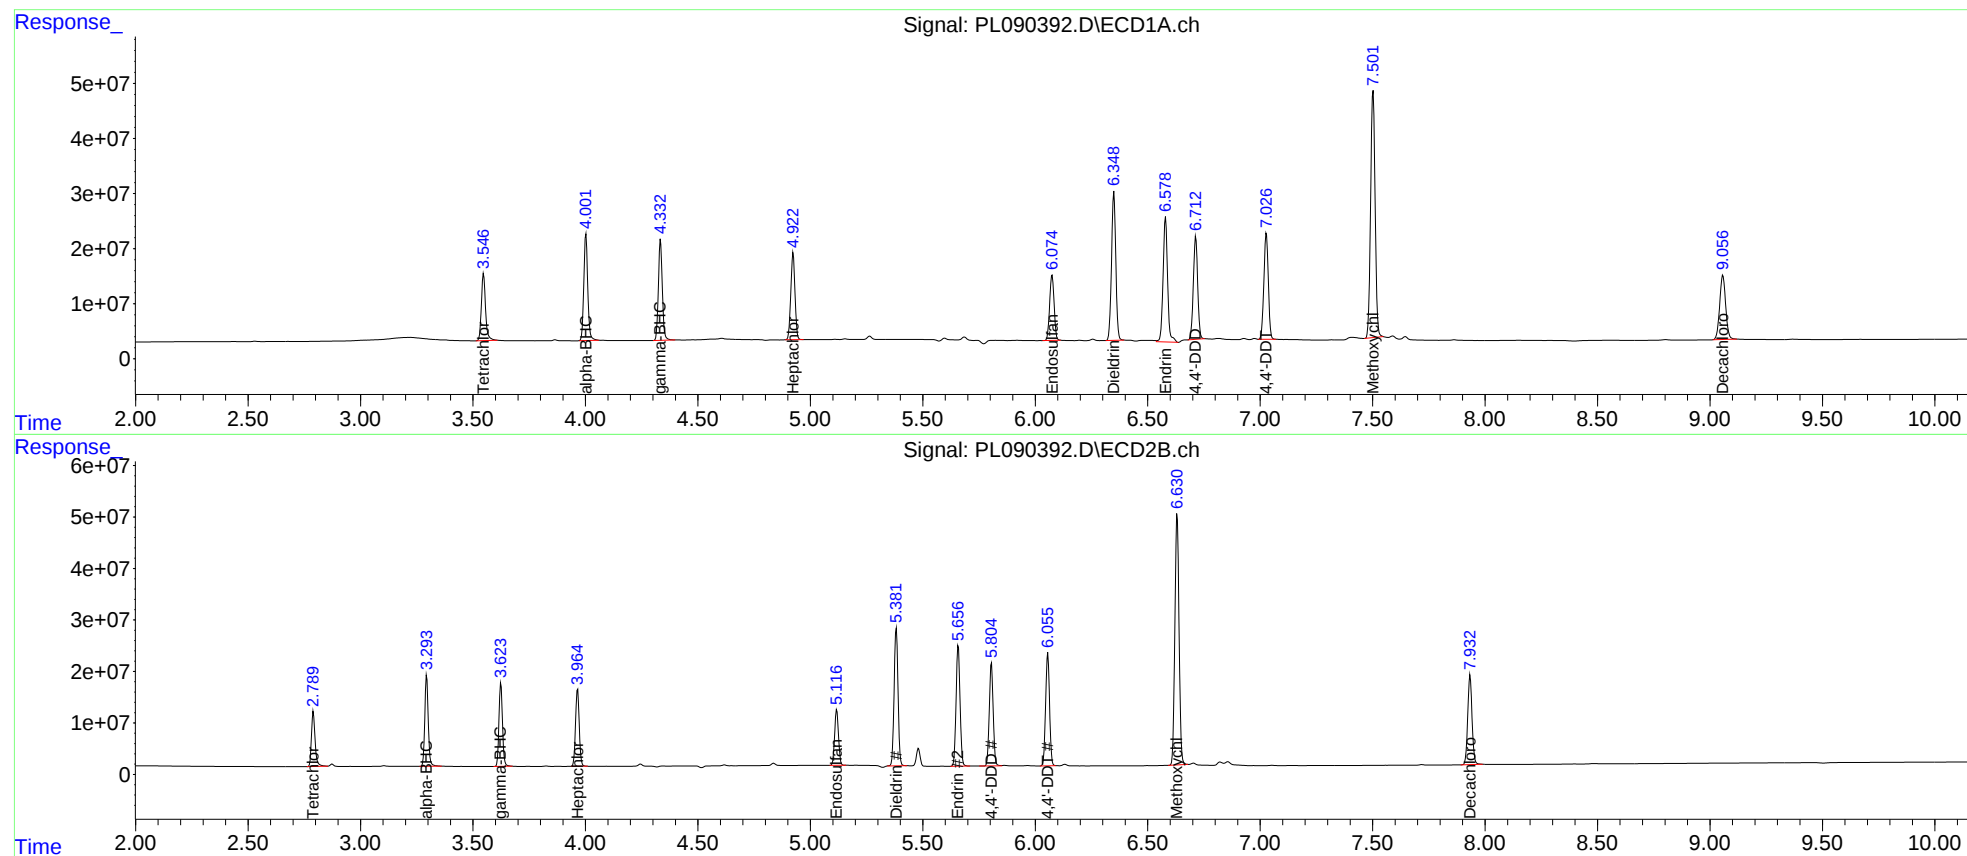

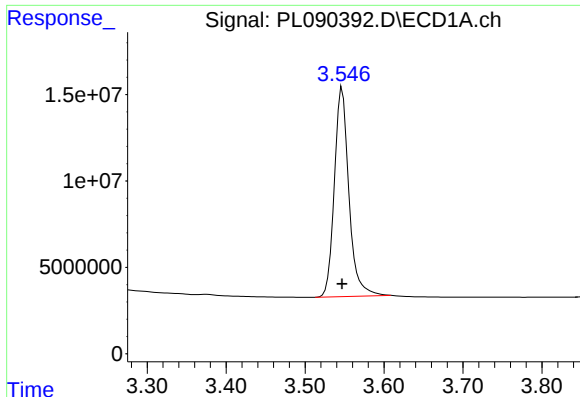


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 155007030
Conc: 79.29 ng/ml

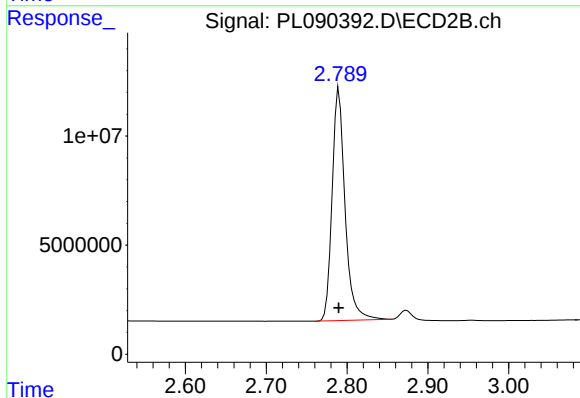


#1 Tetrachloro-m-xylene

R.T.: 2.790 min
Delta R.T.: 0.000 min
Response: 118777785
Conc: 86.24 ng/ml

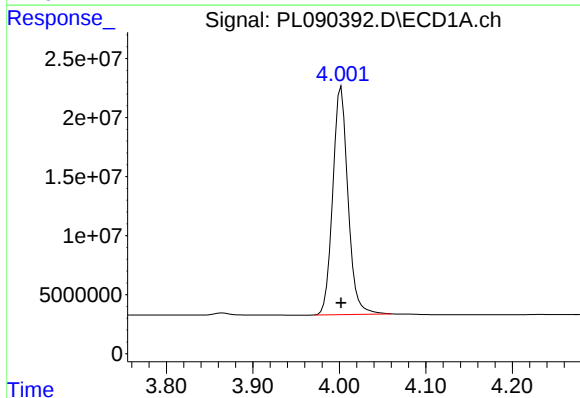


#2 alpha-BHC

R.T.: 4.002 min
Delta R.T.: 0.000 min
Response: 235093987
Conc: 84.67 ng/ml

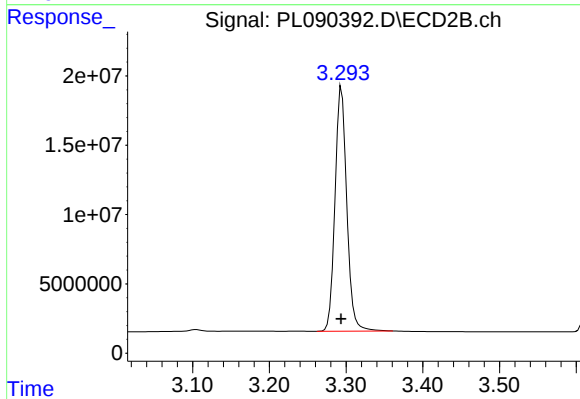


#2 alpha-BHC

R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 187985517
Conc: 98.93 ng/ml

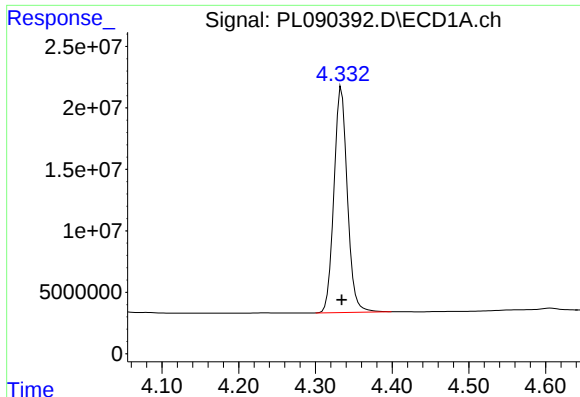


#3 gamma-BHC (Lindane)

R.T.: 4.334 min
Delta R.T.: 0.000 min
Response: 223005873
Conc: 83.93 ng/ml

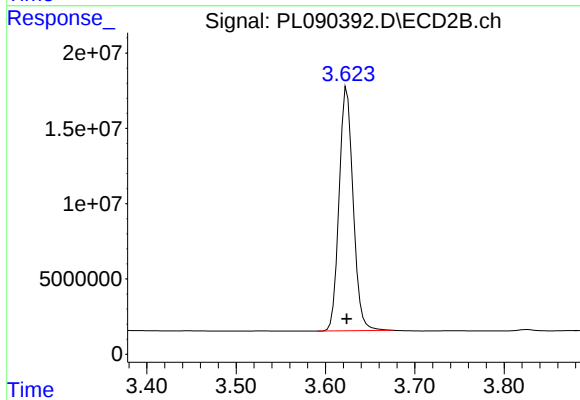


#3 gamma-BHC (Lindane)

R.T.: 3.624 min
Delta R.T.: 0.000 min
Response: 176040017
Conc: 96.00 ng/ml

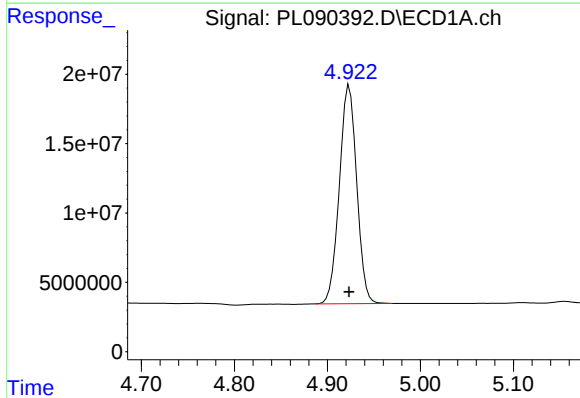


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 204305666
Conc: 78.73 ng/ml

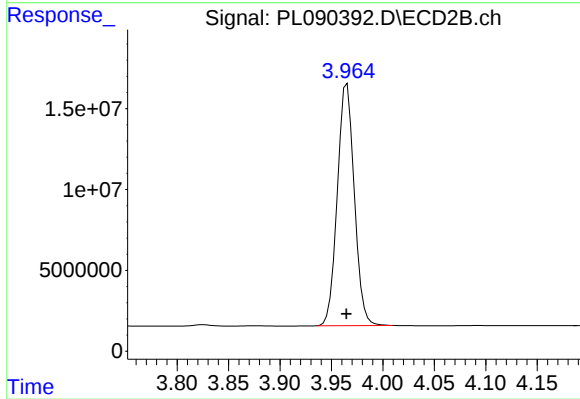


#4 Heptachlor

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 171997050
Conc: 91.71 ng/ml

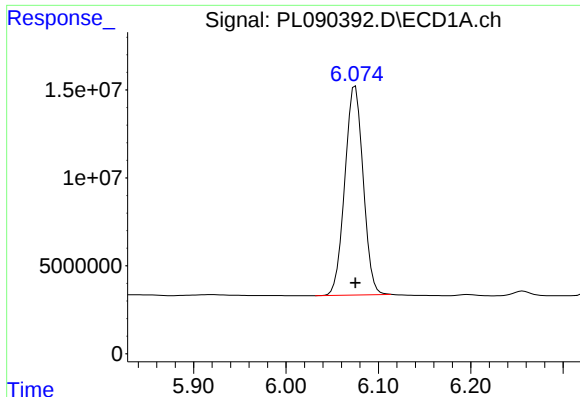


#9 Endosulfan I

R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 163873885
Conc: 75.60 ng/ml

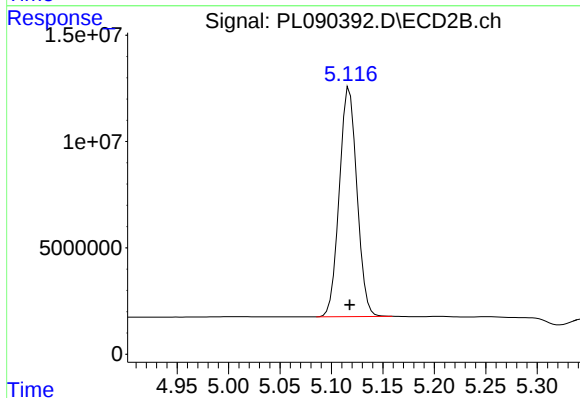


#9 Endosulfan I

R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 128597365
Conc: 81.69 ng/ml

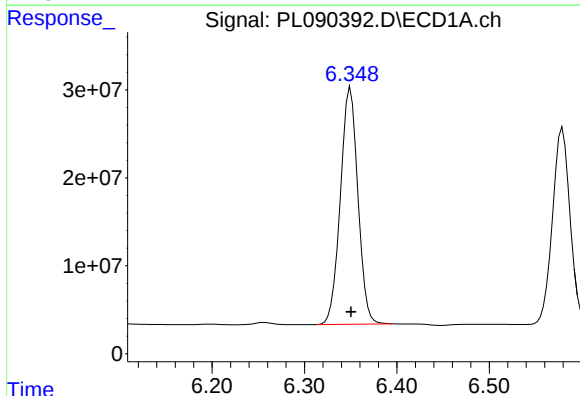


#13 Dieldrin

R.T.: 6.350 min
Delta R.T.: 0.000 min
Response: 354951197
Conc: 162.68 ng/ml

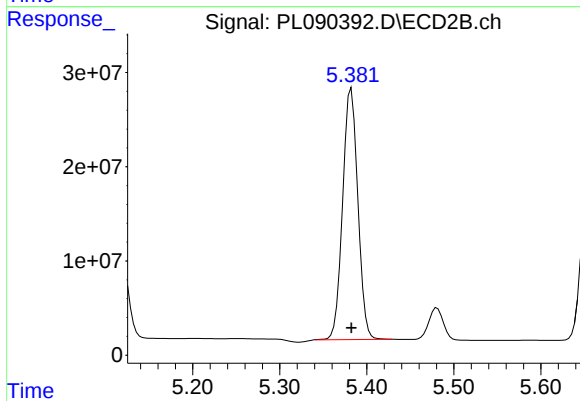


#13 Dieldrin

R.T.: 5.382 min
Delta R.T.: 0.000 min
Response: 323573887
Conc: 185.92 ng/ml

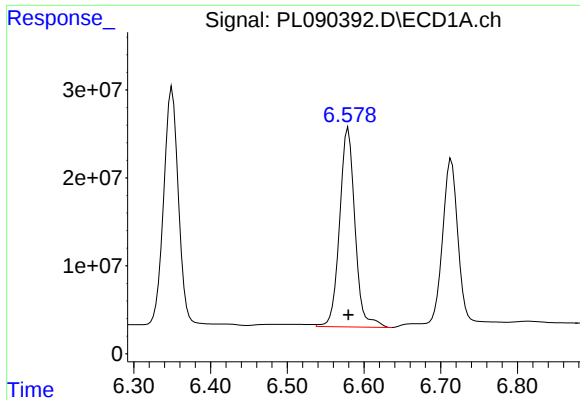


#14 Endrin

R.T.: 6.579 min
Delta R.T.: 0.000 min
Response: 316542670
Conc: 169.49 ng/ml

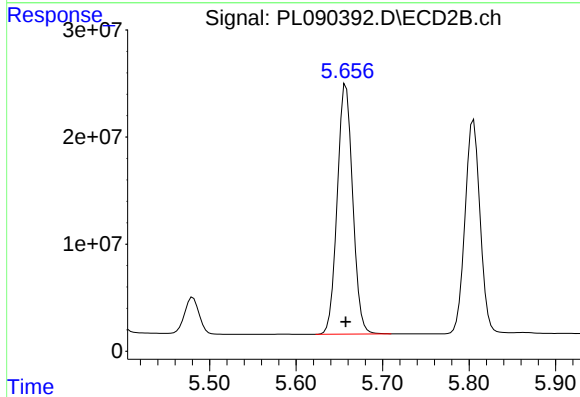


#14 Endrin

R.T.: 5.658 min
Delta R.T.: 0.000 min
Response: 287726430
Conc: 185.06 ng/ml

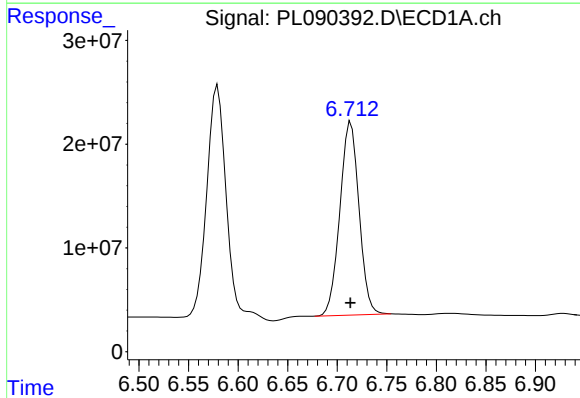


#16 4,4'-DDD

R.T.: 6.714 min
Delta R.T.: 0.000 min
Response: 250634751
Conc: 165.43 ng/ml

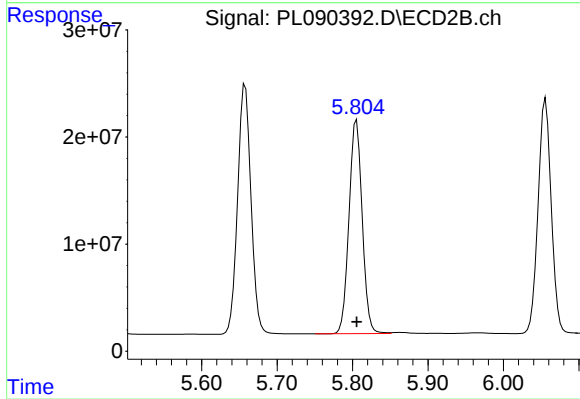


#16 4,4'-DDD

R.T.: 5.805 min
Delta R.T.: 0.000 min
Response: 242117450
Conc: 192.04 ng/ml

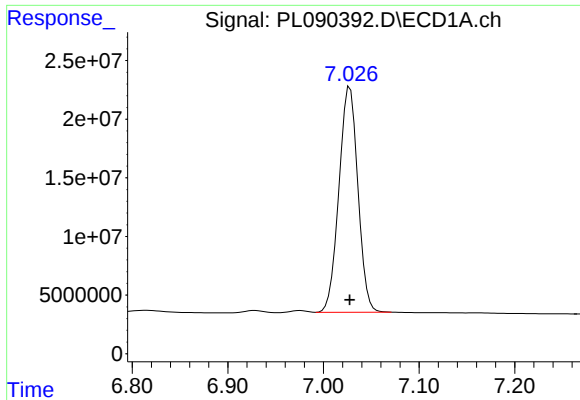


#17 4,4'-DDT

R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 265235433
Conc: 164.68 ng/ml

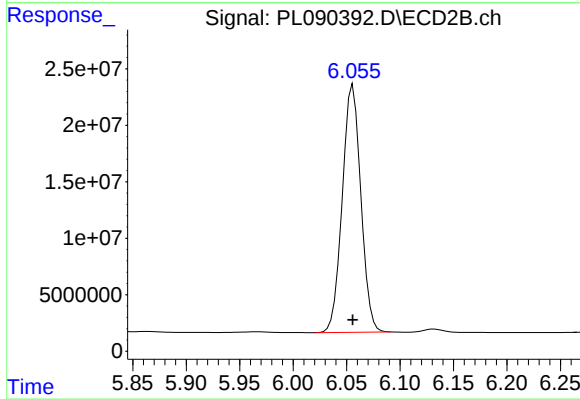


#17 4,4'-DDT

R.T.: 6.056 min
Delta R.T.: 0.000 min
Response: 265032233
Conc: 189.25 ng/ml

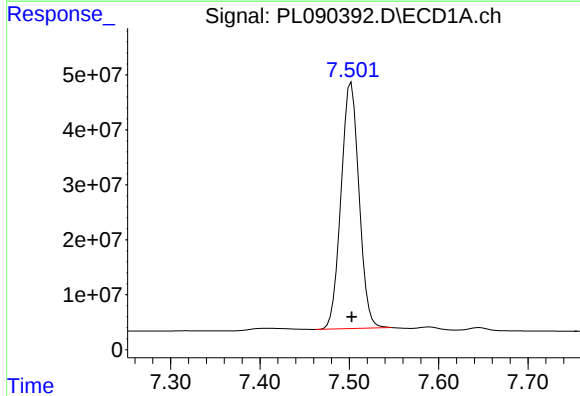


#20 Methoxychlor

R.T.: 7.502 min
Delta R.T.: 0.000 min
Response: 625876436
Conc: 795.66 ng/ml

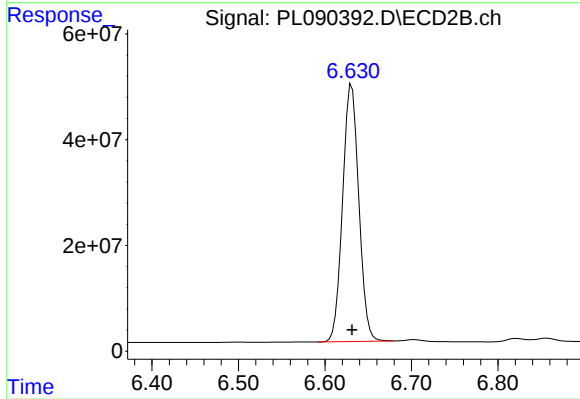

#20 Methoxychlor

R.T.: 6.631 min
Delta R.T.: 0.000 min
Response: 629252709
Conc: 816.97 ng/ml

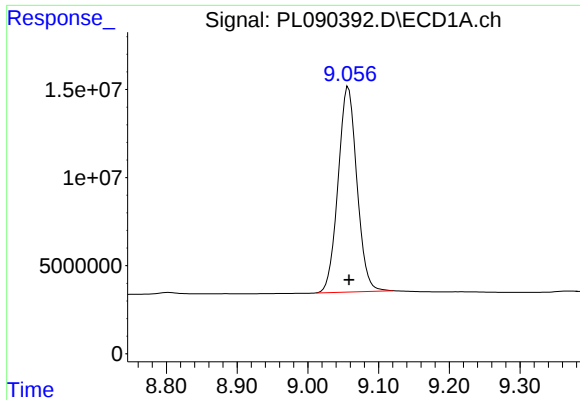


#27 Decachlorobiphenyl

R.T.: 9.057 min

Delta R.T.: -0.001 min

Response: 215456870

Conc: 138.33 ng/ml

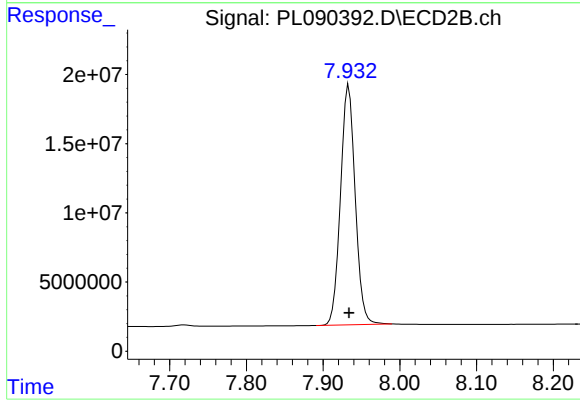

#27 Decachlorobiphenyl

R.T.: 7.933 min

Delta R.T.: 0.000 min

Response: 231631142

Conc: 158.07 ng/ml