

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
 Data File : PL037554.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2018 16:20
 Operator : UA\AJ
 Sample : J3248-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 29 23:27:20 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.936	60637620	18371776	7.666	6.640
28)	SA Decachlor...	8.014	8.948	41907462	13817446	6.945	6.965
Target Compounds							
2)	A alpha-BHC	3.778	0.000	7140985	0	0.583	N.D. #
5)	MB Aldrin	4.571	0.000	11360064	0	1.116	N.D. #
9)	A Endosulfan I	5.284f	0.000	17553238	0	2.075	N.D. #
10)	B gamma-Chl...	5.221	0.000	15967617	0	1.705	N.D. #
11)	B alpha-Chl...	5.284	0.000	17553238	0	1.933	N.D. #
23)	Chlordane-1	4.182	0.000	2806033	0	9.139	N.D. #
24)	Chlordane-2	4.675	0.000	3611885	0	10.146	N.D. #
25)	Chlordane-3	5.221	0.000	15967617	0	15.022	N.D. #
26)	Chlordane-4	5.284	0.000	17553238	0	18.218	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
Data File : PL037554.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2018 16:20
Operator : UA\AJ
Sample : J3248-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 29 23:27:20 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

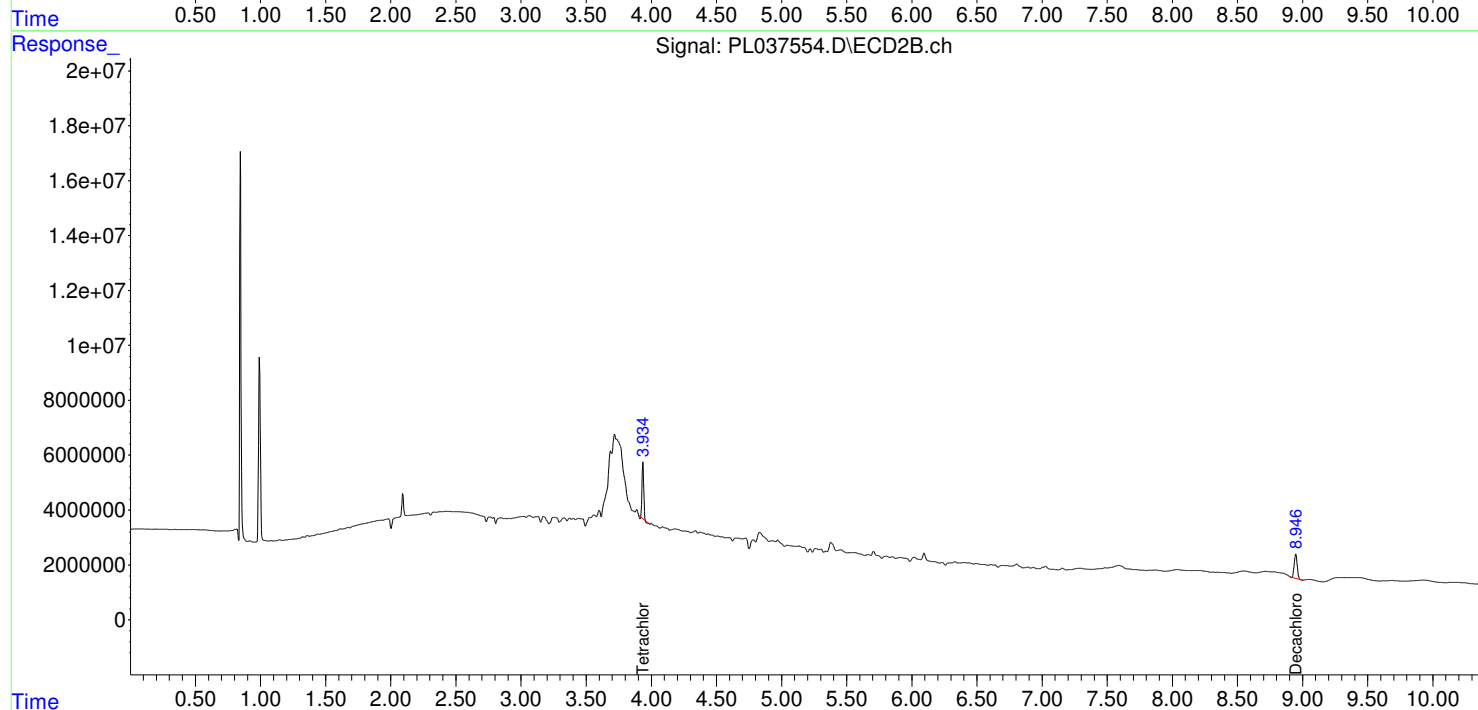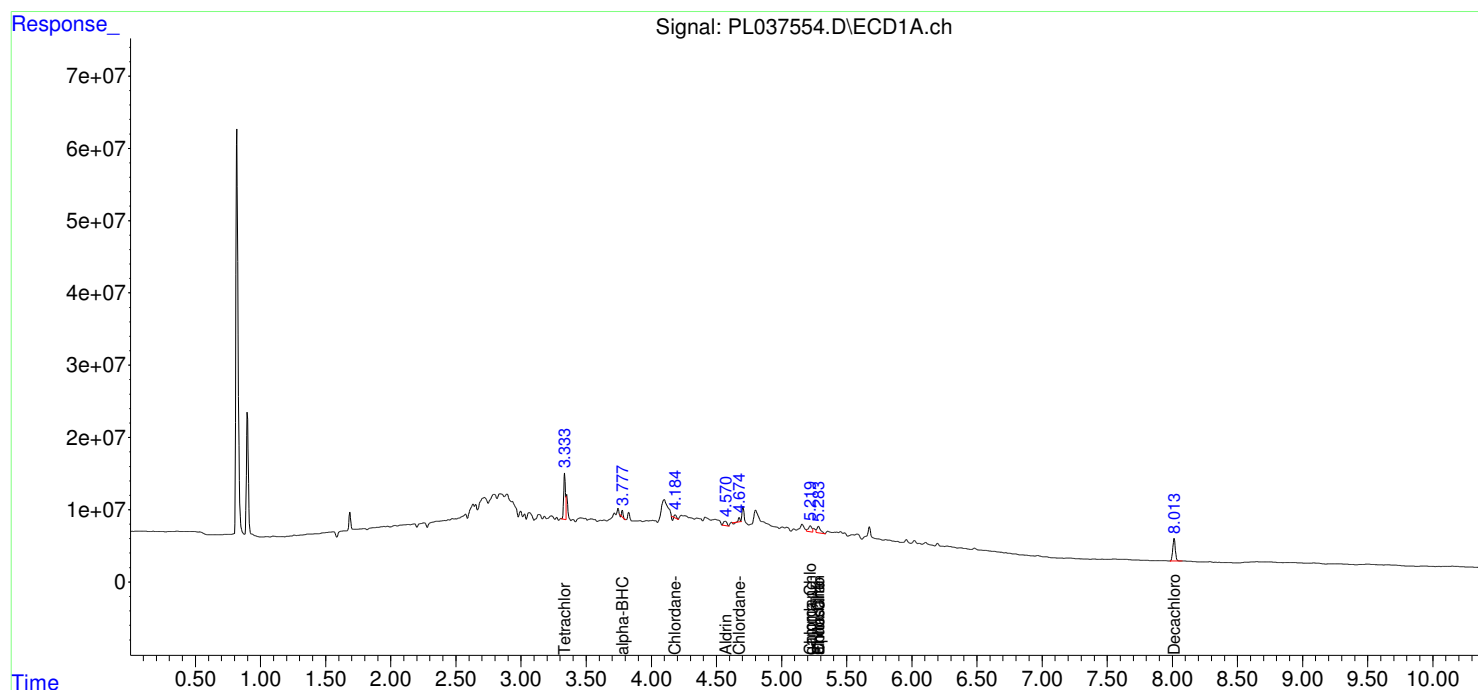


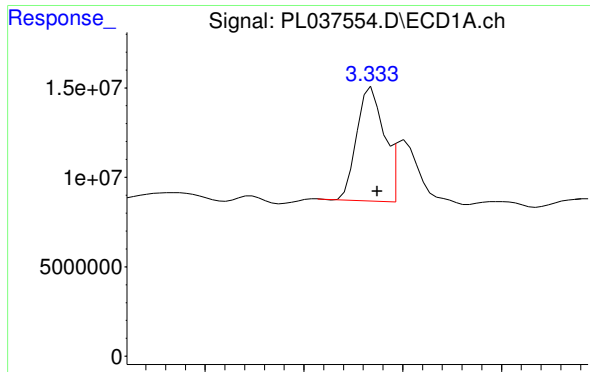

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 60637620
Conc: 7.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

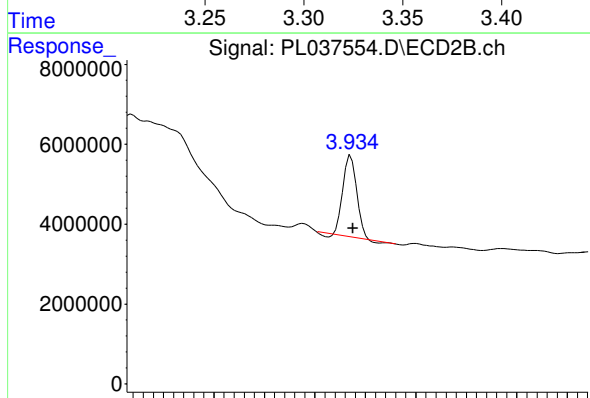


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 18371776
Conc: 6.64 ng/ml

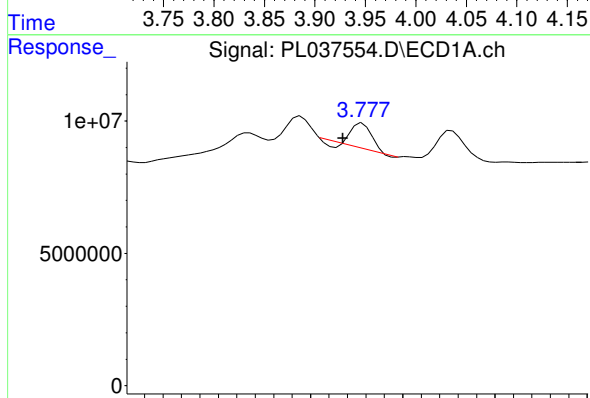


#2 alpha-BHC

R.T.: 3.778 min
Delta R.T.: 0.011 min
Response: 7140985
Conc: 0.58 ng/ml

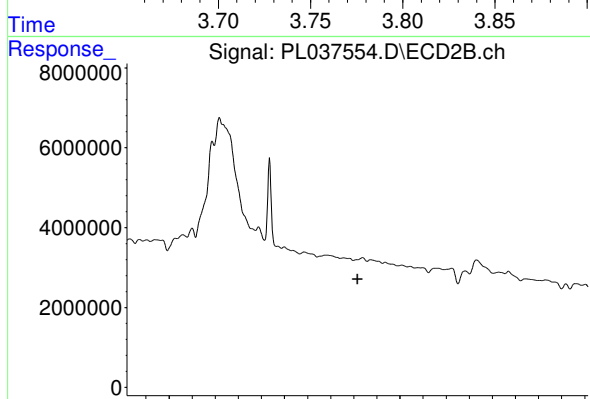

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.317 min
Response: 0
Conc: N.D.

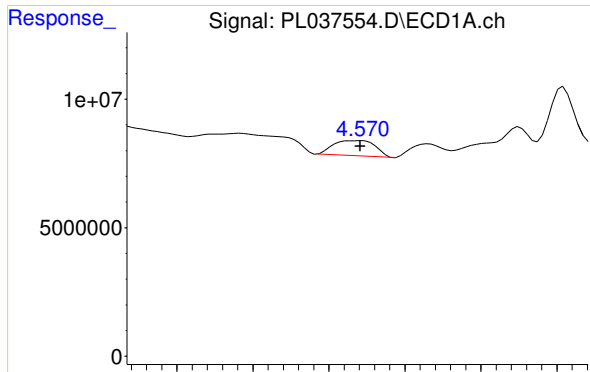

#5 Aldrin


R.T.: 4.571 min
Delta R.T.: 0.000 min
Response: 11360064
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

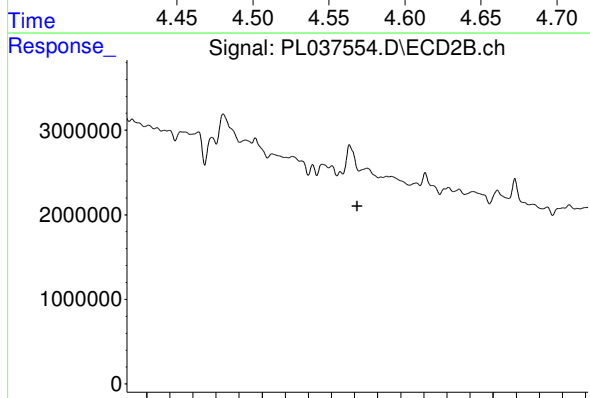


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

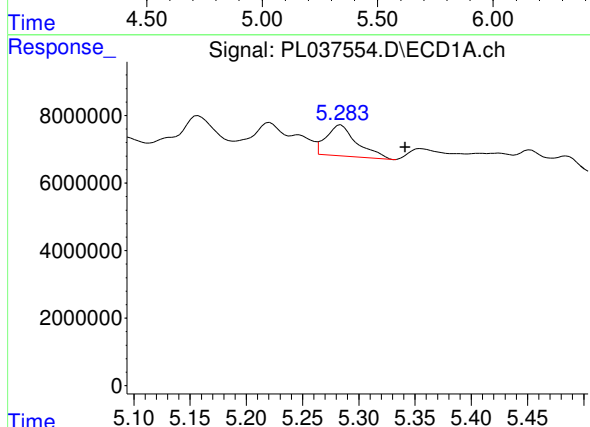


#9 Endosulfan I

R.T.: 5.284 min
Delta R.T.: -0.057 min
Response: 17553238
Conc: 2.07 ng/ml

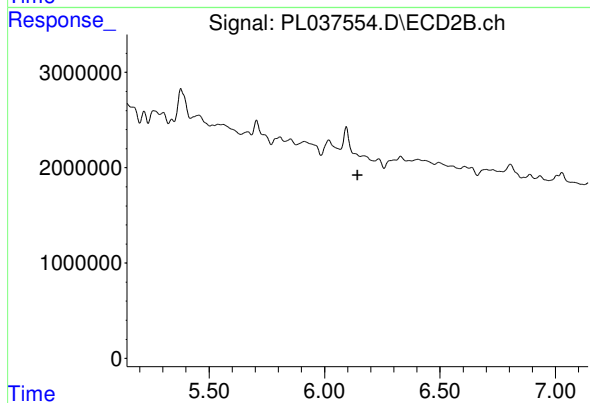

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

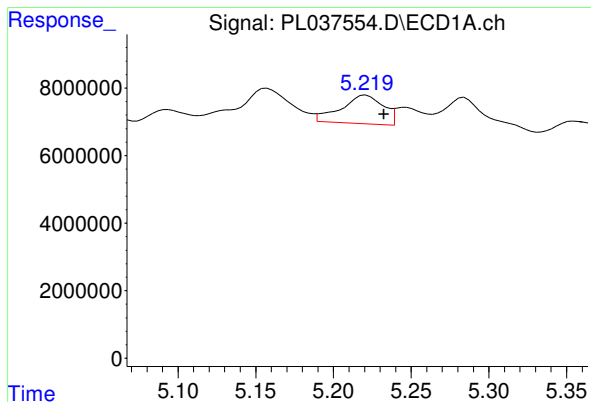

#10 gamma-Chlordane


R.T.: 5.221 min
Delta R.T.: -0.012 min
Response: 15967617
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

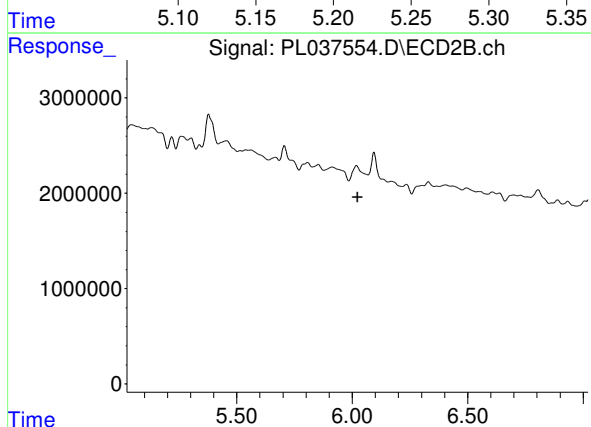


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

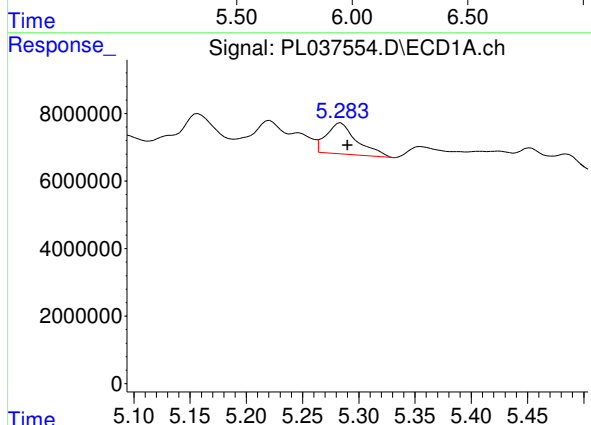


#11 alpha-Chlordane

R.T.: 5.284 min
Delta R.T.: -0.006 min
Response: 17553238
Conc: 1.93 ng/ml

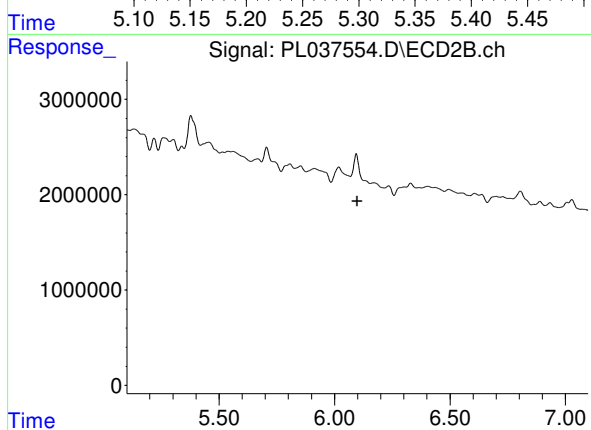

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

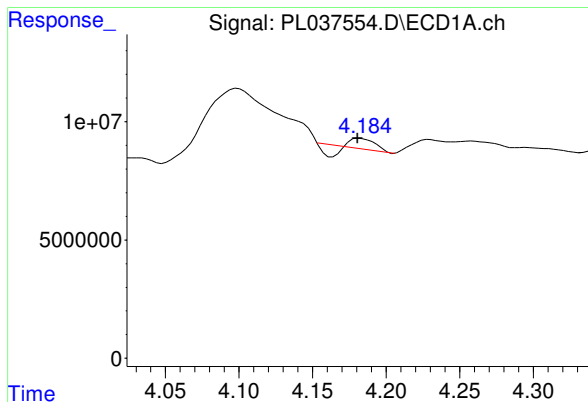

#23 Chlordane-1


R.T.: 4.182 min
Delta R.T.: 0.001 min
Response: 2806033
Conc: 9.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

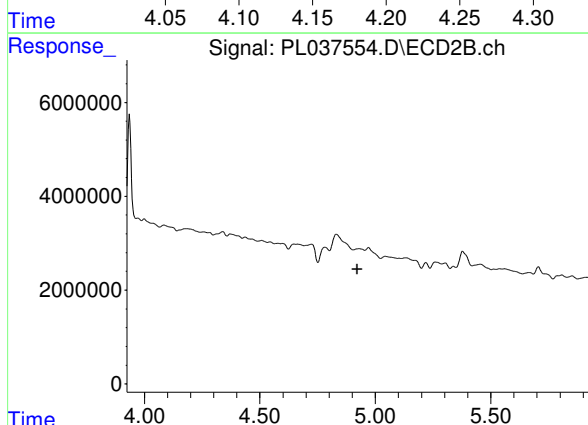


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

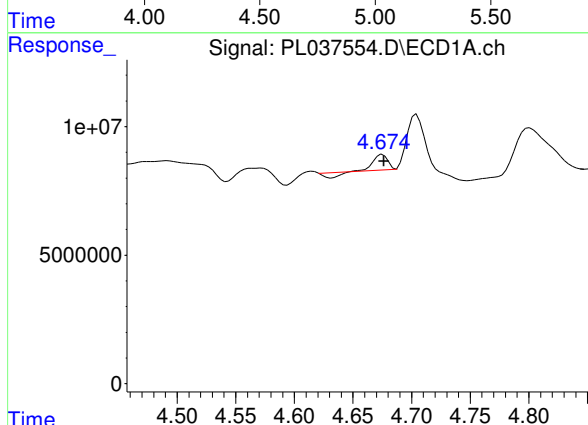


#24 Chlordane-2

R.T.: 4.675 min
Delta R.T.: -0.001 min
Response: 3611885
Conc: 10.15 ng/ml

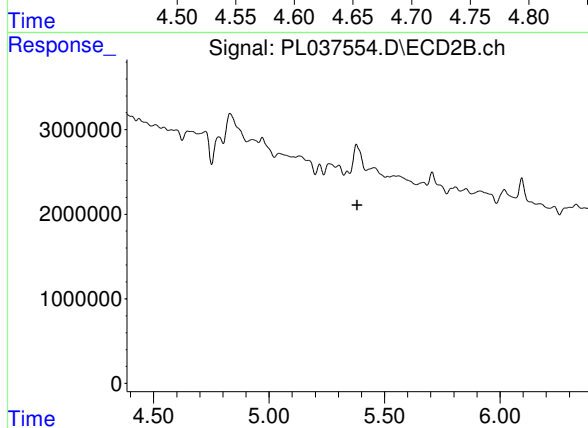

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.382 min
Response: 0
Conc: N.D.

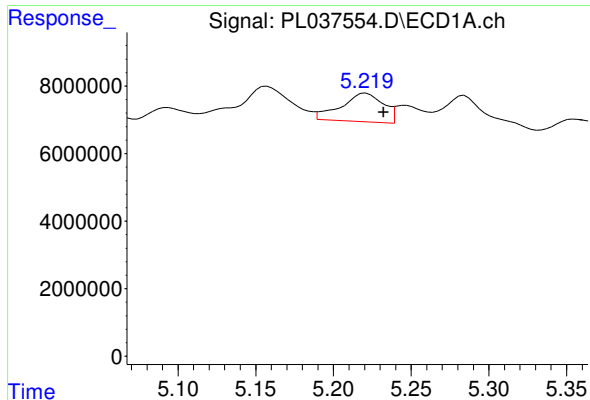

#25 Chlordane-3


R.T.: 5.221 min
Delta R.T.: -0.012 min
Response: 15967617
Conc: 15.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

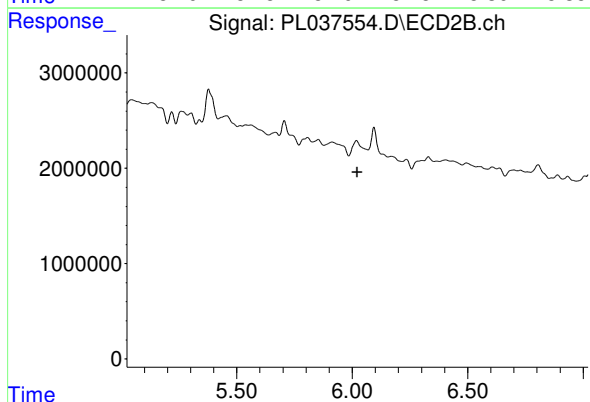


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 6.022 min
Response: 0
Conc: N.D.

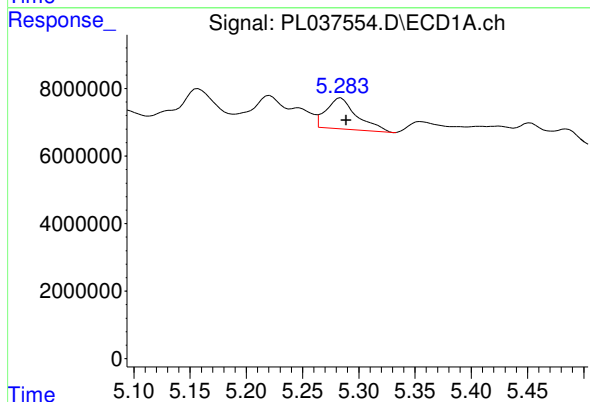


#26 Chlordane-4

R.T.: 5.284 min
Delta R.T.: -0.005 min
Response: 17553238
Conc: 18.22 ng/ml

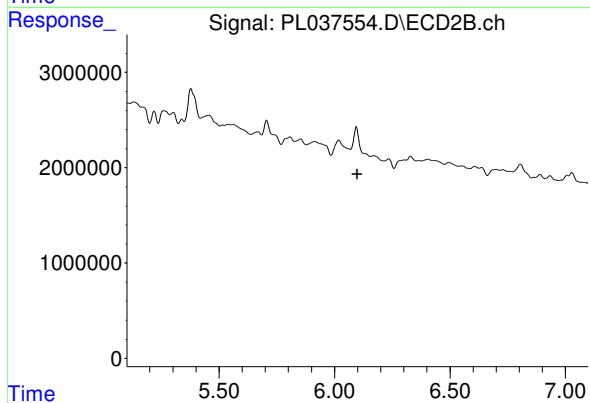

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

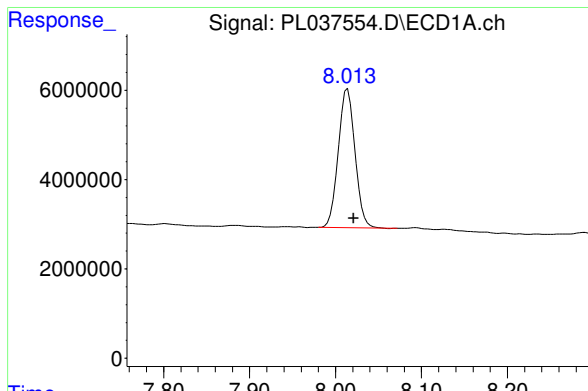

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.007 min
Response: 41907462
Conc: 6.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

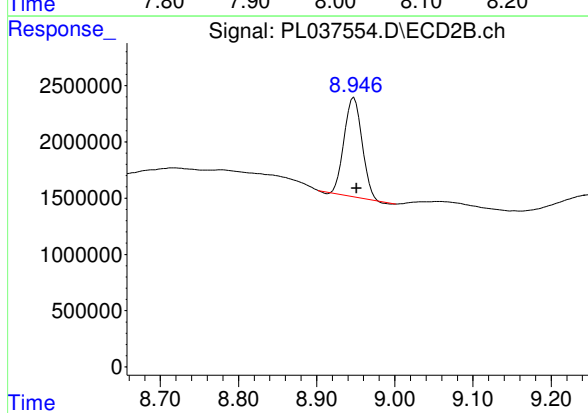

#28 Decachlorobiphenyl

R.T.: 8.948 min
Delta R.T.: -0.003 min
Response: 13817446
Conc: 6.96 ng/ml