

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
 Data File : PL037568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2018 19:37
 Operator : UA\AJ
 Sample : J3774-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 09:03:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.935	71410684	25129739	9.028	9.083
28)	SA Decachlor...	8.013	8.947	57507089	19713205	9.530	9.936
Target Compounds							
9)	A Endosulfan I	5.283f	6.097f	27766234	17107620	3.282	6.670 #
10)	B gamma-Chl...	5.246	6.021	49308927	7623335	5.264	2.707 #
11)	B alpha-Chl...	5.283	6.097	27766234	17107620	3.057	5.944 #
15)	B Endosulfa...	6.107	0.000	8810877	0	1.198	N.D. #
23)	Chlordane-1	4.178	0.000	10508363	0	34.805	N.D. #
24)	Chlordane-2	4.673	0.000	10028544	0	28.170	N.D. #
25)	Chlordane-3	5.246	6.021	49308927	7623335	46.390	19.493 #
26)	Chlordane-4	5.283	6.097	27766234	17107620	28.818	35.701



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
Data File : PL037568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2018 19:37
Operator : UA\AJ
Sample : J3774-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 09:03:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

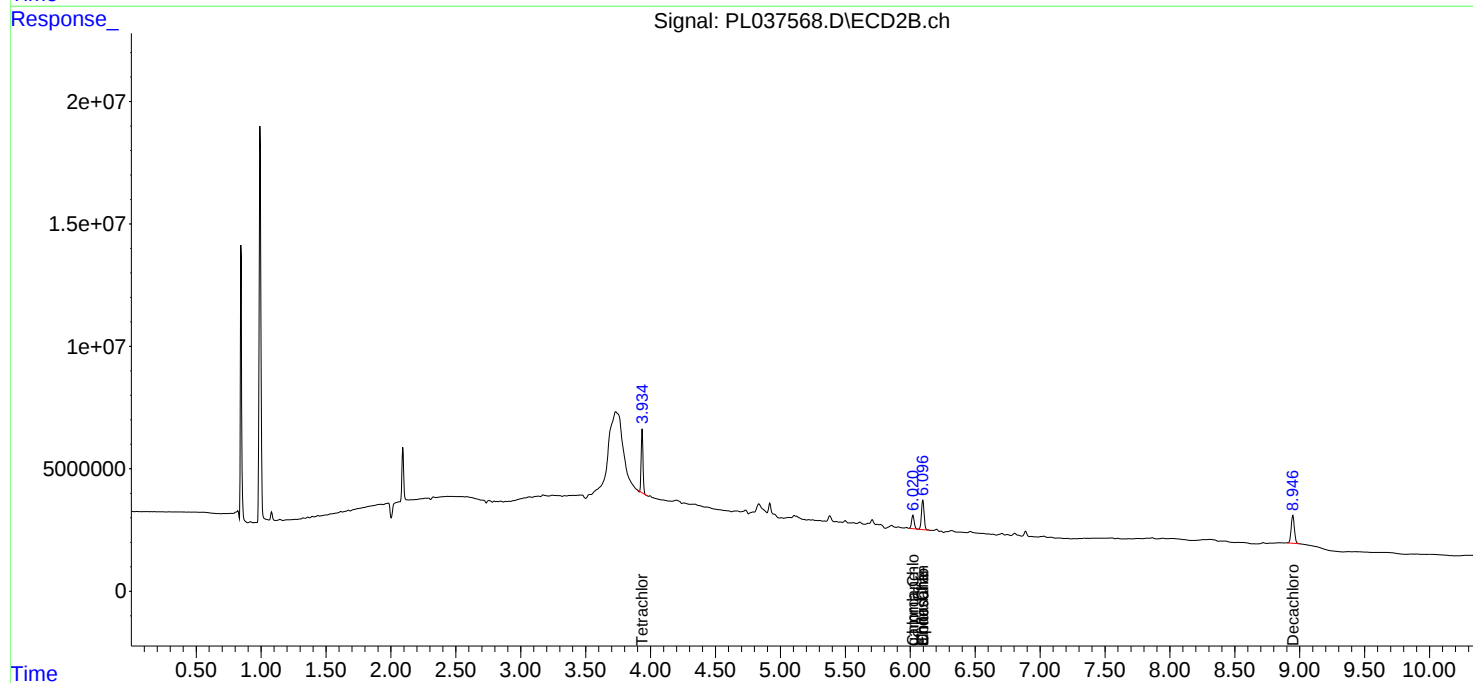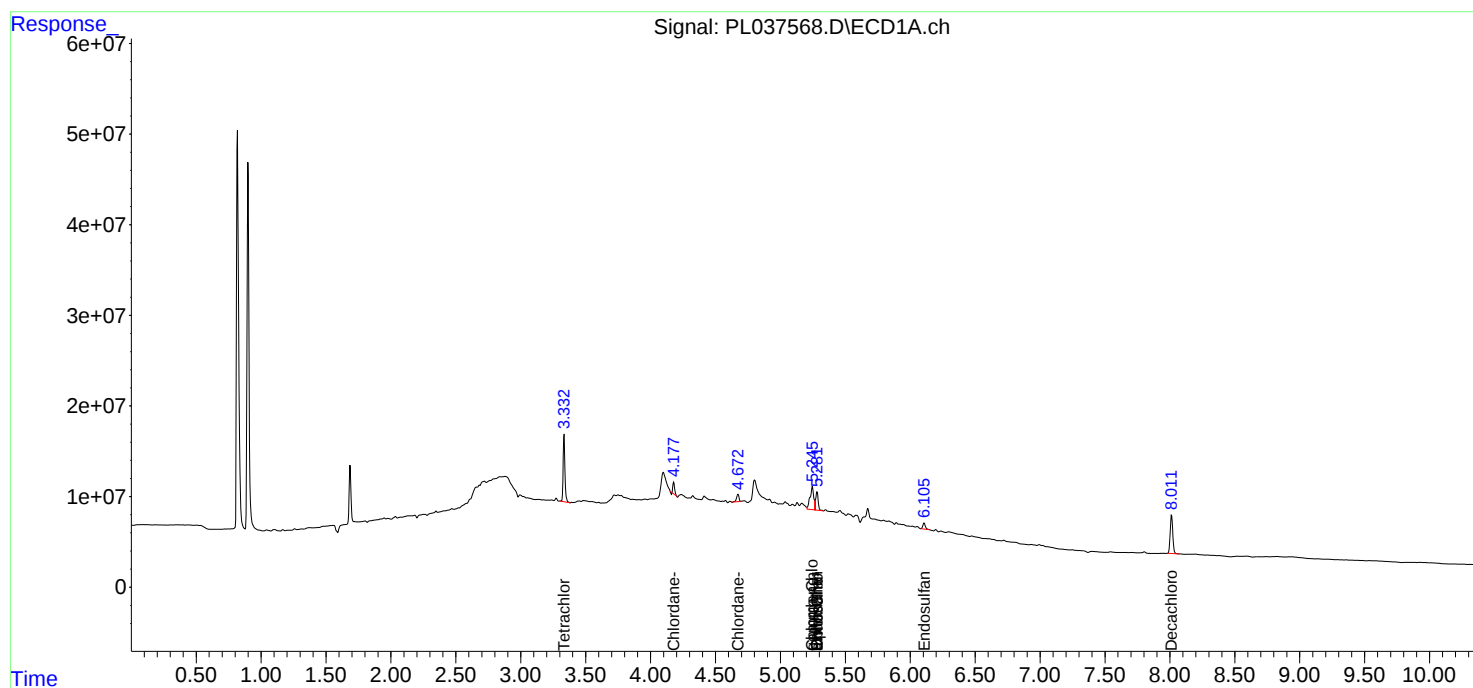


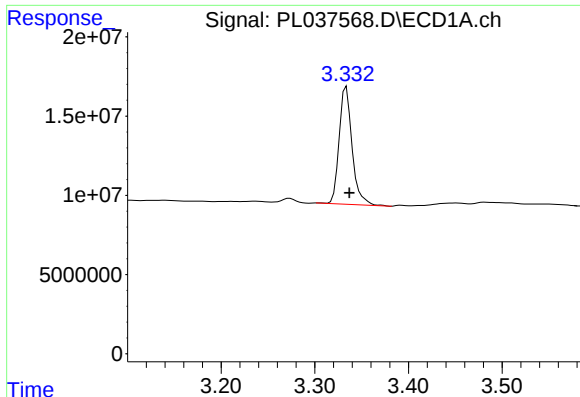

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 71410684
Conc: 9.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

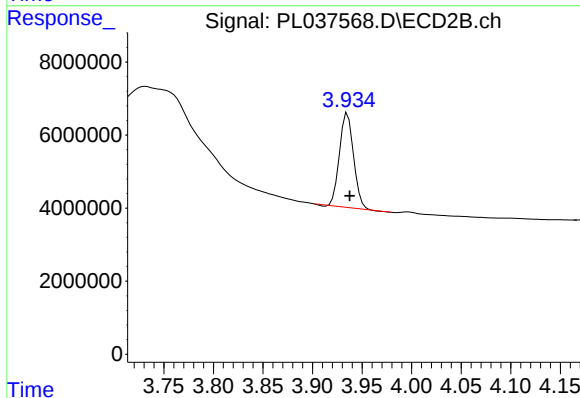


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 25129739
Conc: 9.08 ng/ml

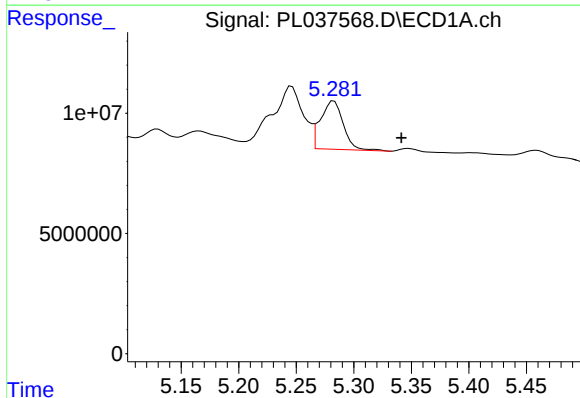


#9 Endosulfan I

R.T.: 5.283 min
Delta R.T.: -0.059 min
Response: 27766234
Conc: 3.28 ng/ml

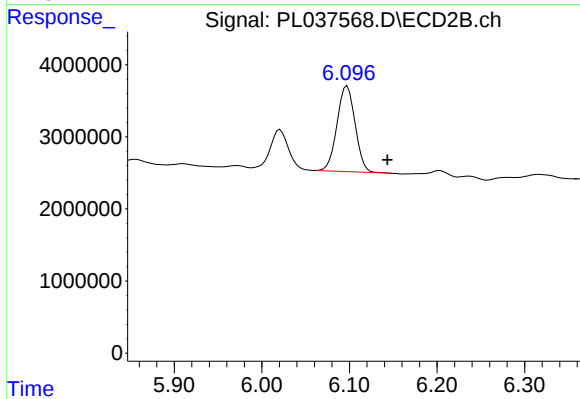

#9 Endosulfan I


R.T.: 6.097 min
Delta R.T.: -0.046 min
Response: 17107620
Conc: 6.67 ng/ml

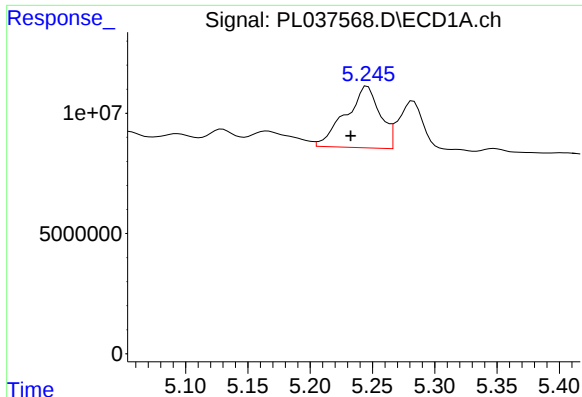

#10 gamma-Chlordane


R.T.: 5.246 min
Delta R.T.: 0.014 min
Response: 49308927
Conc: 5.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

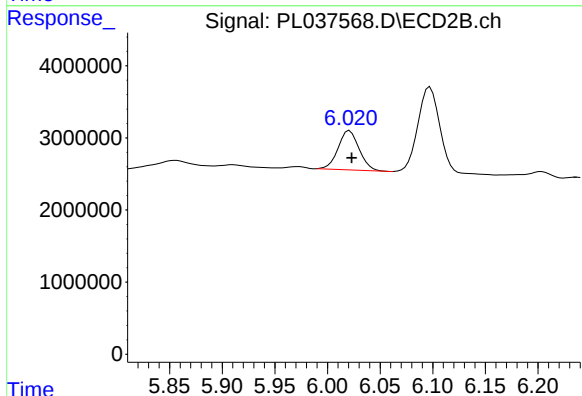


#10 gamma-Chlordane

R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 7623335
Conc: 2.71 ng/ml

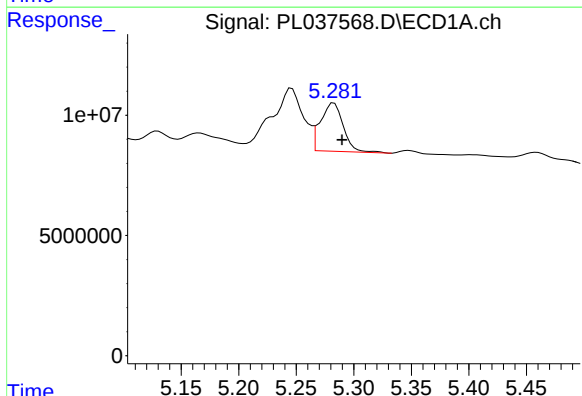


#11 alpha-Chlordane

R.T.: 5.283 min
Delta R.T.: -0.007 min
Response: 27766234
Conc: 3.06 ng/ml

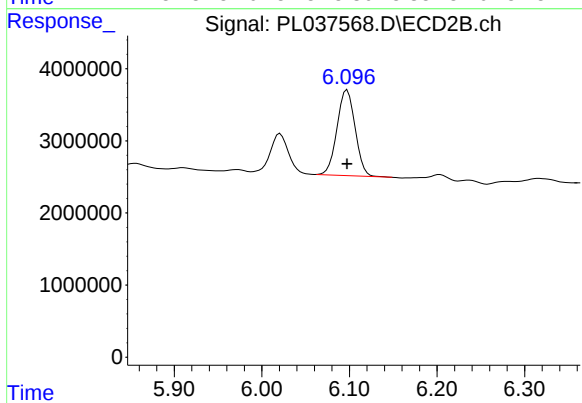

#11 alpha-Chlordane


R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 17107620
Conc: 5.94 ng/ml

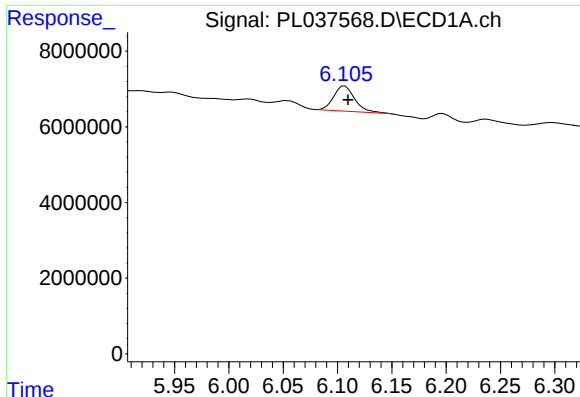

#15 Endosulfan II


R.T.: 6.107 min
Delta R.T.: -0.003 min
Response: 8810877
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

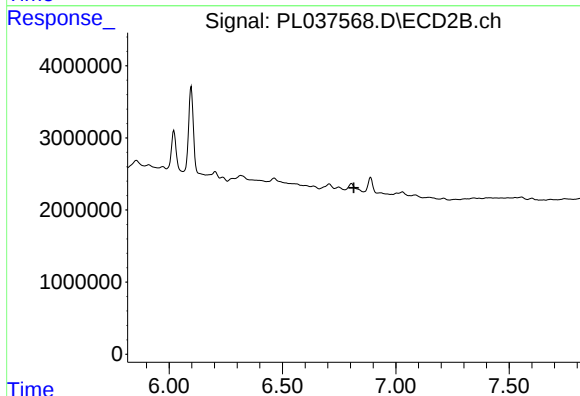


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

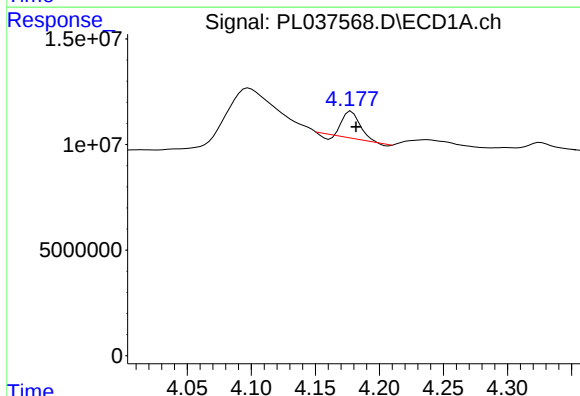


#23 Chlordane-1

R.T.: 4.178 min
Delta R.T.: -0.004 min
Response: 10508363
Conc: 34.81 ng/ml

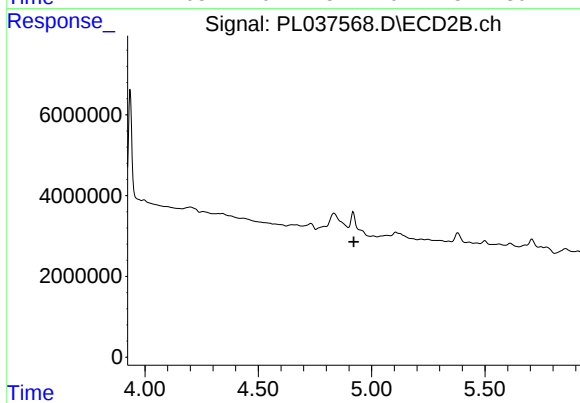

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.921 min
Response: 0
Conc: N.D.

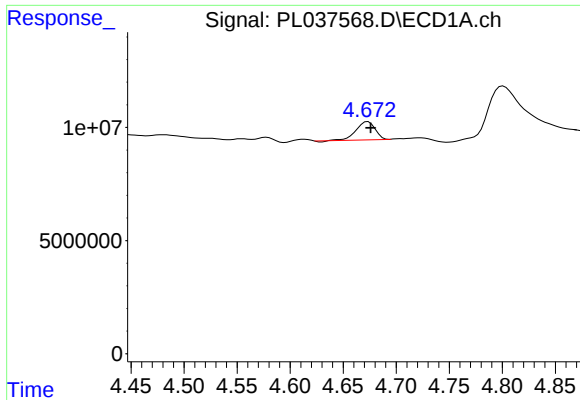

#24 Chlordane-2


R.T.: 4.673 min
Delta R.T.: -0.003 min
Response: 10028544
Conc: 28.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

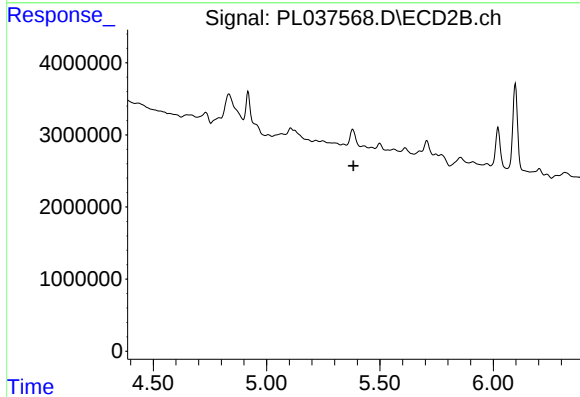


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

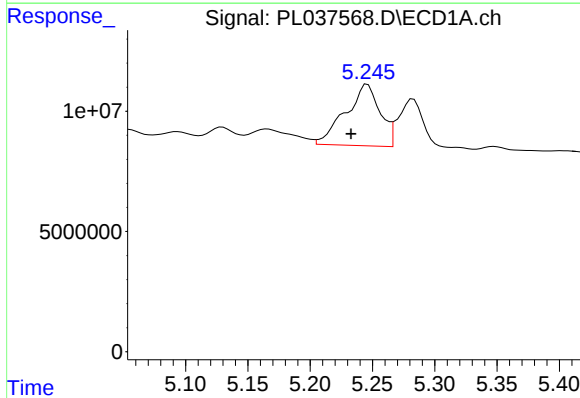


#25 Chlordane-3

R.T.: 5.246 min
Delta R.T.: 0.013 min
Response: 49308927
Conc: 46.39 ng/ml

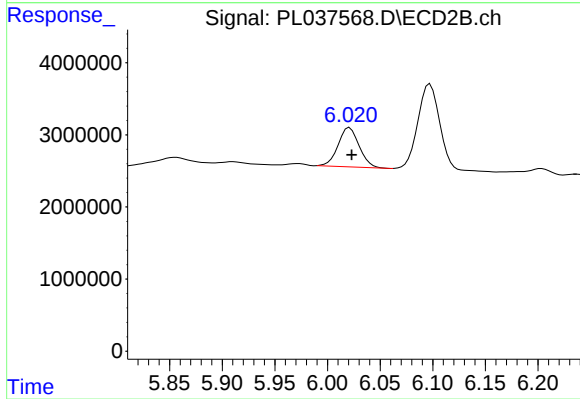

#25 Chlordane-3


R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 7623335
Conc: 19.49 ng/ml

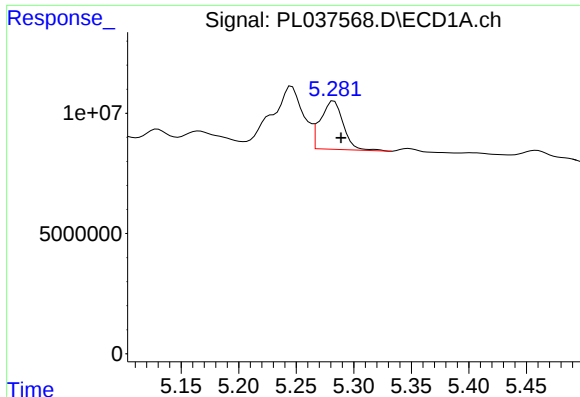

#26 Chlordane-4


R.T.: 5.283 min
Delta R.T.: -0.006 min
Response: 27766234
Conc: 28.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

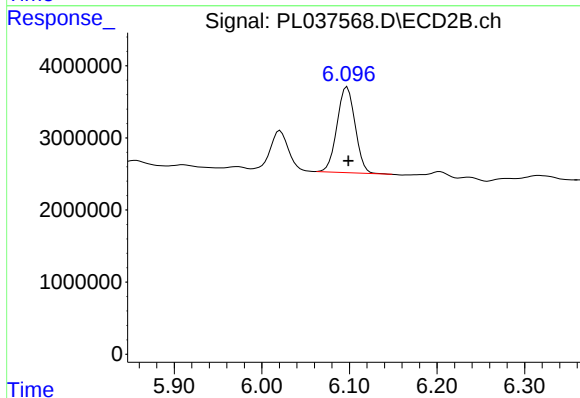


#26 Chlordane-4

R.T.: 6.097 min
Delta R.T.: -0.001 min
Response: 17107620
Conc: 35.70 ng/ml

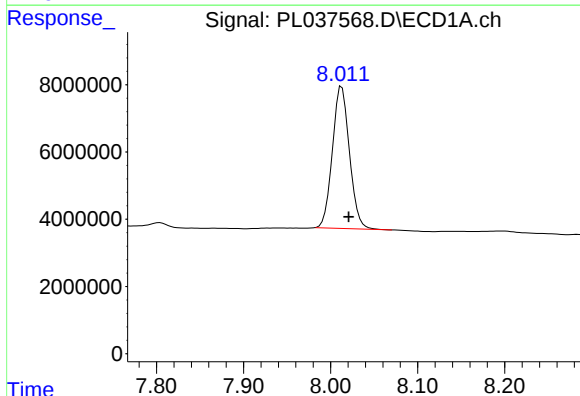

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: -0.008 min
Response: 57507089
Conc: 9.53 ng/ml

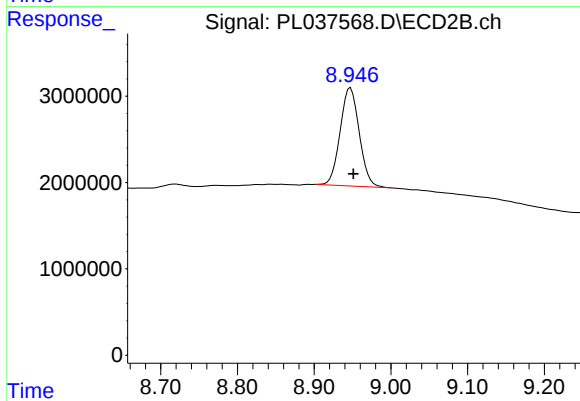

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 19713205
Conc: 9.94 ng/ml