

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
 Data File : PL037572.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2018 20:33
 Operator : UA\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 09:04:10 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.936	119.1E6	42085691	15.056	15.211
28)	SA Decachlor...	8.014	8.947	89165359	27889372	14.777	14.058
Target Compounds							
3)	MA gamma-BHC...	4.016f	0.000	8233514	0	0.798	N.D. #
8)	B Heptachlo...	0.000	5.780	0	34253860	N.D.	12.016 #
10)	B gamma-Chl...	0.000	5.986f	0	28553894	N.D.	10.138 #
14)	MA Endrin	5.848	0.000	32685421	0	4.149	N.D. #
21)	B Endrin ke...	6.935f	0.000	543.3E6	0	76.401	N.D. #
24)	Chlordane-2	0.000	5.316	0	40540190	N.D.	320.347 #
25)	Chlordane-3	0.000	5.986	0	28553894	N.D.	73.012 #
27)	Chlordane-5	5.848	0.000	32685421	0	252.144	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
Data File : PL037572.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2018 20:33
Operator : UA\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 09:04:10 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

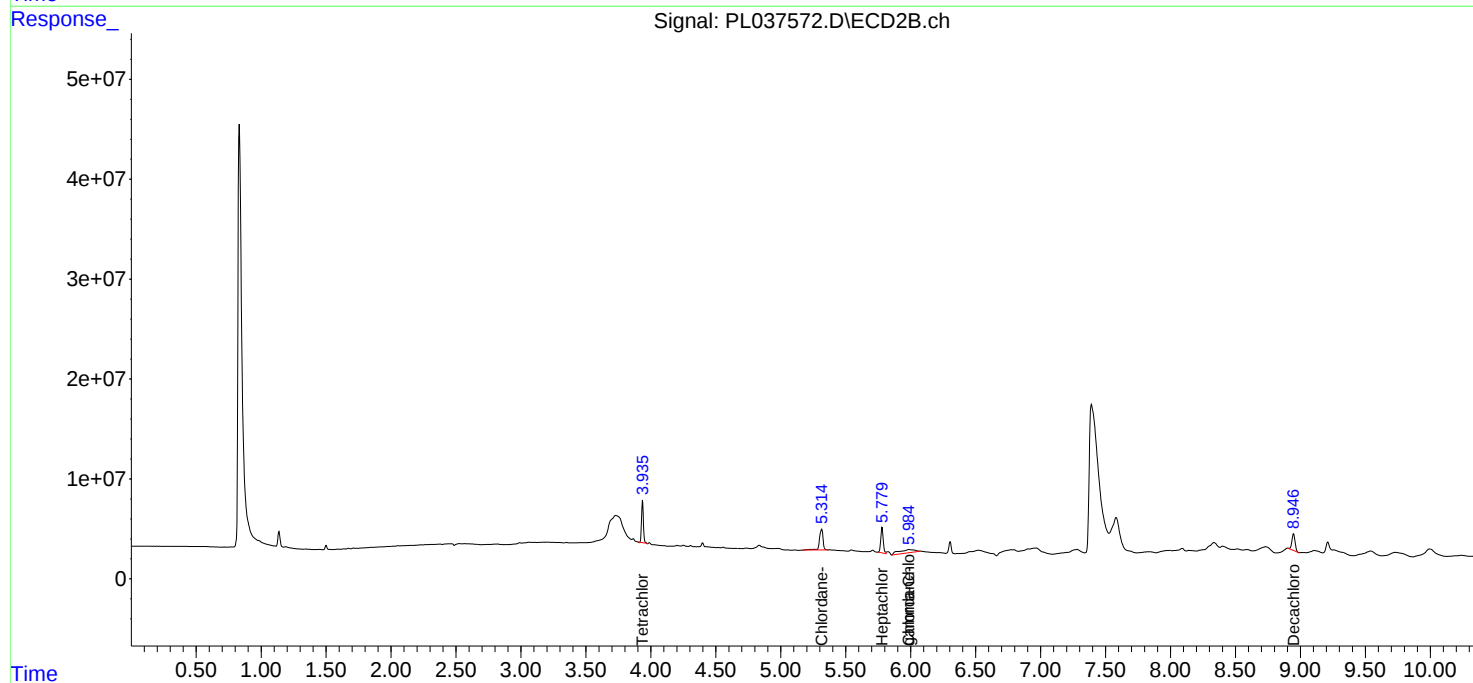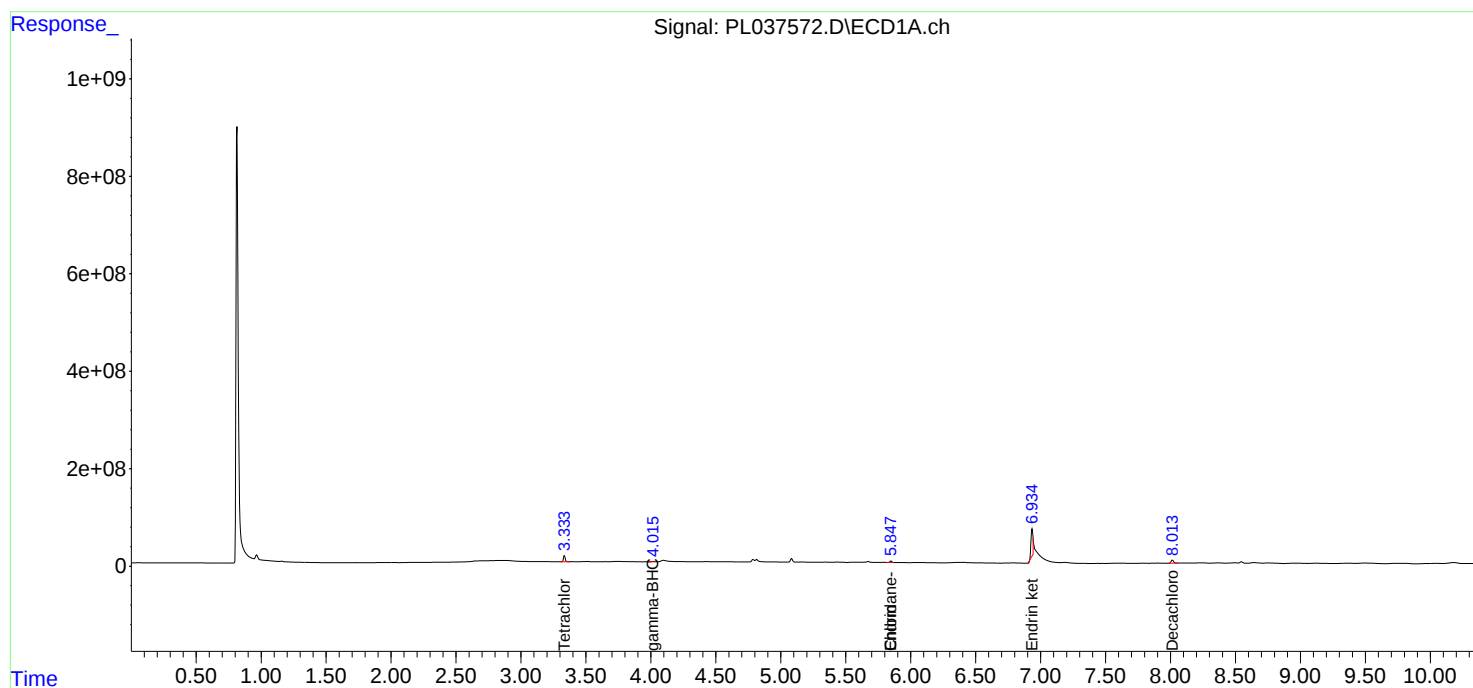


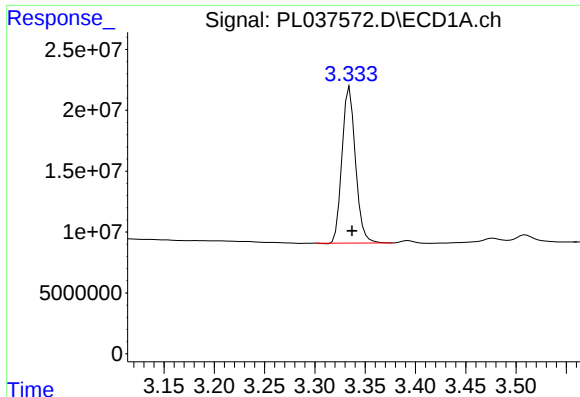

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: -0.002 min
Response: 119094447
Conc: 15.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

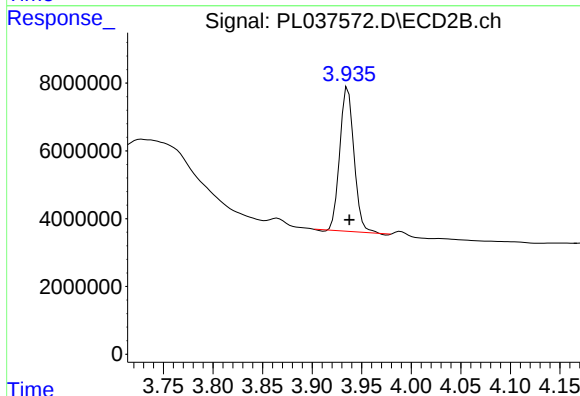


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.001 min
Response: 42085691
Conc: 15.21 ng/ml

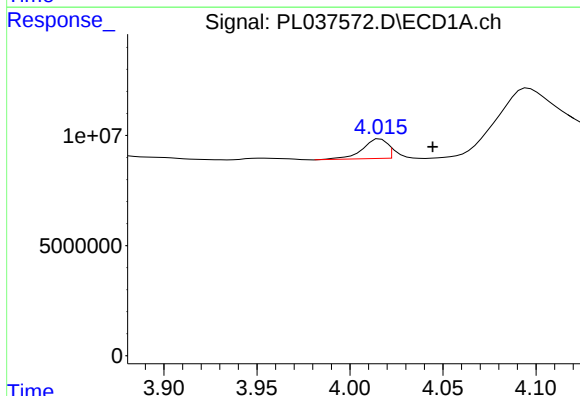


#3 gamma-BHC (Lindane)

R.T.: 4.016 min
Delta R.T.: -0.028 min
Response: 8233514
Conc: 0.80 ng/ml

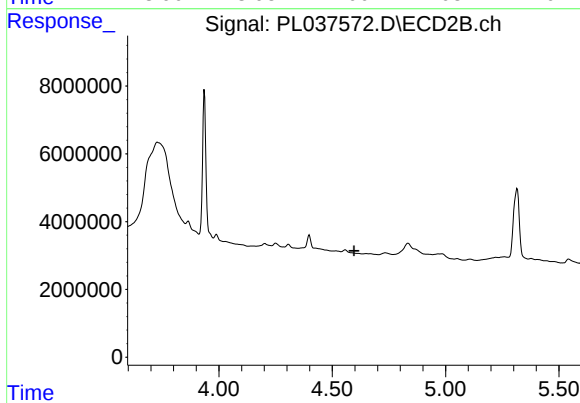

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.597 min
Response: 0
Conc: N.D.

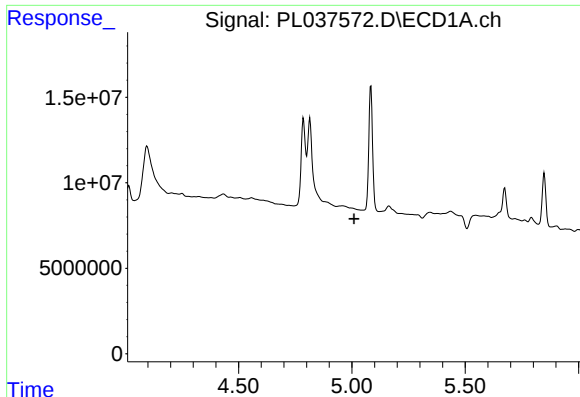

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.010 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

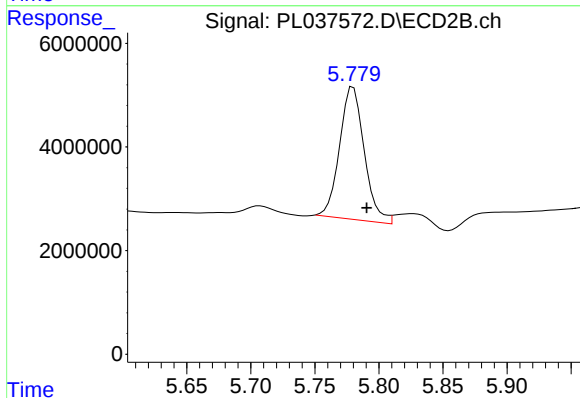


#8 Heptachlor epoxide

R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 34253860
Conc: 12.02 ng/ml

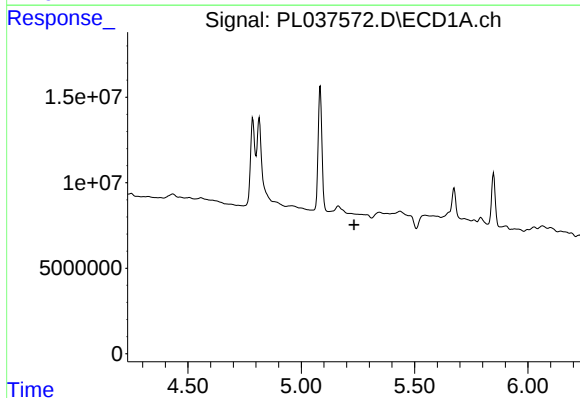


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

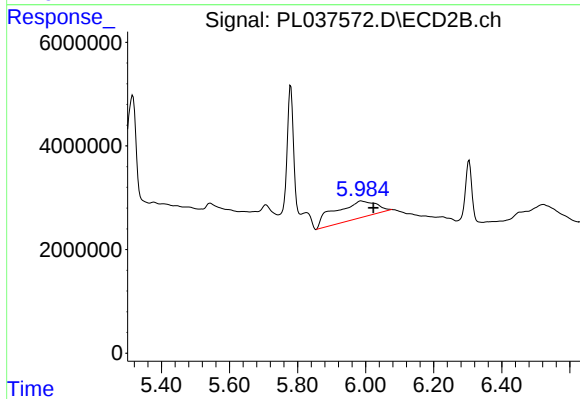

#10 gamma-Chlordane


R.T.: 5.986 min
Delta R.T.: -0.037 min
Response: 28553894
Conc: 10.14 ng/ml

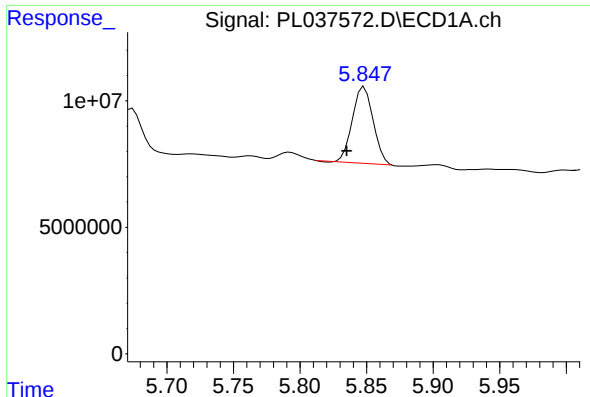

#14 Endrin


R.T.: 5.848 min
Delta R.T.: 0.013 min
Response: 32685421
Conc: 4.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

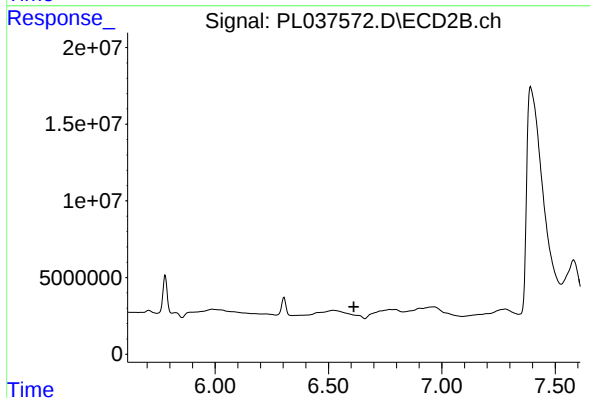


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.612 min
Response: 0
Conc: N.D.

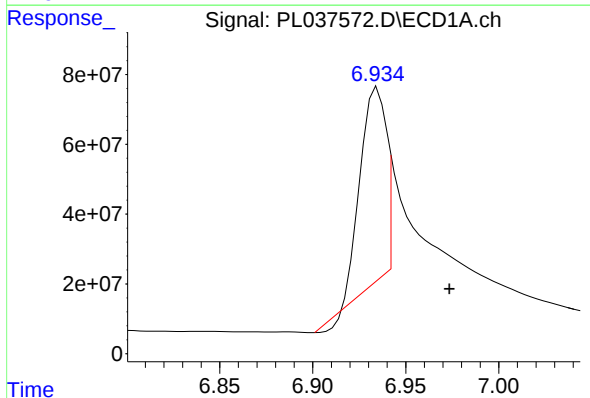


#21 Endrin ketone

R.T.: 6.935 min
Delta R.T.: -0.039 min
Response: 543336426
Conc: 76.40 ng/ml

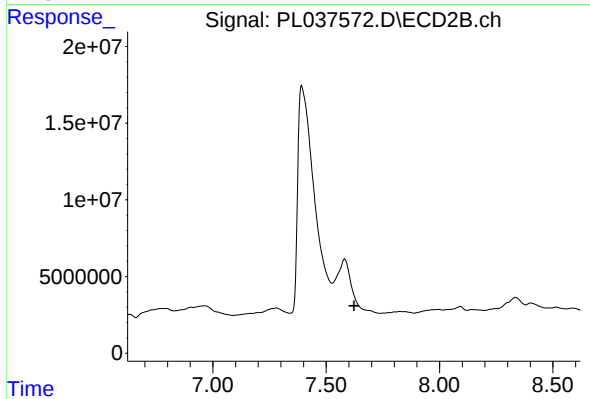

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.623 min
Response: 0
Conc: N.D.

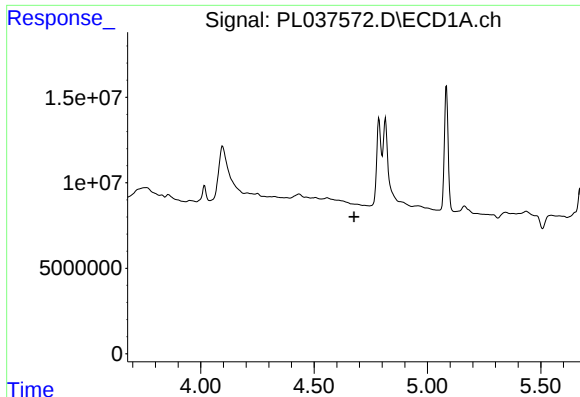

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

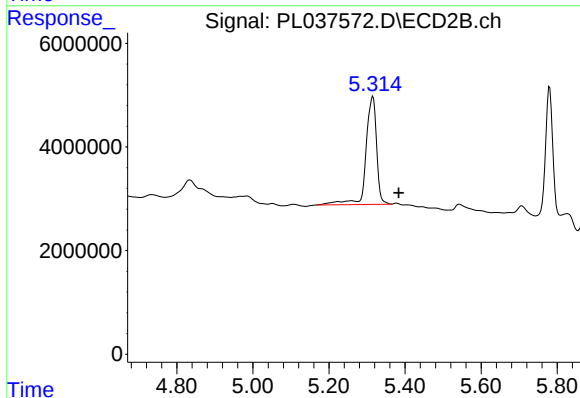


#24 Chlordane-2

R.T.: 5.316 min
Delta R.T.: -0.068 min
Response: 40540190
Conc: 320.35 ng/ml

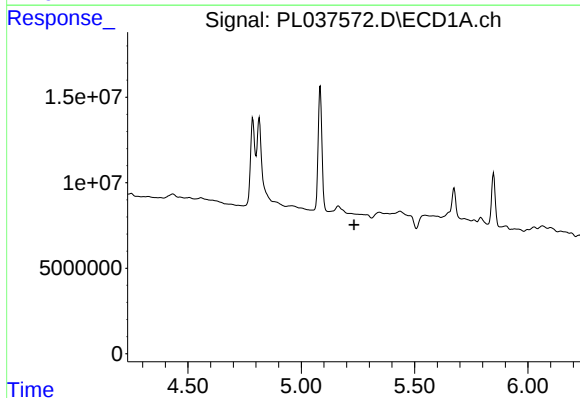


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

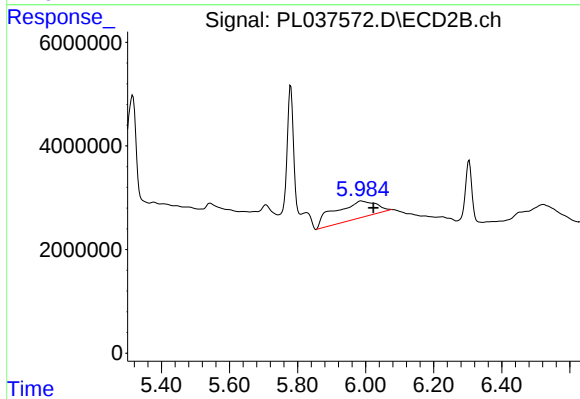

#25 Chlordane-3


R.T.: 5.986 min
Delta R.T.: -0.037 min
Response: 28553894
Conc: 73.01 ng/ml

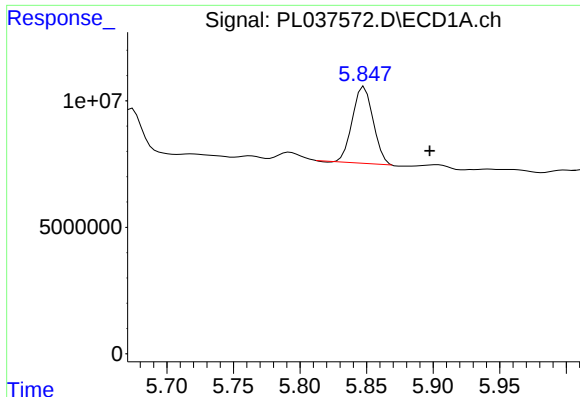

#27 Chlordane-5


R.T.: 5.848 min
Delta R.T.: -0.049 min
Response: 32685421
Conc: 252.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

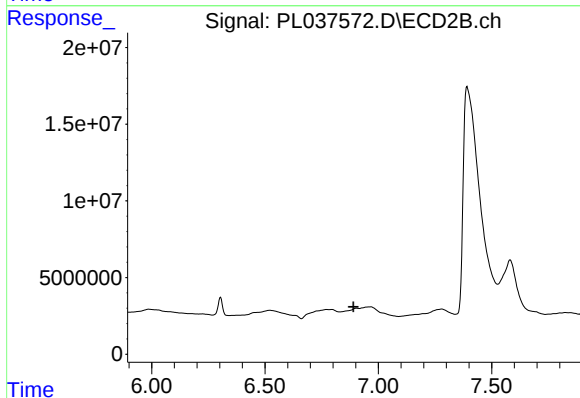


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.890 min
Response: 0
Conc: N.D.

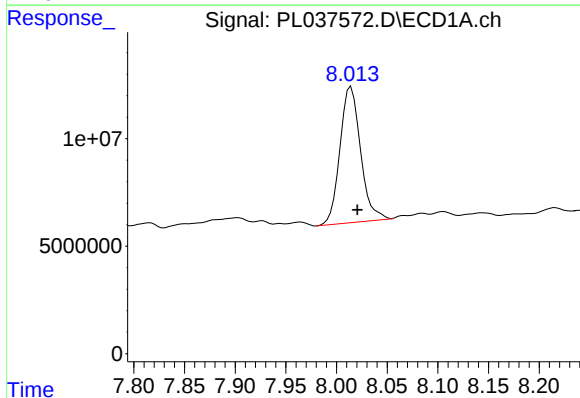

#28 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: -0.006 min
Response: 89165359
Conc: 14.78 ng/ml

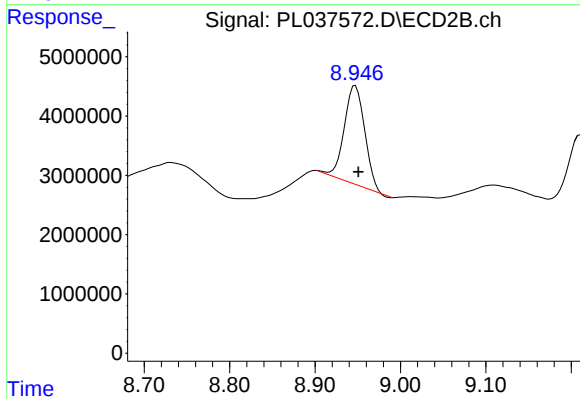

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 27889372
Conc: 14.06 ng/ml