

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
 Data File : PL037568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2018 19:37
 Operator : UA\AJ
 Sample : J3774-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-6(2-4)

Manual Integrations
 APPROVED

mohammad
 7/2/2018 12:26:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 09:03:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.334	3.935	71410684	25129739	9.028	9.083
28) SA Decachlor...	8.013	8.947	57507089	19713205	9.530	9.936
Target Compounds						
10) B gamma-Chl...	5.233	6.021	13834466	7623335	1.477m	2.707 #
11) B alpha-Chl...	5.283	6.097	27766234	17107620	3.057	5.944 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062918\
Data File : PL037568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2018 19:37
Operator : UA\AJ
Sample : J3774-06
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
SB-6(2-4)


Manual Integrations
APPROVED

mohammad
7/2/2018 12:26:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 09:03:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

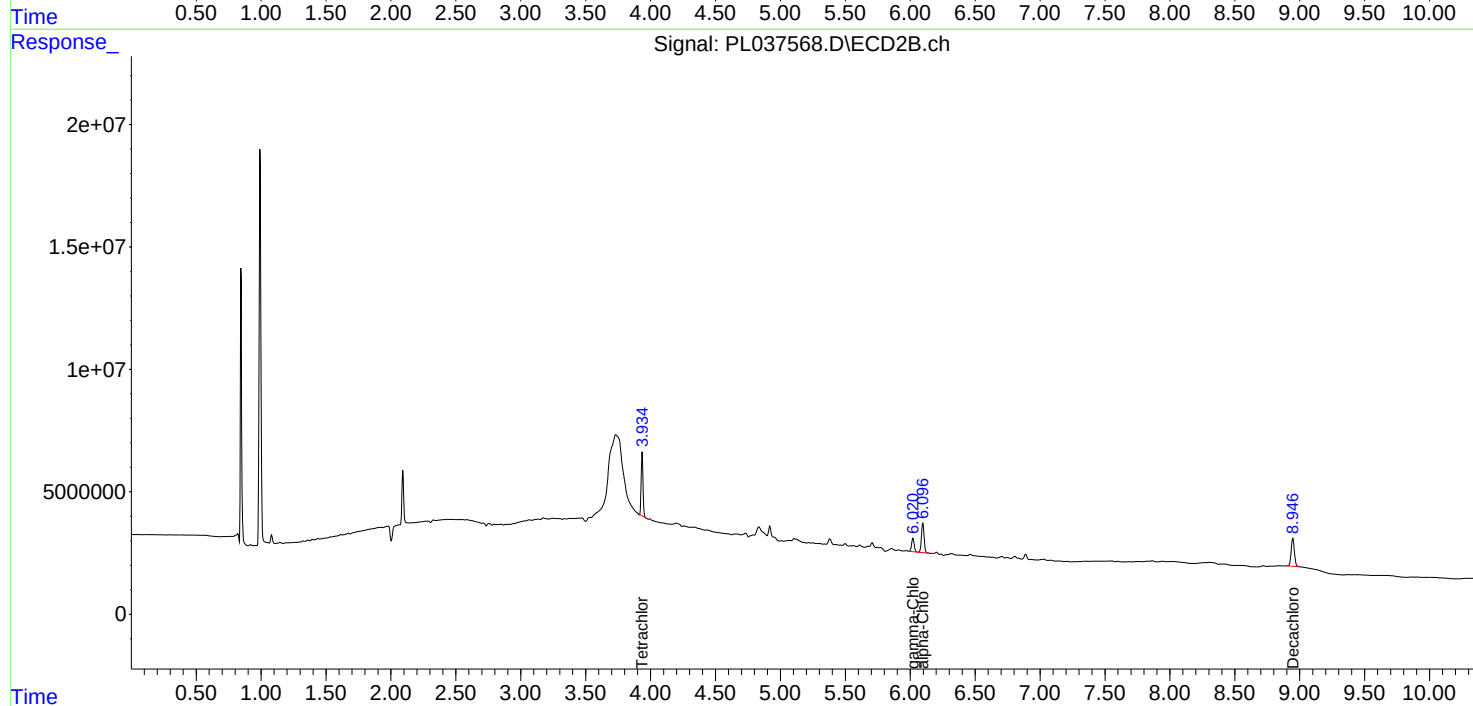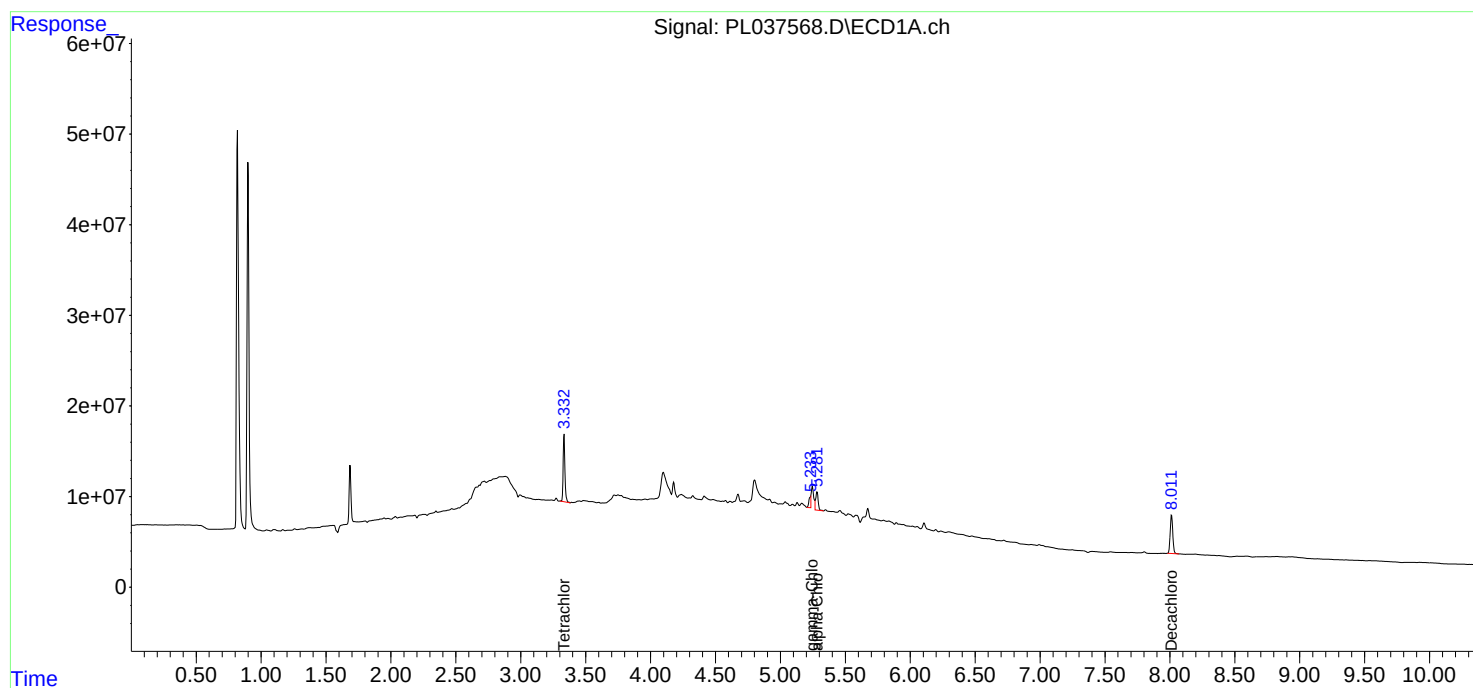

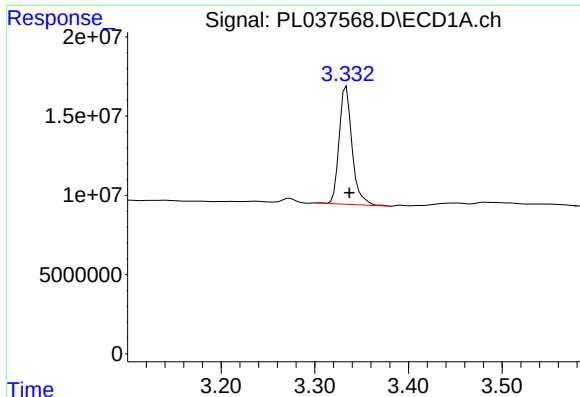


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 71410684
Conc: 9.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(2-4)


Manual Integrations
APPROVED

mohammad
7/2/2018 12:26:41 PM

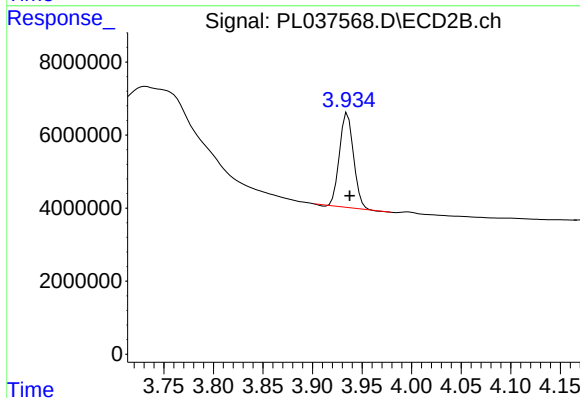


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.002 min
Response: 25129739
Conc: 9.08 ng/ml

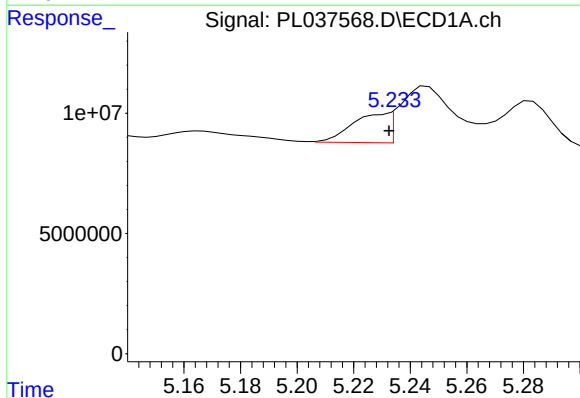


#10 gamma-Chlordane

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 13834466
Conc: 1.48 ng/ml m

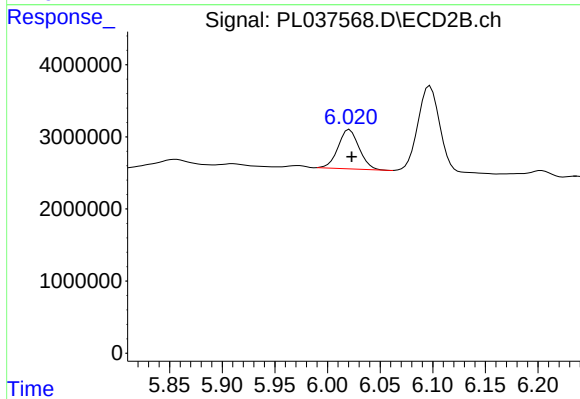

#10 gamma-Chlordane

R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 7623335
Conc: 2.71 ng/ml

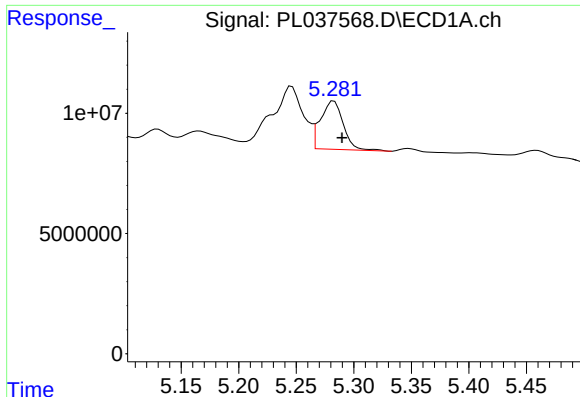


#11 alpha-Chlordane

R.T.: 5.283 min
Delta R.T.: -0.007 min
Response: 27766234
Conc: 3.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-6(2-4)


Manual Integrations
APPROVED

mohammad
7/2/2018 12:26:41 PM

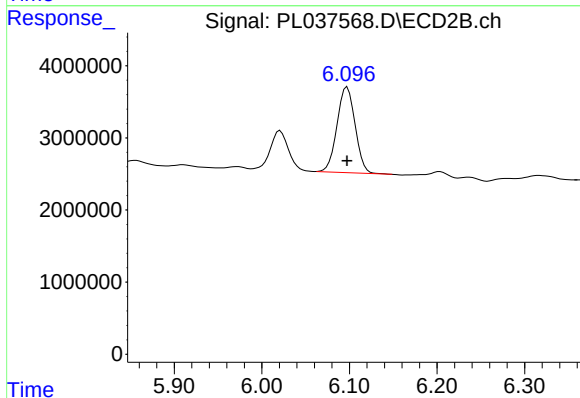


#11 alpha-Chlordane

R.T.: 6.097 min
Delta R.T.: 0.000 min
Response: 17107620
Conc: 5.94 ng/ml

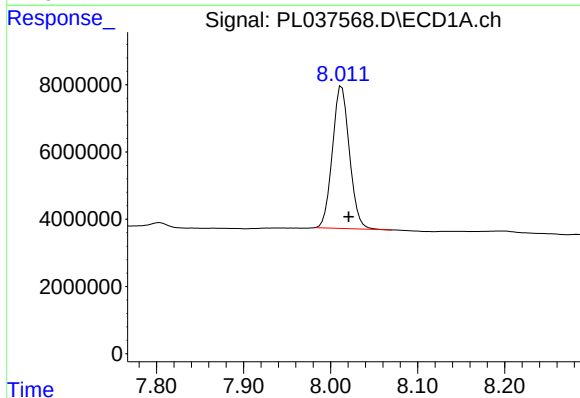

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: -0.008 min
Response: 57507089
Conc: 9.53 ng/ml

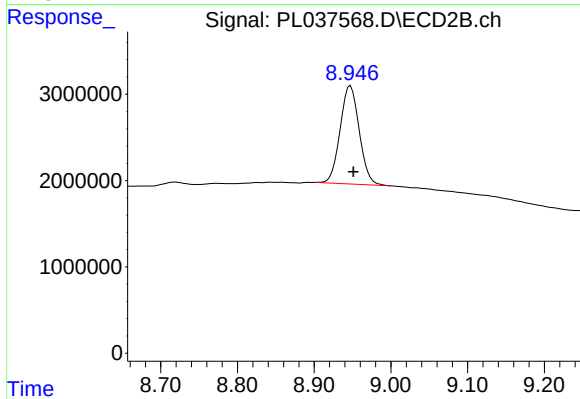

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 19713205
Conc: 9.94 ng/ml