

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062921\
 Data File : PL067871.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2021 14:33
 Operator : AR\AJ
 Sample : M2884-01 (Sig #1); M2854-01 (Sig #2)
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-03-062821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 02:56:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.526	4562768	8088727	8.299m	8.580
28)	SA Decachlor...	10.218	11.422	6001135	9454234	8.468	9.492

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062921\
Data File : PL067871.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2021 14:33
Operator : AR\AJ
Sample : M2884-01 (Sig #1); M2854-01 (Sig #2)
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OK-03-062821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 02:56:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

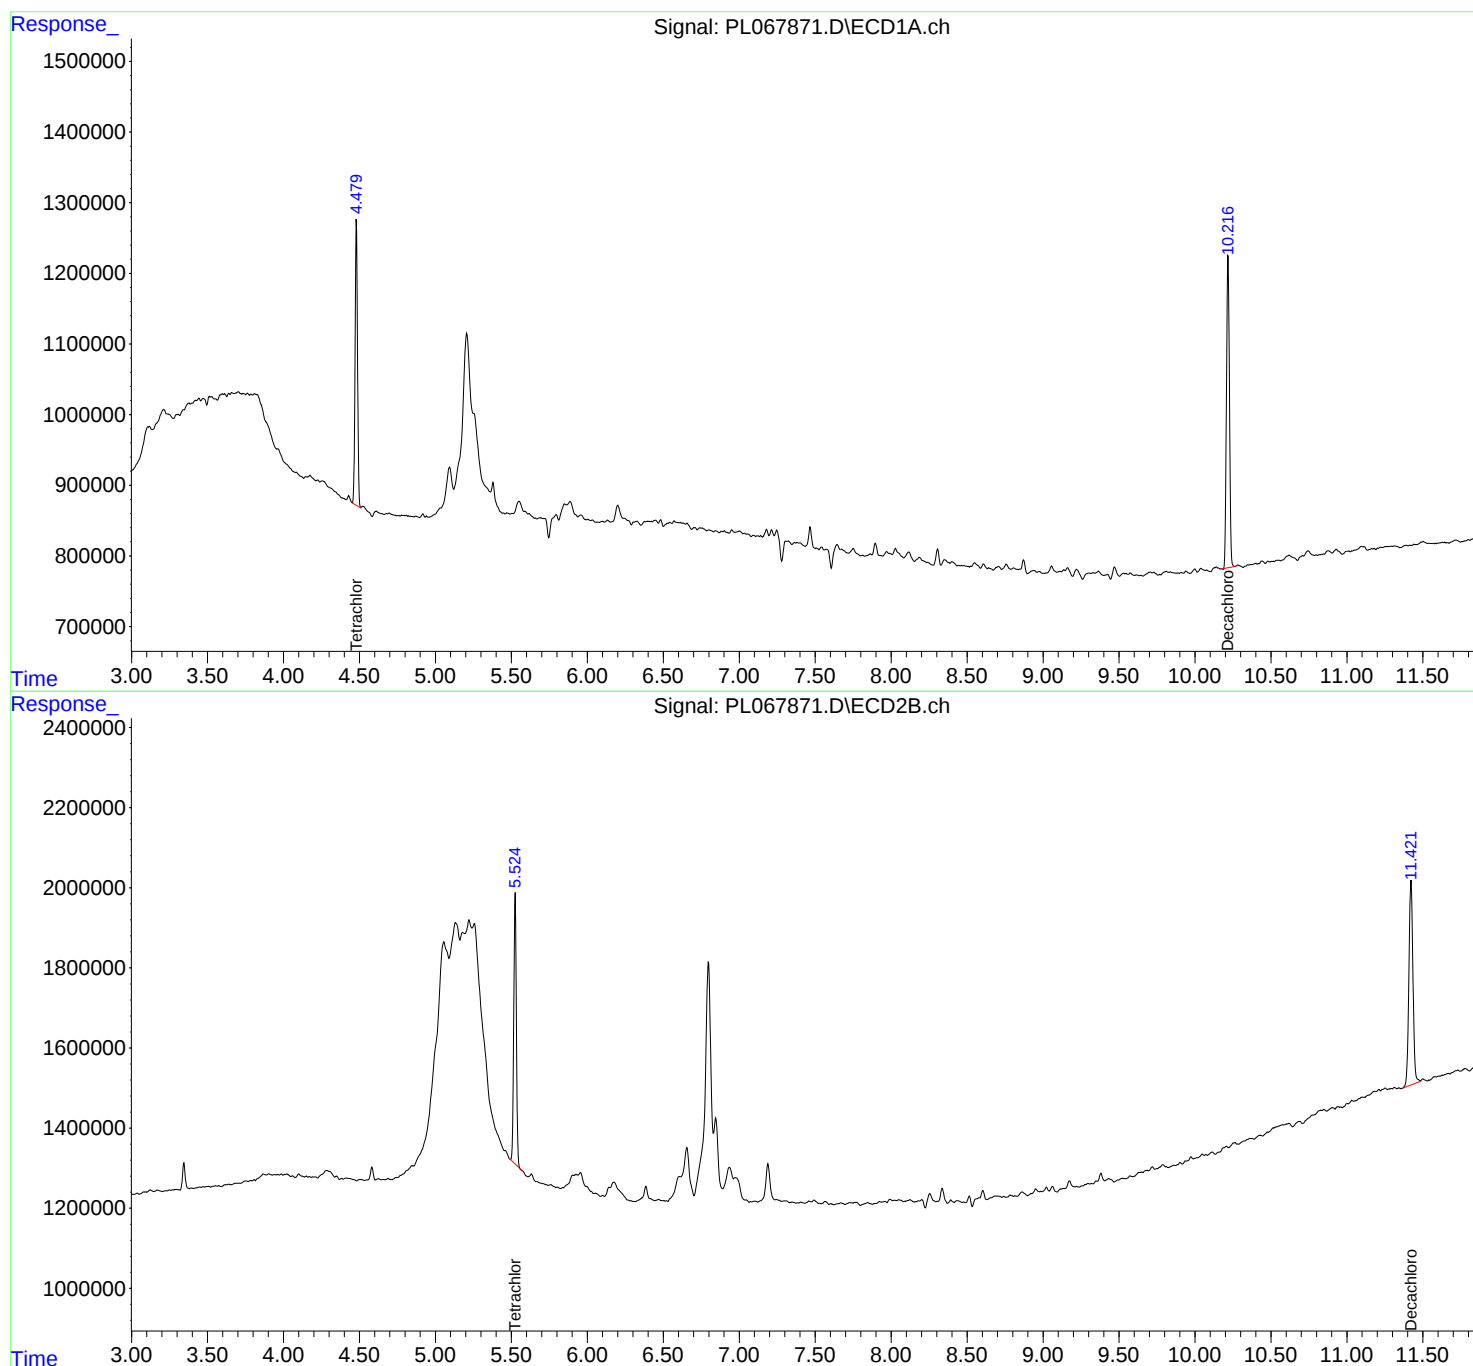


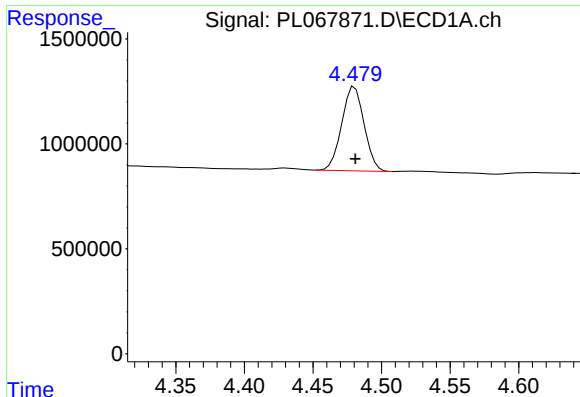

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 4562768
Conc: 8.30 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OK-03-062821

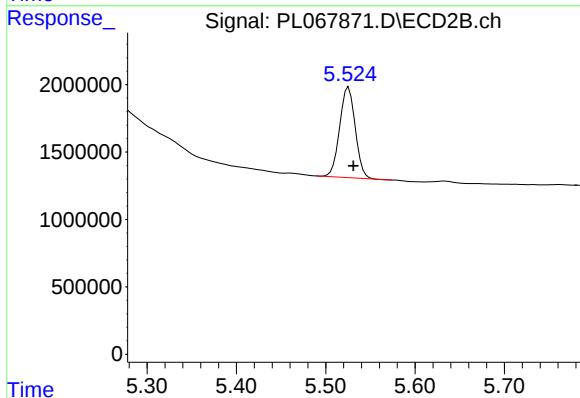


#1 Tetrachloro-m-xylene

R.T.: 5.526 min
Delta R.T.: -0.005 min
Response: 8088727
Conc: 8.58 ng/ml

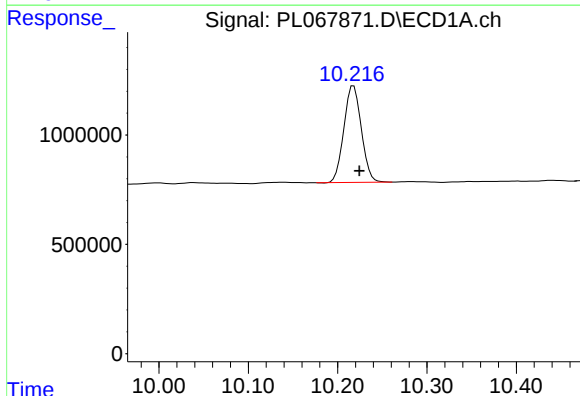

#28 Decachlorobiphenyl

R.T.: 10.218 min
Delta R.T.: -0.007 min
Response: 6001135
Conc: 8.47 ng/ml

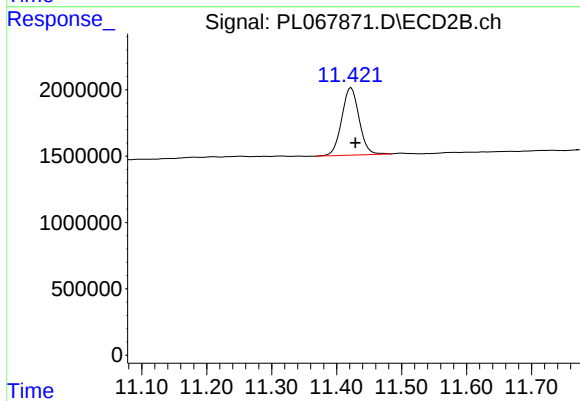

#28 Decachlorobiphenyl

R.T.: 11.422 min
Delta R.T.: -0.006 min
Response: 9454234
Conc: 9.49 ng/ml