

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062922\
 Data File : PL076100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jun 2022 10:54
 Operator : AR\AJ
 Sample : N3442-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANTRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/30/2022
 Supervised By :Ankita Jodhani 06/30/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 04:18:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.645	4.632	9663098	24620768	12.776m	12.981m
28)	SA Decachlor...	11.635	10.373	4961510	16757953	7.885m	10.911 #
Target Compounds							
12)	B 4,4'-DDE	8.664	7.615	3827702	10329020	5.663m	6.085m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062922\
Data File : PL076100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jun 2022 10:54
Operator : AR\AJ
Sample : N3442-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/30/2022
Supervised By : Ankita Jodhani 06/30/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 04:18:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

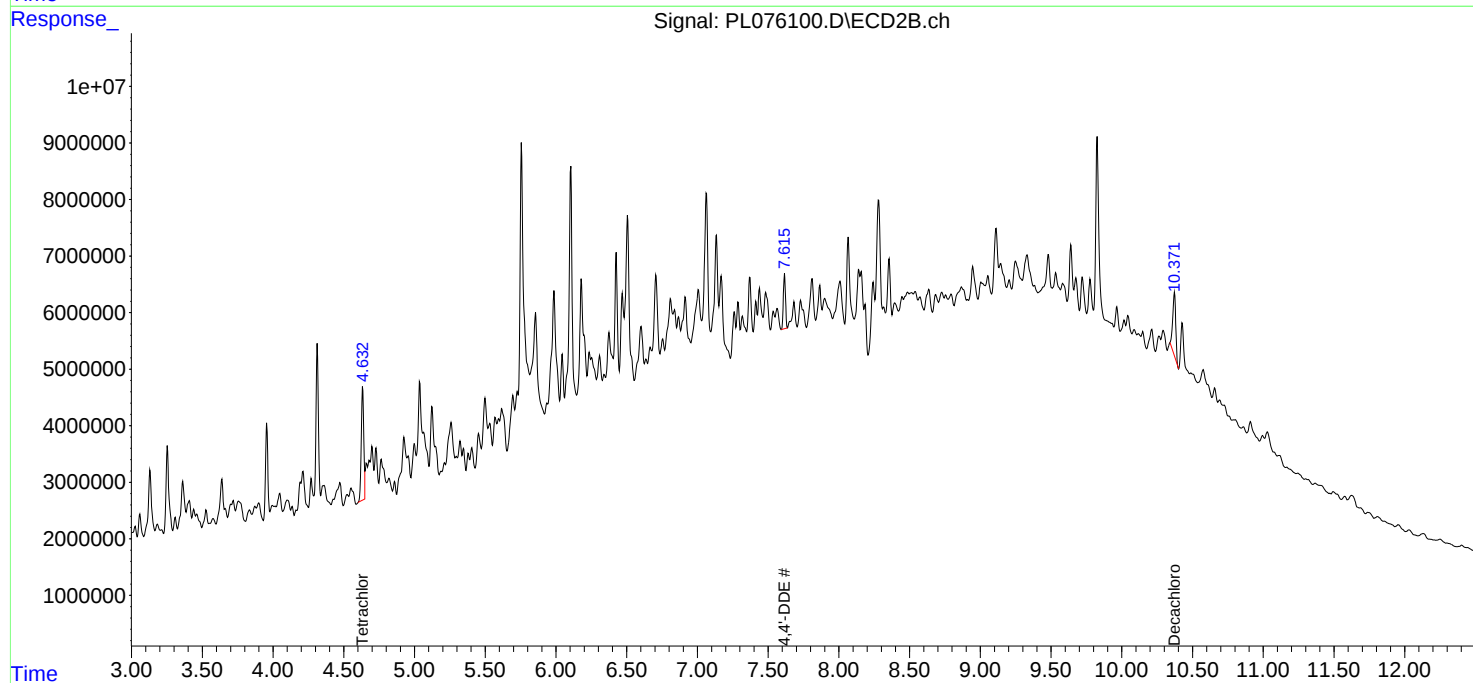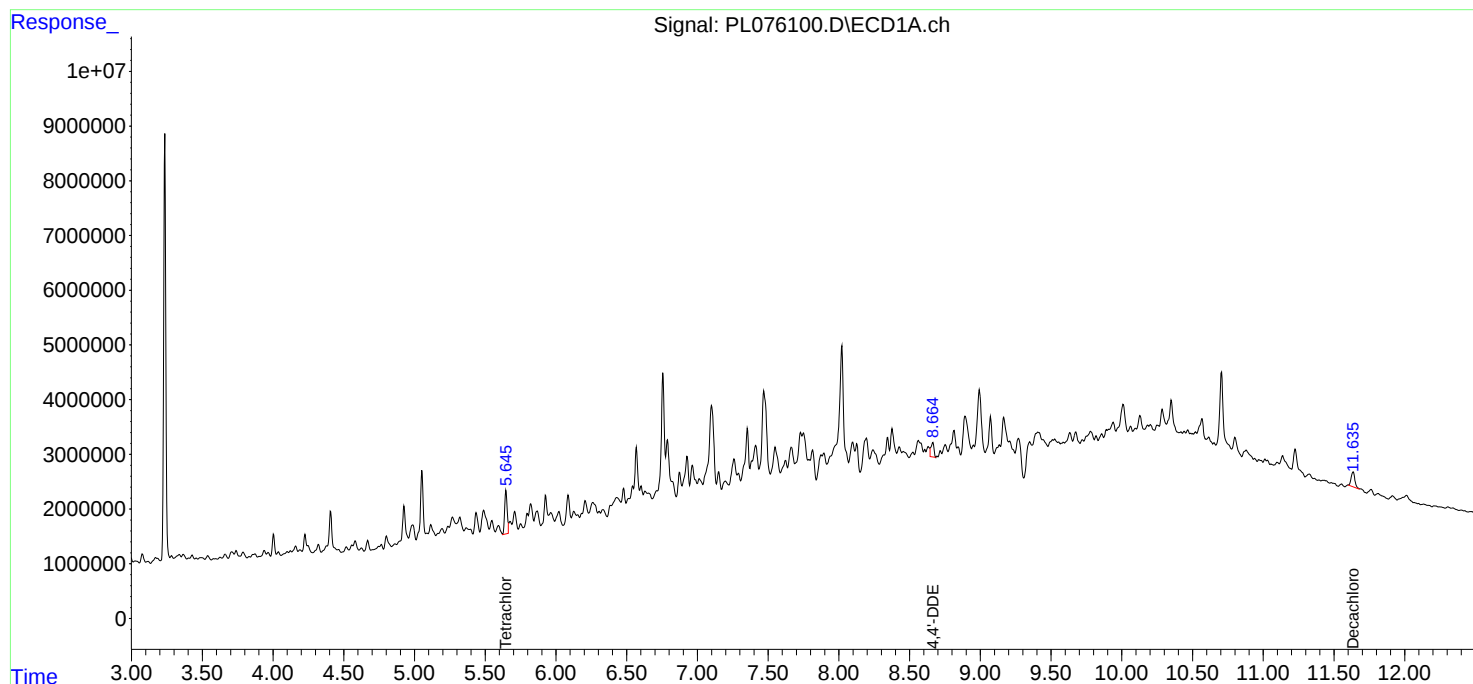

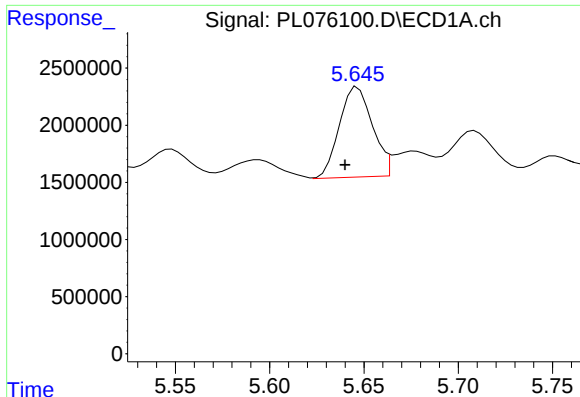


#1 Tetrachloro-m-xylene

R.T.: 5.645 min
Delta R.T.: 0.005 min
Response: 9663098
Conc: 12.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/30/2022
Supervised By :Ankita Jodhani 06/30/2022

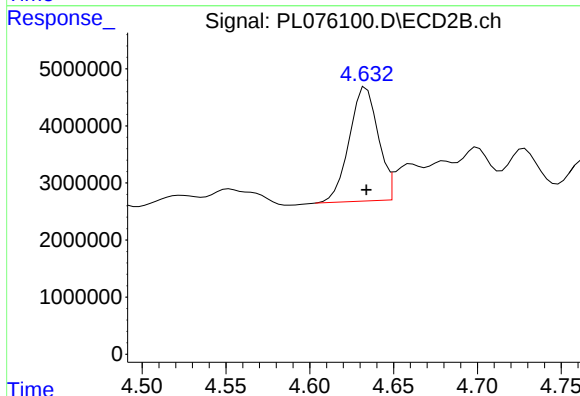


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 24620768
Conc: 12.98 ng/ml m

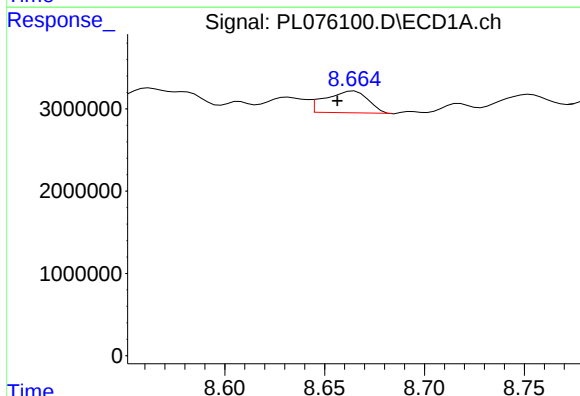


#12 4,4'-DDE

R.T.: 8.664 min
Delta R.T.: 0.007 min
Response: 3827702
Conc: 5.66 ng/ml m

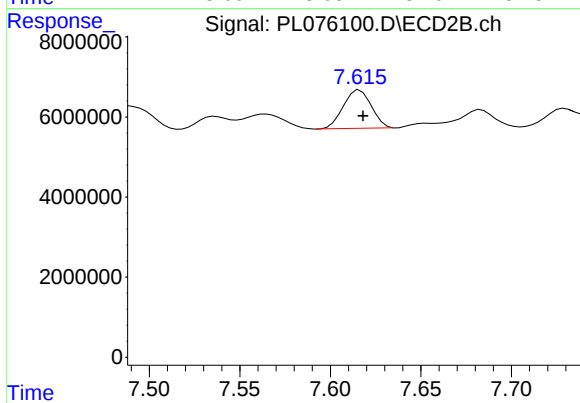

#12 4,4'-DDE

R.T.: 7.615 min
Delta R.T.: -0.003 min
Response: 10329020
Conc: 6.09 ng/ml m

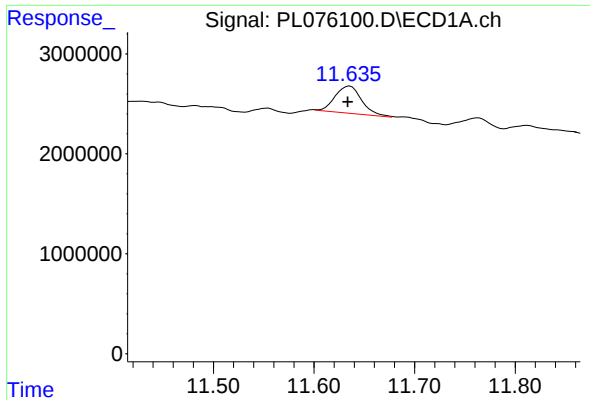


#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: 0.000 min
Response: 4961510
Conc: 7.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANTRE

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/30/2022
Supervised By :Ankita Jodhani 06/30/2022

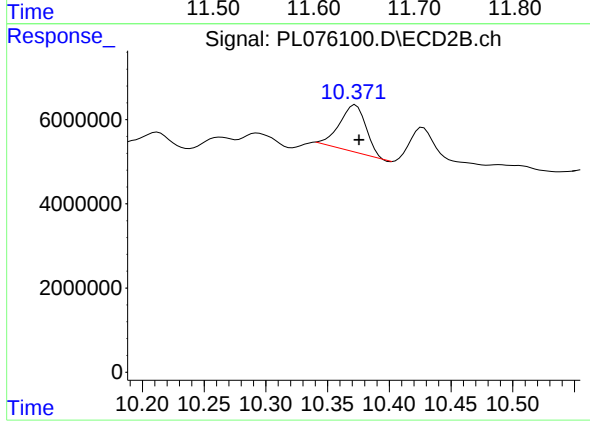

#28 Decachlorobiphenyl

R.T.: 10.373 min
Delta R.T.: -0.003 min
Response: 16757953
Conc: 10.91 ng/ml