

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 20:48
 Operator : AJ\MA
 Sample : PB129876TB
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:34:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	35849514	54462941	19.960	20.479
28)	SA Decachlor...	8.288	9.183	31908437	45434436	20.784	20.902
Target Compounds							
2)	A alpha-BHC	3.966	4.488f	1763044	-57668	0.685	N.D. #
4)	MA Heptachlor	0.000	5.262	0	2012849	N.D.	0.575 #
15)	B Endosulfa...	6.345	7.008	432669	2000342	0.285	0.779 #
16)	A 4,4'-DDD	6.212	0.000	880671	0	0.660	N.D. #
17)	MA 4,4'-DDT	0.000	7.231f	0	300706	N.D.	0.133 #
18)	B Endrin al...	6.494f	7.138	103481	326660	0.082	0.147 #
23)	Chlordane-1	4.422f	0.000	1142897	0	21.931	N.D. #
27)	Chlordane-5	6.345f	7.073	432669	2138865	8.422	24.579 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 20:48
Operator : AJ\MA
Sample : PB129876TB
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:34:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

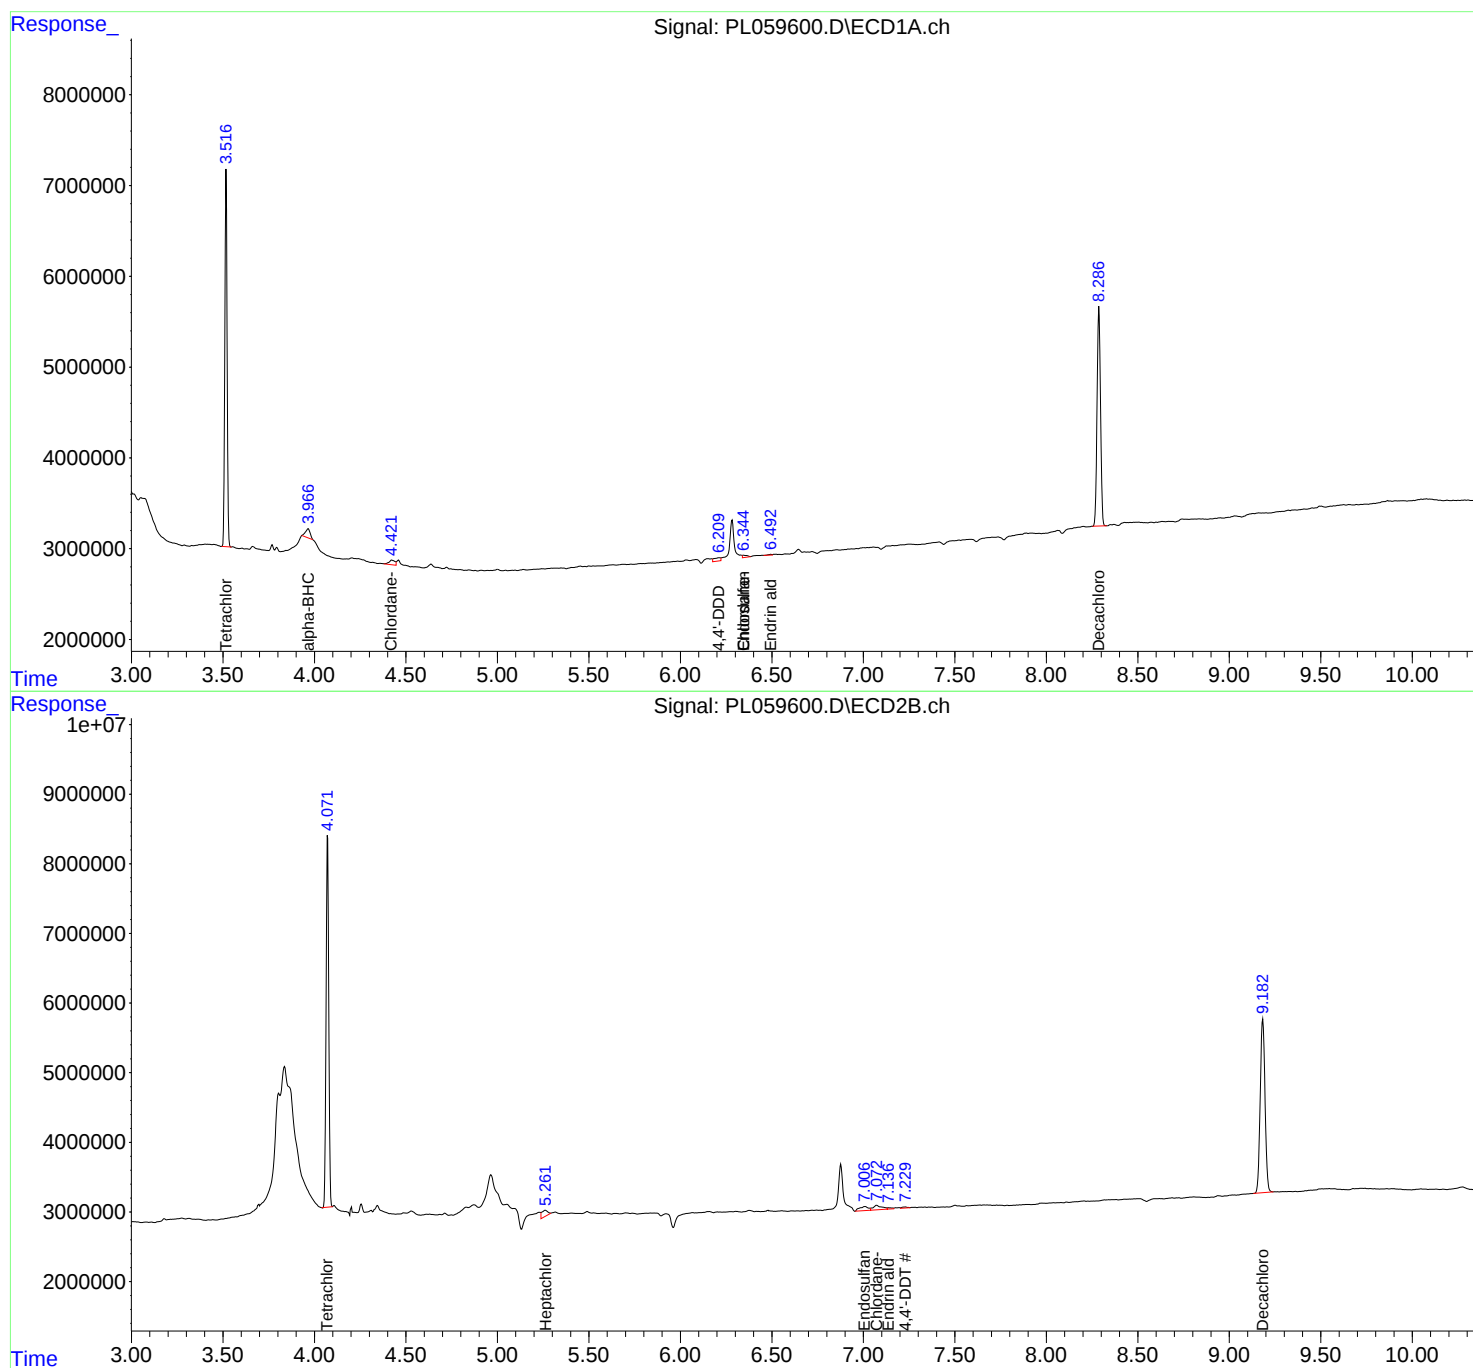


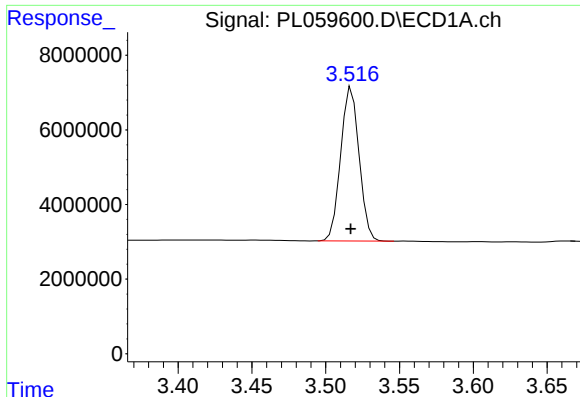

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 35849514
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

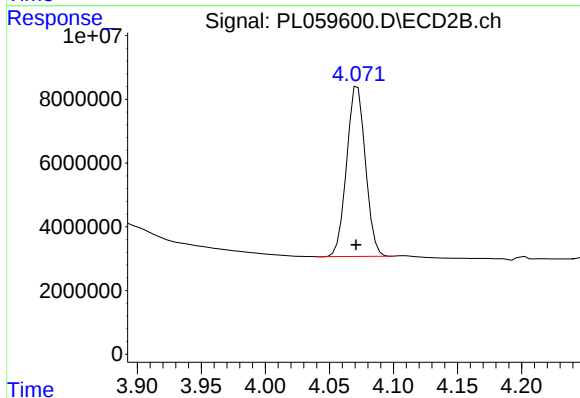


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.001 min
Response: 54462941
Conc: 20.48 ng/ml

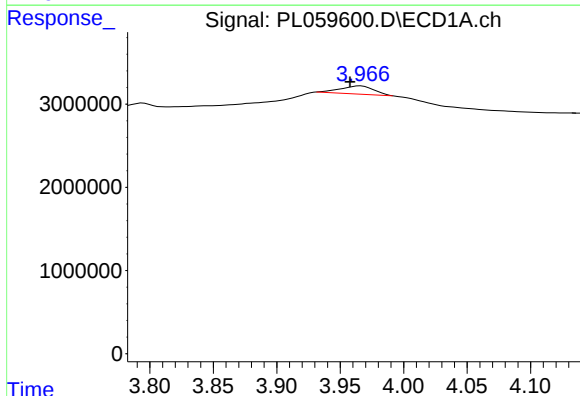


#2 alpha-BHC

R.T.: 3.966 min
Delta R.T.: 0.008 min
Response: 1763044
Conc: 0.69 ng/ml

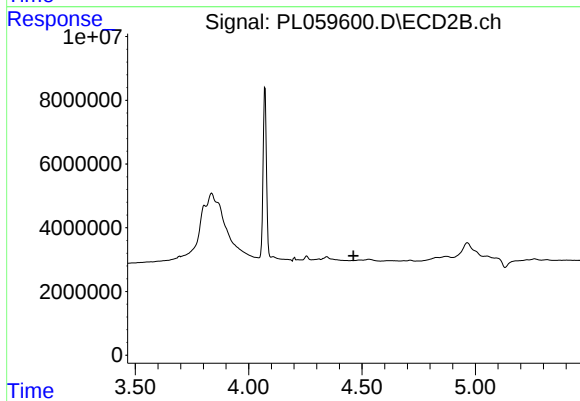

#2 alpha-BHC


R.T.: 4.488 min
Delta R.T.: 0.025 min
Response: -57668
Conc: N.D.

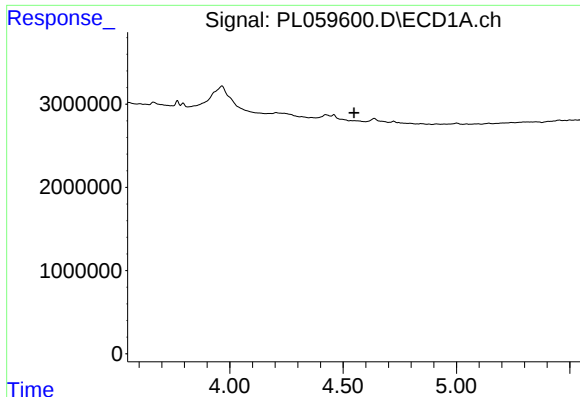

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

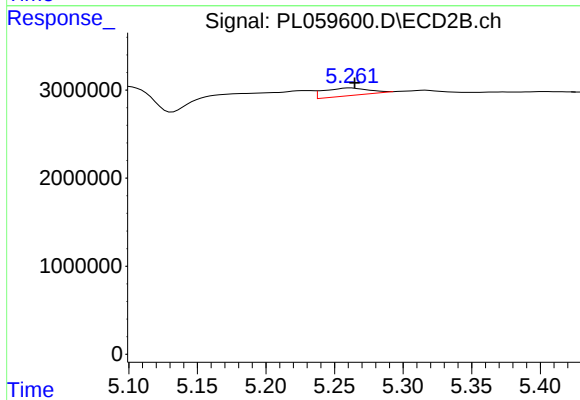


#4 Heptachlor

R.T.: 5.262 min
Delta R.T.: -0.003 min
Response: 2012849
Conc: 0.57 ng/ml

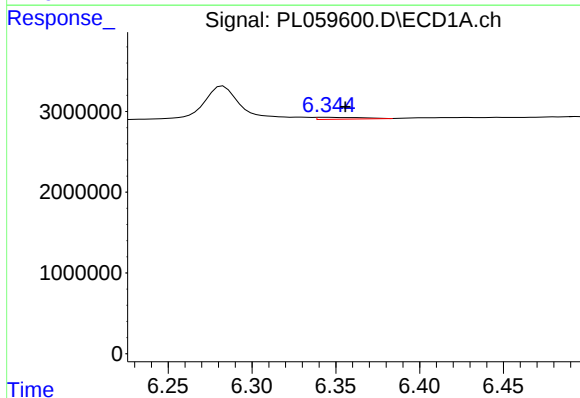


#15 Endosulfan II

R.T.: 6.345 min
Delta R.T.: -0.011 min
Response: 432669
Conc: 0.29 ng/ml

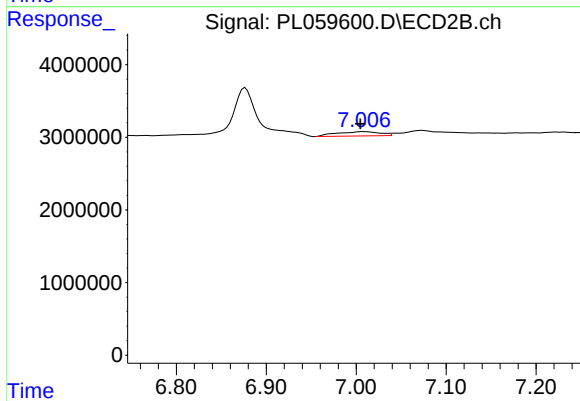

#15 Endosulfan II


R.T.: 7.008 min
Delta R.T.: 0.003 min
Response: 2000342
Conc: 0.78 ng/ml

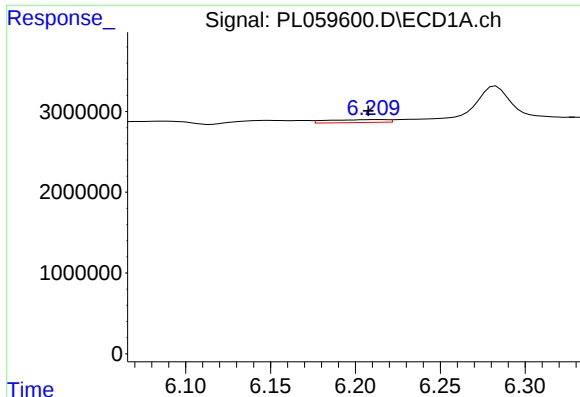

#16 4,4'-DDD


R.T.: 6.212 min
Delta R.T.: 0.004 min
Response: 880671
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

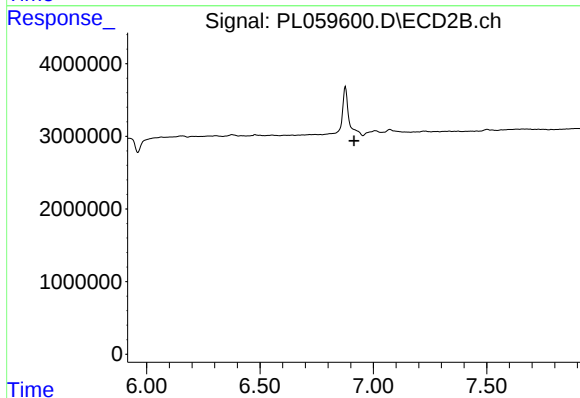


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

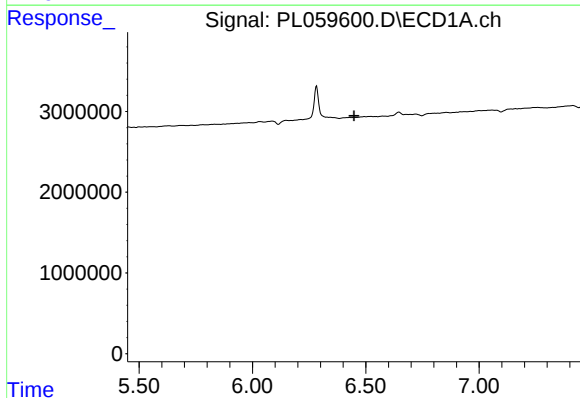


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.449 min
Response: 0
Conc: N.D.

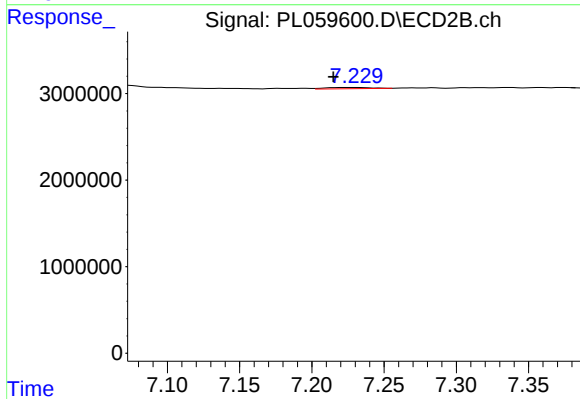

#17 4,4'-DDT


R.T.: 7.231 min
Delta R.T.: 0.016 min
Response: 300706
Conc: 0.13 ng/ml

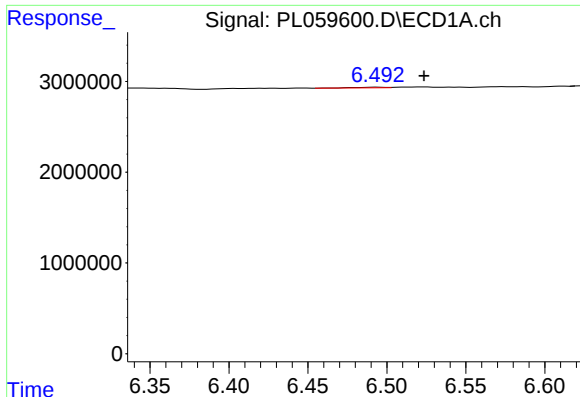

#18 Endrin aldehyde


R.T.: 6.494 min
Delta R.T.: -0.029 min
Response: 103481
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

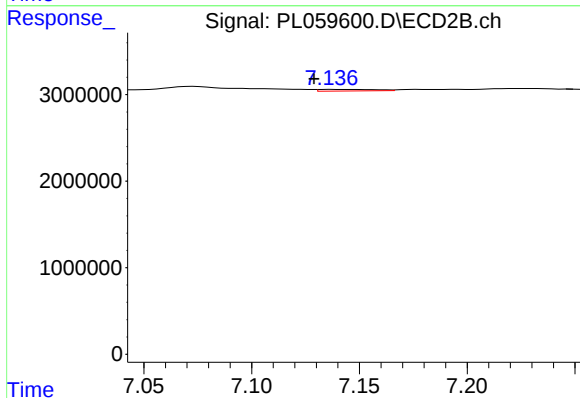


#18 Endrin aldehyde

R.T.: 7.138 min
Delta R.T.: 0.009 min
Response: 326660
Conc: 0.15 ng/ml

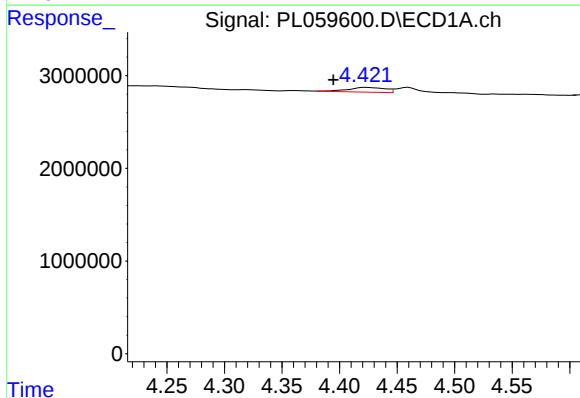


#23 Chlordane-1

R.T.: 4.422 min
Delta R.T.: 0.028 min
Response: 1142897
Conc: 21.93 ng/ml

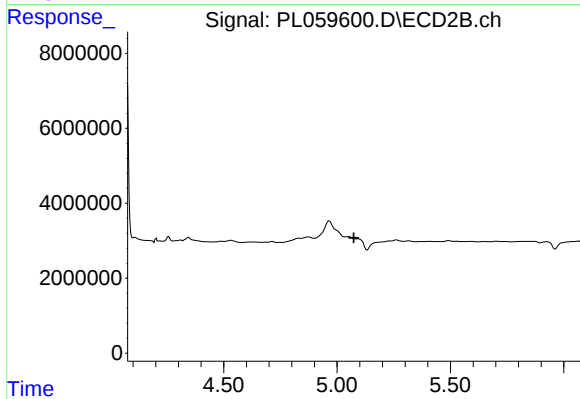

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.074 min
Response: 0
Conc: N.D.

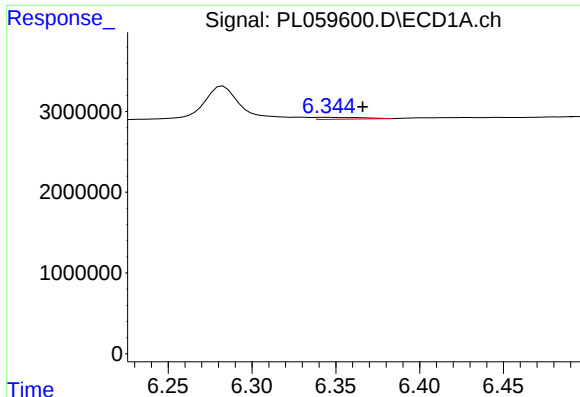

#27 Chlordane-5


R.T.: 6.345 min
Delta R.T.: -0.021 min
Response: 432669
Conc: 8.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

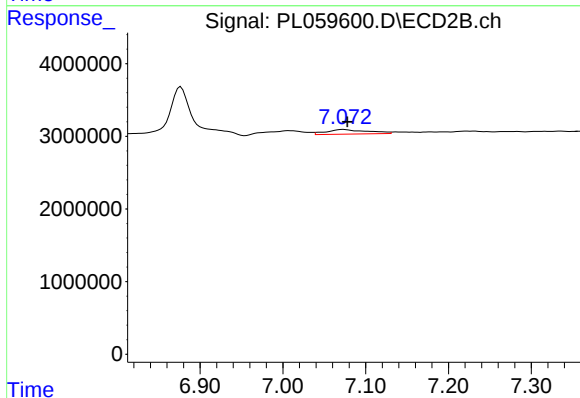


#27 Chlordane-5

R.T.: 7.073 min
Delta R.T.: -0.005 min
Response: 2138865
Conc: 24.58 ng/ml

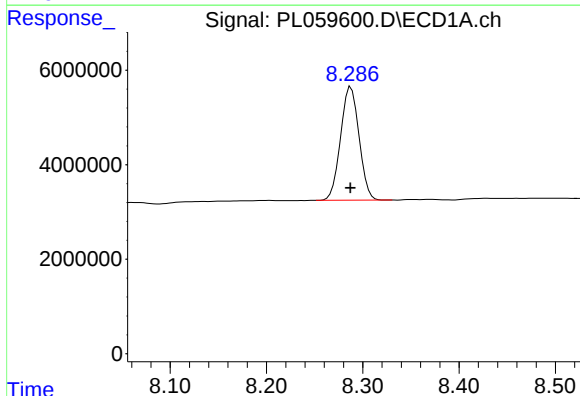

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 31908437
Conc: 20.78 ng/ml

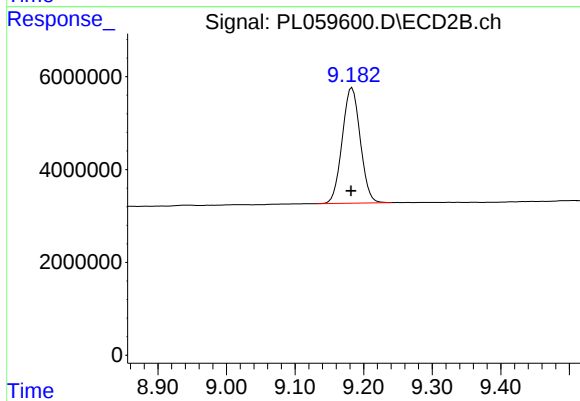

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.001 min
Response: 45434436
Conc: 20.90 ng/ml