

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 23:23
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:37:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.072	46335276	69170996	25.798	26.010
28)	SA Decachlor...	8.286	9.183	41929013	57646750	27.311	26.521
Target Compounds							
2)	A alpha-BHC	3.967	0.000	1142674	0	0.444	N.D. #
4)	MA Heptachlor	0.000	5.265	0	1264792	N.D.	0.361 #
8)	B Heptachlo...	0.000	5.941f	0	1420992	N.D.	0.585 #
15)	B Endosulfa...	6.354	7.007	24287	2105749	0.016	0.820 #
16)	A 4,4'-DDD	6.202	0.000	70956	0	0.053	N.D. #
17)	MA 4,4'-DDT	0.000	7.224	0	214108	N.D.	0.095 #
19)	B Endosulfa...	0.000	7.380f	0	474066	N.D.	0.198 #
23)	Chlordane-1	4.423f	5.103f	1344734	3535814	25.803	32.750 #
27)	Chlordane-5	6.354	7.072	24287	854153	0.473	9.815 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 23:23
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:37:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

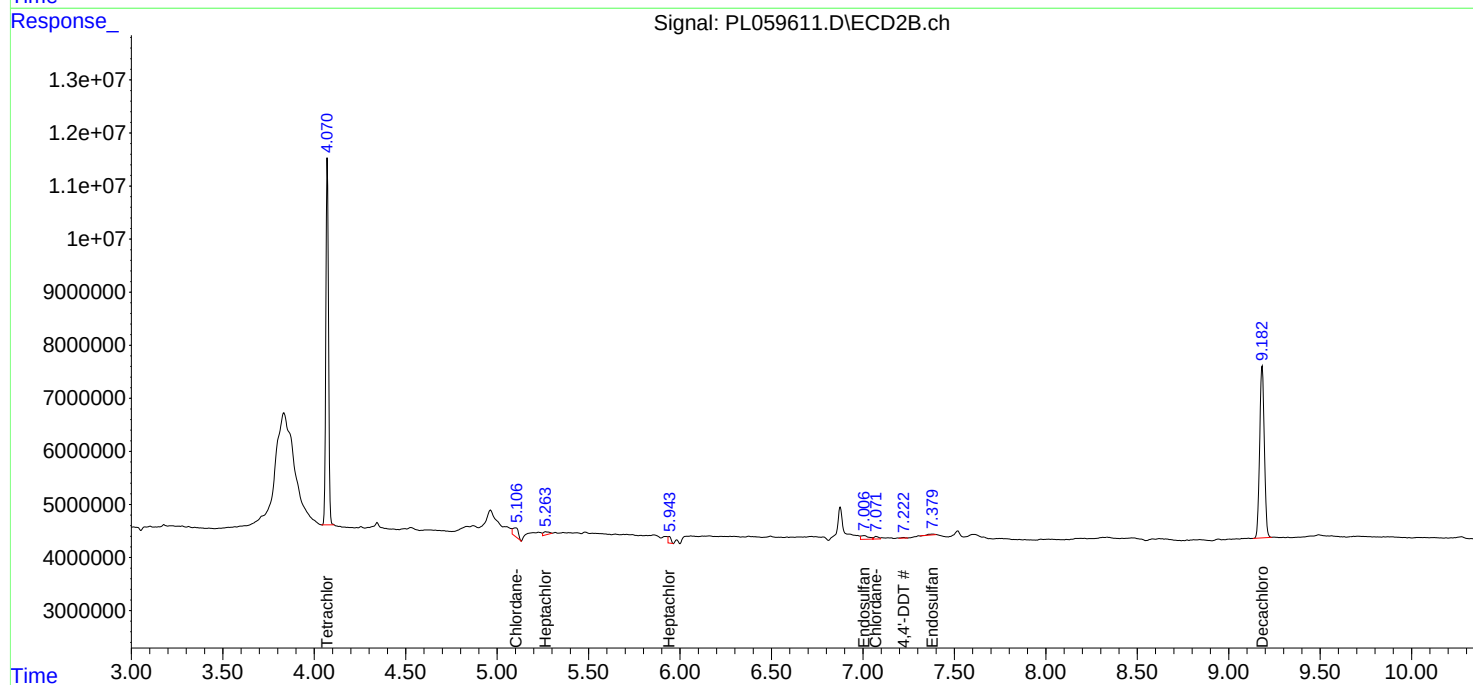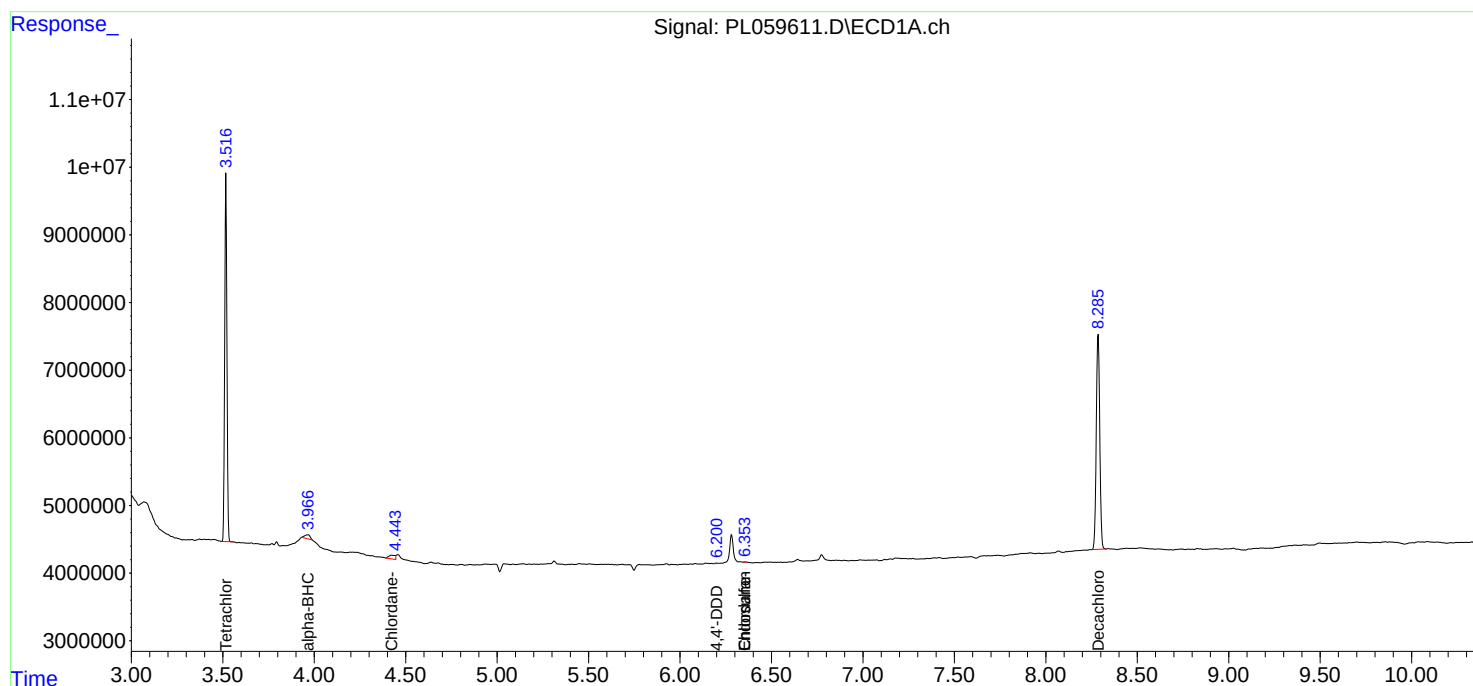


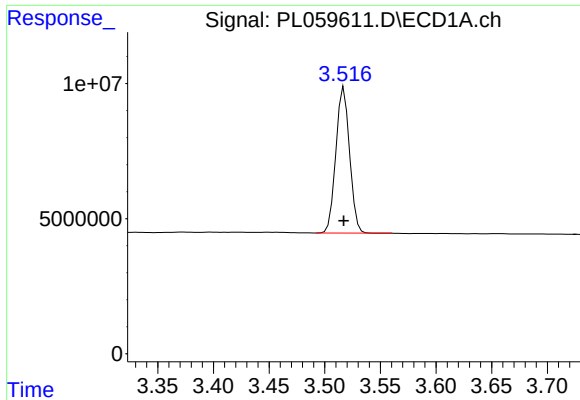

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 46335276
Conc: 25.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

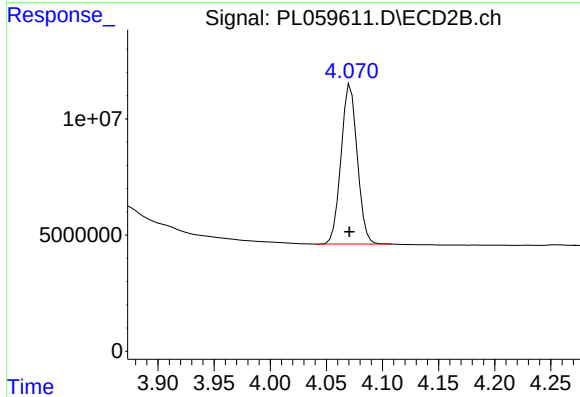


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 69170996
Conc: 26.01 ng/ml

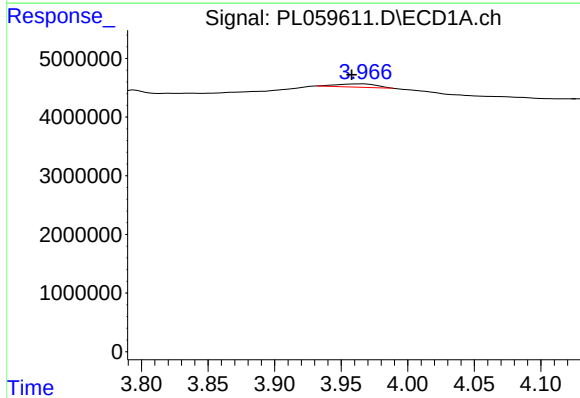


#2 alpha-BHC

R.T.: 3.967 min
Delta R.T.: 0.009 min
Response: 1142674
Conc: 0.44 ng/ml

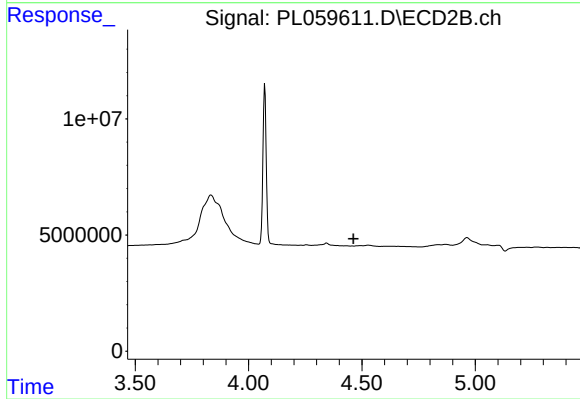

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

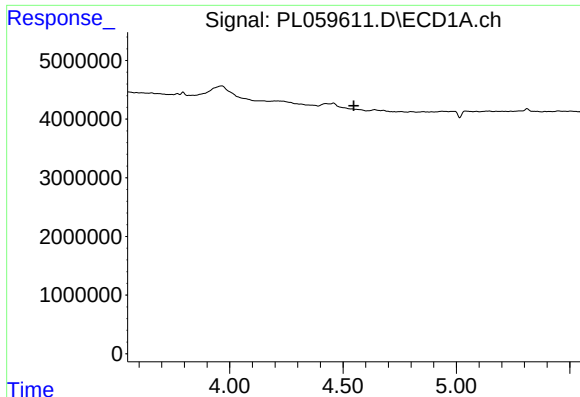

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

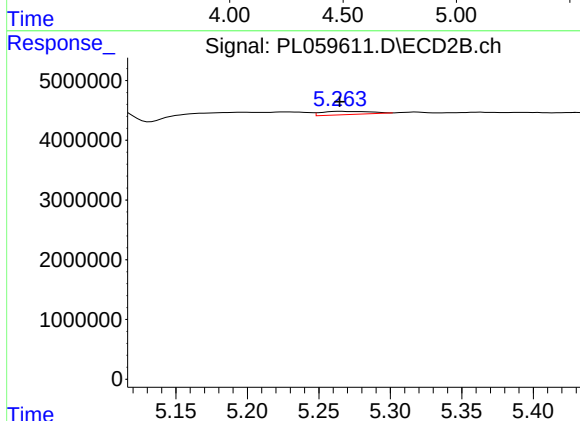


#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 1264792
Conc: 0.36 ng/ml

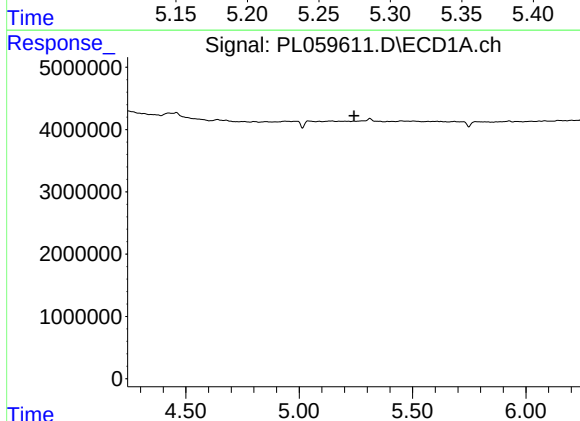


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

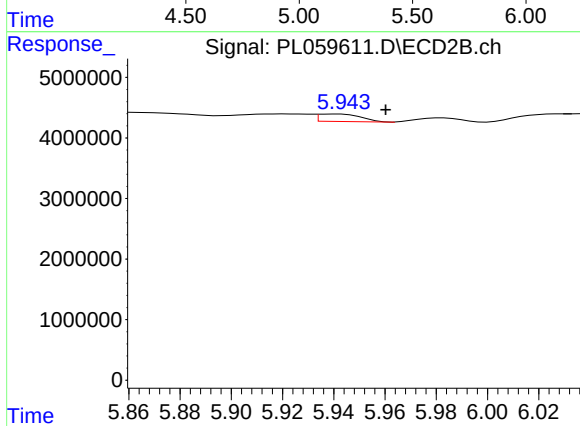

#8 Heptachlor epoxide


R.T.: 5.941 min
Delta R.T.: -0.019 min
Response: 1420992
Conc: 0.58 ng/ml

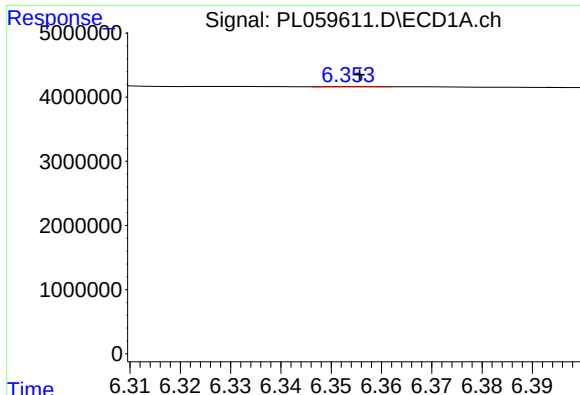

#15 Endosulfan II


R.T.: 6.354 min
Delta R.T.: -0.001 min
Response: 24287
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

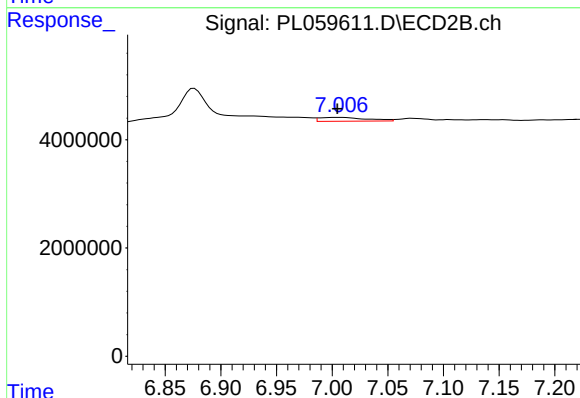


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.003 min
Response: 2105749
Conc: 0.82 ng/ml

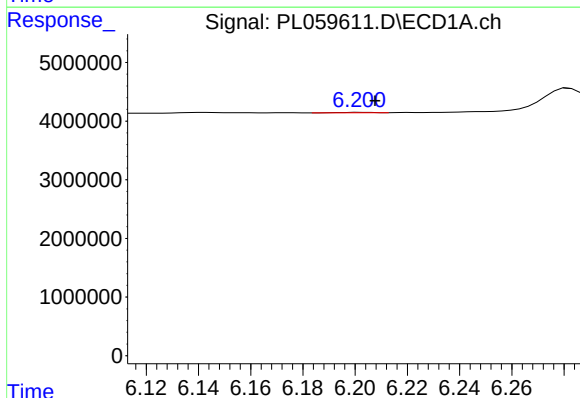


#16 4,4'-DDD

R.T.: 6.202 min
Delta R.T.: -0.006 min
Response: 70956
Conc: 0.05 ng/ml

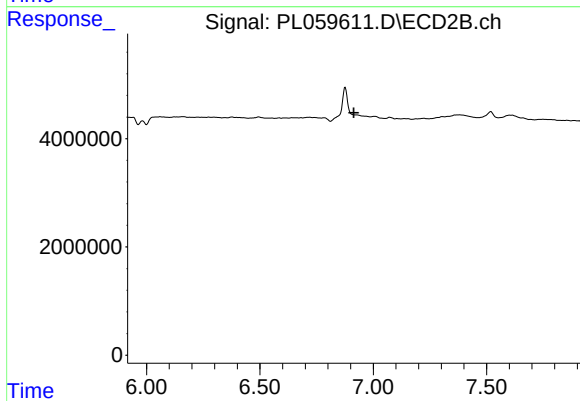

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

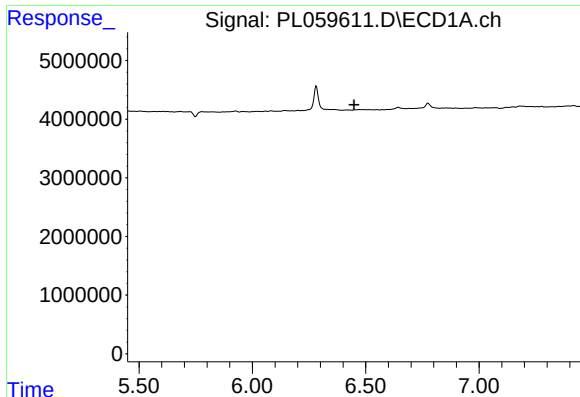

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

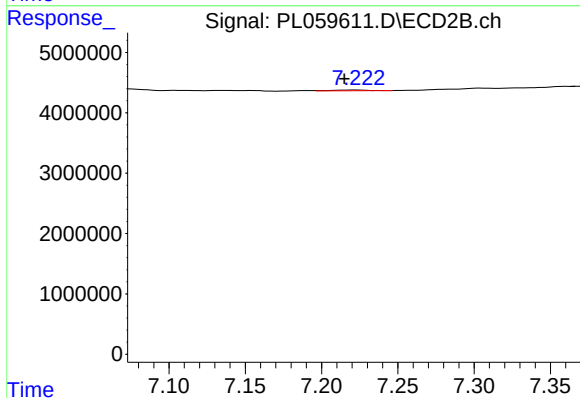


#17 4,4'-DDT

R.T.: 7.224 min
Delta R.T.: 0.009 min
Response: 214108
Conc: 0.09 ng/ml

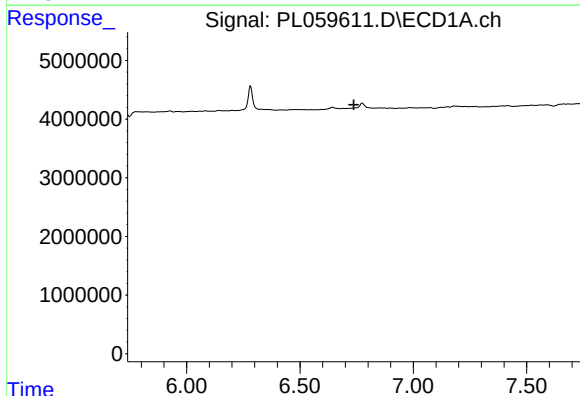


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 6.737 min
Response: 0
Conc: N.D.

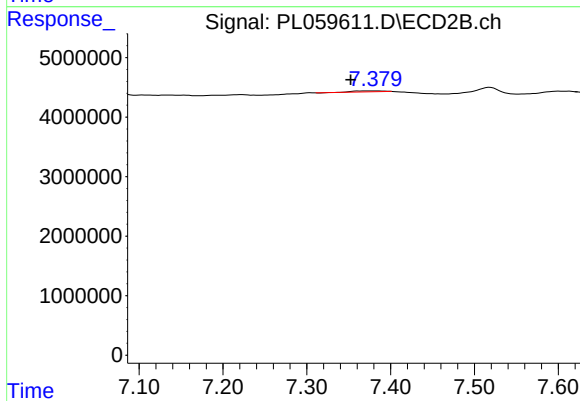

#19 Endosulfan Sulfate


R.T.: 7.380 min
Delta R.T.: 0.027 min
Response: 474066
Conc: 0.20 ng/ml

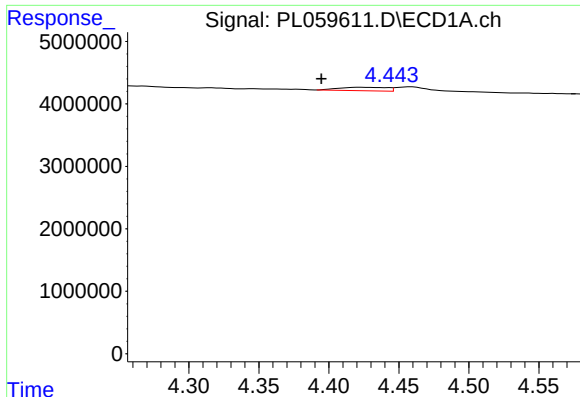

#23 Chlordane-1


R.T.: 4.423 min
Delta R.T.: 0.029 min
Response: 1344734
Conc: 25.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

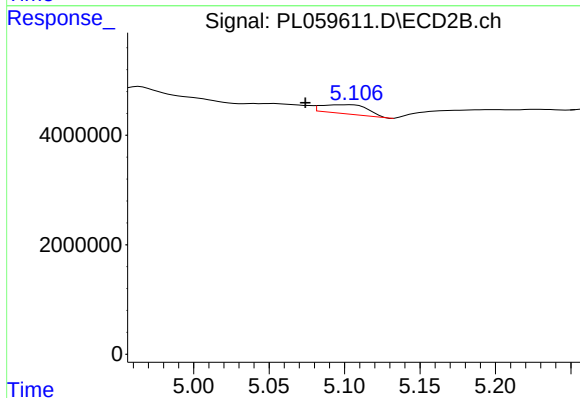


#23 Chlordane-1

R.T.: 5.103 min
Delta R.T.: 0.029 min
Response: 3535814
Conc: 32.75 ng/ml

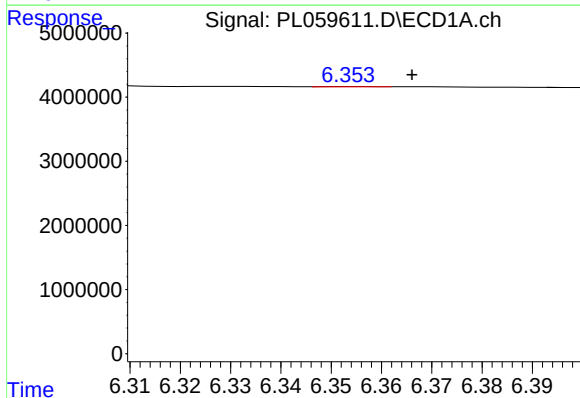


#27 Chlordane-5

R.T.: 6.354 min
Delta R.T.: -0.012 min
Response: 24287
Conc: 0.47 ng/ml

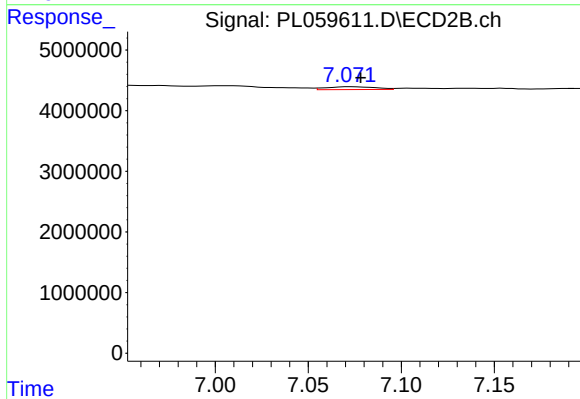

#27 Chlordane-5


R.T.: 7.072 min
Delta R.T.: -0.006 min
Response: 854153
Conc: 9.82 ng/ml

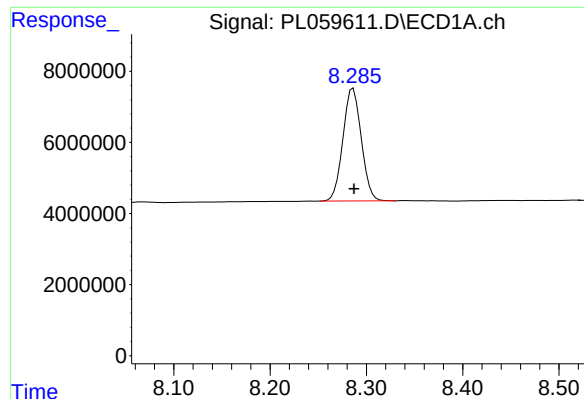

#28 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 41929013
Conc: 27.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

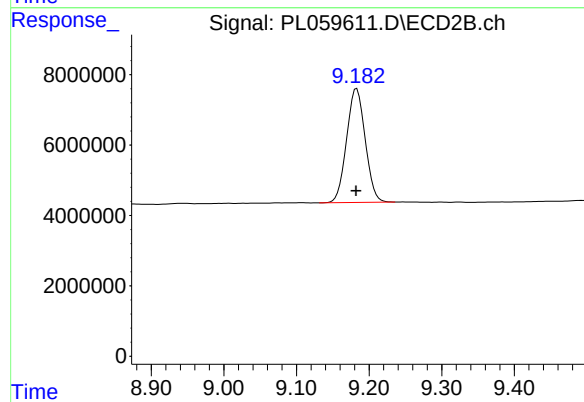

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.001 min
Response: 57646750
Conc: 26.52 ng/ml