

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 02:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:18:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	44712106	65975676	24.895	24.808
28)	SA Decachlor...	8.287	9.182	38360502	52673753	24.987	24.233
Target Compounds							
2)	A alpha-BHC	3.964	4.491f	1705589	258401	0.663	0.066 #
4)	MA Heptachlor	0.000	5.266	0	1845496	N.D.	0.527 #
8)	B Heptachlo...	0.000	5.941f	0	2789428	N.D.	1.148 #
9)	A Endosulfan I	5.599f	0.000	115624	0	0.075	N.D. #
14)	MA Endrin	6.083	0.000	170172	0	0.115	N.D. #
15)	B Endosulfa...	6.365	7.011	223629	2093900	0.147	0.815 #
16)	A 4,4'-DDD	6.205	0.000	205297	0	0.154	N.D. #
17)	MA 4,4'-DDT	0.000	7.187f	0	75138	N.D.	0.033 #
18)	B Endrin al...	0.000	7.135	0	296367	N.D.	0.134 #
22)	Mirex	0.000	8.313f	0	899372	N.D.	0.471 #
23)	Chlordane-1	4.421f	0.000	1206953	0	23.160	N.D. #
27)	Chlordane-5	6.365	7.073	223629	1609661	4.353	18.497 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 02:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:18:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

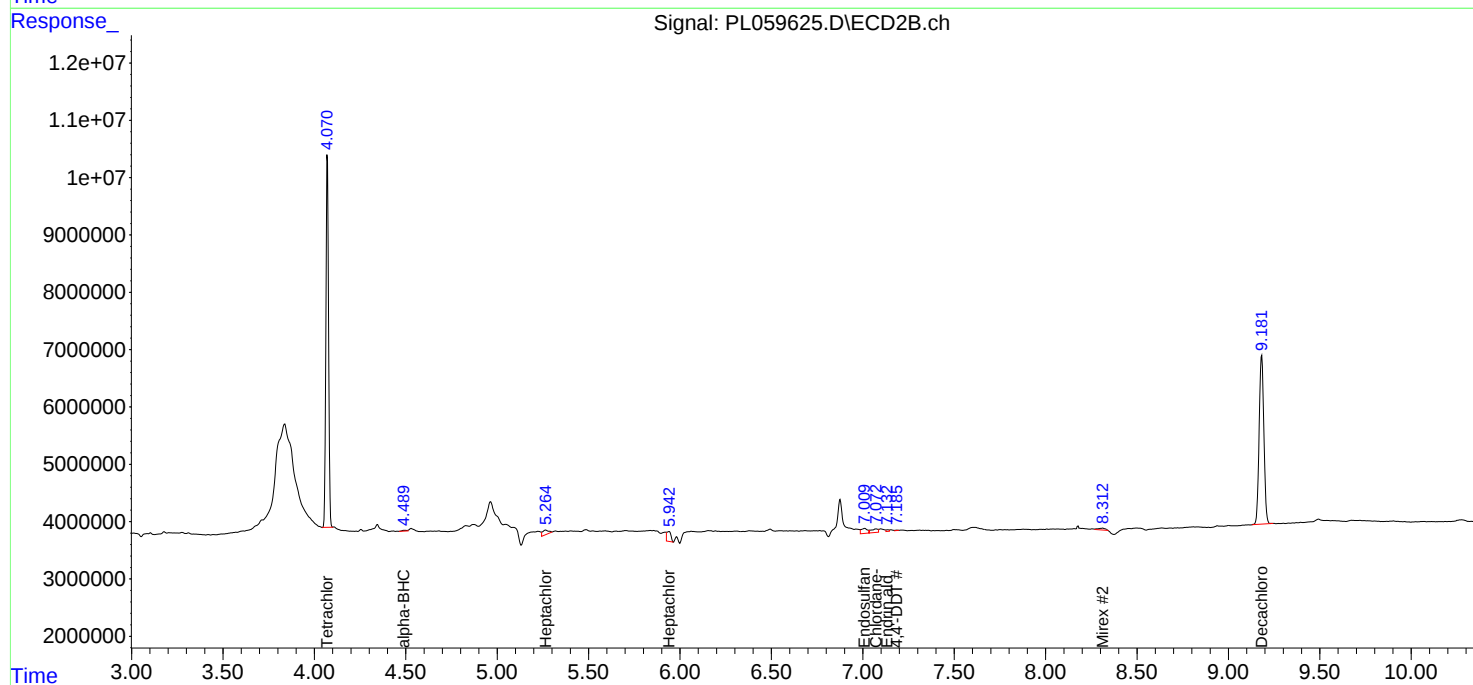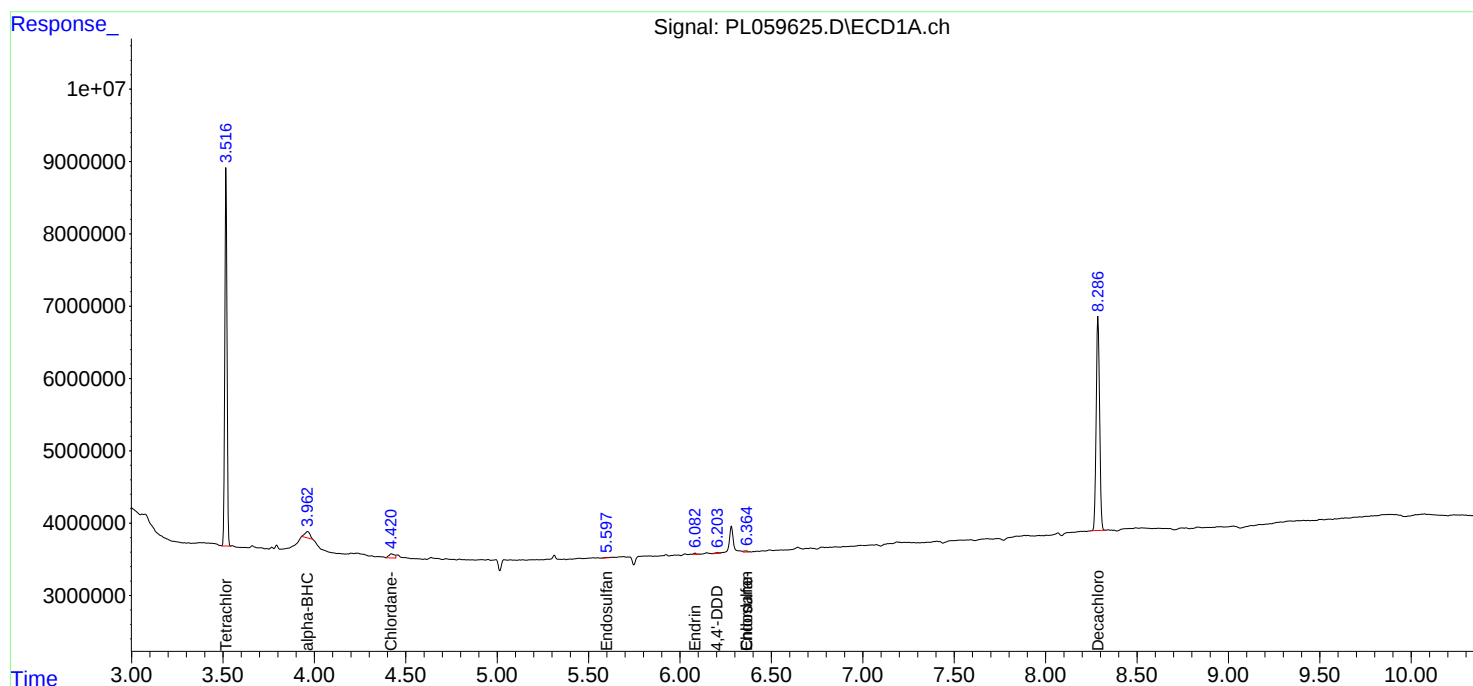


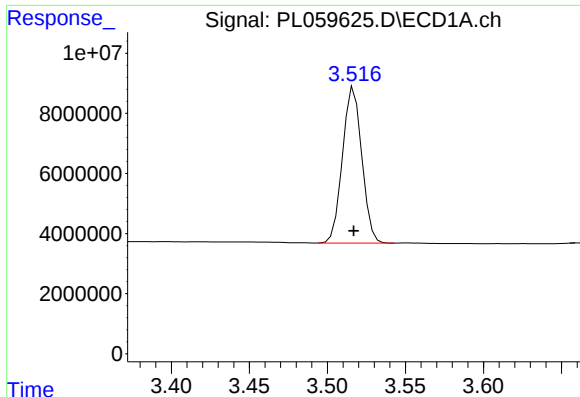

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 44712106
Conc: 24.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

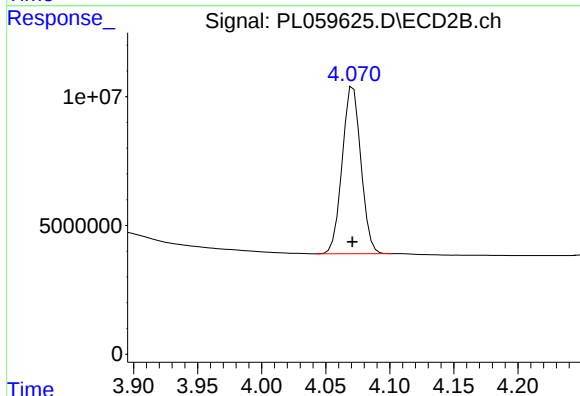


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 65975676
Conc: 24.81 ng/ml

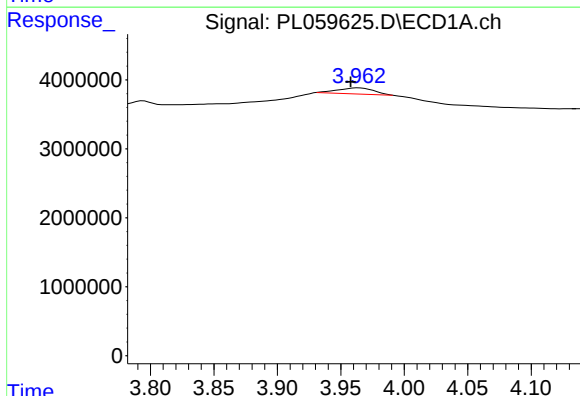


#2 alpha-BHC

R.T.: 3.964 min
Delta R.T.: 0.006 min
Response: 1705589
Conc: 0.66 ng/ml

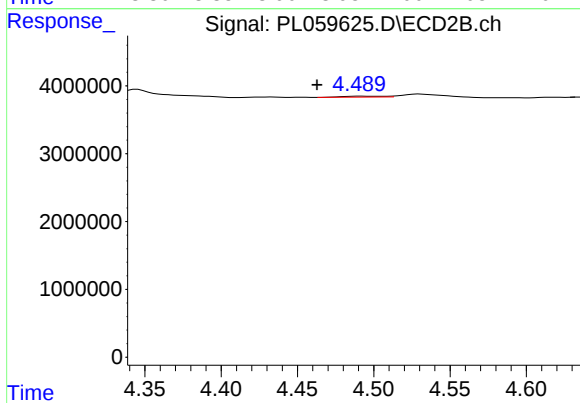

#2 alpha-BHC


R.T.: 4.491 min
Delta R.T.: 0.028 min
Response: 258401
Conc: 0.07 ng/ml

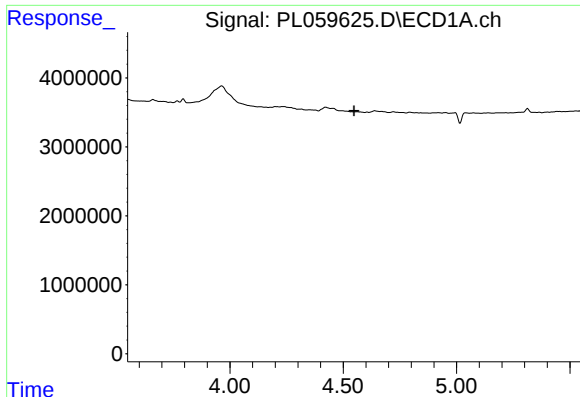

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

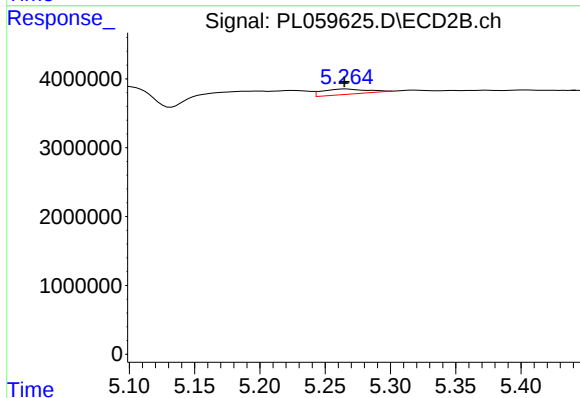


#4 Heptachlor

R.T.: 5.266 min
Delta R.T.: 0.001 min
Response: 1845496
Conc: 0.53 ng/ml

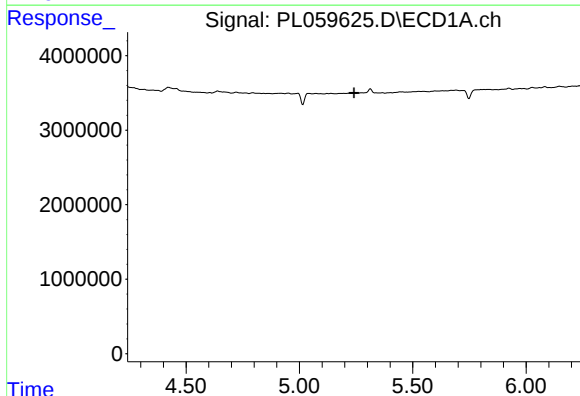


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

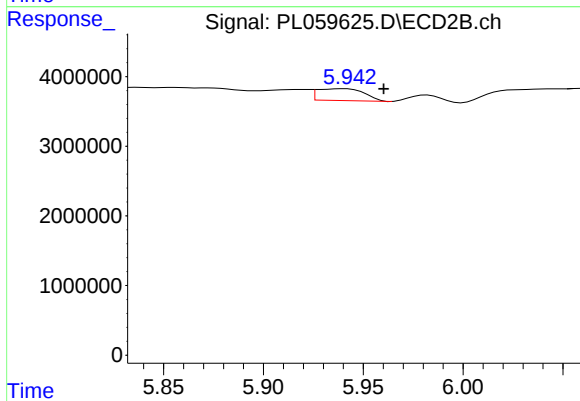

#8 Heptachlor epoxide


R.T.: 5.941 min
Delta R.T.: -0.020 min
Response: 2789428
Conc: 1.15 ng/ml

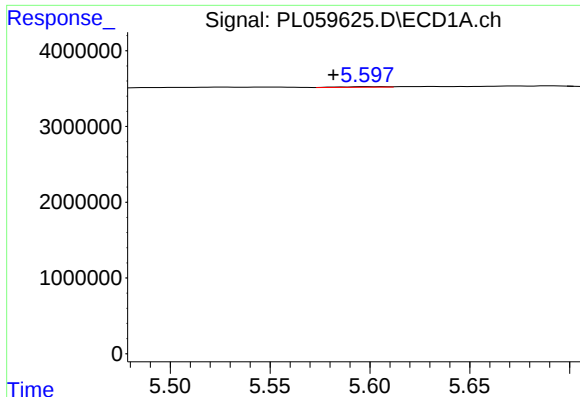

#9 Endosulfan I


R.T.: 5.599 min
Delta R.T.: 0.017 min
Response: 115624
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

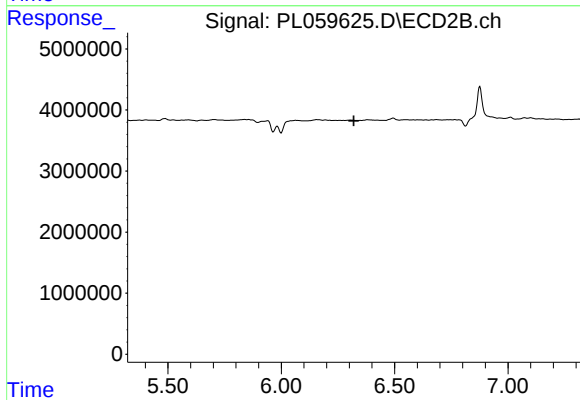


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.319 min
Response: 0
Conc: N.D.

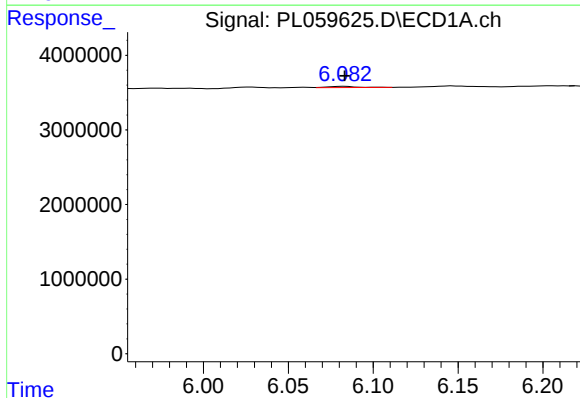


#14 Endrin

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 170172
Conc: 0.12 ng/ml

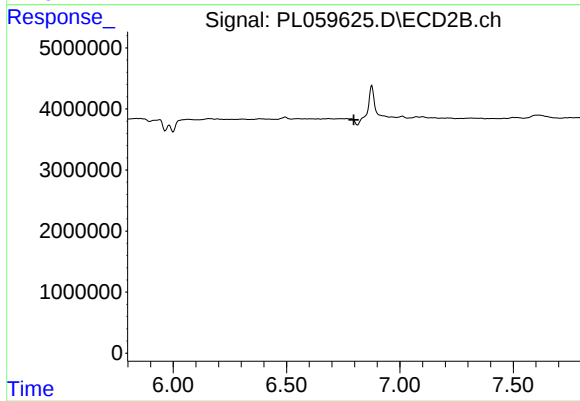

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.797 min
Response: 0
Conc: N.D.

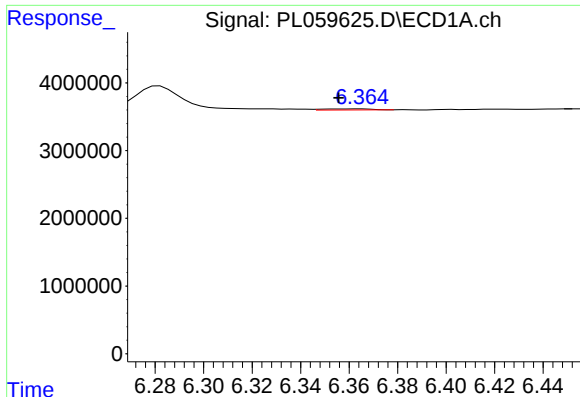

#15 Endosulfan II


R.T.: 6.365 min
Delta R.T.: 0.010 min
Response: 223629
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

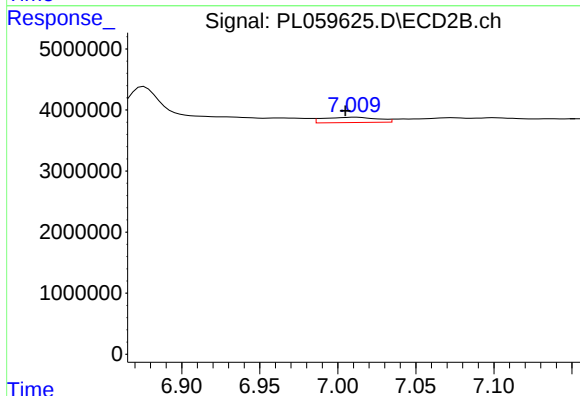


#15 Endosulfan II

R.T.: 7.011 min
Delta R.T.: 0.007 min
Response: 2093900
Conc: 0.82 ng/ml

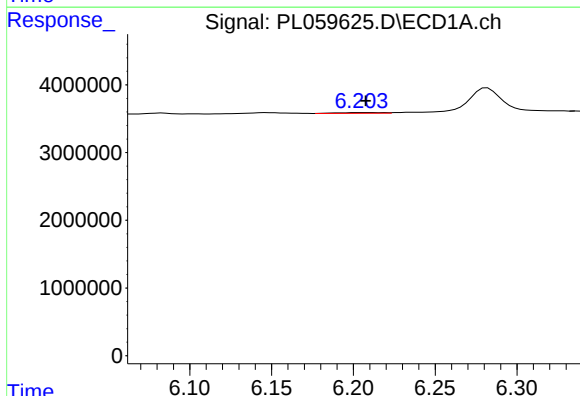


#16 4,4'-DDD

R.T.: 6.205 min
Delta R.T.: -0.003 min
Response: 205297
Conc: 0.15 ng/ml

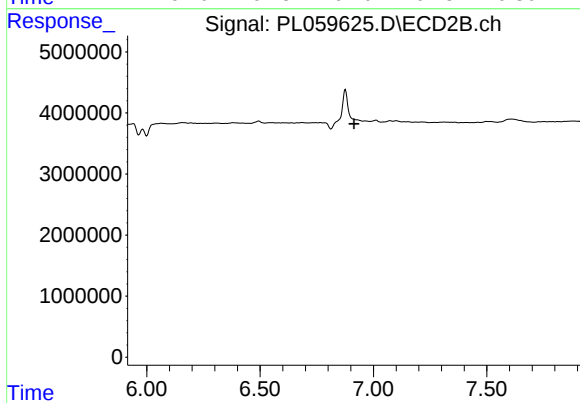

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

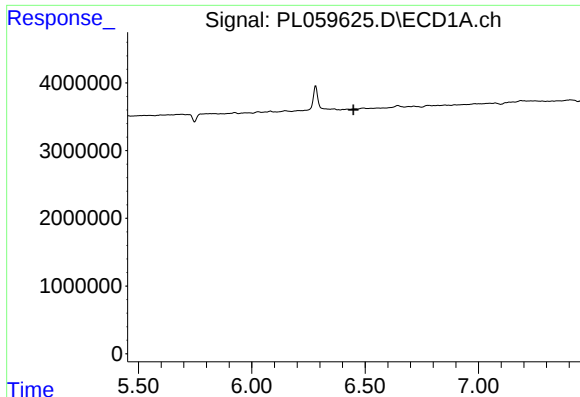

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

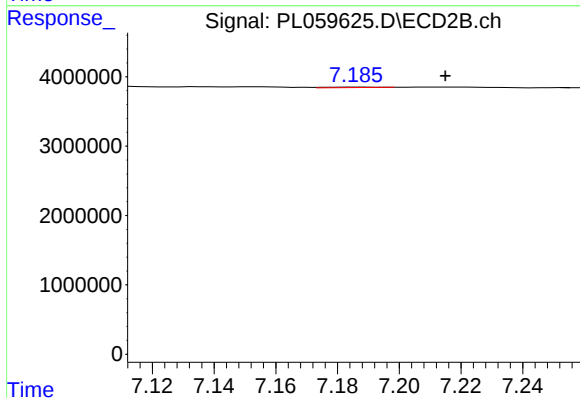


#17 4,4'-DDT

R.T.: 7.187 min
Delta R.T.: -0.028 min
Response: 75138
Conc: 0.03 ng/ml

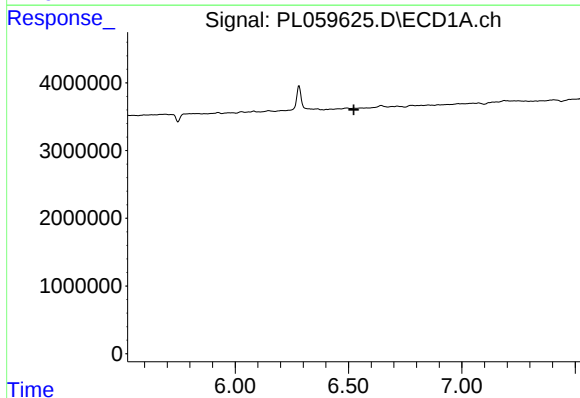


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.524 min
Response: 0
Conc: N.D.

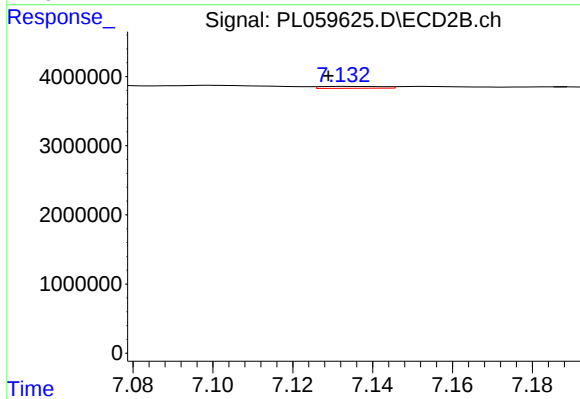

#18 Endrin aldehyde


R.T.: 7.135 min
Delta R.T.: 0.006 min
Response: 296367
Conc: 0.13 ng/ml

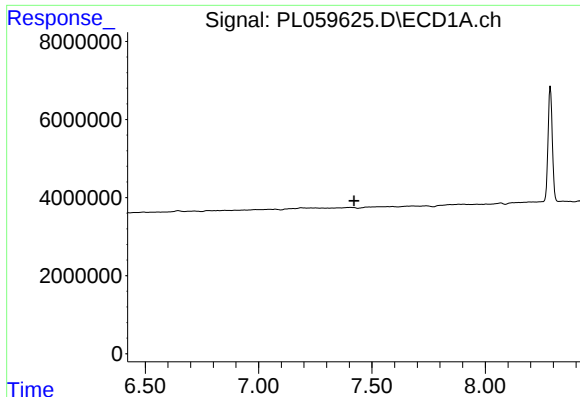

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.422 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

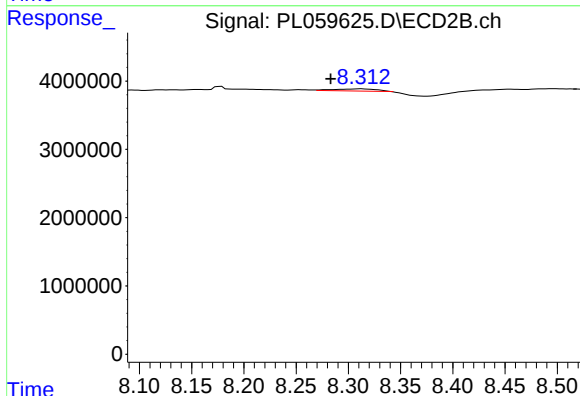


#22 Mirex

R.T.: 8.313 min
Delta R.T.: 0.029 min
Response: 899372
Conc: 0.47 ng/ml

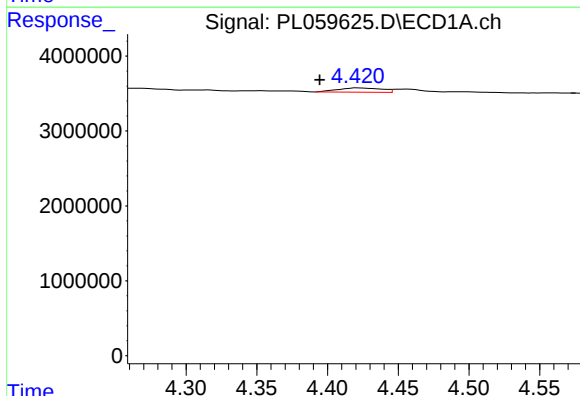


#23 Chlordane-1

R.T.: 4.421 min
Delta R.T.: 0.027 min
Response: 1206953
Conc: 23.16 ng/ml

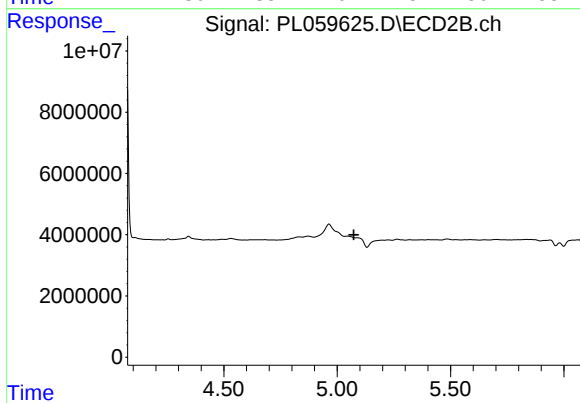

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.074 min
Response: 0
Conc: N.D.

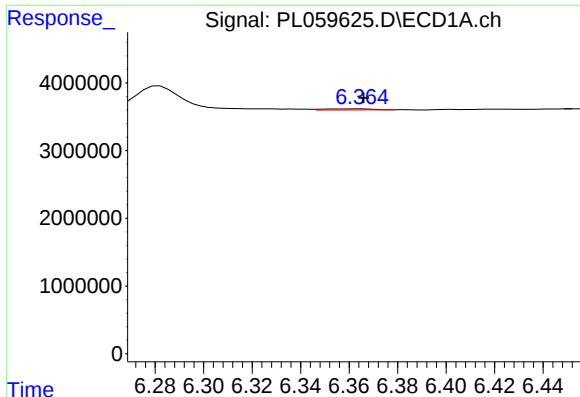

#27 Chlordane-5


R.T.: 6.365 min
Delta R.T.: 0.000 min
Response: 223629
Conc: 4.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

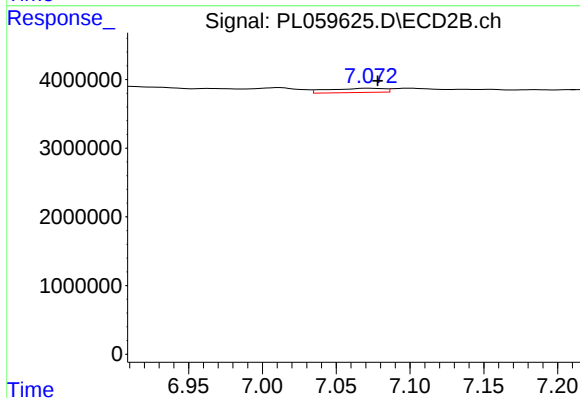


#27 Chlordane-5

R.T.: 7.073 min
Delta R.T.: -0.005 min
Response: 1609661
Conc: 18.50 ng/ml

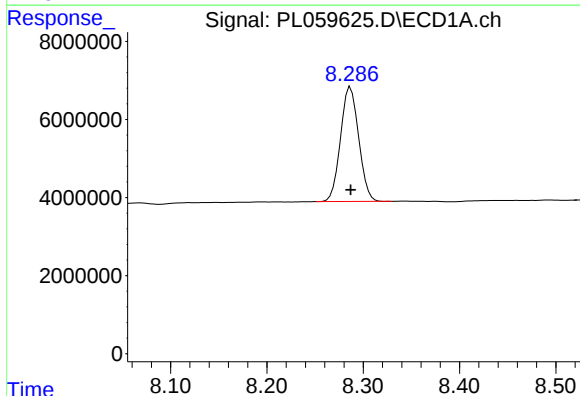

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 38360502
Conc: 24.99 ng/ml

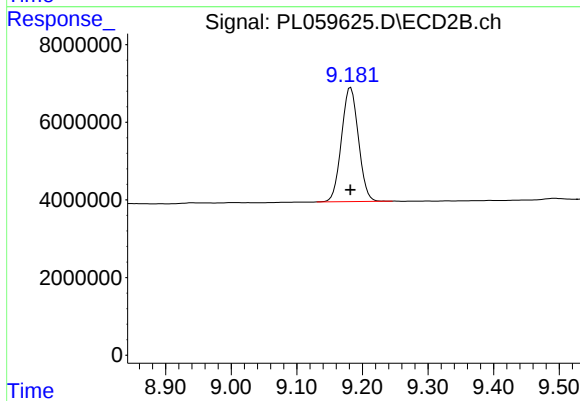

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 52673753
Conc: 24.23 ng/ml