

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 11:09
 Operator : AJ\MA
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 30 14:24:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 30 13:56:32 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	37702377	56215797	20.992	21.138
28)	SA Decachlor...	8.287	9.182	33125497	47764118	21.577	21.974
Target Compounds							
9)	A Endosulfan I	5.582	6.319	15760640	26846609	10.242	9.950
10)	B gamma-Chl...	5.469	6.195	16365020	28749994	10.002	9.751
12)	B 4,4'-DDE	5.691	6.424	29206198	51621030	19.482	19.350
13)	MA Dieldrin	5.826	6.577	31352970	56144297	19.639	19.923
19)	B Endosulfa...	6.736	7.352	27952732	47200731	19.471	19.722
20)	A Methoxychlor	6.994	7.672	76358952	125.2E6	99.777	96.980
21)	B Endrin ke...	7.228	7.825	32170657	49682861	19.483	19.718



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 11:09
Operator : AJ\MA
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 30 14:24:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Tue Jun 30 13:56:32 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

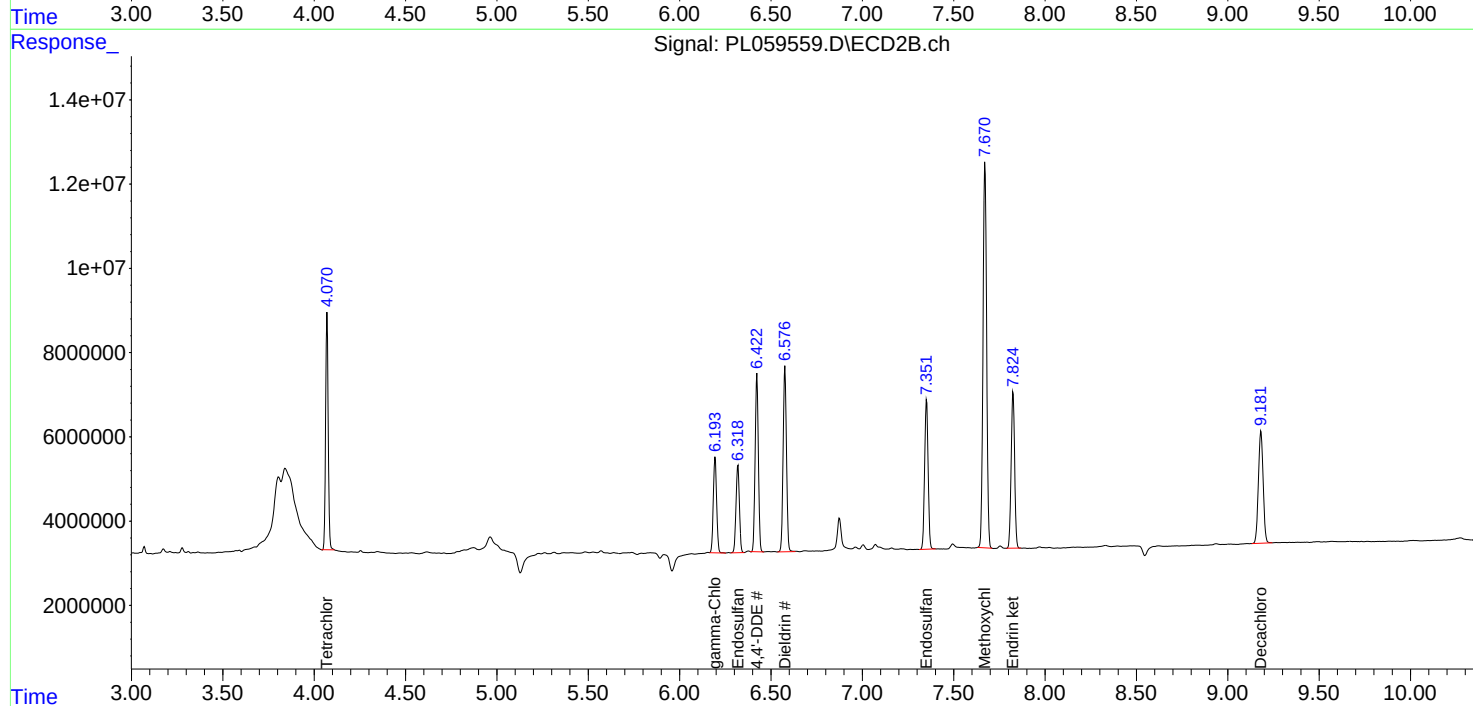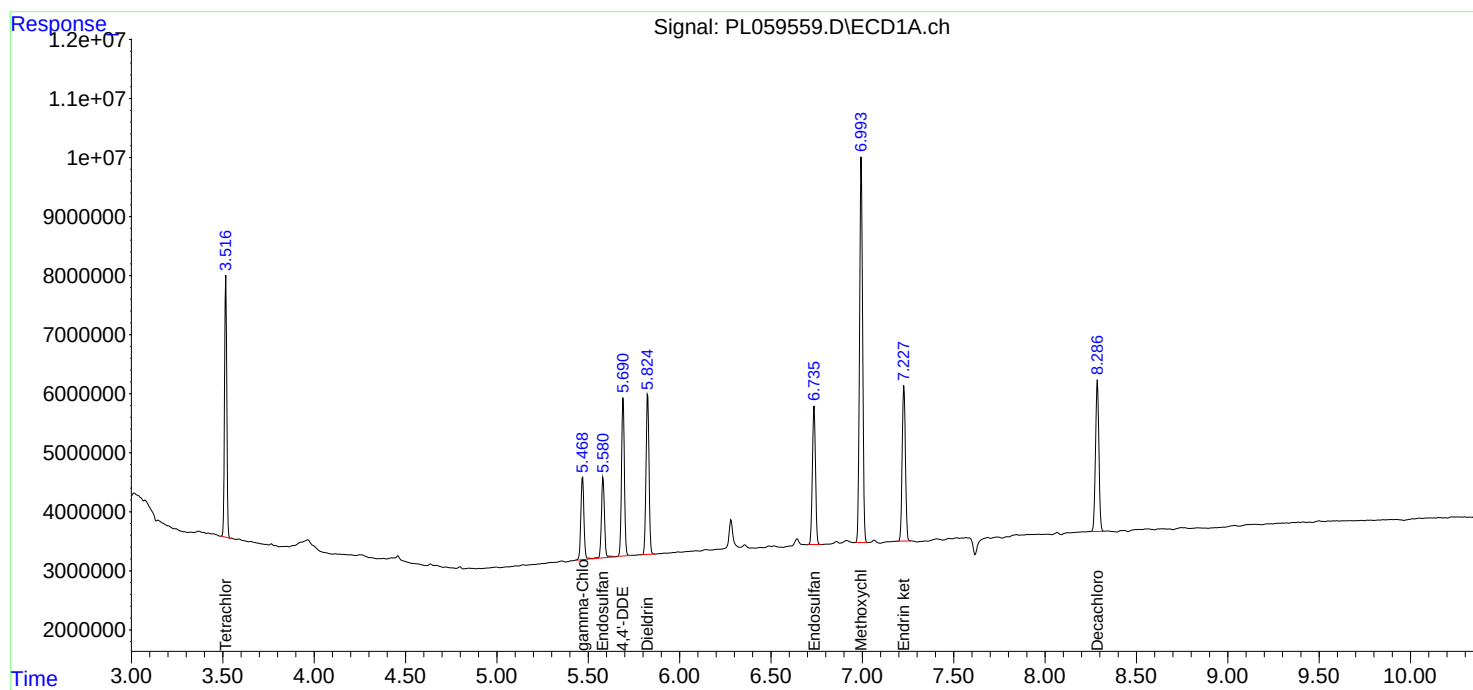


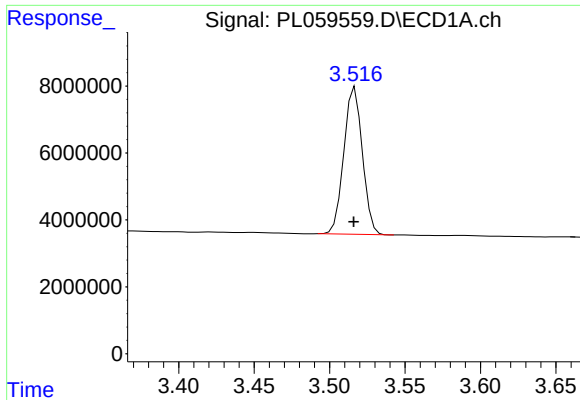

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 37702377
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

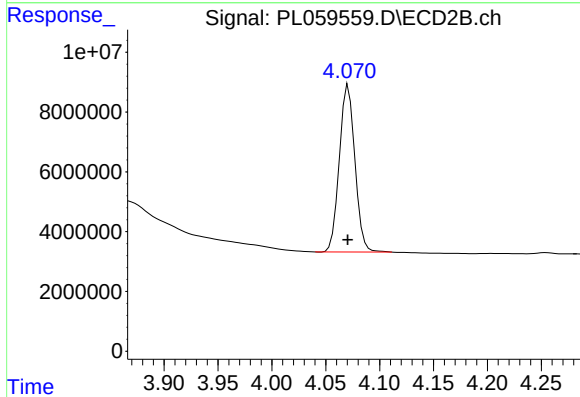


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 56215797
Conc: 21.14 ng/ml

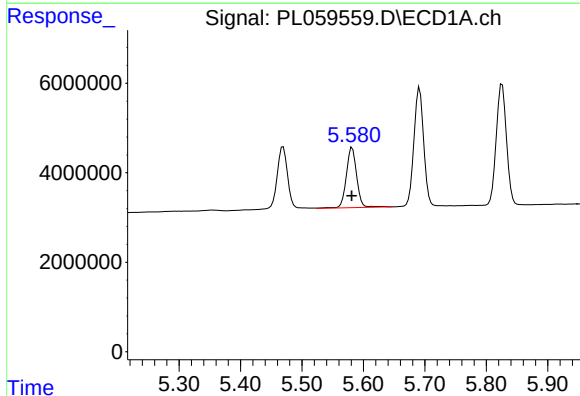


#9 Endosulfan I

R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 15760640
Conc: 10.24 ng/ml

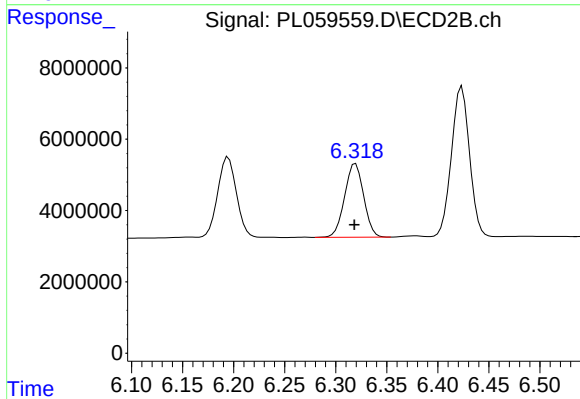

#9 Endosulfan I


R.T.: 6.319 min
Delta R.T.: 0.001 min
Response: 26846609
Conc: 9.95 ng/ml

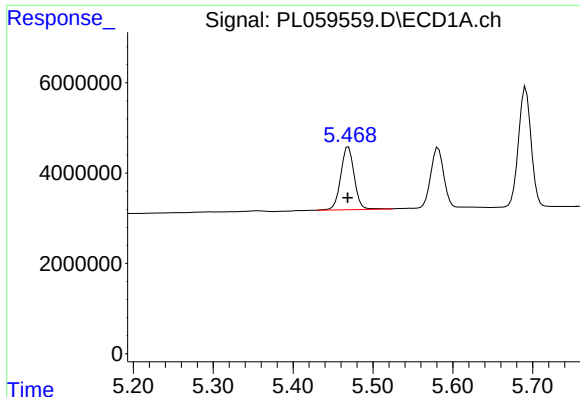

#10 gamma-Chlordane


R.T.: 5.469 min
Delta R.T.: 0.000 min
Response: 16365020
Conc: 10.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

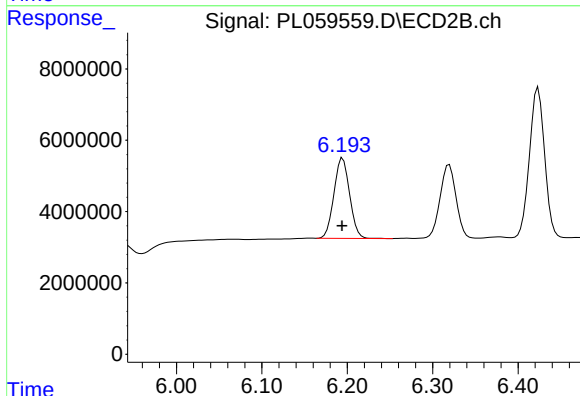


#10 gamma-Chlordane

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 28749994
Conc: 9.75 ng/ml

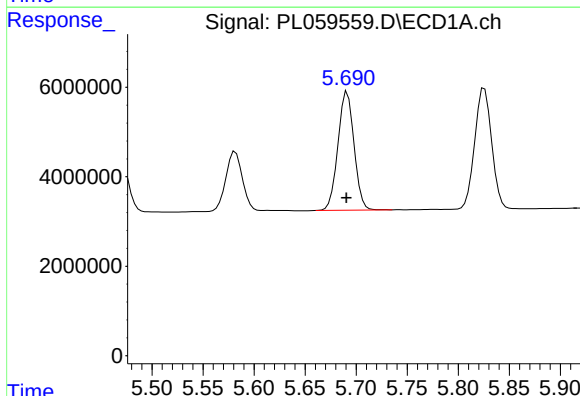


#12 4,4'-DDE

R.T.: 5.691 min
Delta R.T.: 0.000 min
Response: 29206198
Conc: 19.48 ng/ml

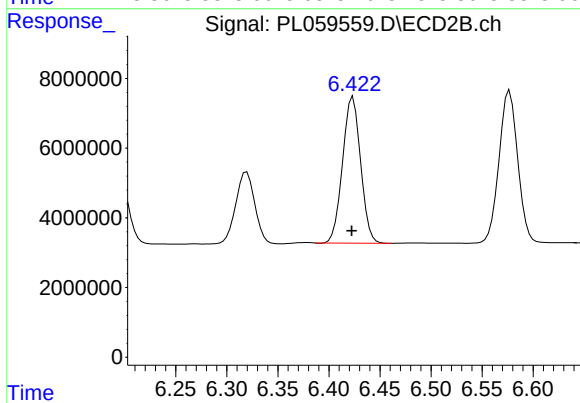

#12 4,4'-DDE


R.T.: 6.424 min
Delta R.T.: 0.001 min
Response: 51621030
Conc: 19.35 ng/ml

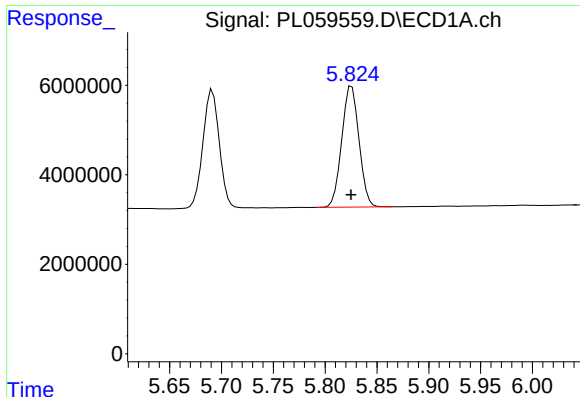

#13 Dieldrin


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 31352970
Conc: 19.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

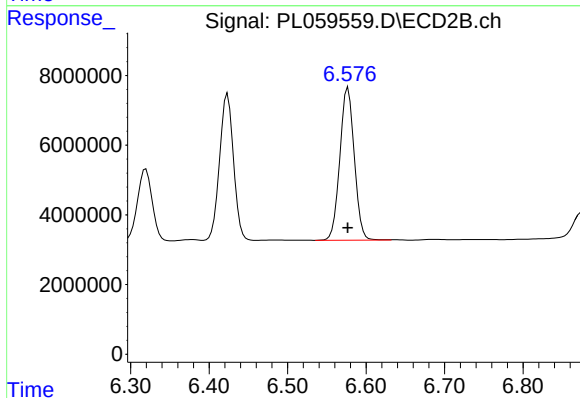


#13 Dieldrin

R.T.: 6.577 min
Delta R.T.: 0.000 min
Response: 56144297
Conc: 19.92 ng/ml

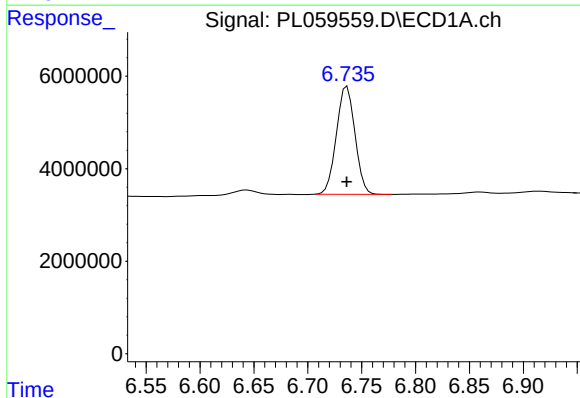


#19 Endosulfan Sulfate

R.T.: 6.736 min
Delta R.T.: 0.000 min
Response: 27952732
Conc: 19.47 ng/ml

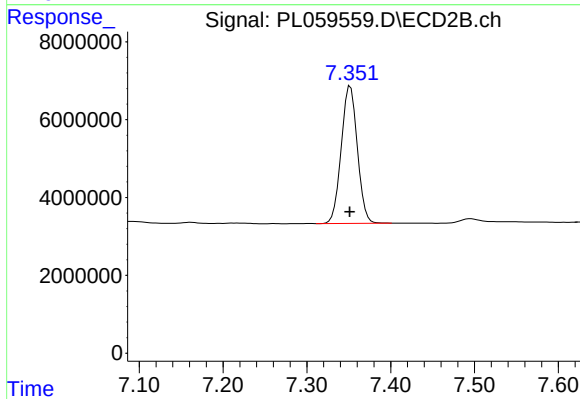

#19 Endosulfan Sulfate


R.T.: 7.352 min
Delta R.T.: 0.000 min
Response: 47200731
Conc: 19.72 ng/ml

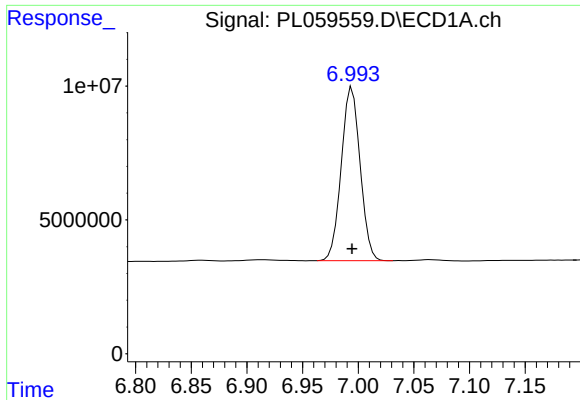

#20 Methoxychlor


R.T.: 6.994 min
Delta R.T.: 0.000 min
Response: 76358952
Conc: 99.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

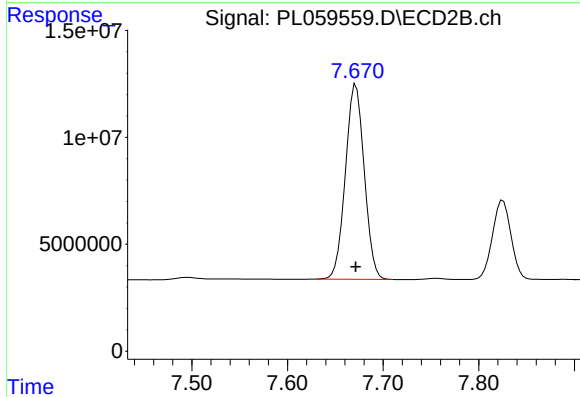


#20 Methoxychlor

R.T.: 7.672 min
Delta R.T.: 0.000 min
Response: 125182072
Conc: 96.98 ng/ml

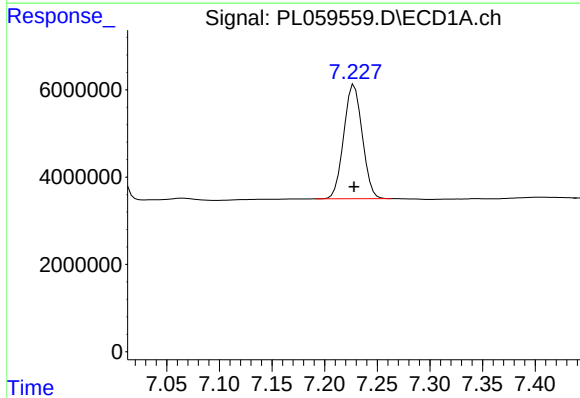


#21 Endrin ketone

R.T.: 7.228 min
Delta R.T.: 0.000 min
Response: 32170657
Conc: 19.48 ng/ml

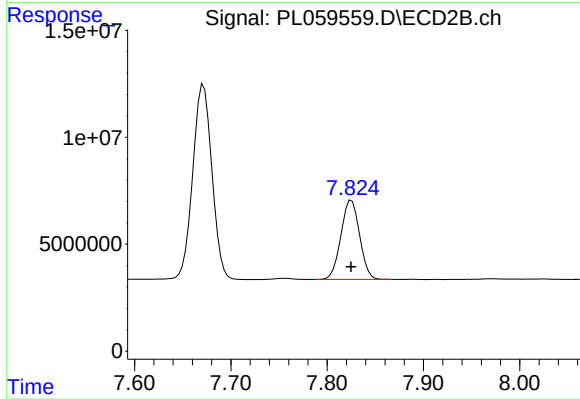

#21 Endrin ketone


R.T.: 7.825 min
Delta R.T.: 0.000 min
Response: 49682861
Conc: 19.72 ng/ml

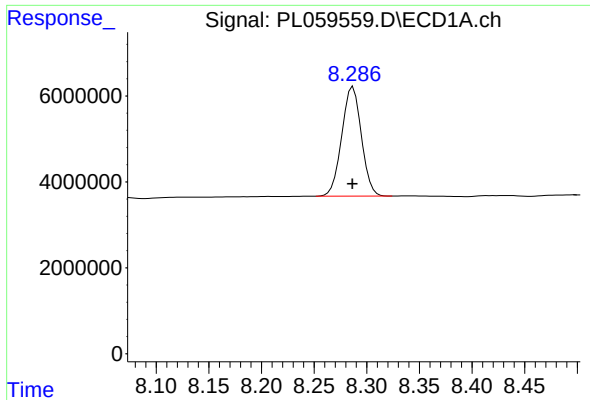

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 33125497
Conc: 21.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

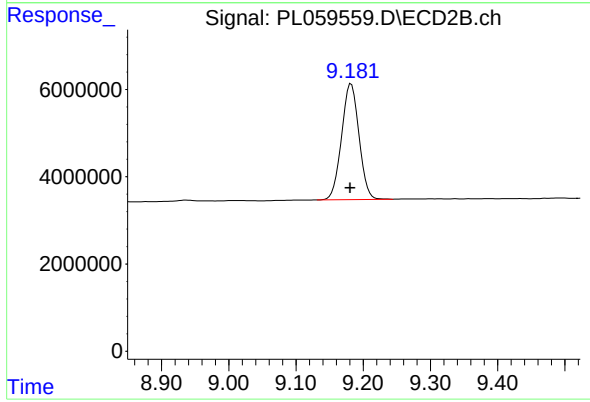

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.001 min
Response: 47764118
Conc: 21.97 ng/ml