

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059589.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 18:13
 Operator : AJ\MA
 Sample : L3153-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP1-B

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:11:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:31:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.518	4.071	38419434	58612352	21.391	22.039
28) SA Decachlor...	8.288	9.183	28047295	40595195	18.269	18.676
Target Compounds						
12) B 4,4'-DDE	5.691	6.422	1125459	2279107	0.751	0.854m
13) MA Dieldrin	5.825	6.578	962391	1611892	0.603m	0.572

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059589.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 18:13
Operator : AJ\MA
Sample : L3153-05
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP1-B


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:31:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

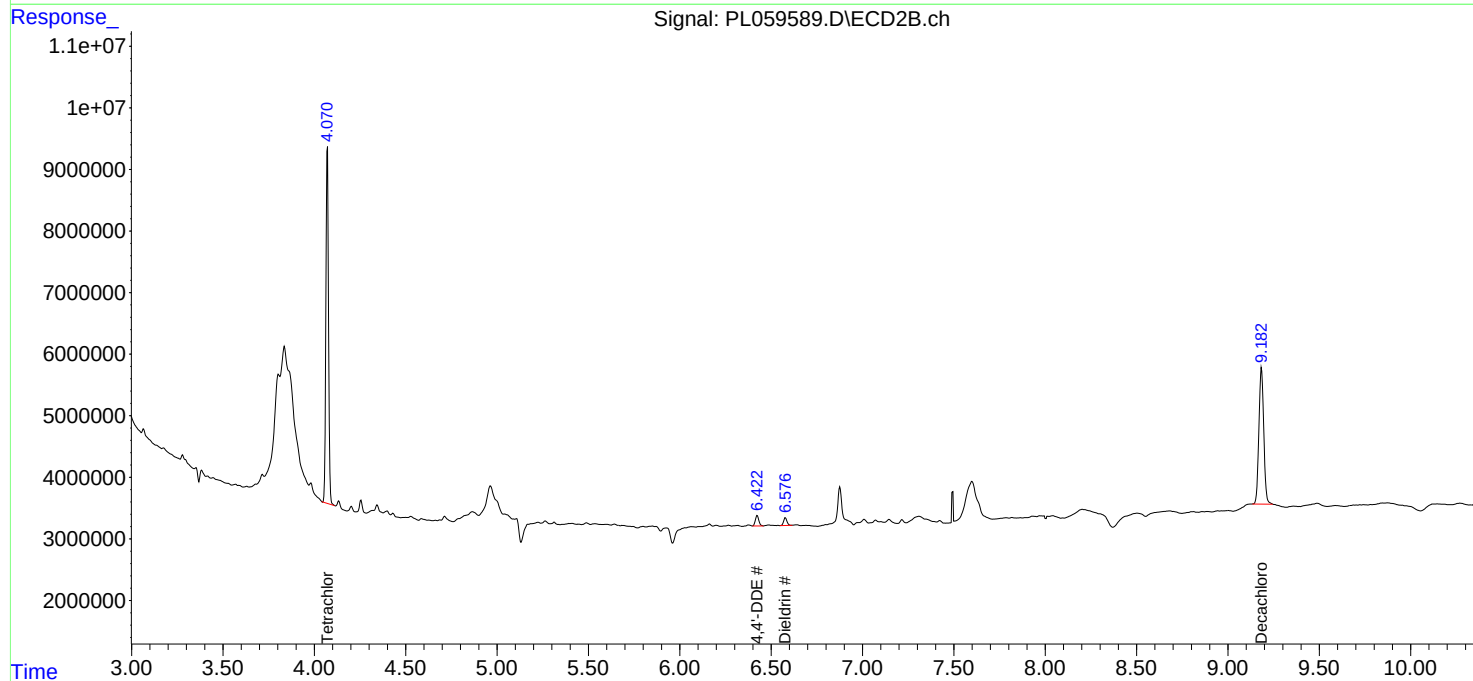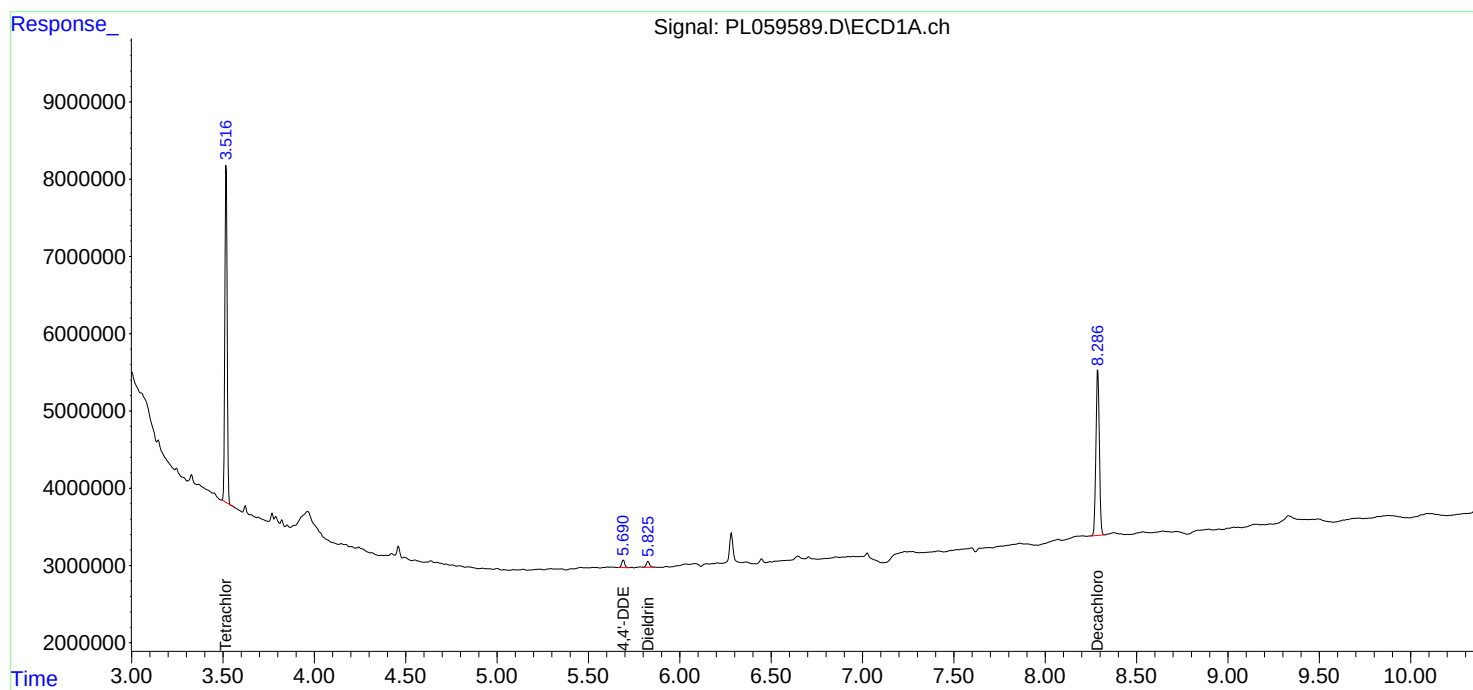

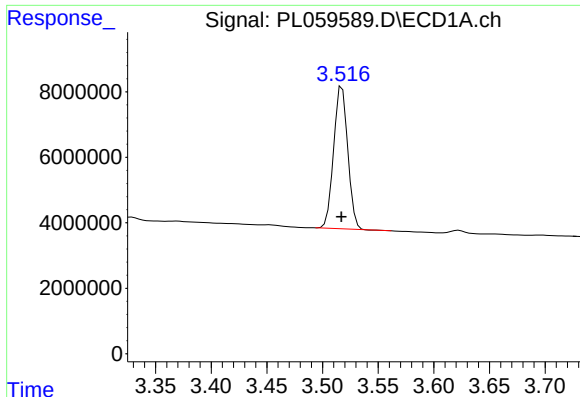


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 38419434
Conc: 21.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP1-B


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:39 PM

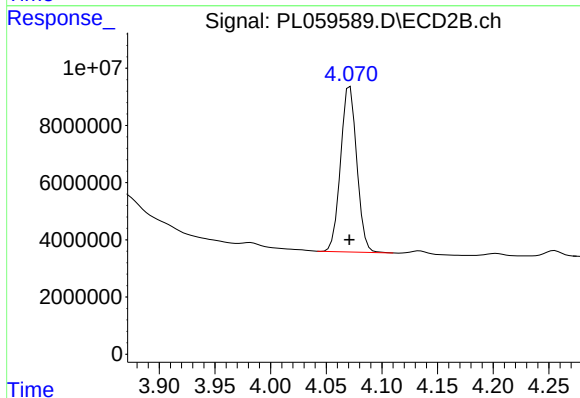


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 58612352
Conc: 22.04 ng/ml

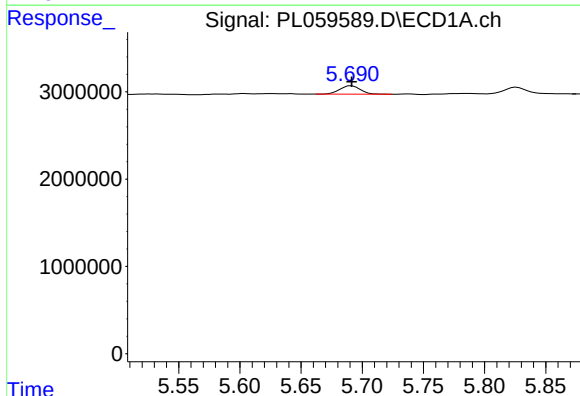


#12 4,4'-DDE

R.T.: 5.691 min
Delta R.T.: 0.000 min
Response: 1125459
Conc: 0.75 ng/ml

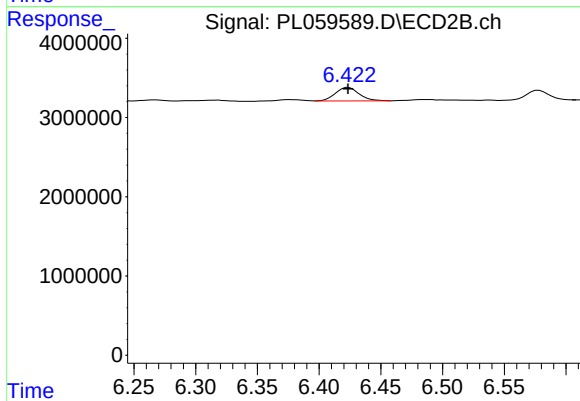

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.001 min
Response: 2279107
Conc: 0.85 ng/ml m

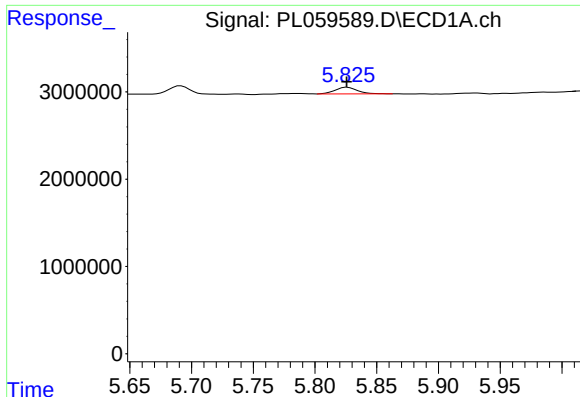


#13 Dieldrin

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 962391
Conc: 0.60 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SP1-B


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:39 PM

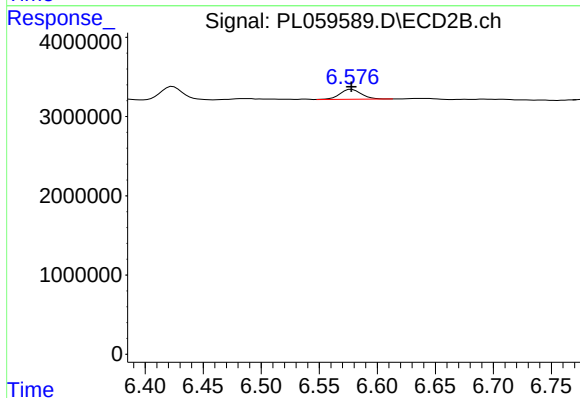


#13 Dieldrin

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 1611892
Conc: 0.57 ng/ml

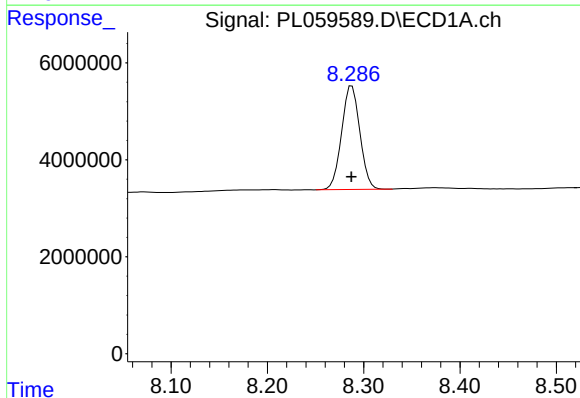

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 28047295
Conc: 18.27 ng/ml

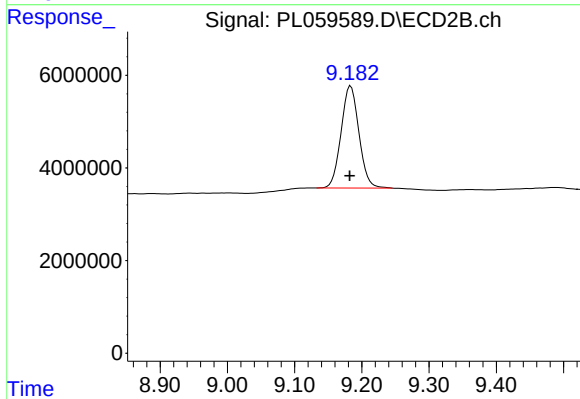

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.001 min
Response: 40595195
Conc: 18.68 ng/ml