

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2020 19:23
 Operator : AJ\MA
 Sample : L3153-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP2-D

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:11:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:33:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.072	38262385	58052739	21.303	21.829
28)	SA Decachlor...	8.288	9.183	28936058	40976494	18.848	18.851
Target Compounds							
12)	B 4,4'-DDE	5.689	6.422	1095952	2084476	0.731m	0.781m
17)	MA 4,4'-DDT	6.447	7.216	596415	948492	0.470	0.419

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2020 19:23
Operator : AJ\MA
Sample : L3153-20
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP2-D


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:33:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

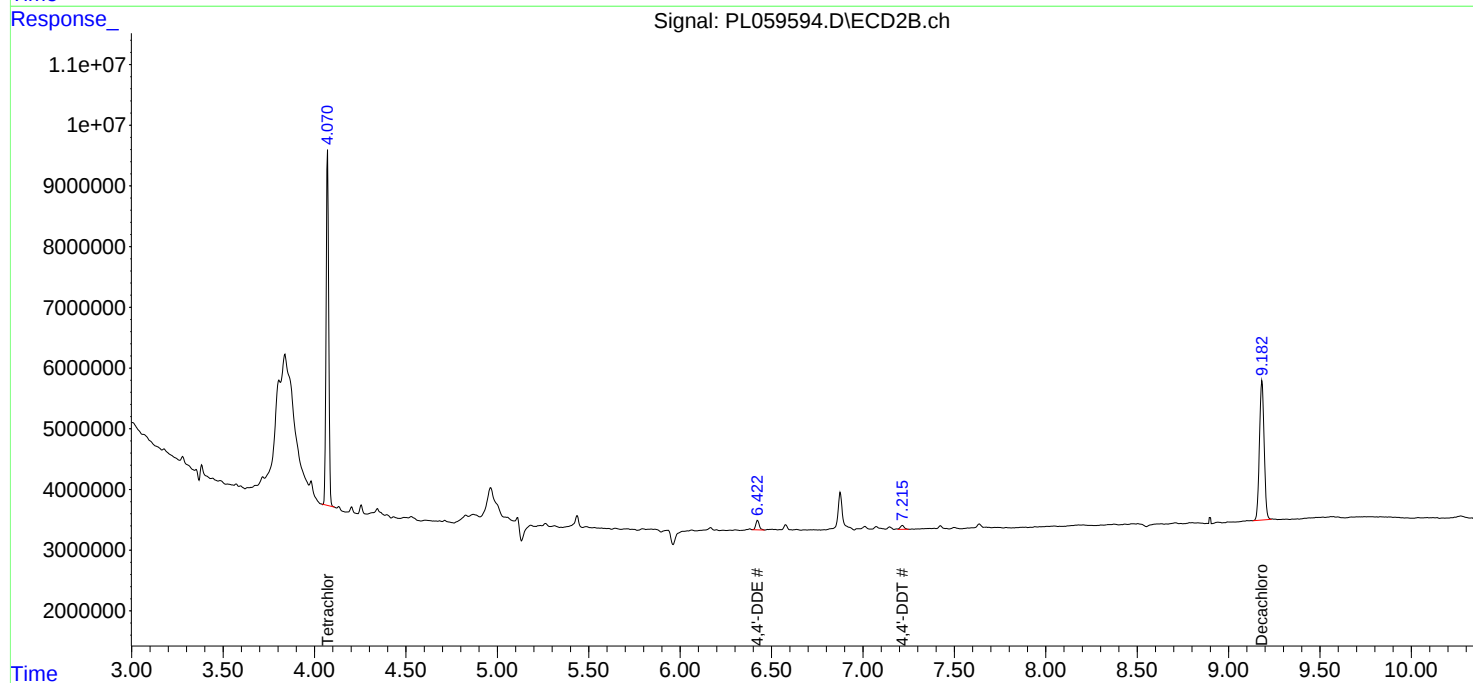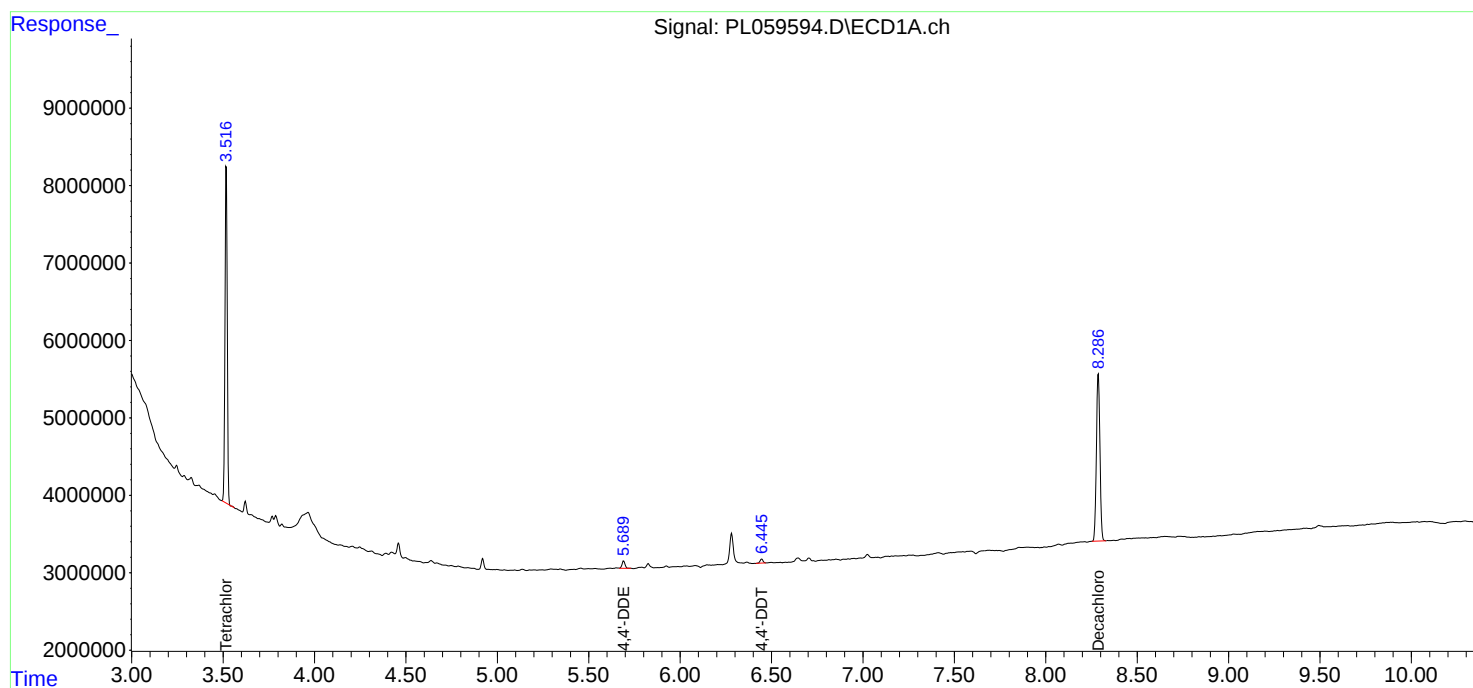

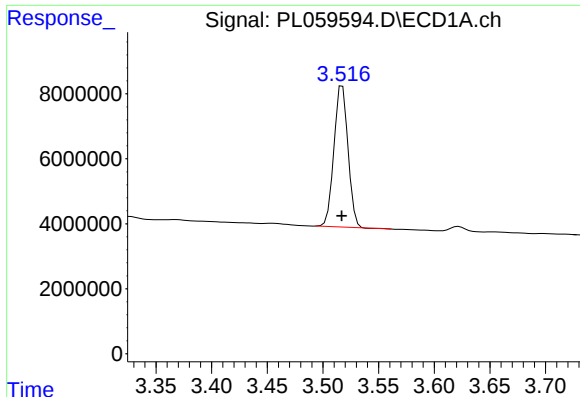


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 38262385
Conc: 21.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-D


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:48 PM

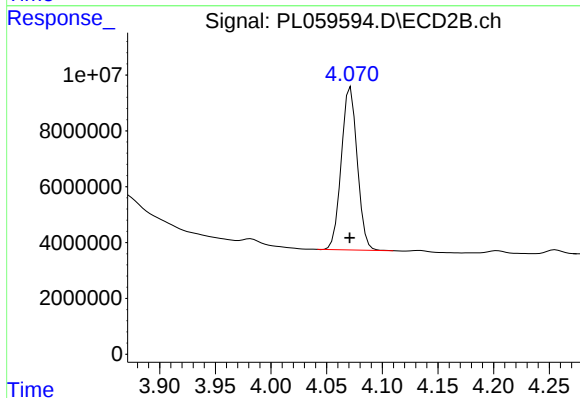


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 58052739
Conc: 21.83 ng/ml

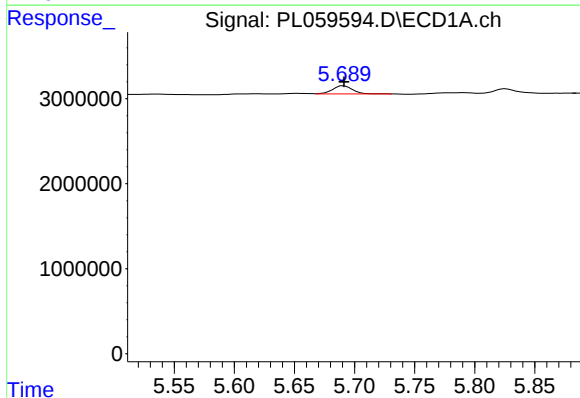


#12 4,4'-DDE

R.T.: 5.689 min
Delta R.T.: -0.002 min
Response: 1095952
Conc: 0.73 ng/ml m

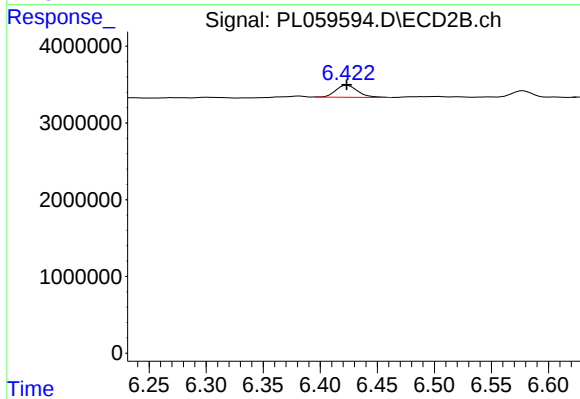

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.001 min
Response: 2084476
Conc: 0.78 ng/ml m

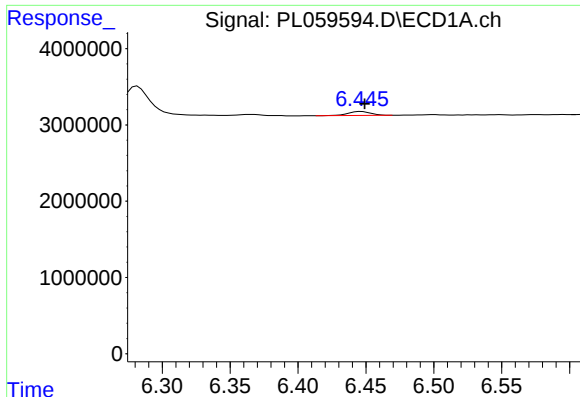


#17 4,4'-DDT

R.T.: 6.447 min
Delta R.T.: -0.002 min
Response: 596415
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-D


Manual Integrations
APPROVED

Ankita
7/1/2020 12:11:48 PM

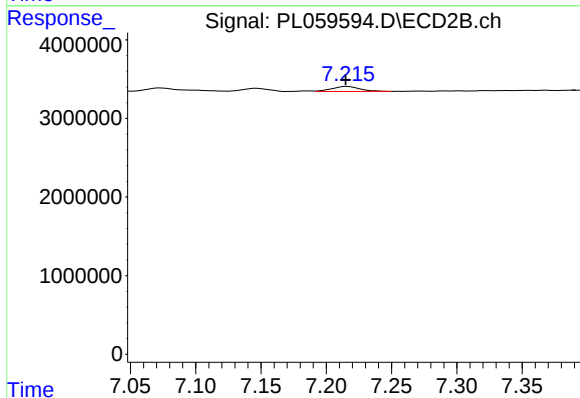


#17 4,4'-DDT

R.T.: 7.216 min
Delta R.T.: 0.001 min
Response: 948492
Conc: 0.42 ng/ml

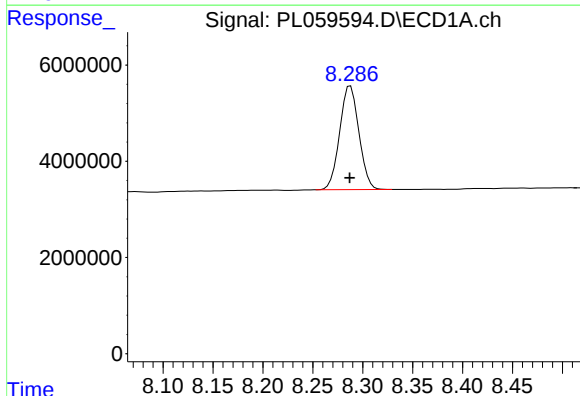

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 28936058
Conc: 18.85 ng/ml

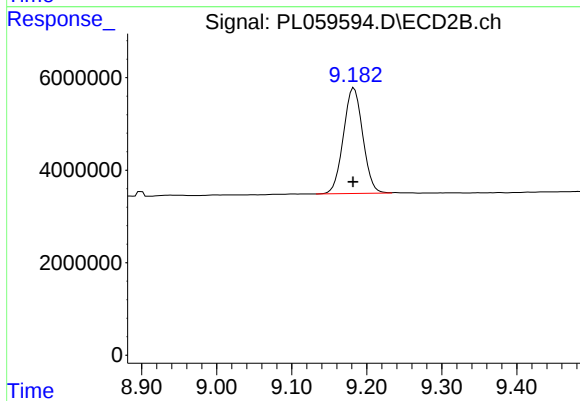

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.001 min
Response: 40976494
Conc: 18.85 ng/ml