

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059622.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 01:59
 Operator : AJ\MA
 Sample : L3153-35
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP2-I

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:12:38 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:17:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	38349435	56460277	21.352	21.230
28)	SA Decachlor...	8.287	9.183	28441301	40106662	18.526	18.451
Target Compounds							
12)	B 4,4'-DDE	5.690	6.422	826819	1376011	0.552m	0.516m
13)	MA Dieldrin	5.826	6.578	680175	1255421	0.426	0.445

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059622.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 01:59
Operator : AJ\MA
Sample : L3153-35
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP2-I


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:38 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:17:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

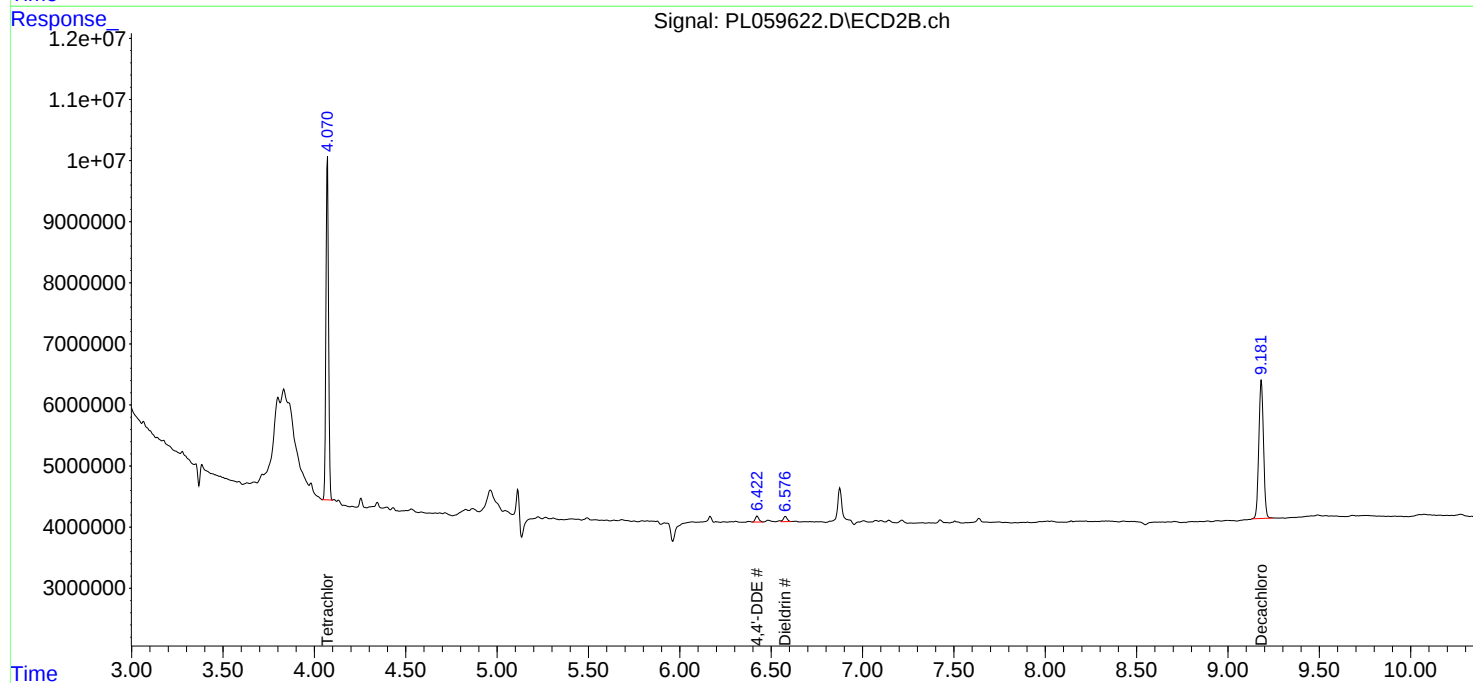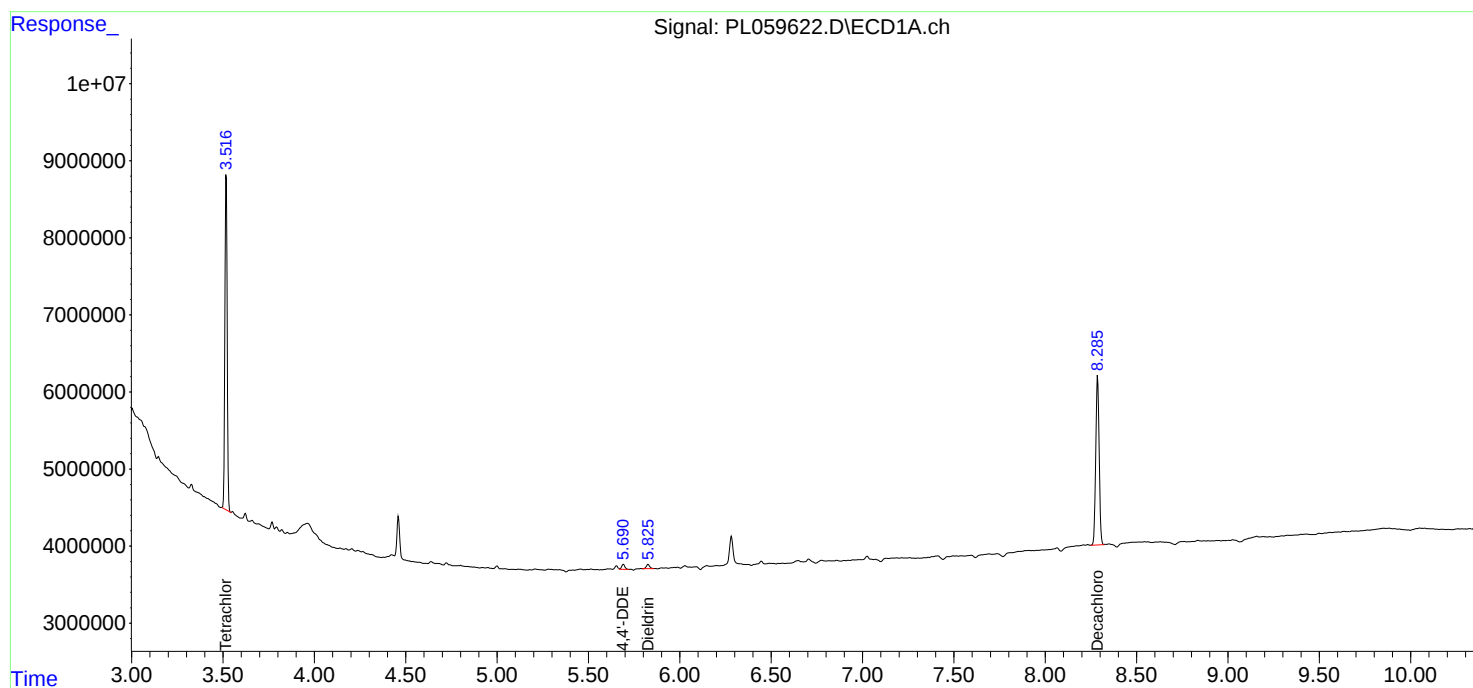

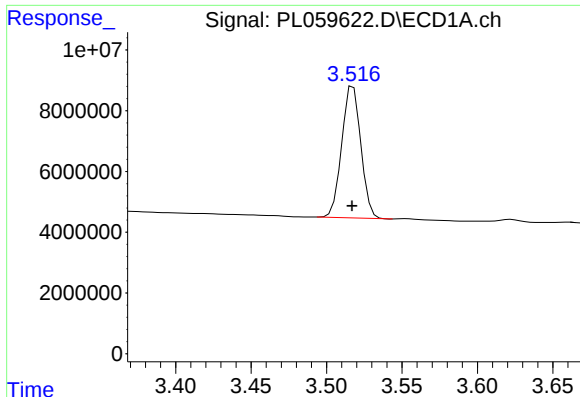


#1 Tetrachloro-m-xylene

R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 38349435
Conc: 21.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-I


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:38 PM

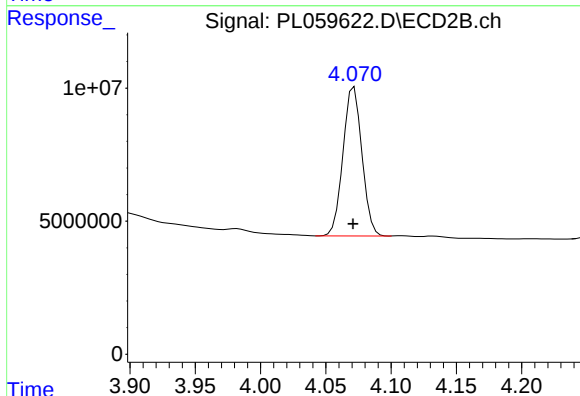


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 56460277
Conc: 21.23 ng/ml

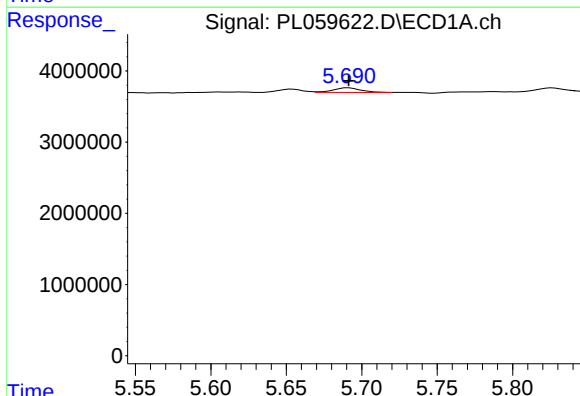


#12 4,4'-DDE

R.T.: 5.690 min
Delta R.T.: -0.002 min
Response: 826819
Conc: 0.55 ng/ml m

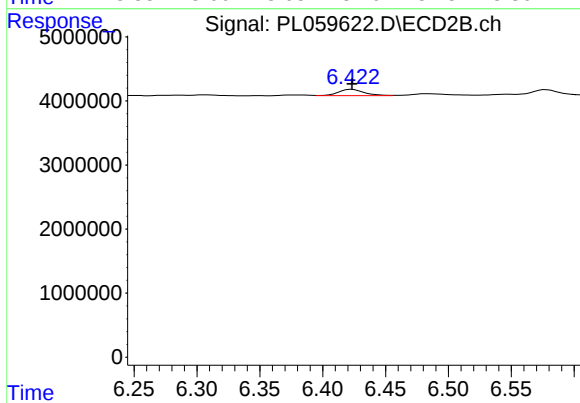

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.001 min
Response: 1376011
Conc: 0.52 ng/ml m

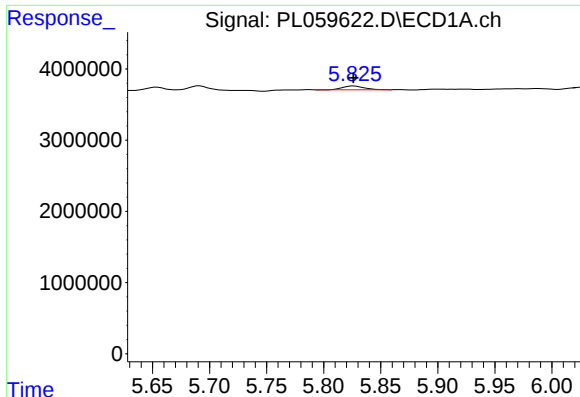


#13 Dieldrin

R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 680175
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-I


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:38 PM

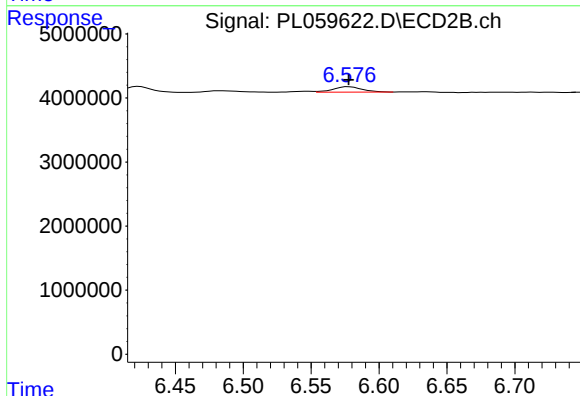


#13 Dieldrin

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 1255421
Conc: 0.45 ng/ml

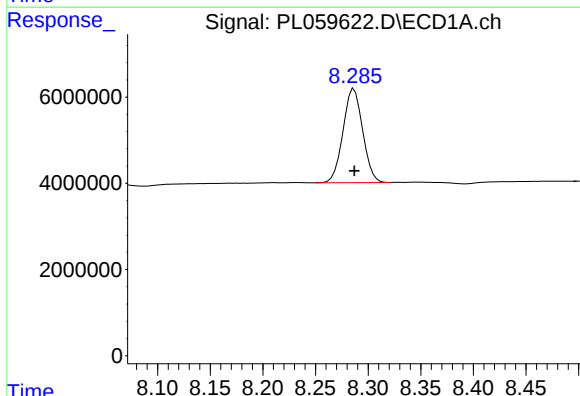

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 28441301
Conc: 18.53 ng/ml

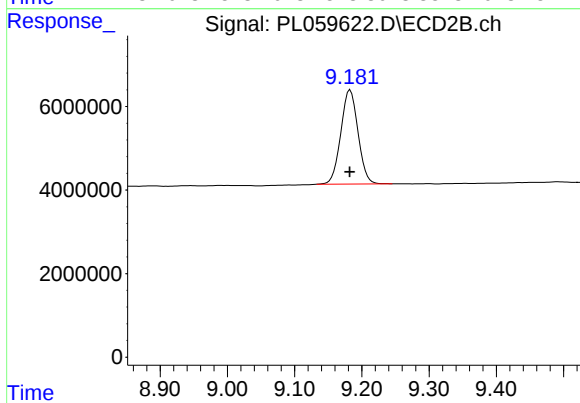

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.000 min
Response: 40106662
Conc: 18.45 ng/ml