

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
 Data File : PL059623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 02:13
 Operator : AJ\MA
 Sample : L3153-38
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP2-J

Manual Integrations
 APPROVED

Ankita
 7/1/2020 12:12:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 04:18:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	40765355	60369907	22.697	22.700
28)	SA Decachlor...	8.287	9.182	29386096	40760013	19.141	18.752
Target Compounds							
12)	B 4,4'-DDE	5.690	6.422	843625	1504122	0.563m	0.564m
13)	MA Dieldrin	5.825	6.578	892734	1146552	0.559	0.407 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063020\
Data File : PL059623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 02:13
Operator : AJ\MA
Sample : L3153-38
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SP2-J


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 04:18:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

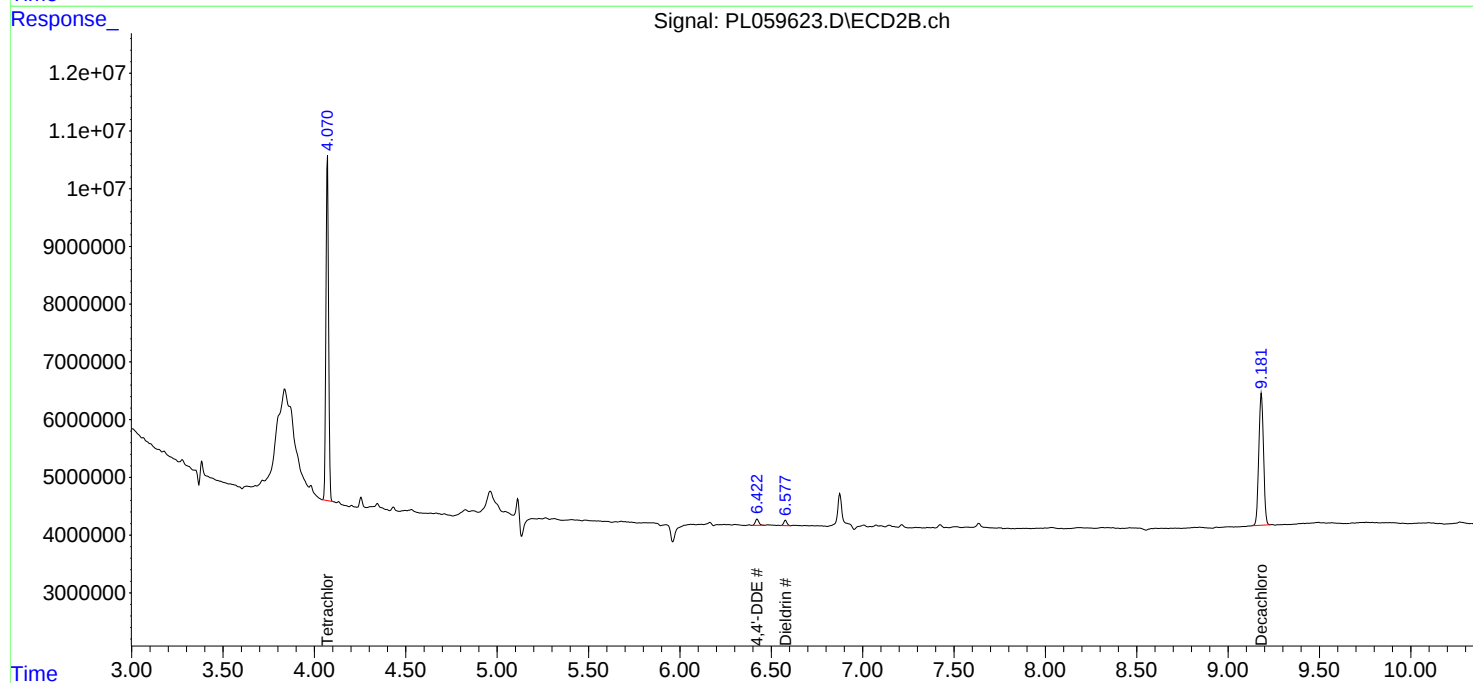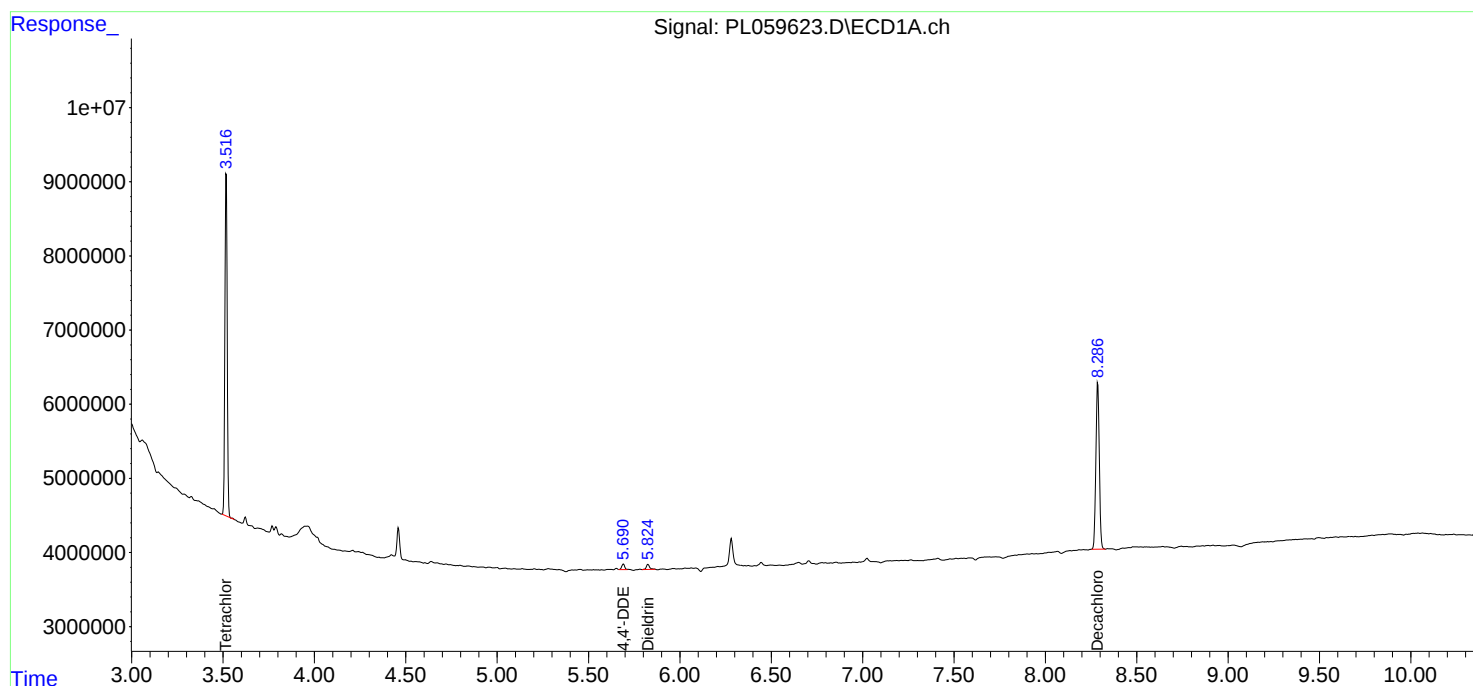

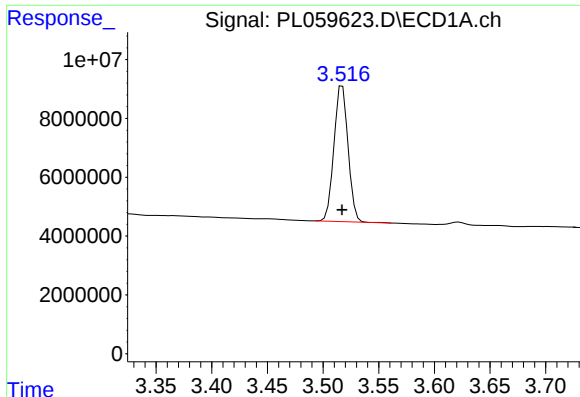


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 40765355
Conc: 22.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-J


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:40 PM

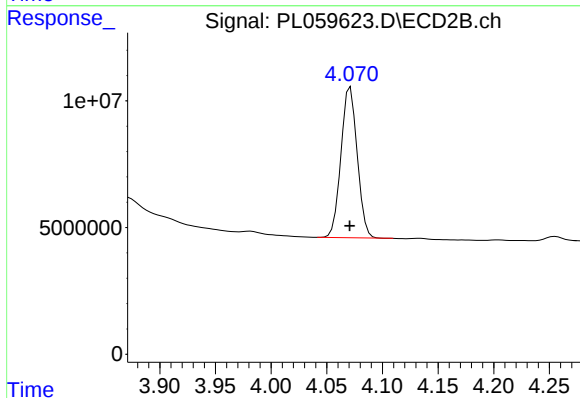


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 60369907
Conc: 22.70 ng/ml

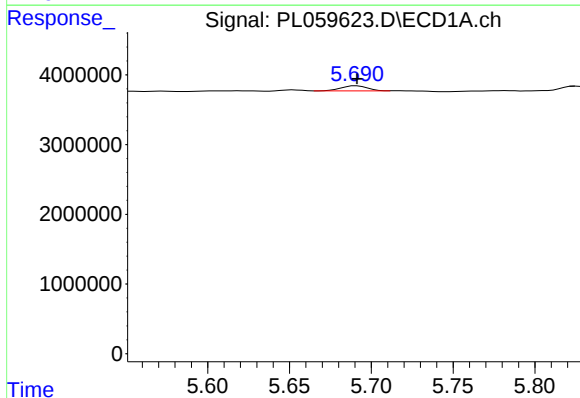


#12 4,4'-DDE

R.T.: 5.690 min
Delta R.T.: -0.002 min
Response: 843625
Conc: 0.56 ng/ml m

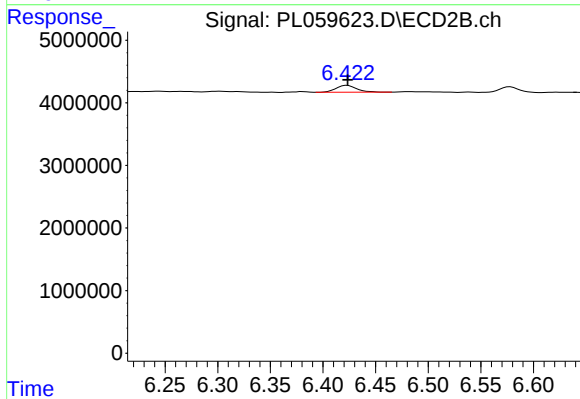

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.002 min
Response: 1504122
Conc: 0.56 ng/ml m

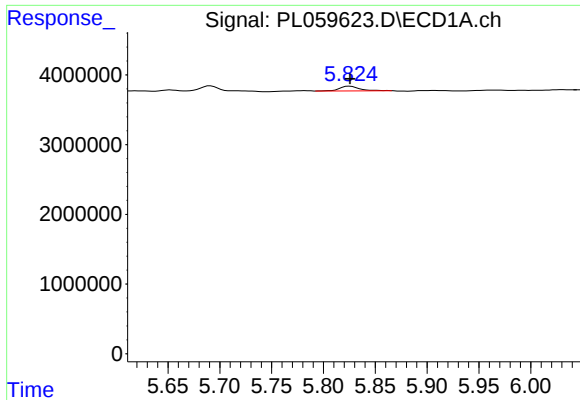


#13 Dieldrin

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 892734
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP2-J


Manual Integrations
APPROVED

Ankita
7/1/2020 12:12:40 PM

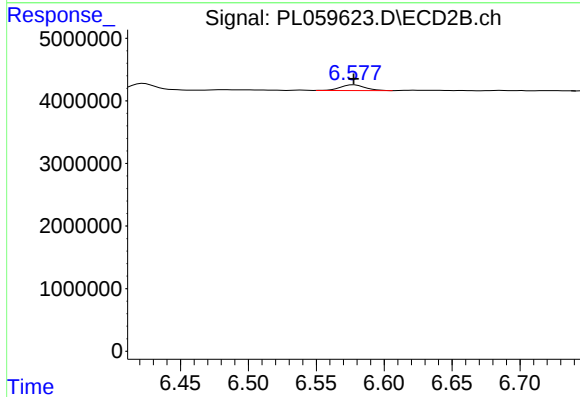


#13 Dieldrin

R.T.: 6.578 min
Delta R.T.: 0.000 min
Response: 1146552
Conc: 0.41 ng/ml

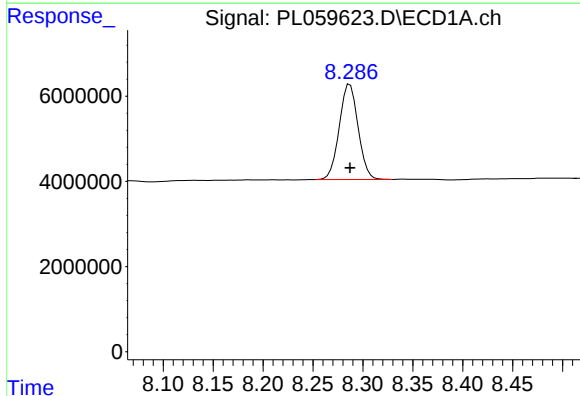

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 29386096
Conc: 19.14 ng/ml

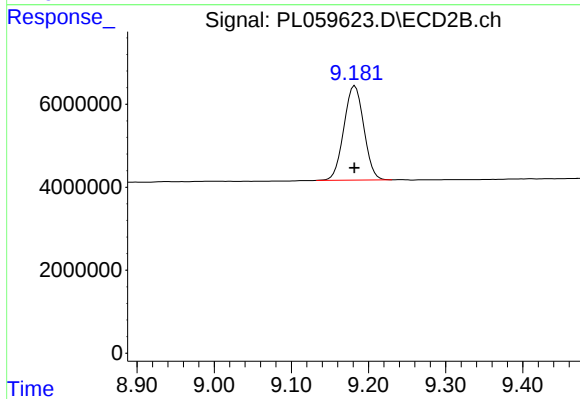

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 40760013
Conc: 18.75 ng/ml