

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063021\
 Data File : PL067893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 12:50
 Operator : AR\AJ
 Sample : M2895-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 00:34:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	5.529	10213385	17517297	18.577	18.581
28)	SA Decachlor...	10.221	11.429	11607303	16335976	16.379	16.401
Target Compounds							
2)	A alpha-BHC	5.207f	0.000	199588	0	0.271	N.D. #
15)	B Endosulfa...	0.000	9.181f	0	326879	N.D.	0.410 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063021\
Data File : PL067893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2021 12:50
Operator : AR\AJ
Sample : M2895-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 00:34:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

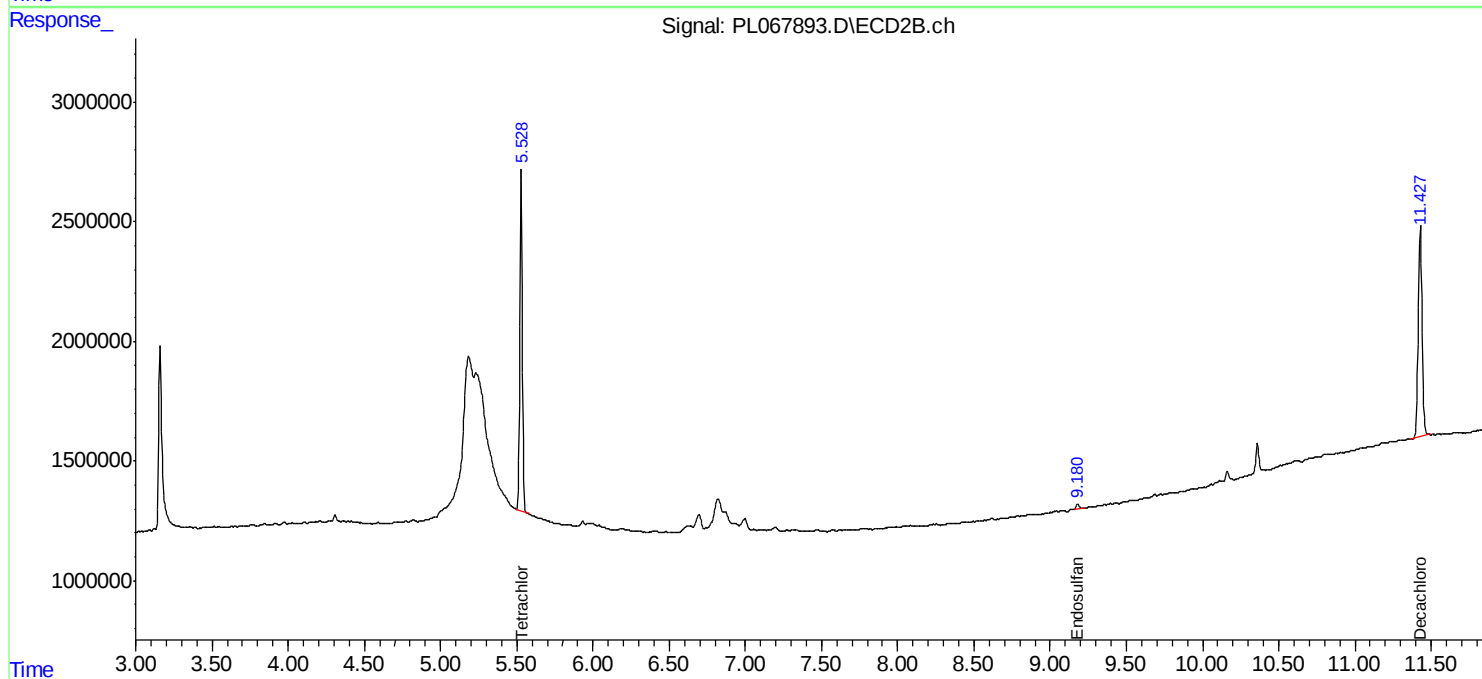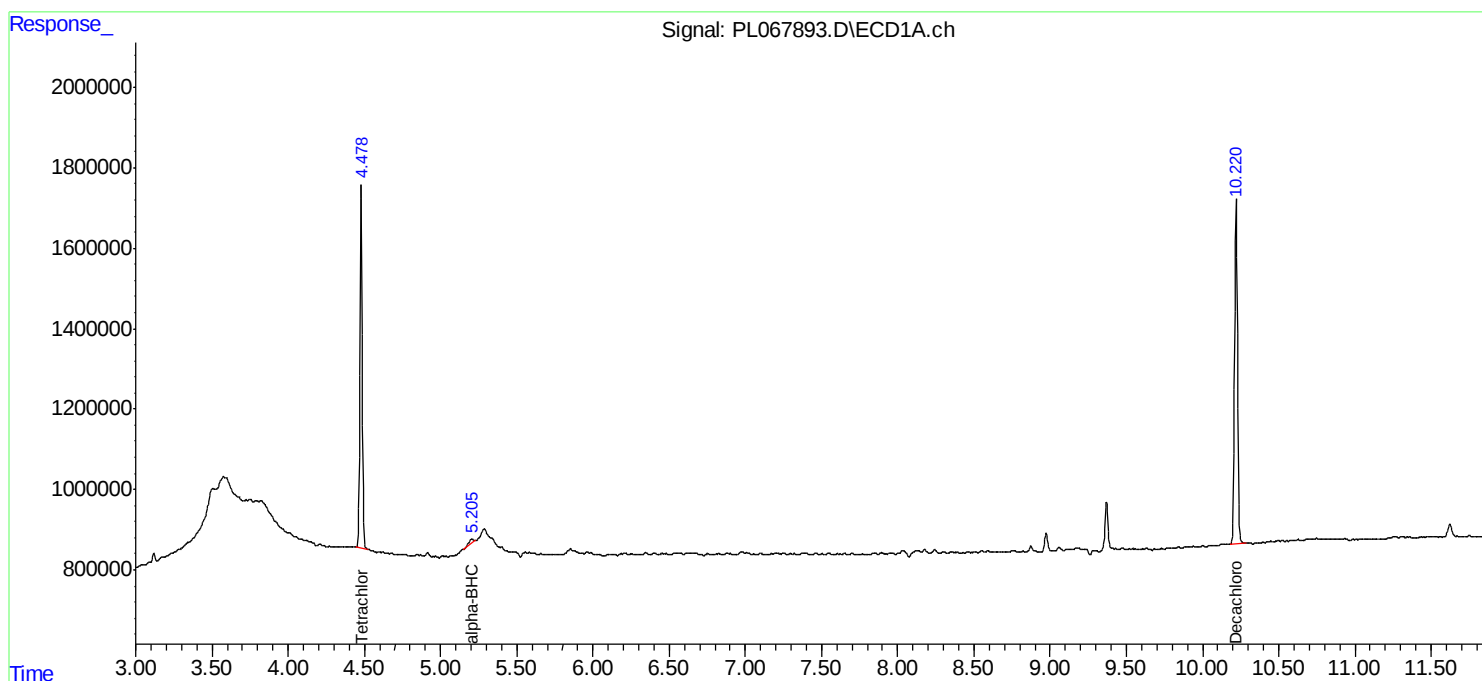


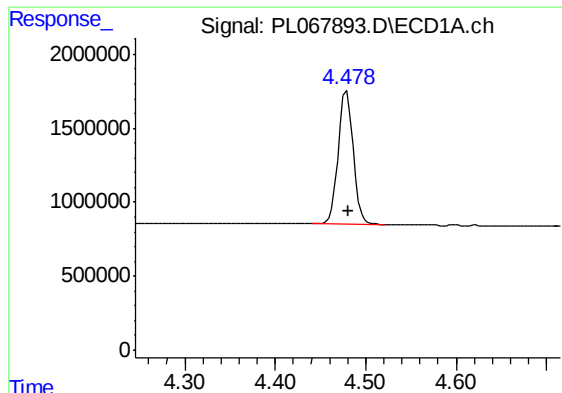

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: -0.002 min
Response: 10213385
Conc: 18.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

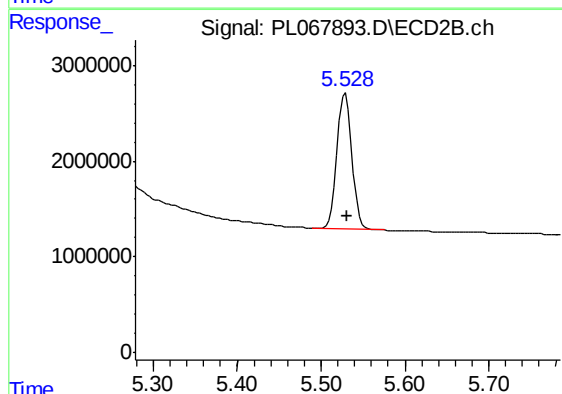


#1 Tetrachloro-m-xylene

R.T.: 5.529 min
Delta R.T.: -0.002 min
Response: 17517297
Conc: 18.58 ng/ml

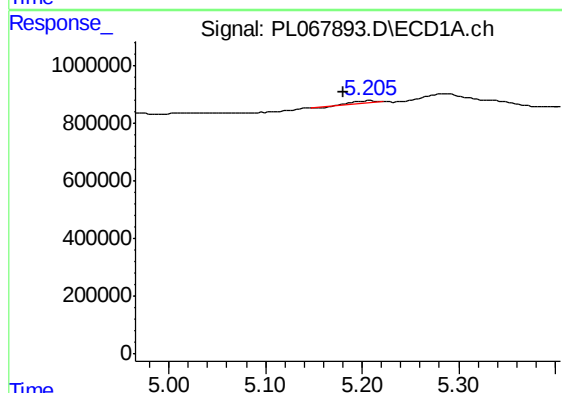


#2 alpha-BHC

R.T.: 5.207 min
Delta R.T.: 0.027 min
Response: 199588
Conc: 0.27 ng/ml

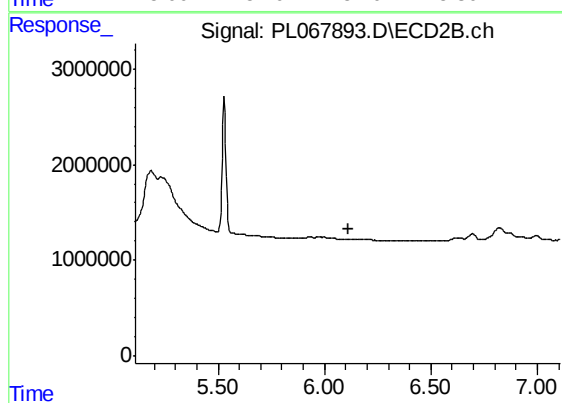

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

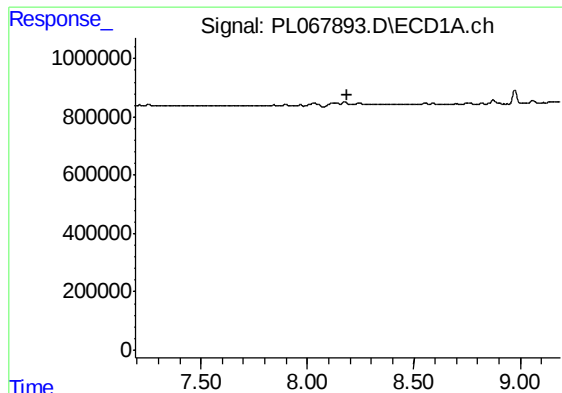

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.190 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

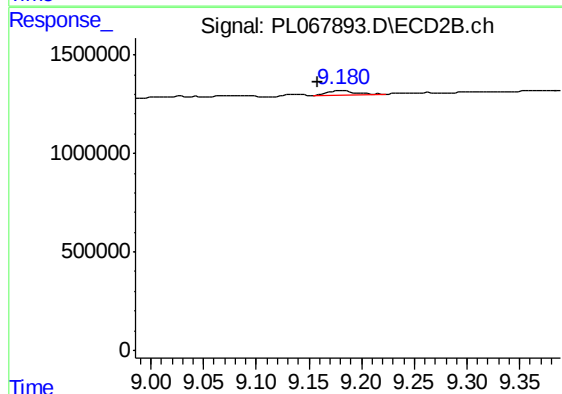


#15 Endosulfan II

R.T.: 9.181 min
Delta R.T.: 0.023 min
Response: 326879
Conc: 0.41 ng/ml

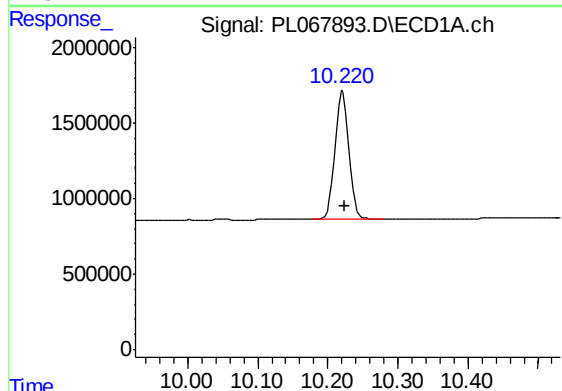

#28 Decachlorobiphenyl

R.T.: 10.221 min
Delta R.T.: -0.003 min
Response: 11607303
Conc: 16.38 ng/ml

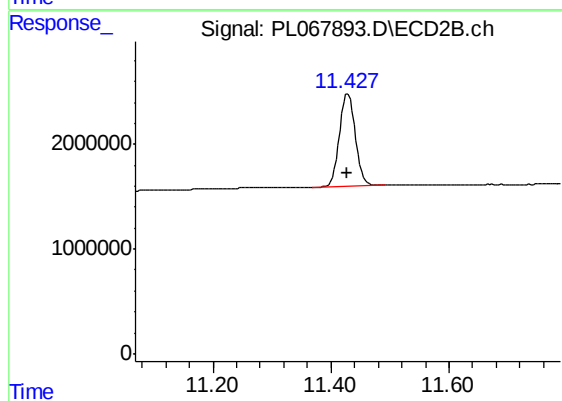

#28 Decachlorobiphenyl

R.T.: 11.429 min
Delta R.T.: 0.000 min
Response: 16335976
Conc: 16.40 ng/ml