

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063021\
 Data File : PL067897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2021 14:06
 Operator : AR\AJ
 Sample : M2895-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 00:36:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	5.547f	9646084	17245024	17.545	18.293
28)	SA Decachlor...	10.220	11.444f	10372737	14749355	14.637	14.808
Target Compounds							
2)	A alpha-BHC	5.204f	0.000	2726670	0	3.707	N.D. #
14)	MA Endrin	7.895f	0.000	243237	0	0.371	N.D. #
15)	B Endosulfa...	8.179	0.000	250713	0	0.407	N.D. #
16)	A 4,4'-DDD	8.029f	0.000	859288	0	1.478	N.D. #
18)	B Endrin al...	8.354f	0.000	282521	0	0.558	N.D. #
19)	B Endosulfa...	8.588f	0.000	628900	0	0.991	N.D. #
21)	B Endrin ke...	0.000	10.022	0	576859	N.D.	0.636 #
27)	Chlordane-5	8.179	9.197f	250713	777661	11.459	26.744 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063021\
Data File : PL067897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2021 14:06
Operator : AR\AJ
Sample : M2895-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 00:36:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

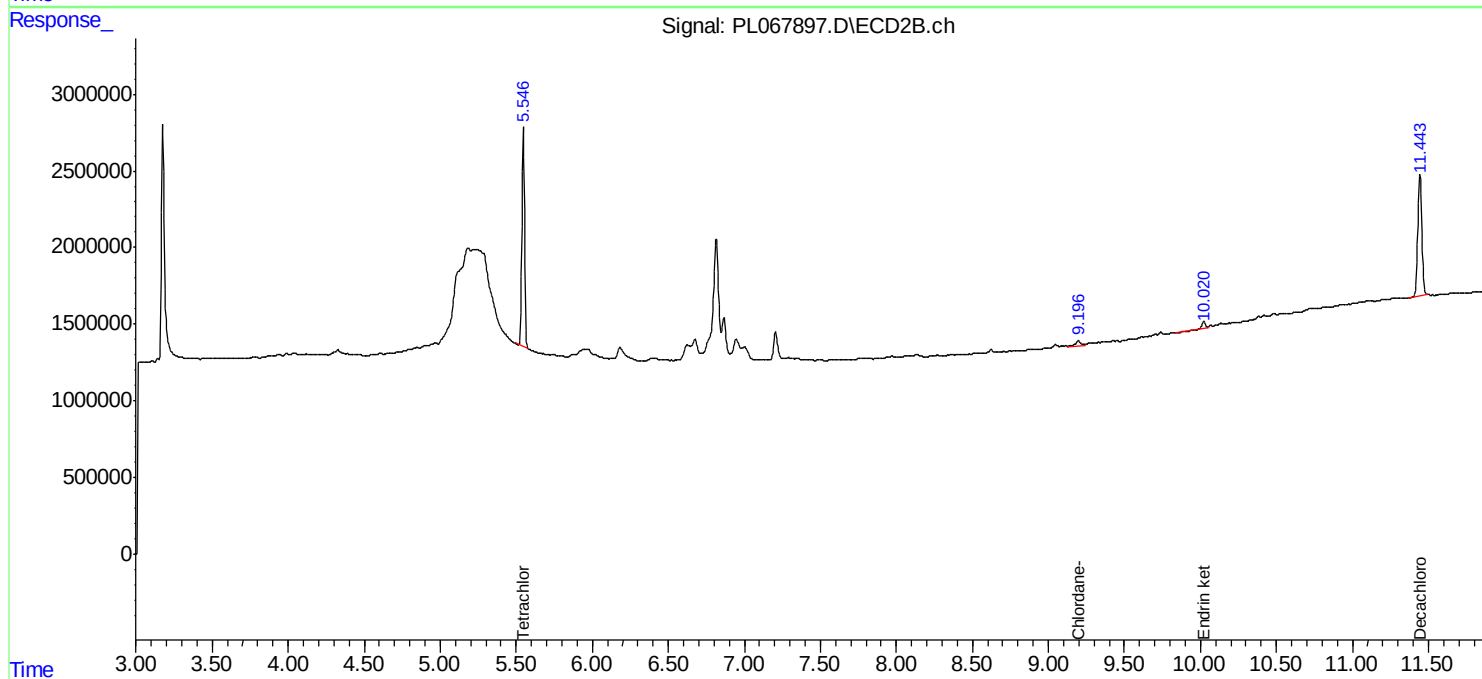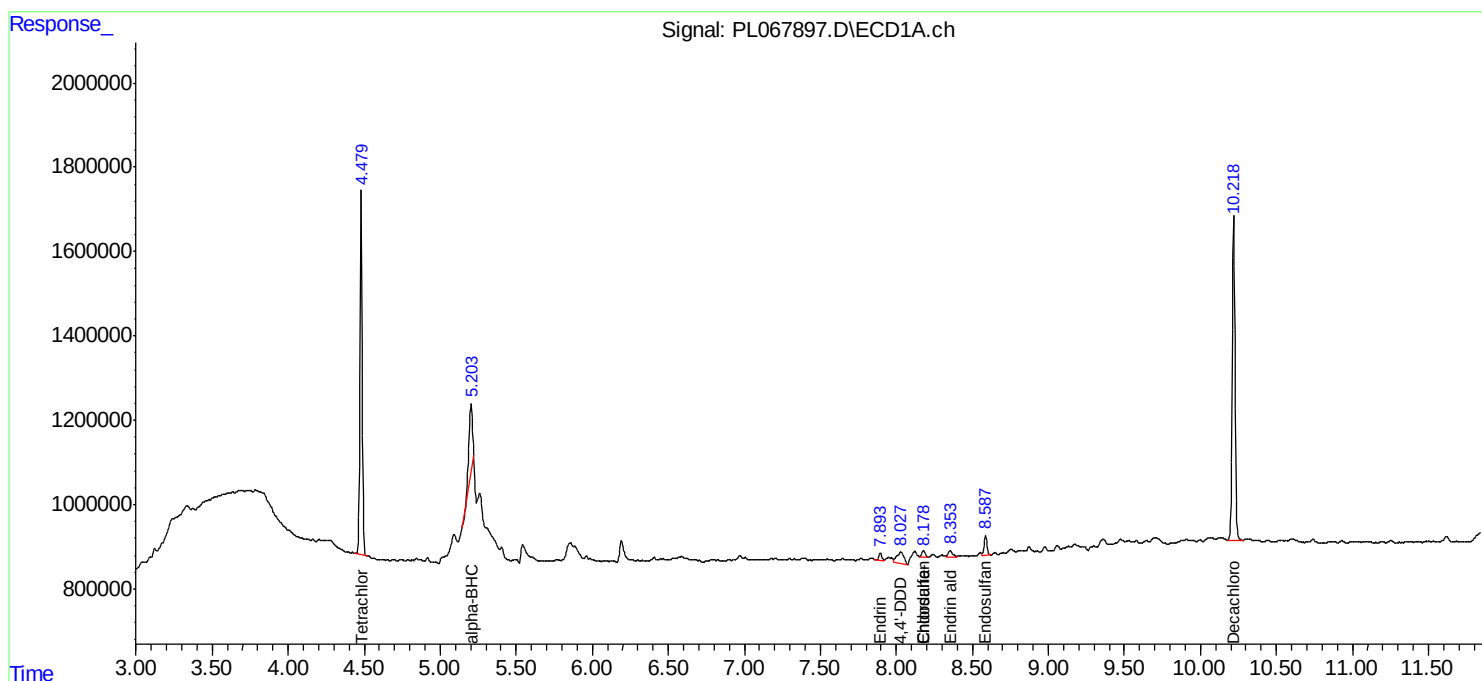


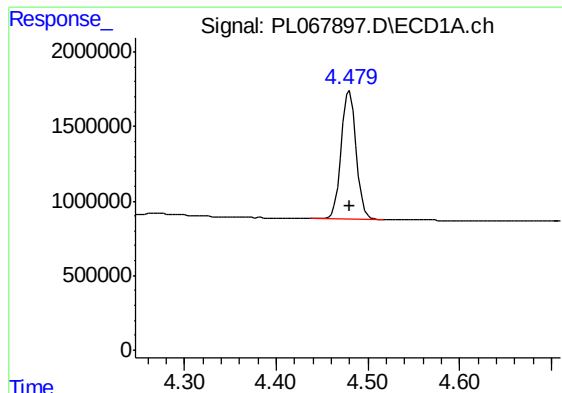

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.000 min
Response: 9646084
Conc: 17.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

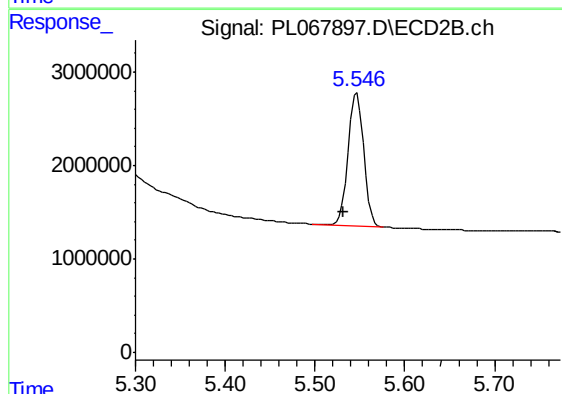


#1 Tetrachloro-m-xylene

R.T.: 5.547 min
Delta R.T.: 0.016 min
Response: 17245024
Conc: 18.29 ng/ml

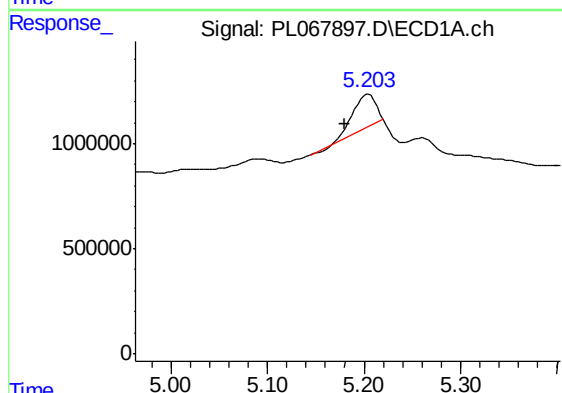


#2 alpha-BHC

R.T.: 5.204 min
Delta R.T.: 0.024 min
Response: 2726670
Conc: 3.71 ng/ml

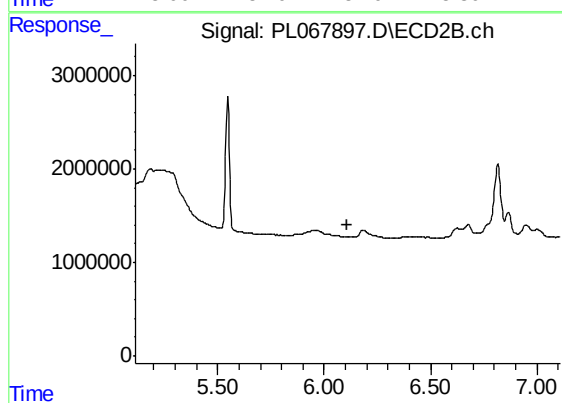

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

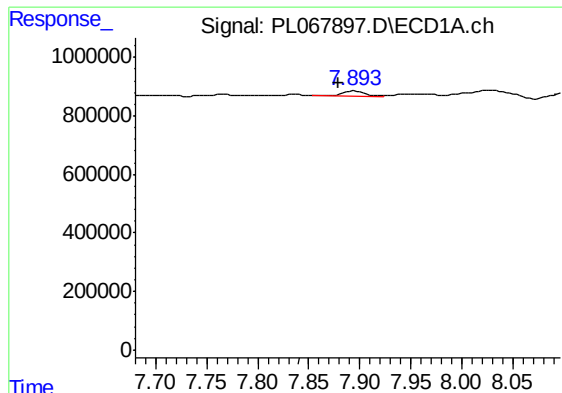

#14 Endrin


R.T.: 7.895 min
Delta R.T.: 0.016 min
Response: 243237
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

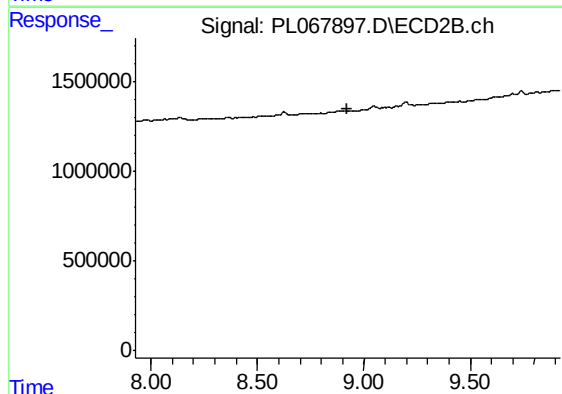


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

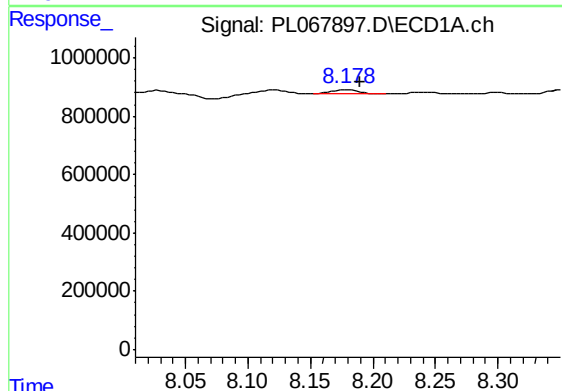


#15 Endosulfan II

R.T.: 8.179 min
Delta R.T.: -0.011 min
Response: 250713
Conc: 0.41 ng/ml

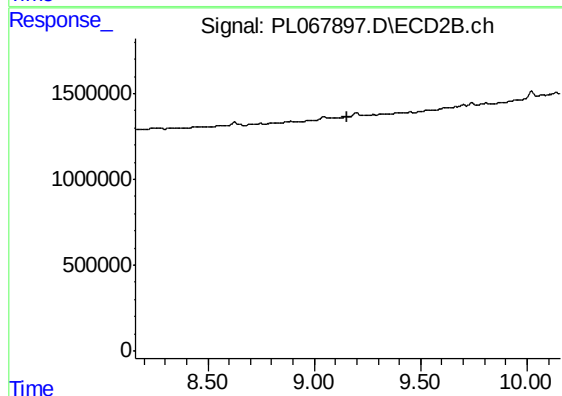

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.158 min
Response: 0
Conc: N.D.

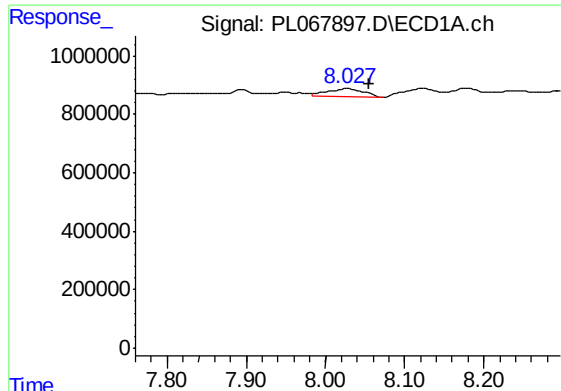

#16 4,4'-DDD


R.T.: 8.029 min
Delta R.T.: -0.026 min
Response: 859288
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

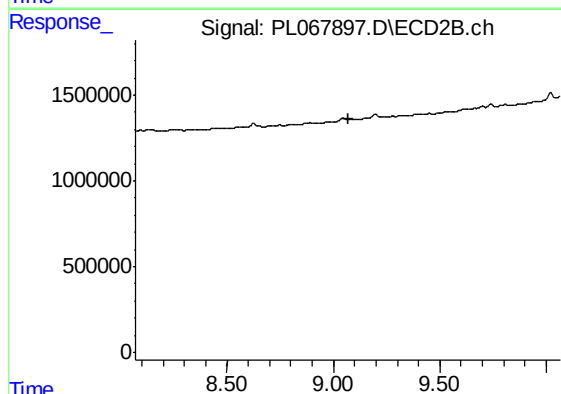


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

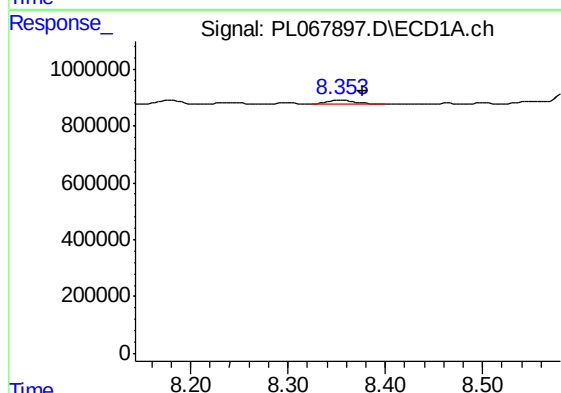


#18 Endrin aldehyde

R.T.: 8.354 min
Delta R.T.: -0.023 min
Response: 282521
Conc: 0.56 ng/ml

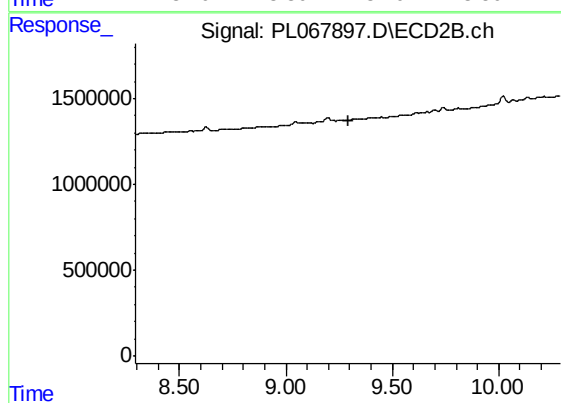

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 9.292 min
Response: 0
Conc: N.D.

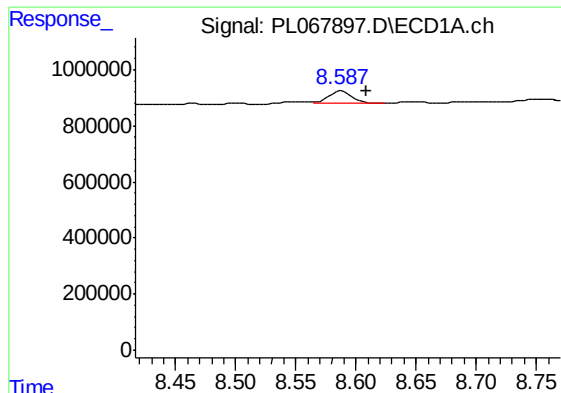

#19 Endosulfan Sulfate


R.T.: 8.588 min
Delta R.T.: -0.020 min
Response: 628900
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

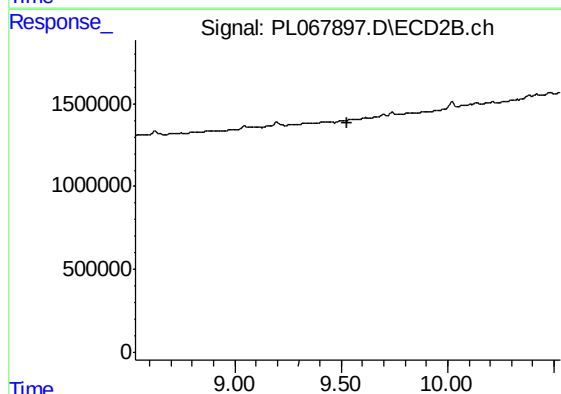


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

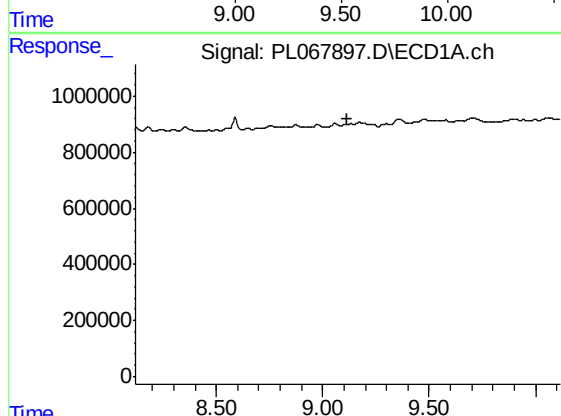


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

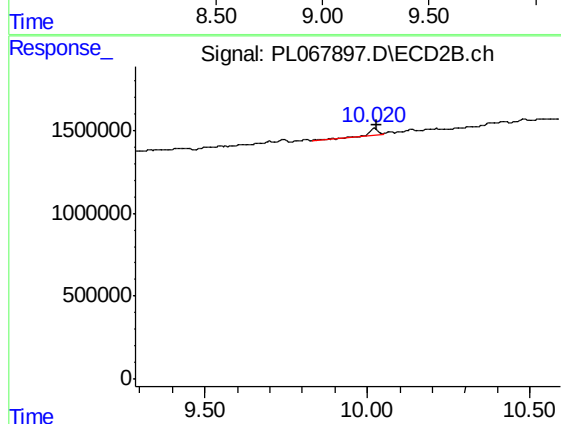

#21 Endrin ketone


R.T.: 10.022 min
Delta R.T.: -0.005 min
Response: 576859
Conc: 0.64 ng/ml

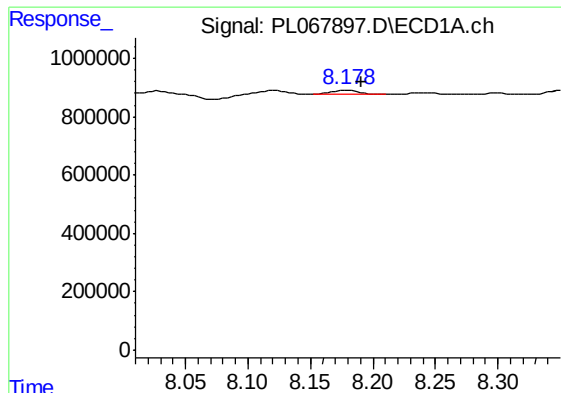

#27 Chlordane-5


R.T.: 8.179 min
Delta R.T.: -0.012 min
Response: 250713
Conc: 11.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

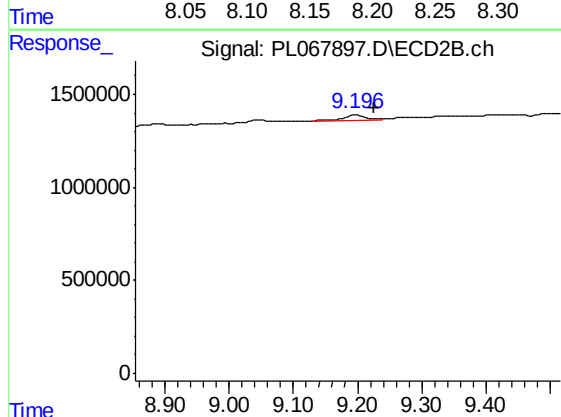


#27 Chlordane-5

R.T.: 9.197 min
Delta R.T.: -0.029 min
Response: 777661
Conc: 26.74 ng/ml

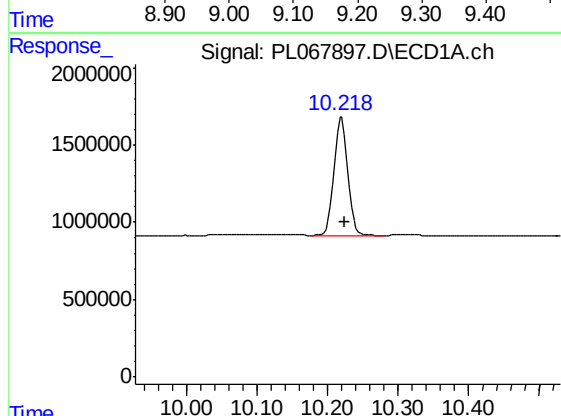

#28 Decachlorobiphenyl

R.T.: 10.220 min
Delta R.T.: -0.005 min
Response: 10372737
Conc: 14.64 ng/ml

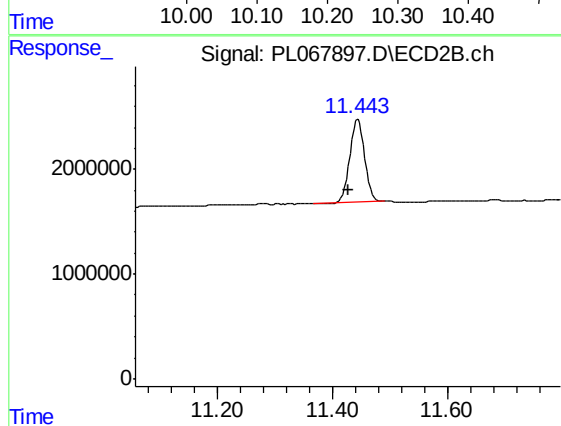

#28 Decachlorobiphenyl

R.T.: 11.444 min
Delta R.T.: 0.016 min
Response: 14749355
Conc: 14.81 ng/ml