

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063022\
 Data File : PL076157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2022 23:15
 Operator : AR\AJ
 Sample : N3549-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ML-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/01/2022
 Supervised By : Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 00:29:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 24 02:17:51 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.632	9529998	24424724	12.600	12.878
28)	SA Decachlor...	11.631	10.370	7264231	16129966	11.544	10.502
Target Compounds							
10)	B gamma-Chl...	8.387	7.333	1105523	1796831	1.422m	0.935 #
11)	B alpha-Chl...	8.472	7.401	2035126	3574614	2.621	1.868 #
12)	B 4,4'-DDE	8.655	7.613	671270	2196298	0.993	1.294 #
17)	MA 4,4'-DDT	9.518	8.456	666669	1853000	1.092	1.253

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL063022\
Data File : PL076157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2022 23:15
Operator : AR\AJ
Sample : N3549-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
ML-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/01/2022
Supervised By : Ankita Jodhani 07/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 00:29:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062222.M
Quant Title : GC Extractables
QLast Update : Fri Jun 24 02:17:51 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

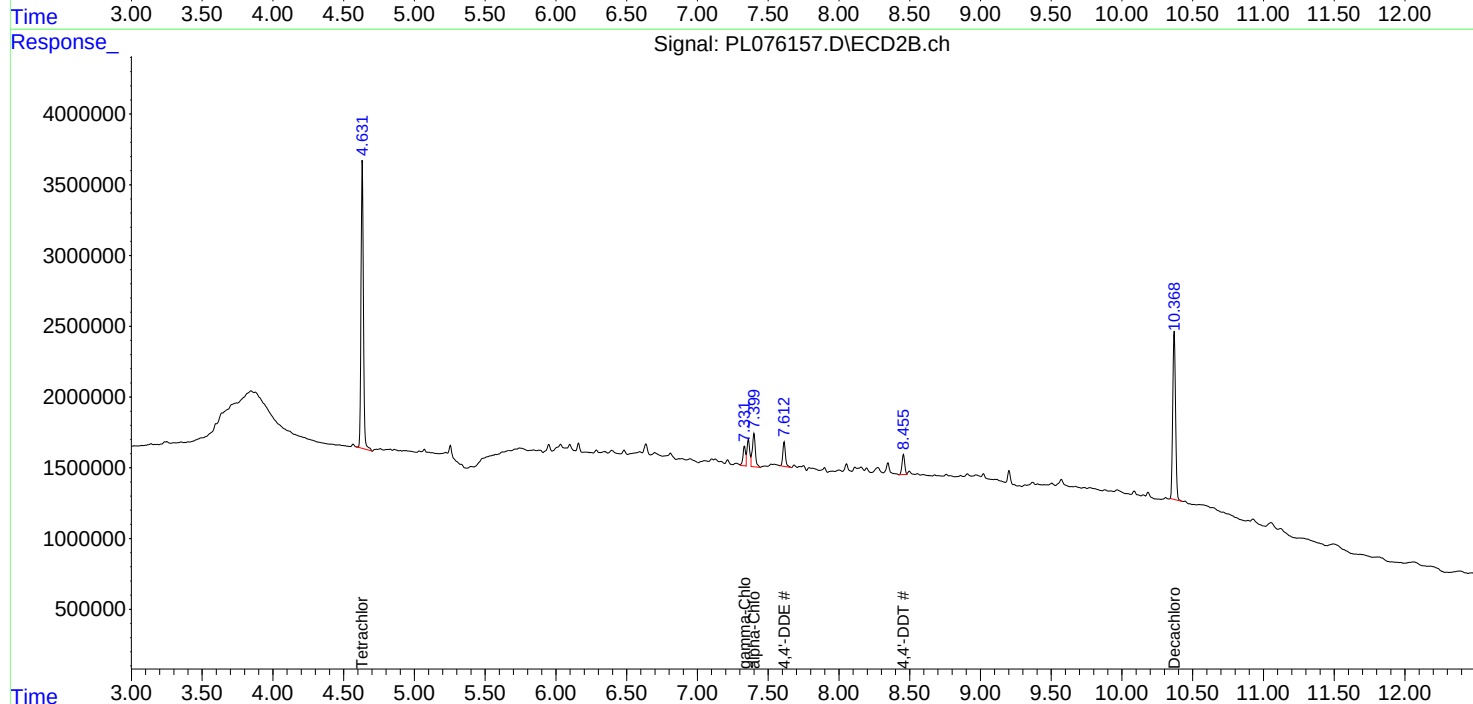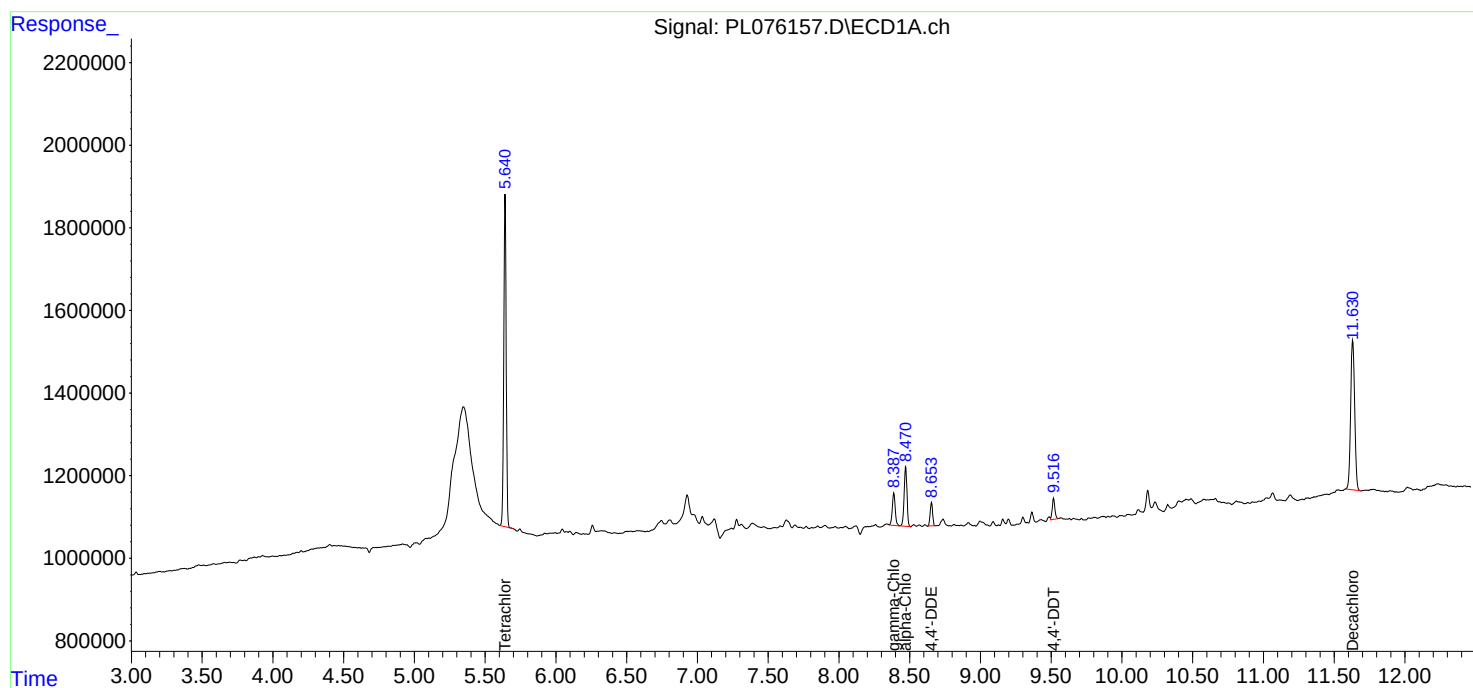

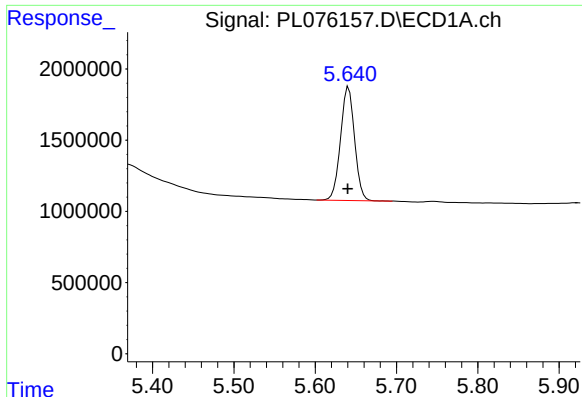


#1 Tetrachloro-m-xylene

R.T.: 5.641 min
Delta R.T.: 0.001 min
Response: 9529998
Conc: 12.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
ML-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/01/2022
Supervised By :Ankita Jodhani 07/01/2022

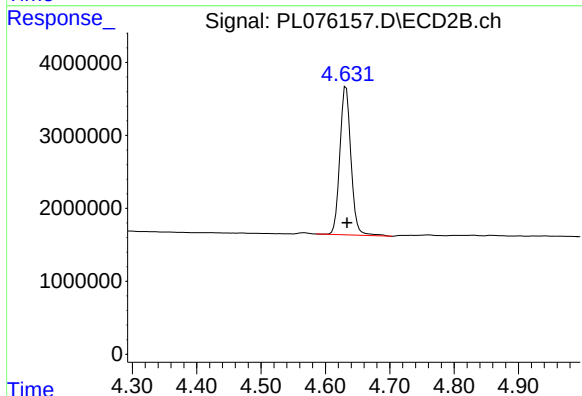


#1 Tetrachloro-m-xylene

R.T.: 4.632 min
Delta R.T.: -0.002 min
Response: 24424724
Conc: 12.88 ng/ml

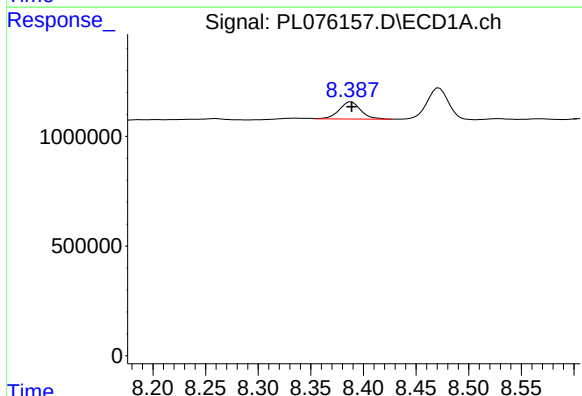


#10 gamma-Chlordane

R.T.: 8.387 min
Delta R.T.: -0.002 min
Response: 1105523
Conc: 1.42 ng/ml m

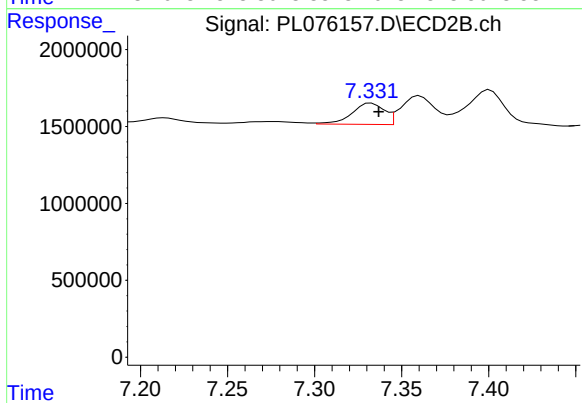

#10 gamma-Chlordane

R.T.: 7.333 min
Delta R.T.: -0.004 min
Response: 1796831
Conc: 0.93 ng/ml

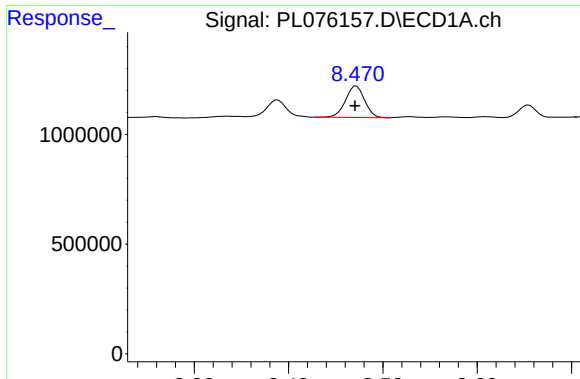


#11 alpha-Chlordane

R.T.: 8.472 min
Delta R.T.: 0.002 min
Response: 2035126
Conc: 2.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
ML-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/01/2022
Supervised By :Ankita Jodhani 07/01/2022

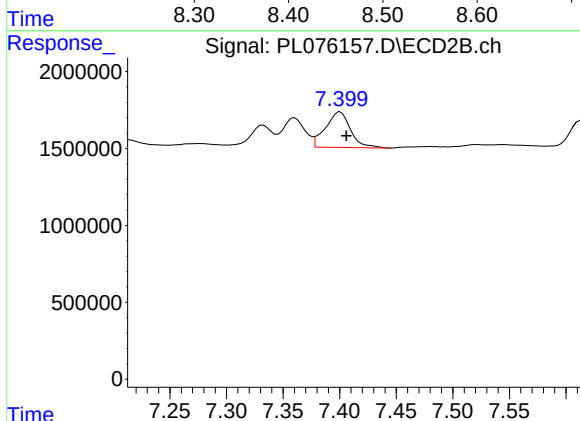


#11 alpha-Chlordane

R.T.: 7.401 min
Delta R.T.: -0.005 min
Response: 3574614
Conc: 1.87 ng/ml

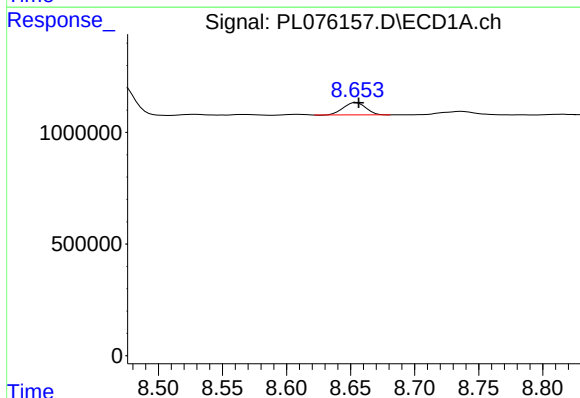


#12 4,4'-DDE

R.T.: 8.655 min
Delta R.T.: -0.002 min
Response: 671270
Conc: 0.99 ng/ml

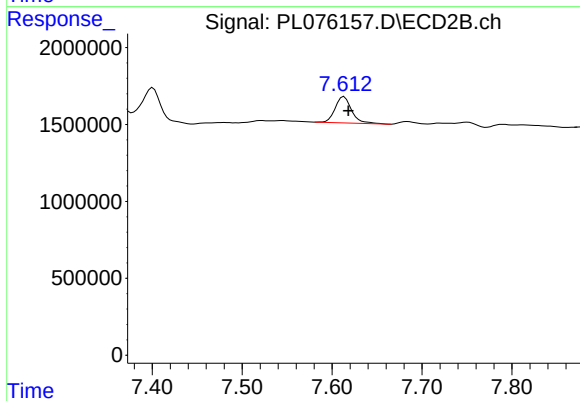

#12 4,4'-DDE

R.T.: 7.613 min
Delta R.T.: -0.005 min
Response: 2196298
Conc: 1.29 ng/ml

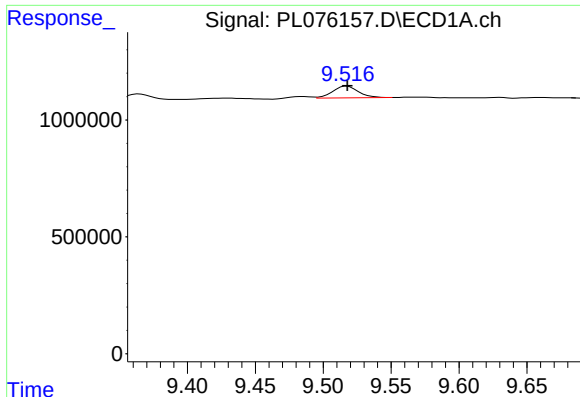


#17 4,4'-DDT

R.T.: 9.518 min
Delta R.T.: 0.000 min
Response: 666669
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
ML-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/01/2022
Supervised By :Ankita Jodhani 07/01/2022

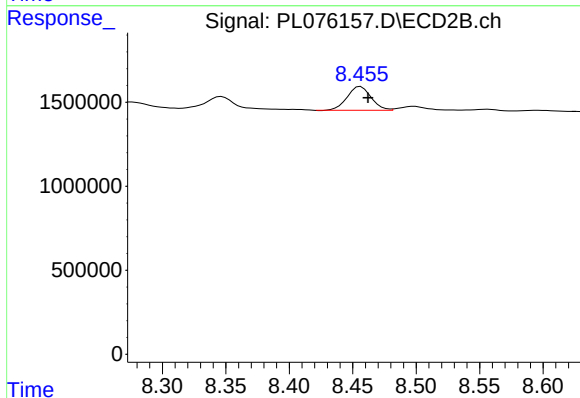


#17 4,4'-DDT

R.T.: 8.456 min
Delta R.T.: -0.006 min
Response: 1853000
Conc: 1.25 ng/ml

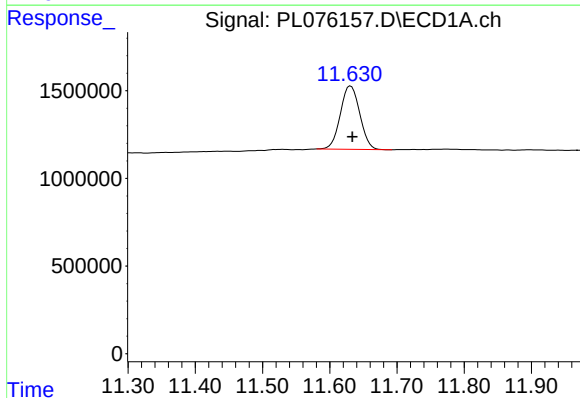

#28 Decachlorobiphenyl

R.T.: 11.631 min
Delta R.T.: -0.003 min
Response: 7264231
Conc: 11.54 ng/ml

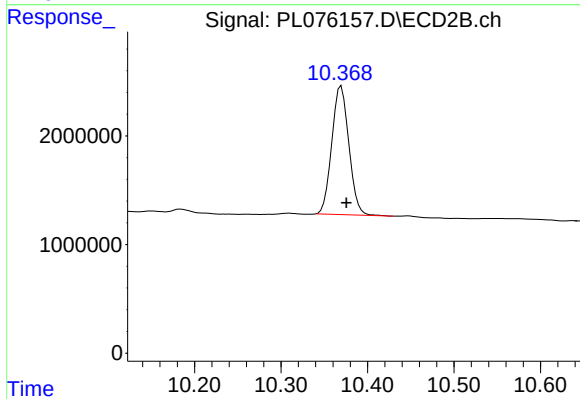

#28 Decachlorobiphenyl

R.T.: 10.370 min
Delta R.T.: -0.006 min
Response: 16129966
Conc: 10.50 ng/ml