

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 11:22
 Operator : SM\AJ
 Sample : K3558-19RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-016-SW095-062619RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:24:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.932	166.6E6	41212227	14.772	13.460
28)	SA Decachlor...	7.985	8.965	132.4E6	34774433	10.421	10.359
Target Compounds							
7)	B delta-BHC	0.000	4.984	0	12352200	N.D.	3.136 #
8)	B Heptachlo...	0.000	5.809	0	9713235	N.D.	2.672 #
9)	A Endosulfan I	5.343f	0.000	50530619	0	3.266	N.D. #
10)	B gamma-Chl...	0.000	6.019	0	9449093	N.D.	2.536 #
13)	MA Dieldrin	5.554	6.406	159.8E6	14757949	9.590	4.160 #
17)	MA 4,4'-DDT	6.172	0.000	23531097	0	1.772	N.D. #
20)	A Methoxychlor	6.755f	0.000	22449302	0	3.444	N.D. #
25)	Chlordane-3	0.000	6.019f	0	9449093	N.D.	18.988 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 11:22
Operator : SM\AJ
Sample : K3558-19RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:24:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

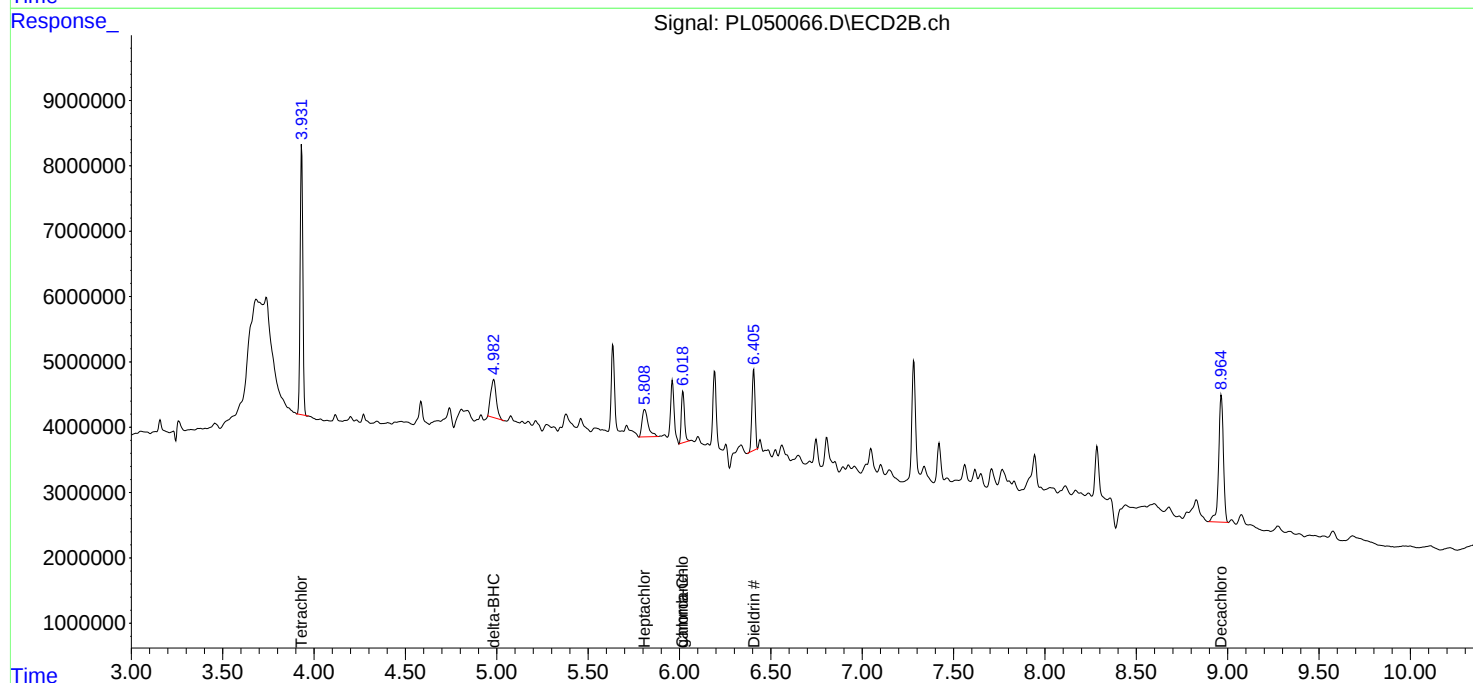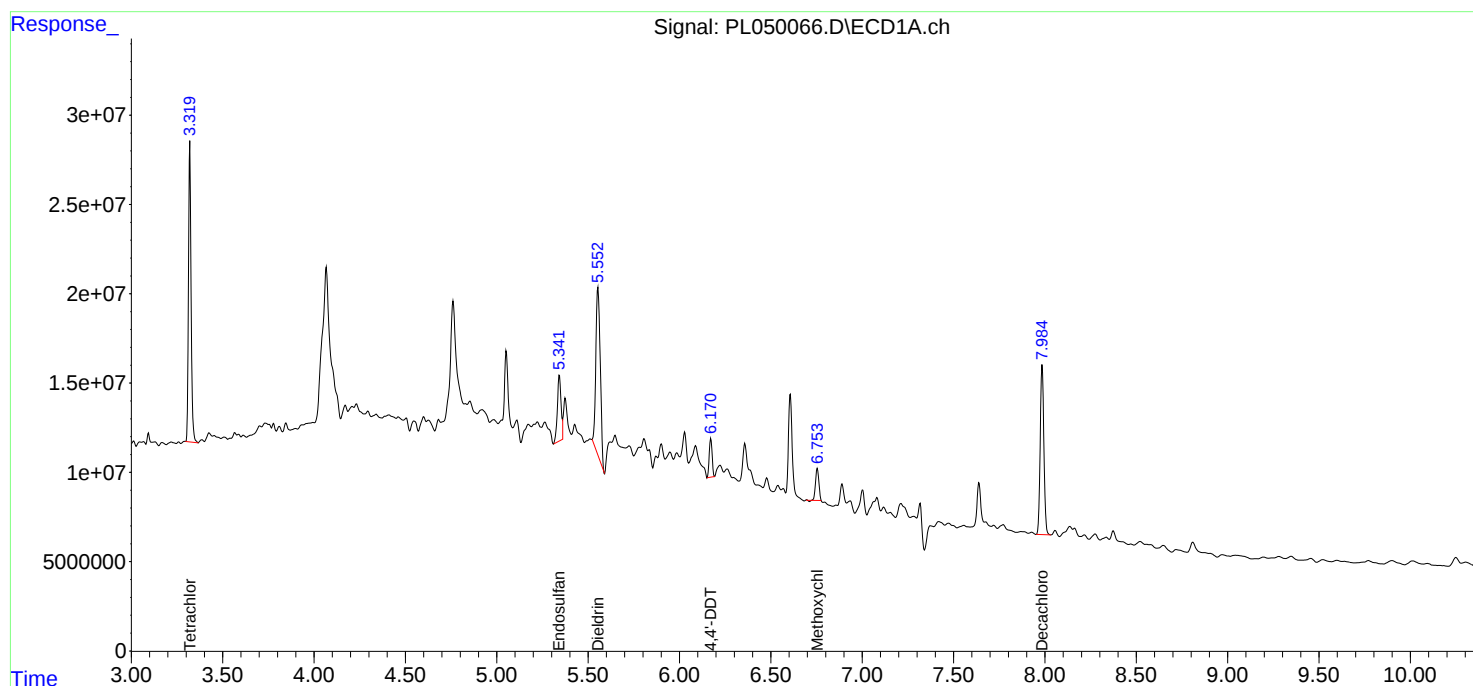


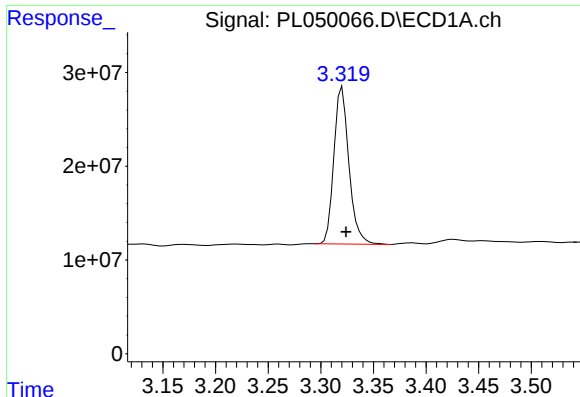

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 166591983
Conc: 14.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

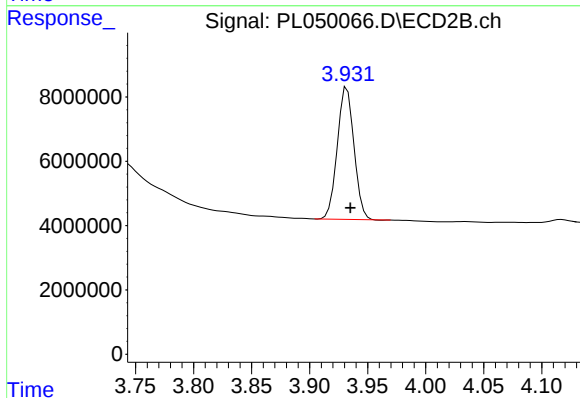


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.003 min
Response: 41212227
Conc: 13.46 ng/ml

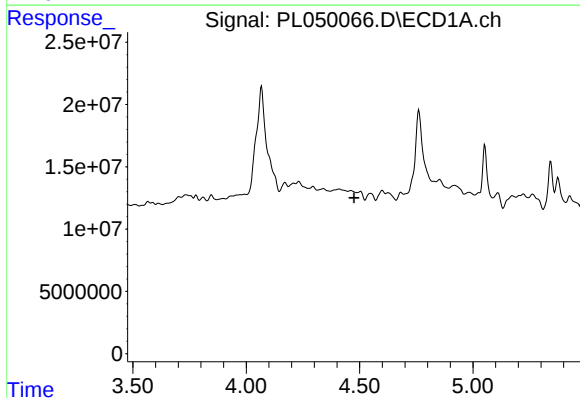


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.476 min
Response: 0
Conc: N.D.

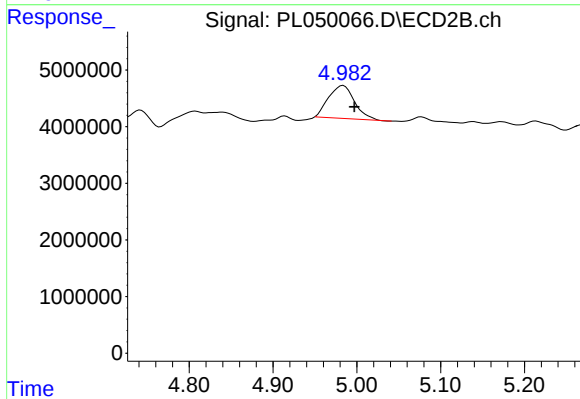

#7 delta-BHC


R.T.: 4.984 min
Delta R.T.: -0.013 min
Response: 12352200
Conc: 3.14 ng/ml

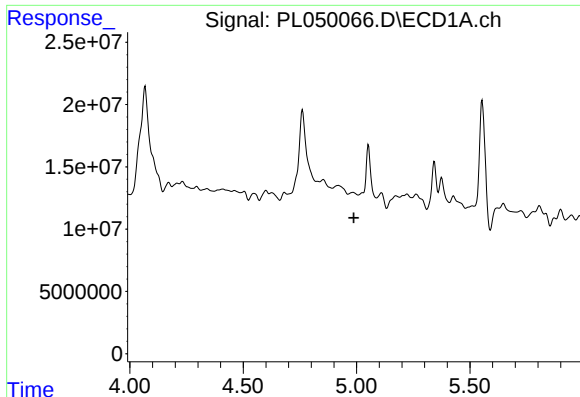

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

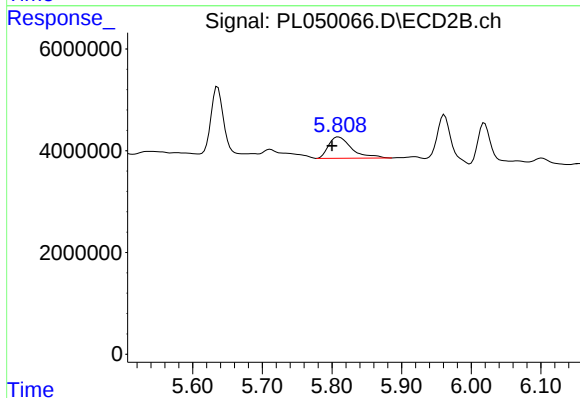


#8 Heptachlor epoxide

R.T.: 5.809 min
Delta R.T.: 0.009 min
Response: 9713235
Conc: 2.67 ng/ml

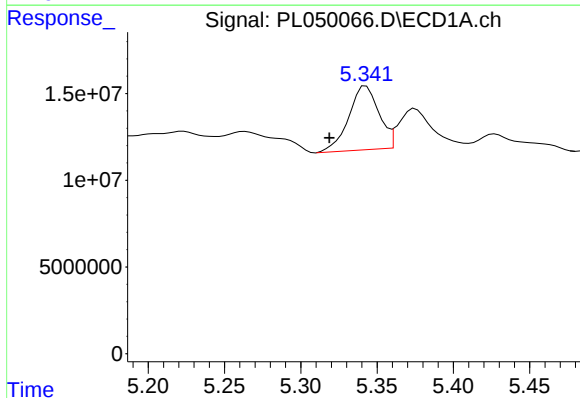


#9 Endosulfan I

R.T.: 5.343 min
Delta R.T.: 0.024 min
Response: 50530619
Conc: 3.27 ng/ml

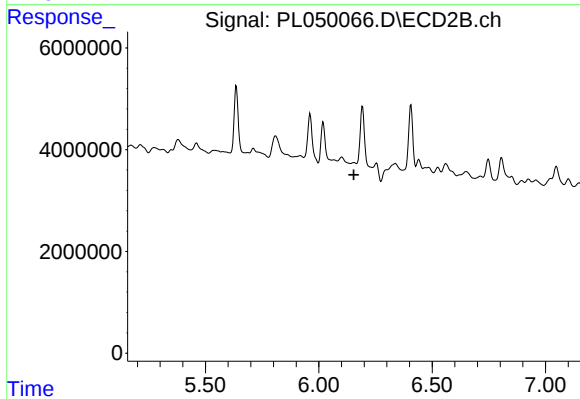

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

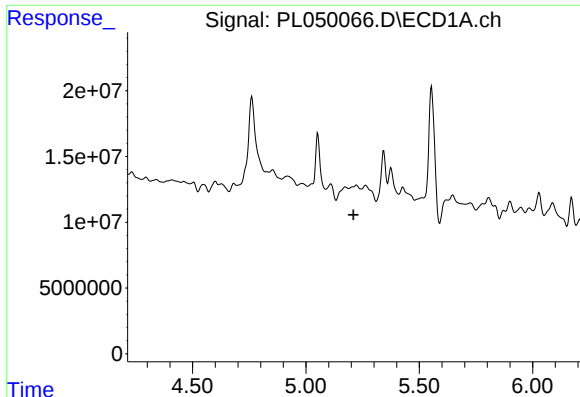

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

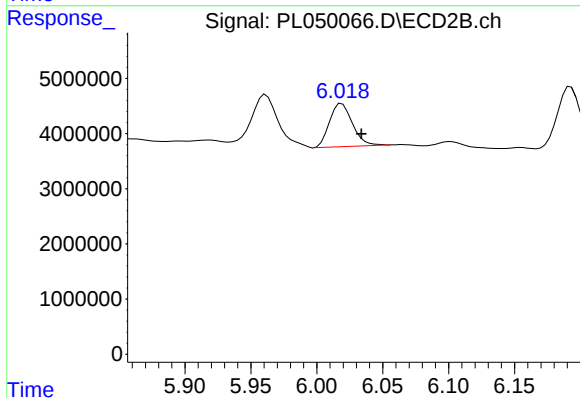


#10 gamma-Chlordane

R.T.: 6.019 min
Delta R.T.: -0.015 min
Response: 9449093
Conc: 2.54 ng/ml

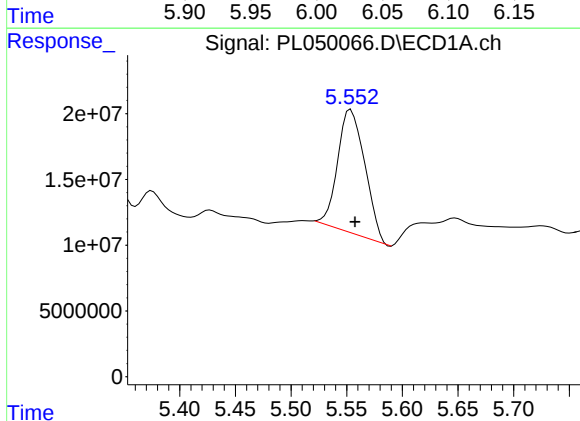


#13 Dieldrin

R.T.: 5.554 min
Delta R.T.: -0.004 min
Response: 159756439
Conc: 9.59 ng/ml

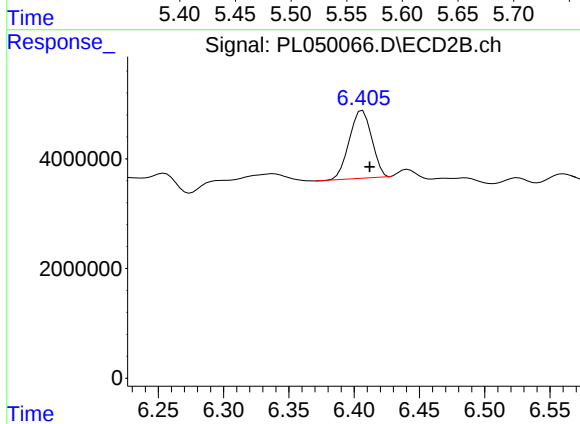

#13 Dieldrin


R.T.: 6.406 min
Delta R.T.: -0.006 min
Response: 14757949
Conc: 4.16 ng/ml

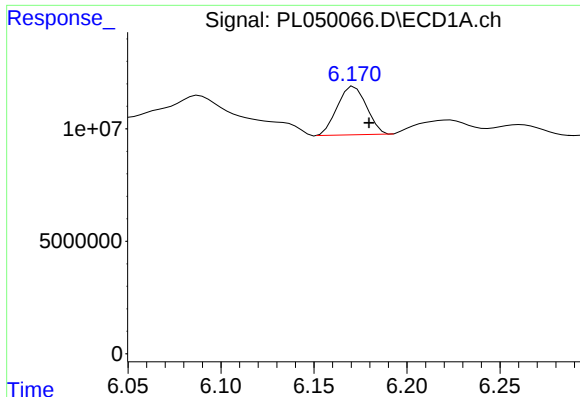

#17 4,4'-DDT


R.T.: 6.172 min
Delta R.T.: -0.008 min
Response: 23531097
Conc: 1.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

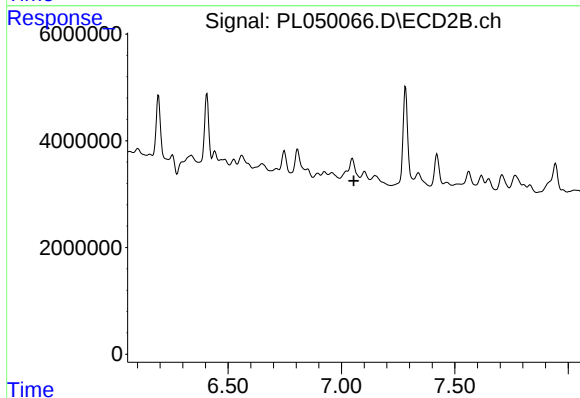


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.054 min
Response: 0
Conc: N.D.

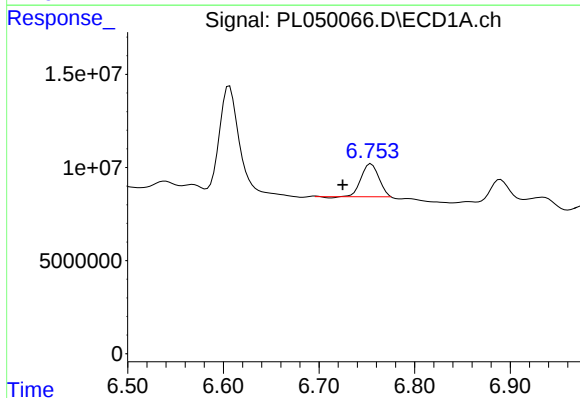


#20 Methoxychlor

R.T.: 6.755 min
Delta R.T.: 0.030 min
Response: 22449302
Conc: 3.44 ng/ml

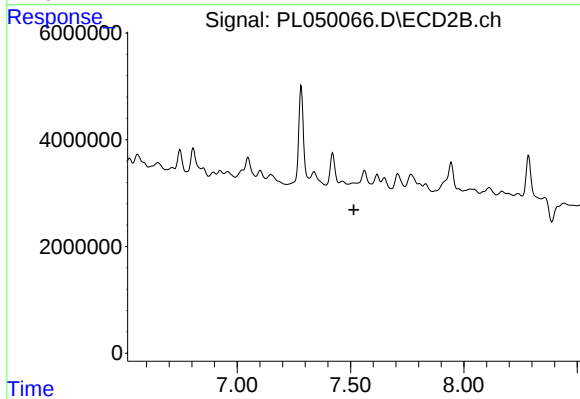

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.515 min
Response: 0
Conc: N.D.

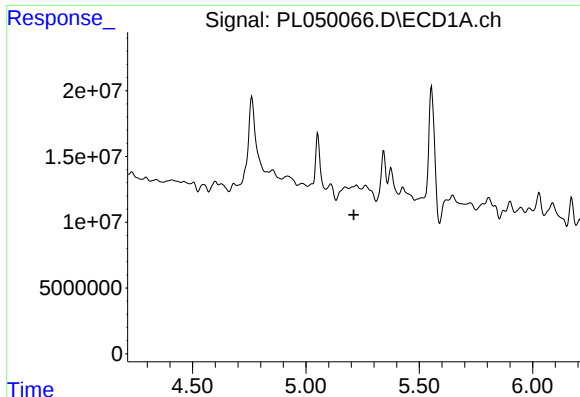

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-016-SW095-062619RE

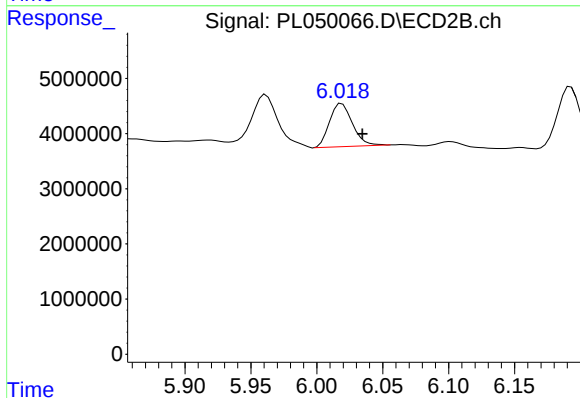


#25 Chlordane-3

R.T.: 6.019 min
Delta R.T.: -0.016 min
Response: 9449093
Conc: 18.99 ng/ml

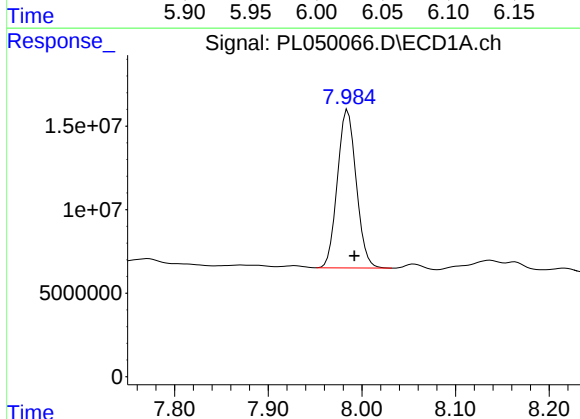

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 132419014
Conc: 10.42 ng/ml

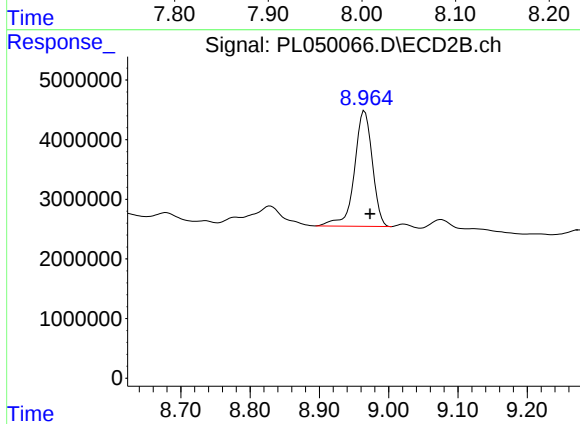

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 34774433
Conc: 10.36 ng/ml