

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 14:03
 Operator : SM\AJ
 Sample : K3560-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-009-SW137-062419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:26:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	238.7E6	54653721	21.165	17.850
28)	SA Decachlor...	7.985	8.966	213.3E6	57852609	16.784	17.233
Target Compounds							
7)	B delta-BHC	0.000	4.987	0	13159306	N.D.	3.341 #
8)	B Heptachlo...	0.000	5.811	0	8922400	N.D.	2.454 #
9)	A Endosulfan I	5.343f	0.000	37941657	0	2.452	N.D. #
10)	B gamma-Chl...	0.000	6.021	0	9999140	N.D.	2.683 #
12)	B 4,4'-DDE	5.428	6.260	101.0E6	16092218	6.065	4.637
13)	MA Dieldrin	5.562	0.000	73906250	0	4.437	N.D. #
17)	MA 4,4'-DDT	6.172	7.049	34578441	8061892	2.605	2.753
25)	Chlordane-3	0.000	6.021	0	9999140	N.D.	20.094 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 14:03
Operator : SM\AJ
Sample : K3560-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:26:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

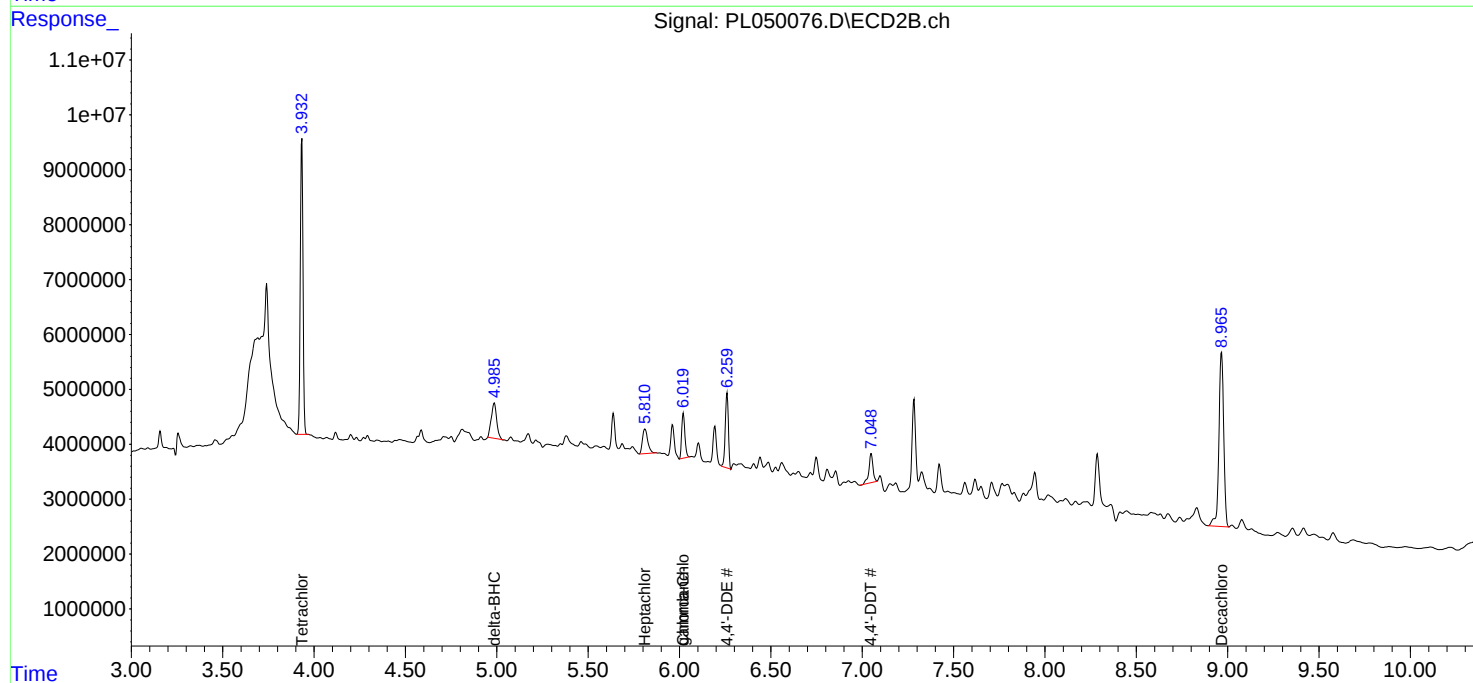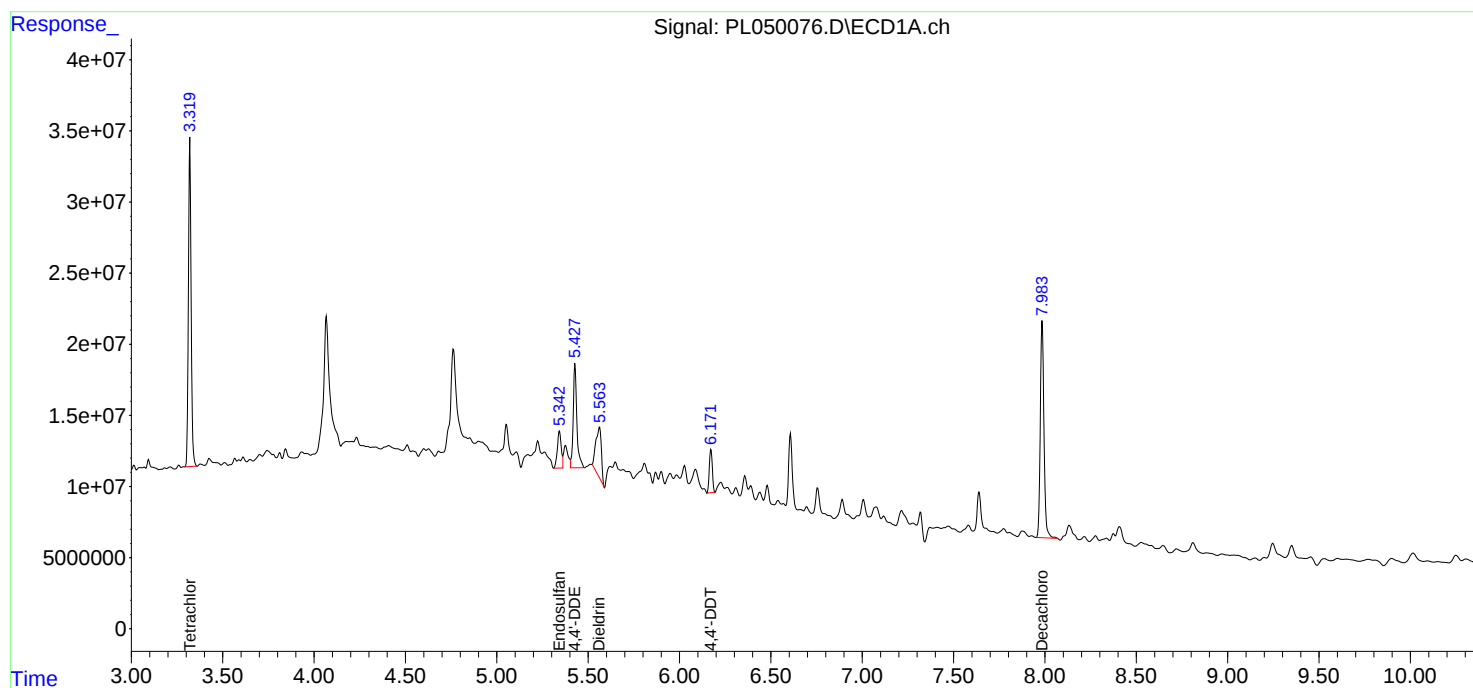


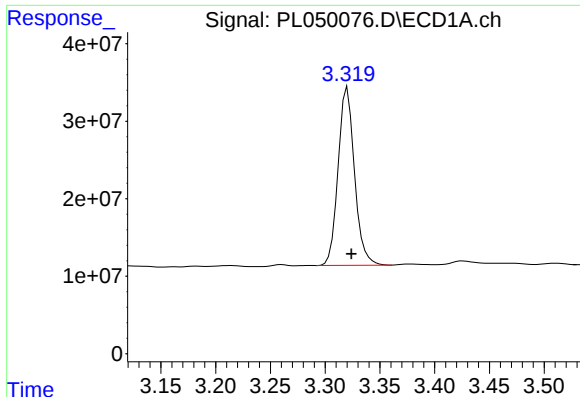

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 238688256
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

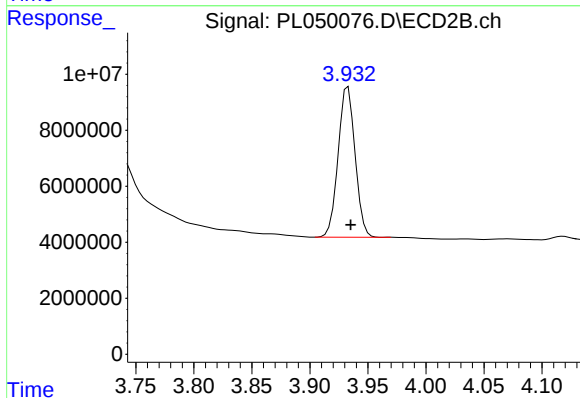


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 54653721
Conc: 17.85 ng/ml

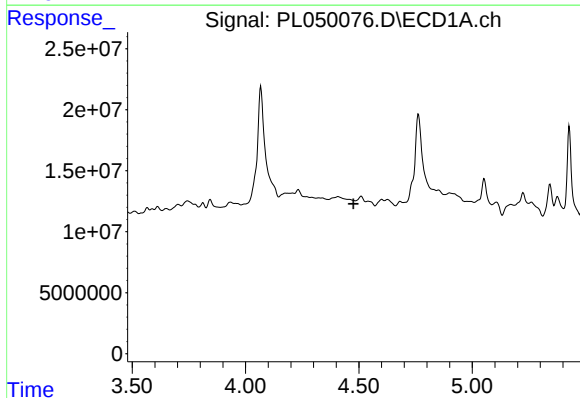


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.476 min
Response: 0
Conc: N.D.

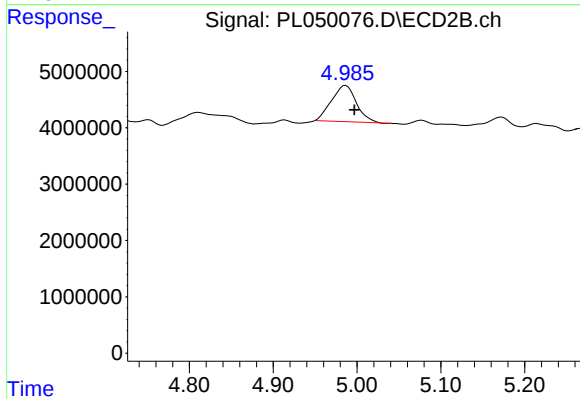

#7 delta-BHC


R.T.: 4.987 min
Delta R.T.: -0.010 min
Response: 13159306
Conc: 3.34 ng/ml

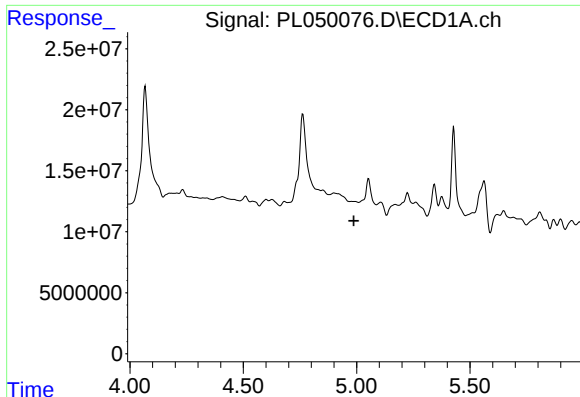

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.988 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

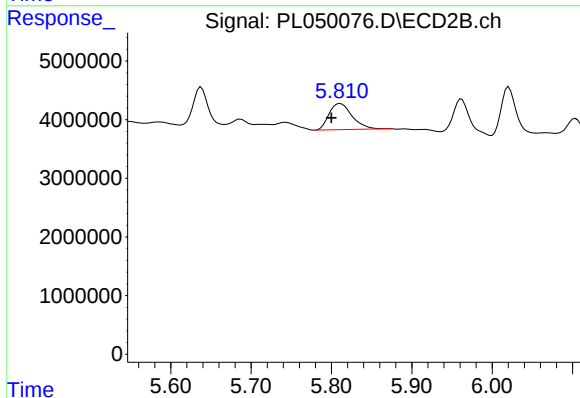


#8 Heptachlor epoxide

R.T.: 5.811 min
Delta R.T.: 0.011 min
Response: 8922400
Conc: 2.45 ng/ml

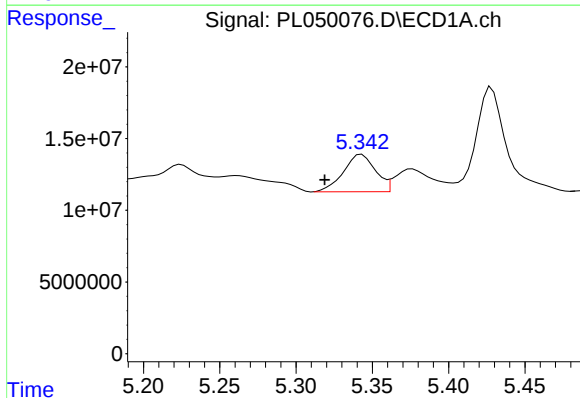


#9 Endosulfan I

R.T.: 5.343 min
Delta R.T.: 0.024 min
Response: 37941657
Conc: 2.45 ng/ml

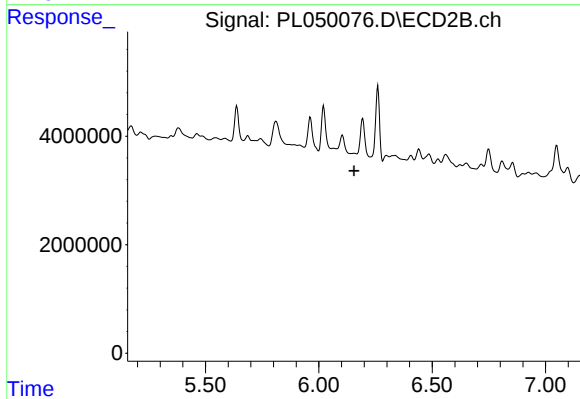

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

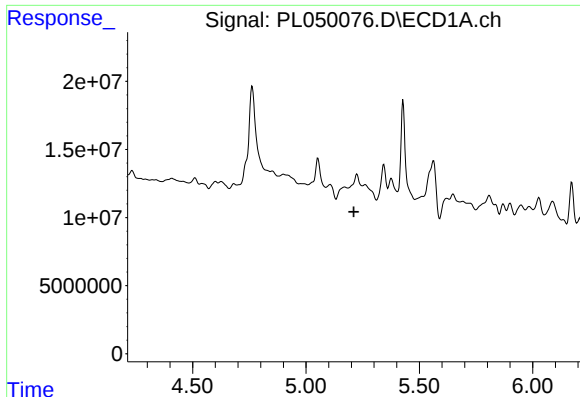

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

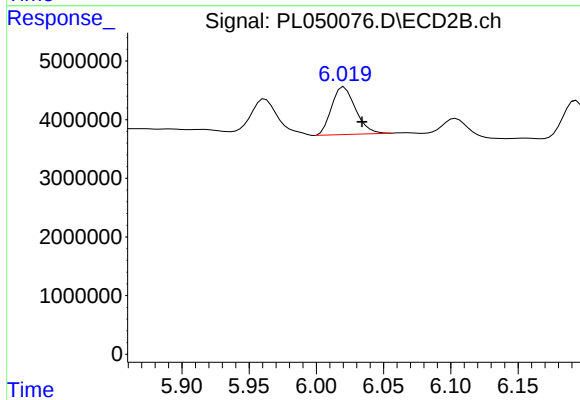


#10 gamma-Chlordane

R.T.: 6.021 min
Delta R.T.: -0.013 min
Response: 9999140
Conc: 2.68 ng/ml

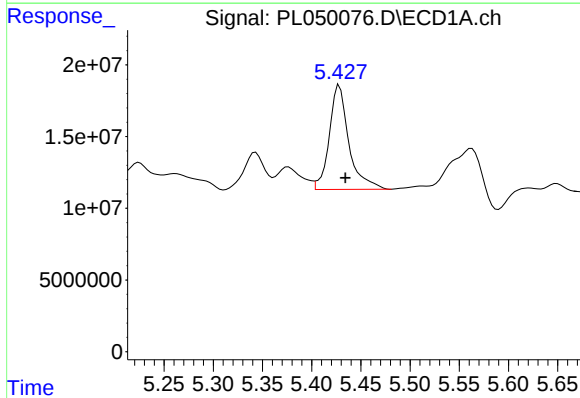


#12 4,4'-DDE

R.T.: 5.428 min
Delta R.T.: -0.006 min
Response: 101031016
Conc: 6.06 ng/ml

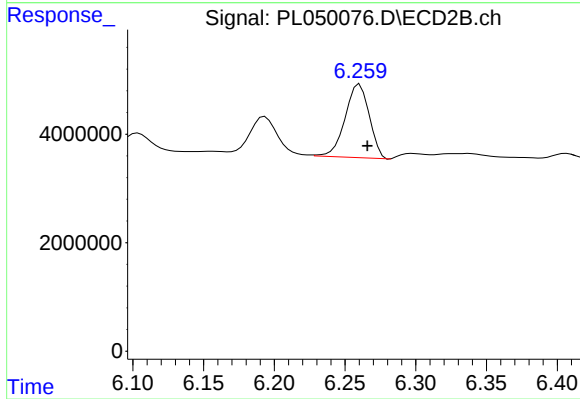

#12 4,4'-DDE


R.T.: 6.260 min
Delta R.T.: -0.005 min
Response: 16092218
Conc: 4.64 ng/ml

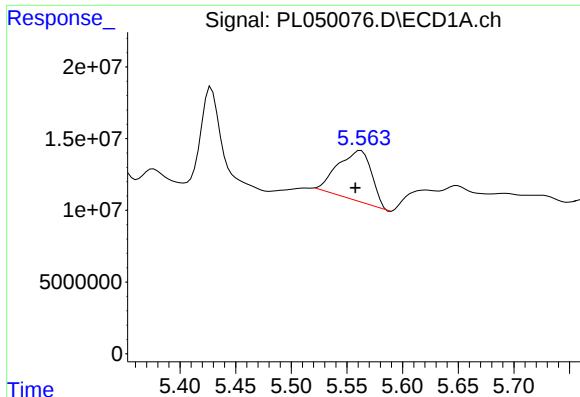

#13 Dieldrin


R.T.: 5.562 min
Delta R.T.: 0.005 min
Response: 73906250
Conc: 4.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

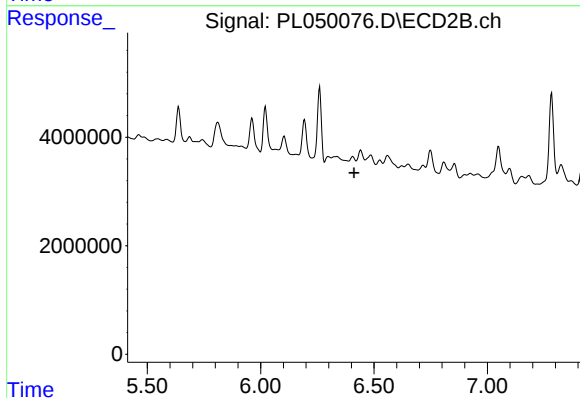


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.412 min
Response: 0
Conc: N.D.

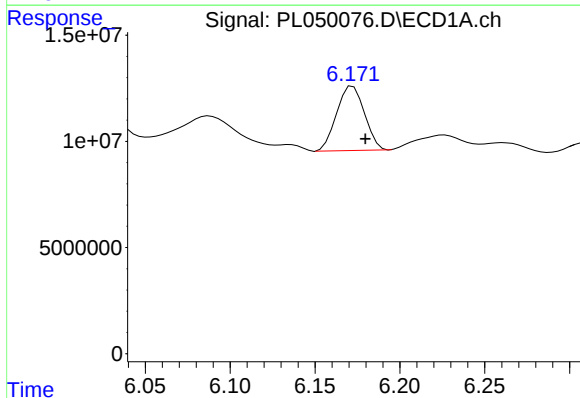


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: -0.007 min
Response: 34578441
Conc: 2.60 ng/ml

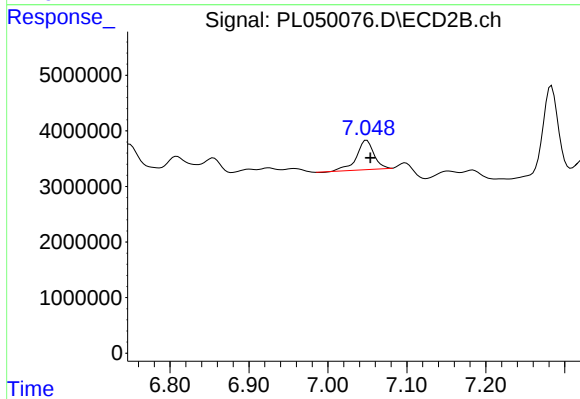

#17 4,4'-DDT


R.T.: 7.049 min
Delta R.T.: -0.005 min
Response: 8061892
Conc: 2.75 ng/ml

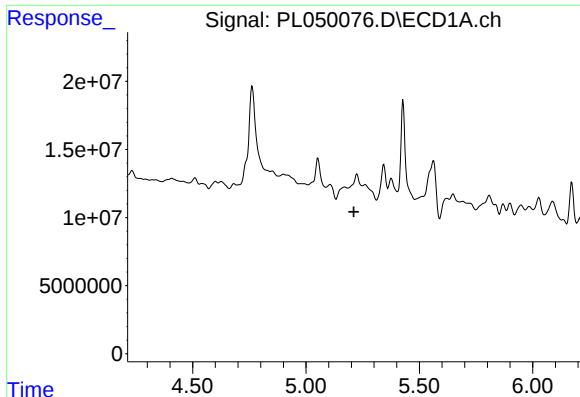

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419

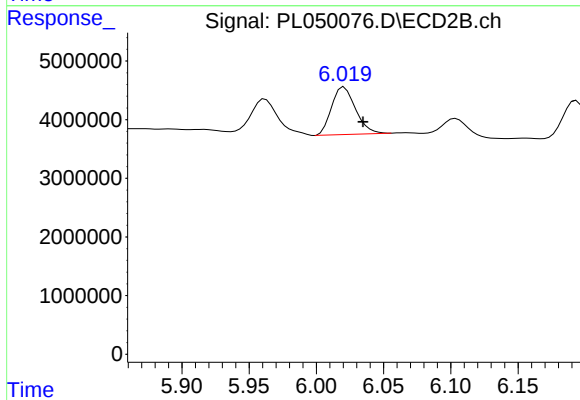


#25 Chlordane-3

R.T.: 6.021 min
Delta R.T.: -0.014 min
Response: 9999140
Conc: 20.09 ng/ml

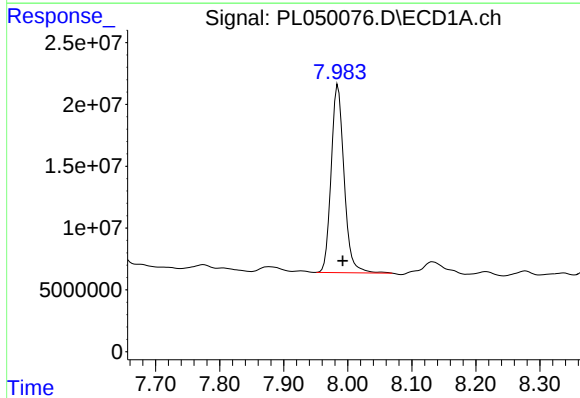

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 213262192
Conc: 16.78 ng/ml

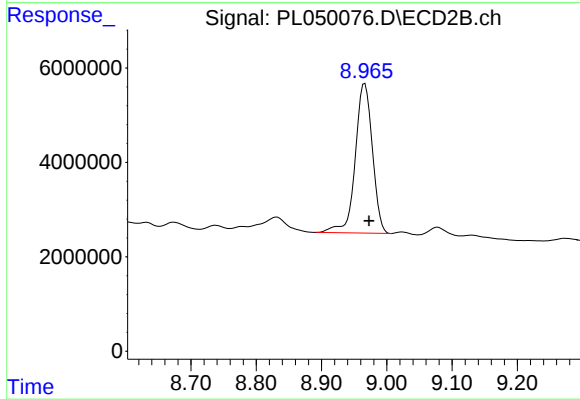

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 57852609
Conc: 17.23 ng/ml