

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 21:39
 Operator : SM\AJ
 Sample : K3592-03
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RBR-200052

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:31:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	204.0E6	52608705	18.088	17.183
28)	SA Decachlor...	7.985	8.966	193.3E6	55270602	15.210	16.464
Target Compounds							
2)	A alpha-BHC	0.000	4.345f	0	5399480	N.D.	1.206 #
7)	B delta-BHC	0.000	4.986	0	12416070	N.D.	3.152 #
9)	A Endosulfan I	5.342f	0.000	63597673	0	4.110	N.D. #
10)	B gamma-Chl...	0.000	6.022	0	8792819	N.D.	2.360 #
11)	B alpha-Chl...	5.264	0.000	61370060	0	3.697	N.D. #
23)	Chlordane-1	0.000	4.894f	0	9621357	N.D.	65.467 #
25)	Chlordane-3	0.000	6.022	0	8792819	N.D.	17.670 #
26)	Chlordane-4	5.264	0.000	61370060	0	35.166	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 21:39
Operator : SM\AJ
Sample : K3592-03
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RBR-200052

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:31:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

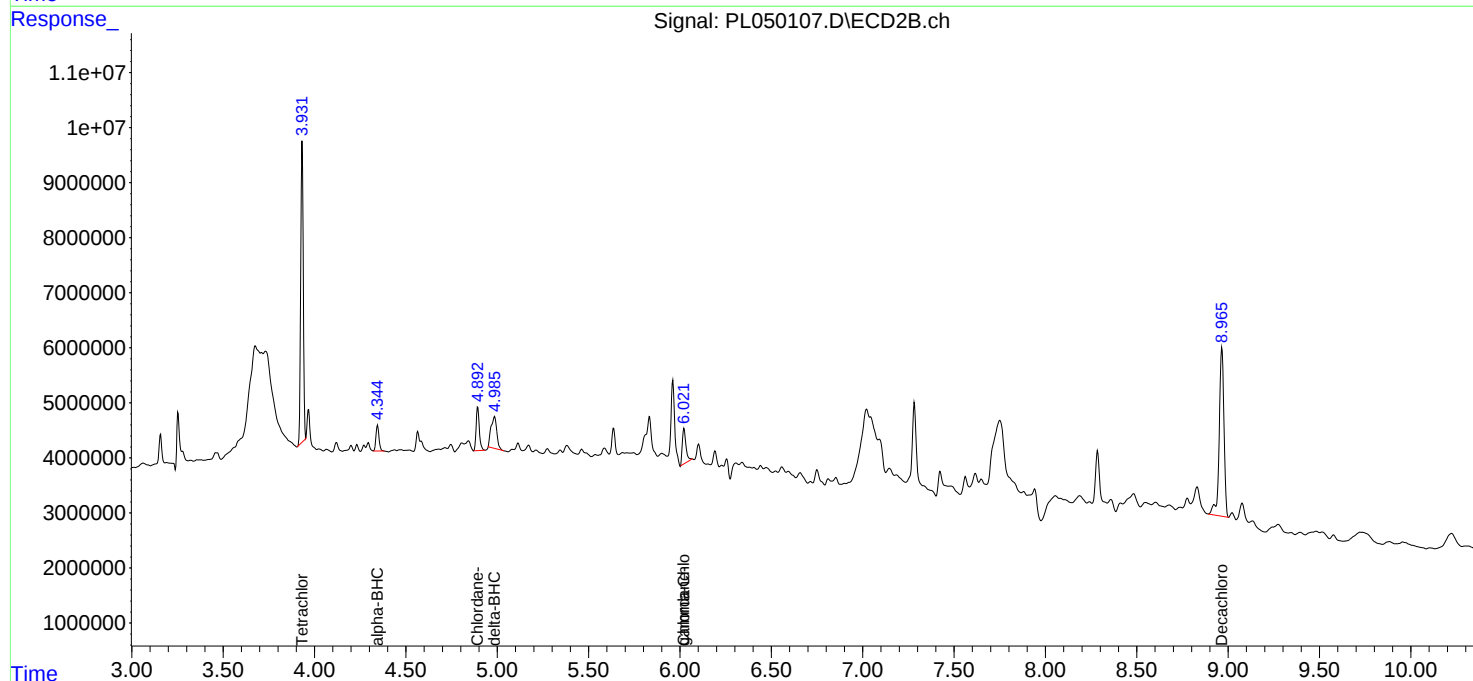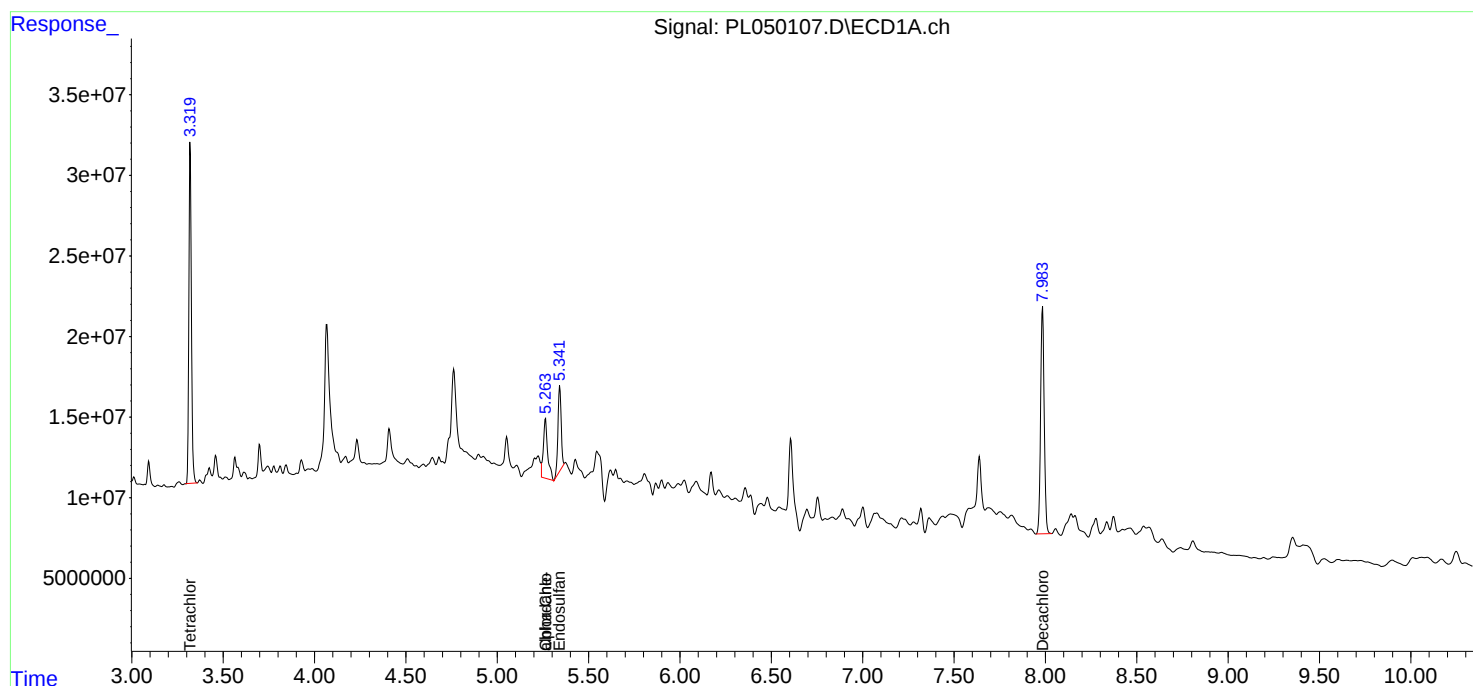


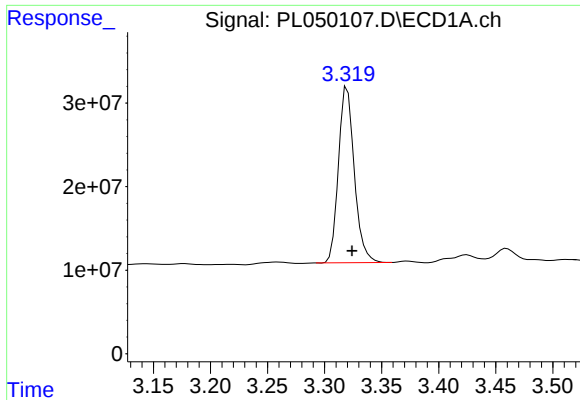

#1 Tetrachloro-m-xylene


R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 203991986
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

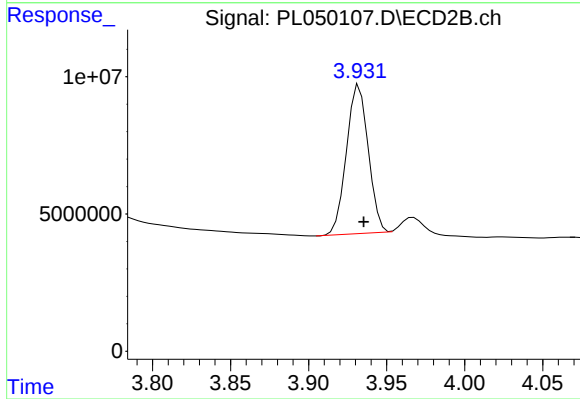


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.003 min
Response: 52608705
Conc: 17.18 ng/ml

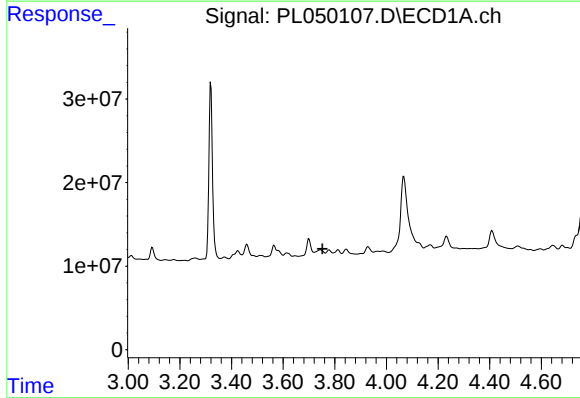


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.752 min
Response: 0
Conc: N.D.

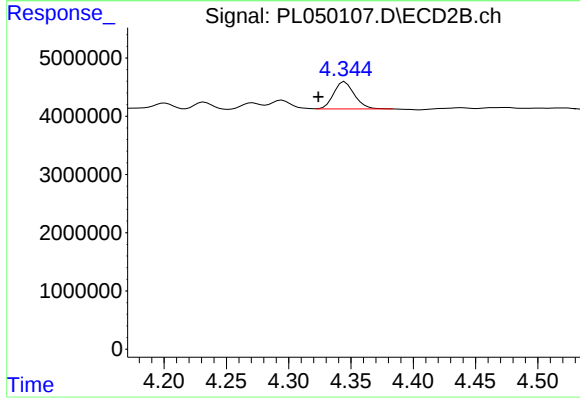

#2 alpha-BHC


R.T.: 4.345 min
Delta R.T.: 0.021 min
Response: 5399480
Conc: 1.21 ng/ml

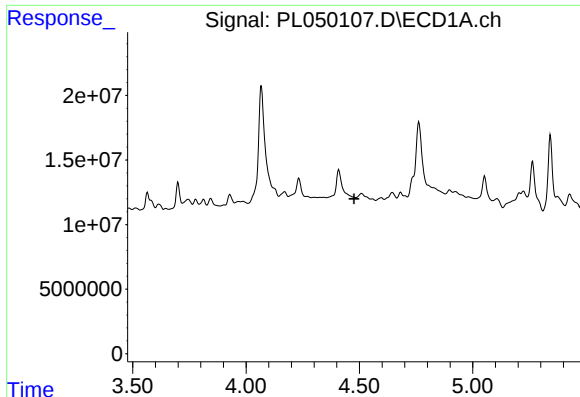

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RBR-200052

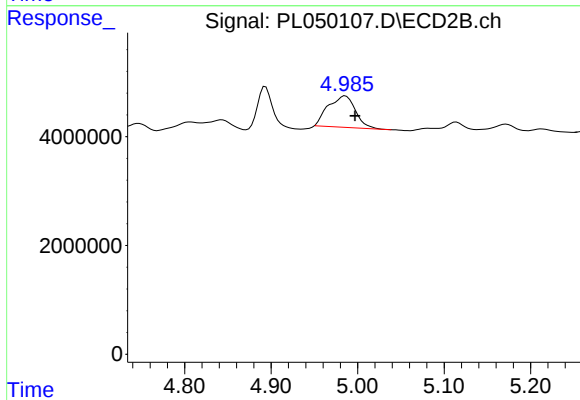


#7 delta-BHC

R.T.: 4.986 min
Delta R.T.: -0.011 min
Response: 12416070
Conc: 3.15 ng/ml

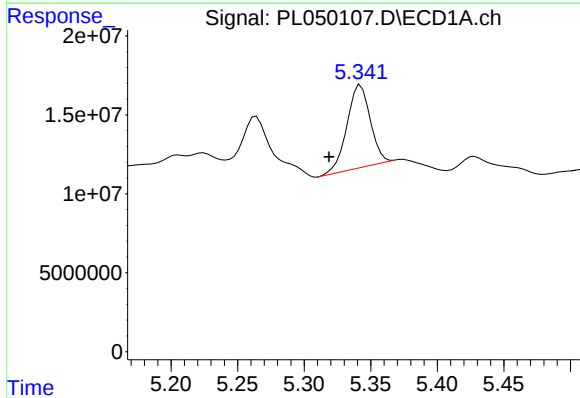


#9 Endosulfan I

R.T.: 5.342 min
Delta R.T.: 0.024 min
Response: 63597673
Conc: 4.11 ng/ml

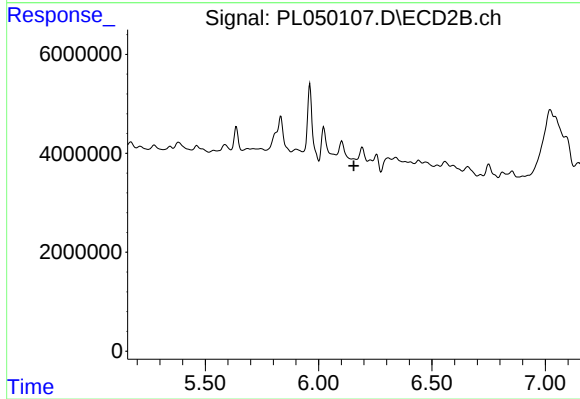

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

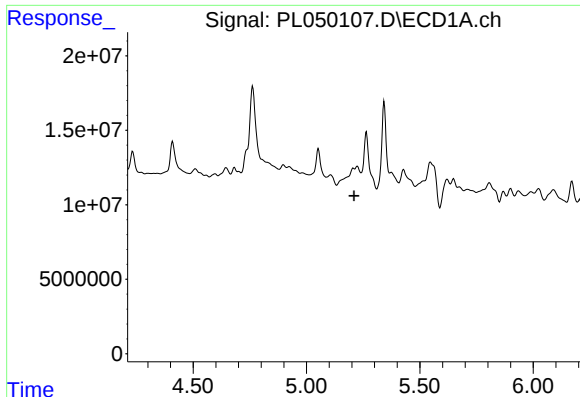

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RBR-200052

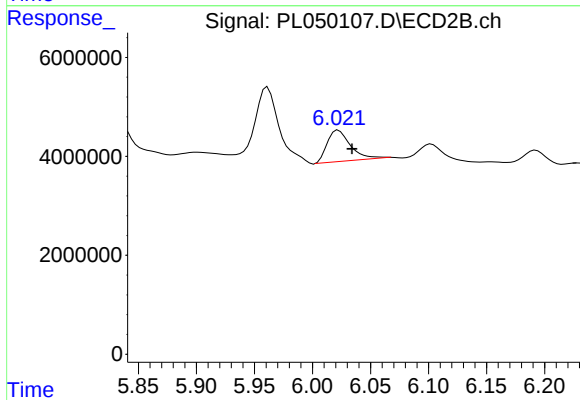


#10 gamma-Chlordane

R.T.: 6.022 min
Delta R.T.: -0.012 min
Response: 8792819
Conc: 2.36 ng/ml

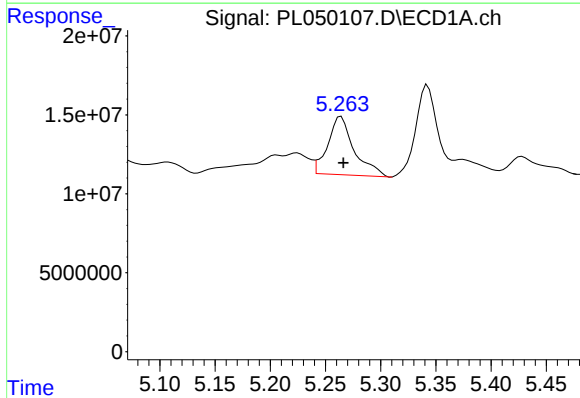


#11 alpha-Chlordane

R.T.: 5.264 min
Delta R.T.: -0.002 min
Response: 61370060
Conc: 3.70 ng/ml

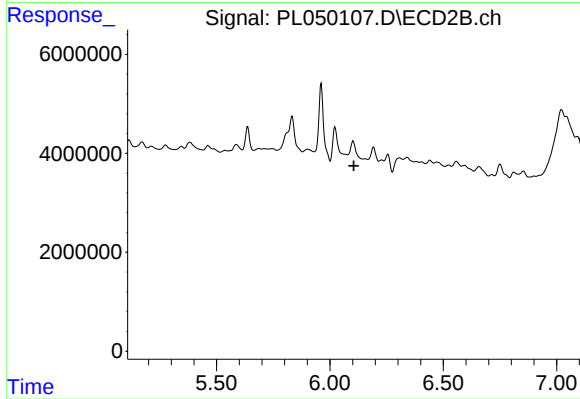

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.105 min
Response: 0
Conc: N.D.

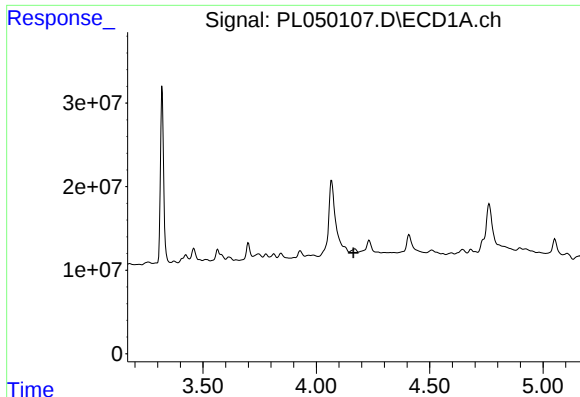

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.164 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RBR-200052

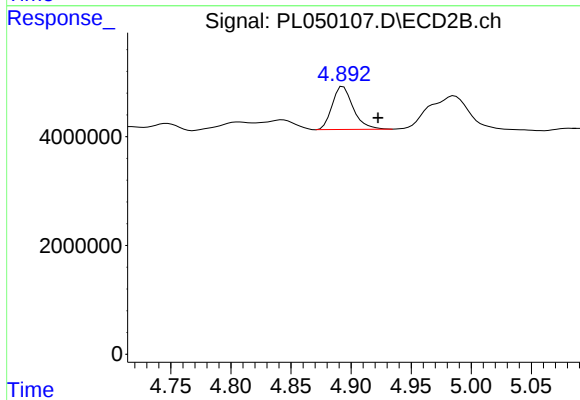


#23 Chlordane-1

R.T.: 4.894 min
Delta R.T.: -0.029 min
Response: 9621357
Conc: 65.47 ng/ml

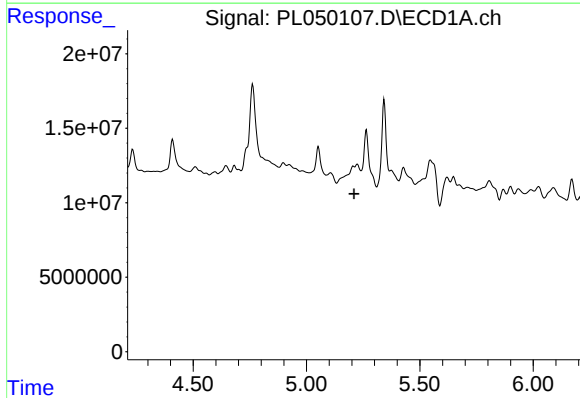


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.211 min
Response: 0
Conc: N.D.

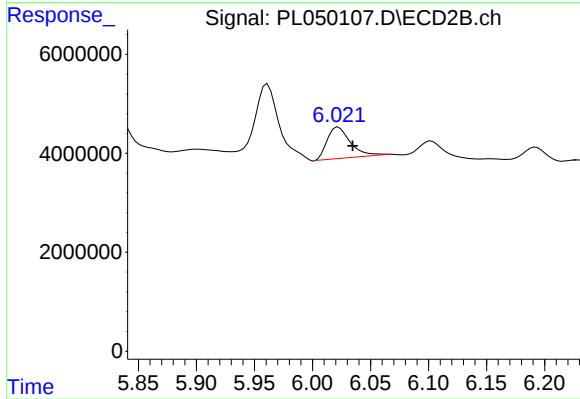

#25 Chlordane-3


R.T.: 6.022 min
Delta R.T.: -0.012 min
Response: 8792819
Conc: 17.67 ng/ml

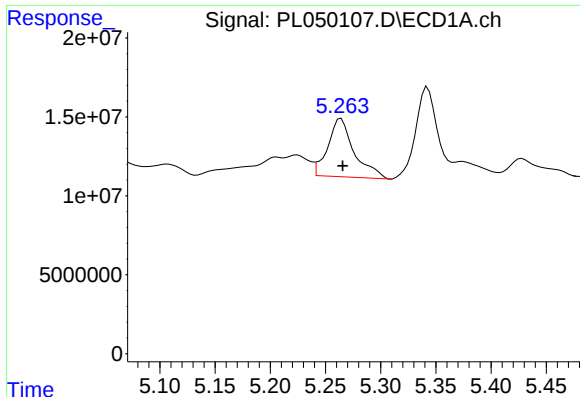

#26 Chlordane-4


R.T.: 5.264 min
Delta R.T.: -0.002 min
Response: 61370060
Conc: 35.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

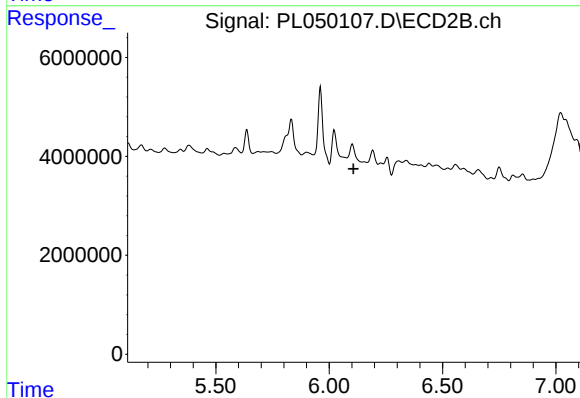


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.107 min
Response: 0
Conc: N.D.

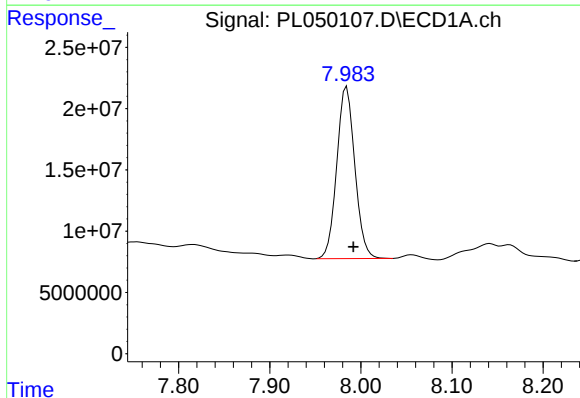

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.008 min
Response: 193260036
Conc: 15.21 ng/ml

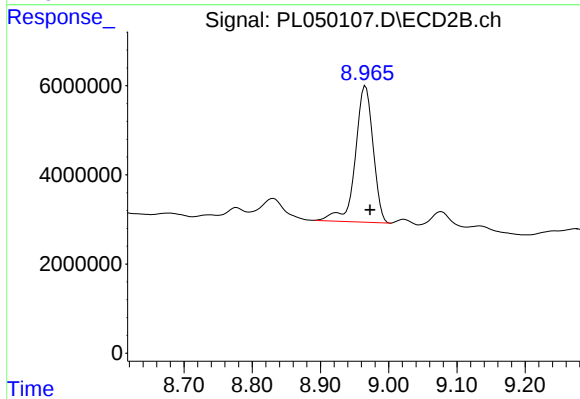

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 55270602
Conc: 16.46 ng/ml