

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 10:08
 Operator : SM\AJ
 Sample : K3589-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FM1180

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:11:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:23:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	3.933	202.4E6	47260942	17.949	15.436
28) SA Decachlor...	7.986	8.966	180.8E6	46443571	14.227	13.835
Target Compounds						
13) MA Dieldrin	5.554	6.406	163.0E6	35016759	9.785	9.871m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 10:08
Operator : SM\AJ
Sample : K3589-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FM1180


Manual Integrations
APPROVED

Ankita
7/2/2019 1:11:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:23:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

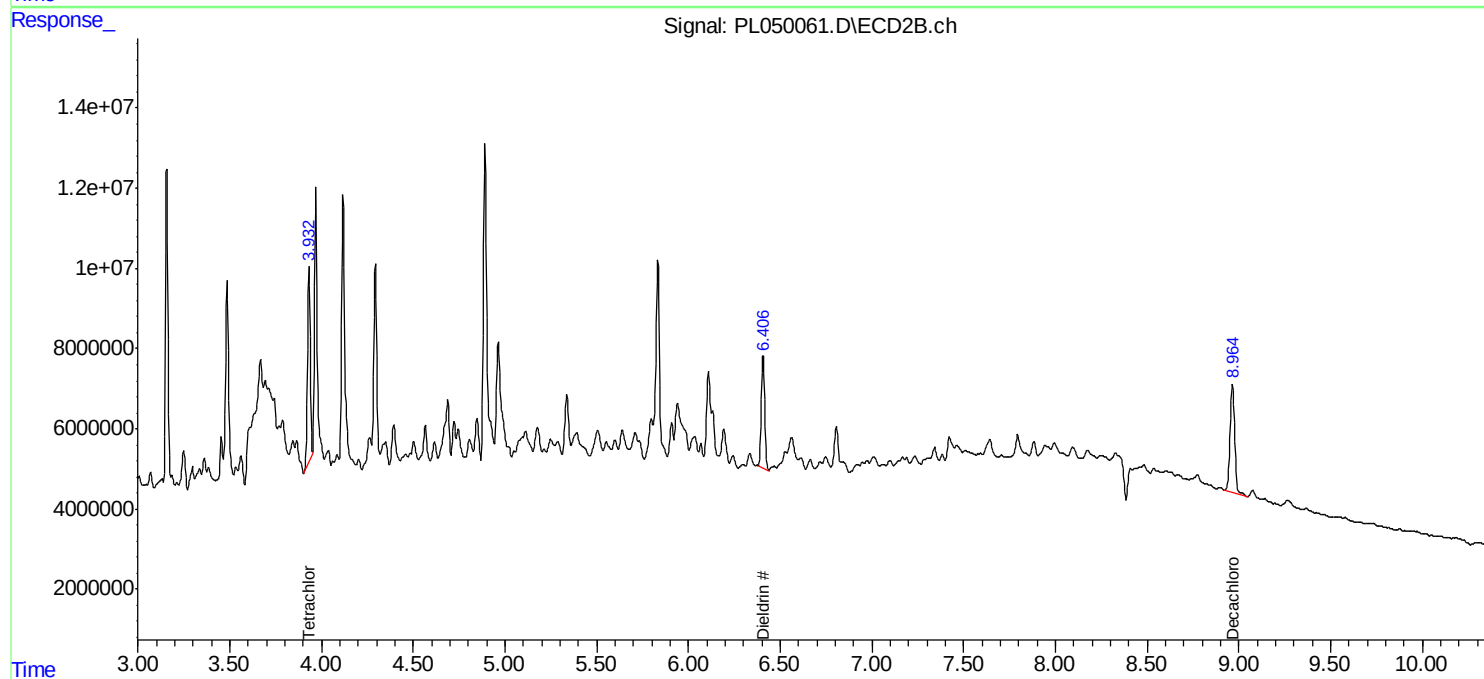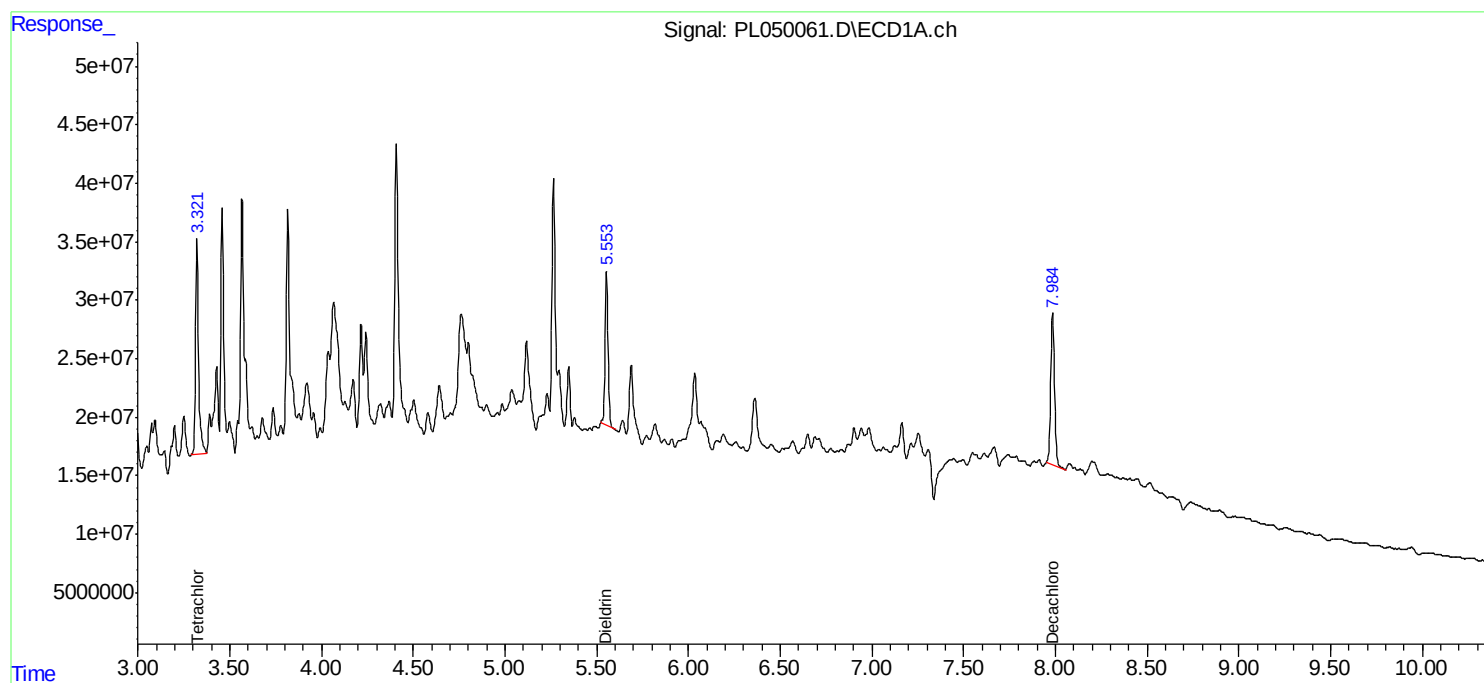

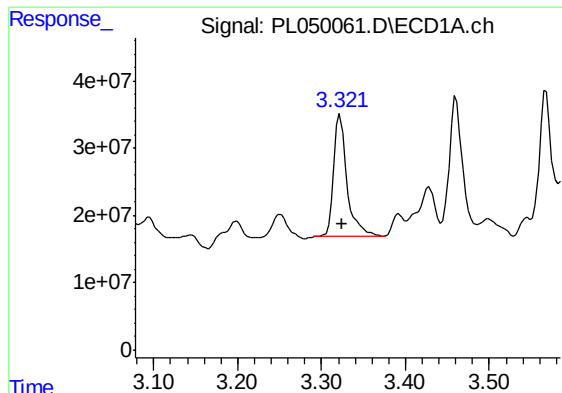


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: -0.001 min
Response: 202419379
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
FM1180


Manual Integrations
APPROVED

Ankita
7/2/2019 1:11:27 PM

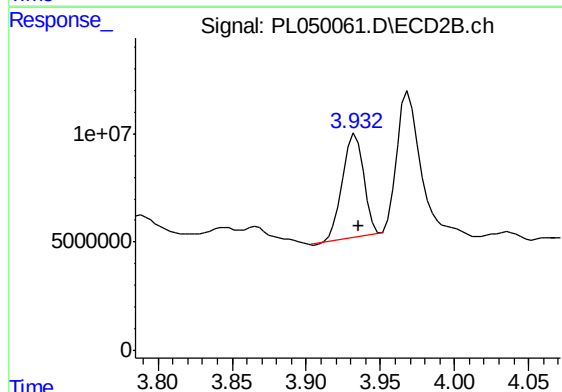


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 47260942
Conc: 15.44 ng/ml

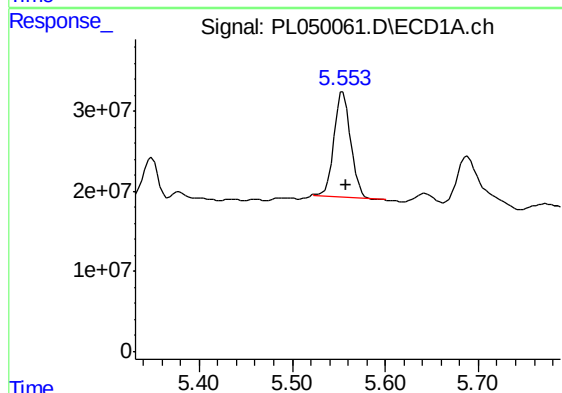


#13 Dieldrin

R.T.: 5.554 min
Delta R.T.: -0.003 min
Response: 162994627
Conc: 9.78 ng/ml

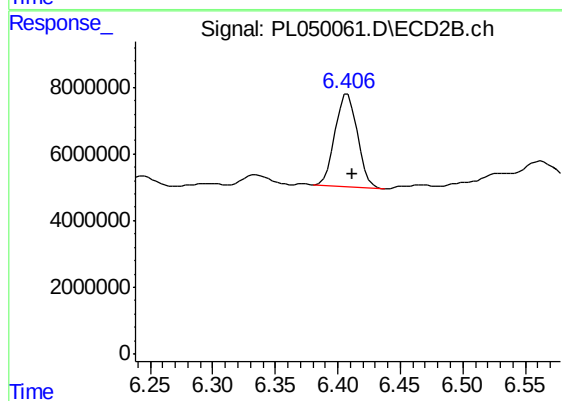

#13 Dieldrin

R.T.: 6.406 min
Delta R.T.: -0.006 min
Response: 35016759
Conc: 9.87 ng/ml m

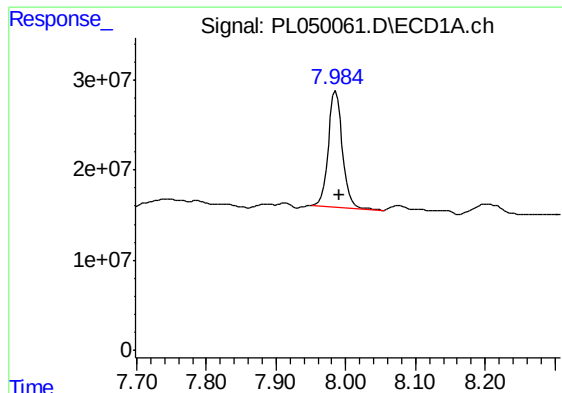


#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 180778726
Conc: 14.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
FM1180

Manual Integrations
APPROVED

Ankita
7/2/2019 1:11:27 PM

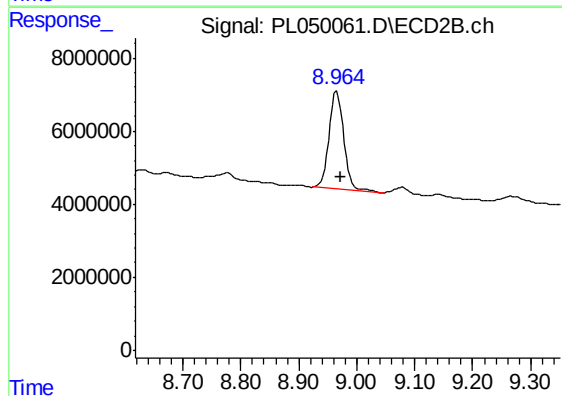

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 46443571
Conc: 13.83 ng/ml