

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 10:38
 Operator : SM\AJ
 Sample : K3558-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-032-SW173-062519

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:13:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:24:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.322	3.933	149.5E6	38571530	13.252	12.598
28)	SA Decachlor...	7.987	8.966	153.3E6	35949465	12.063	10.709
Target Compounds							
12)	B 4,4'-DDE	5.429	6.259	90085548	18099065	5.408m	5.216
17)	MA 4,4'-DDT	6.175	7.047	47512563	11738309	3.579	4.008m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 10:38
Operator : SM\AJ
Sample : K3558-09
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-032-SW173-062519


Manual Integrations
APPROVED

Ankita
7/2/2019 1:13:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:24:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

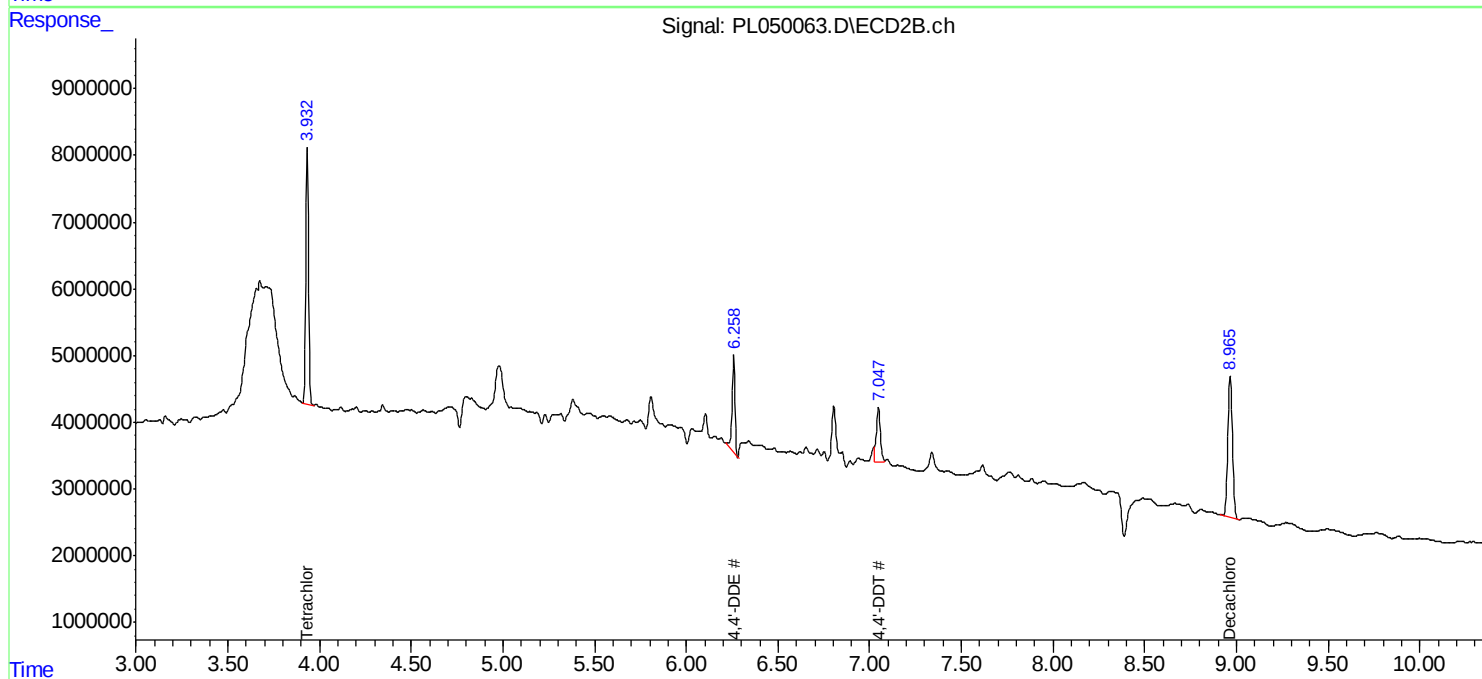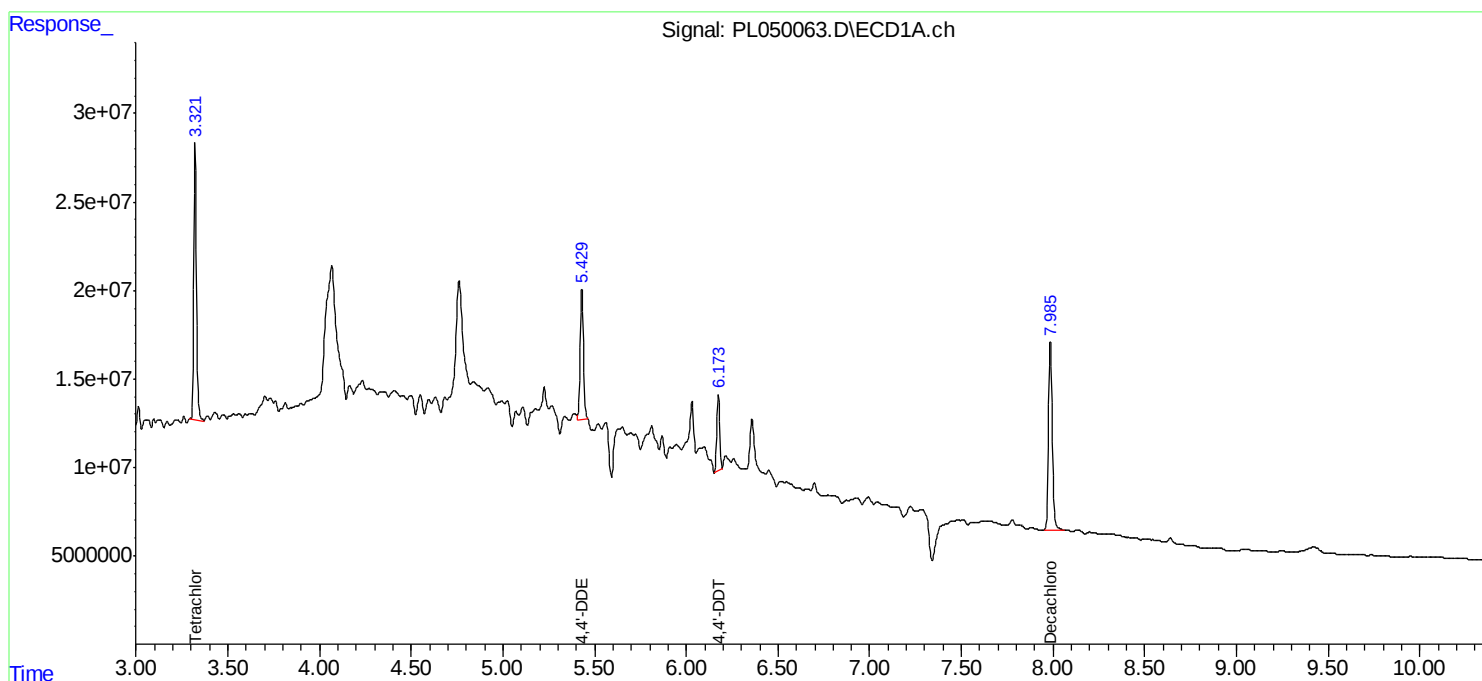

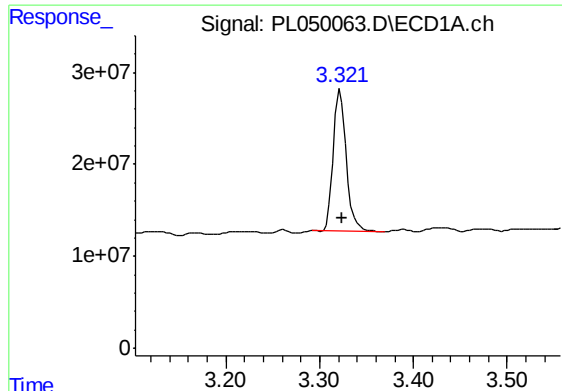


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 149453001
Conc: 13.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-032-SW173-062519


Manual Integrations
APPROVED

Ankita
7/2/2019 1:13:55 PM

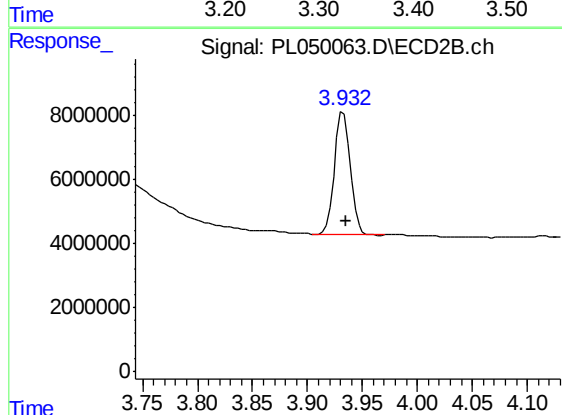


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 38571530
Conc: 12.60 ng/ml

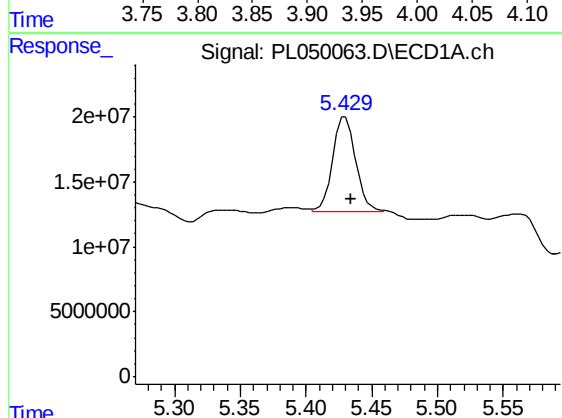


#12 4,4'-DDE

R.T.: 5.429 min
Delta R.T.: -0.006 min
Response: 90085548
Conc: 5.41 ng/ml m

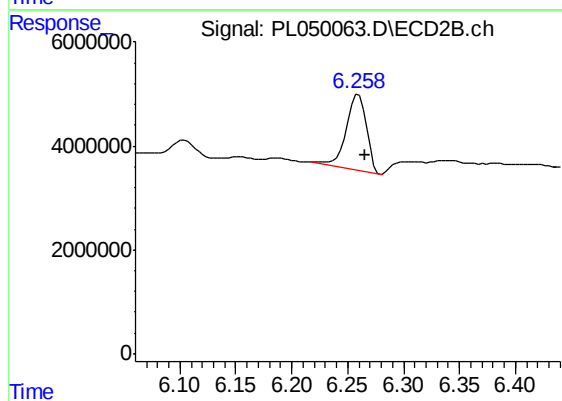

#12 4,4'-DDE

R.T.: 6.259 min
Delta R.T.: -0.006 min
Response: 18099065
Conc: 5.22 ng/ml

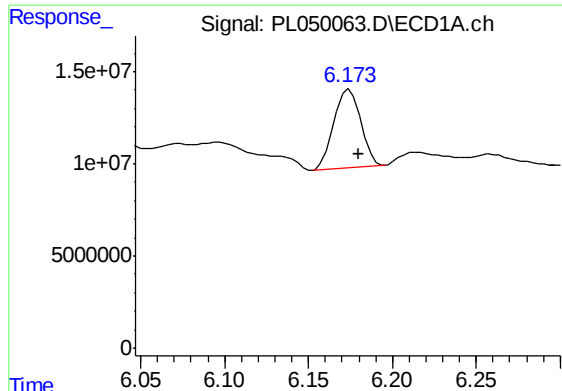


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: -0.005 min
Response: 47512563
Conc: 3.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-032-SW173-062519


Manual Integrations
APPROVED

Ankita
7/2/2019 1:13:55 PM

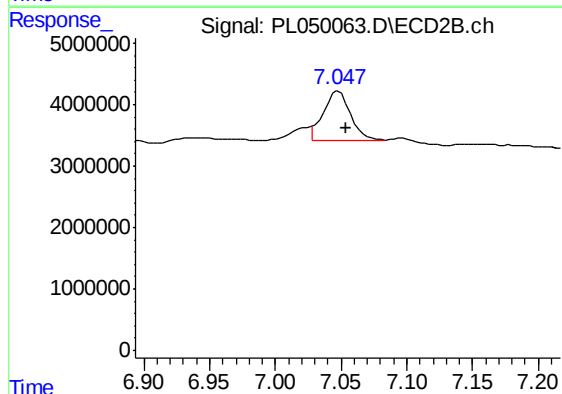


#17 4,4'-DDT

R.T.: 7.047 min
Delta R.T.: -0.007 min
Response: 11738309
Conc: 4.01 ng/ml m

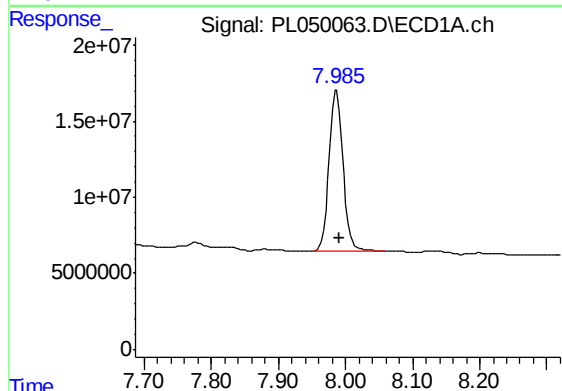

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: -0.006 min
Response: 153283177
Conc: 12.06 ng/ml

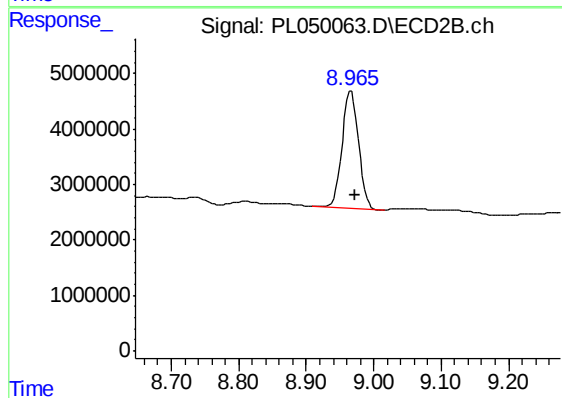

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 35949465
Conc: 10.71 ng/ml