

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 13:05
 Operator : SM\AJ
 Sample : K3560-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-009-SW147-062419

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:09:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:25:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	230.0E6	53371000	20.394	17.431
28)	SA Decachlor...	7.985	8.966	202.2E6	52725441	15.911	15.706
Target Compounds							
13)	MA Dieldrin	5.552	6.406	49709968	5401473	2.984	1.523m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 13:05
Operator : SM\AJ
Sample : K3560-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-009-SW147-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:09:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:25:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

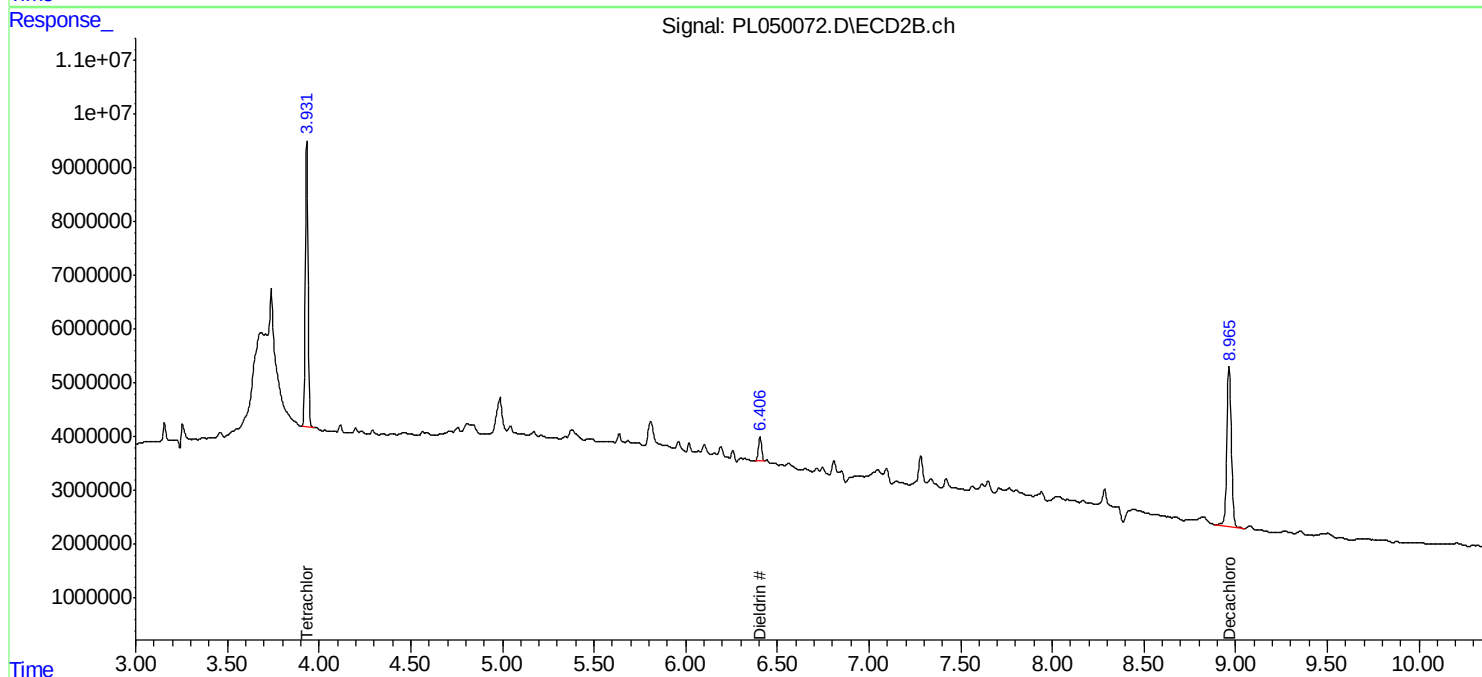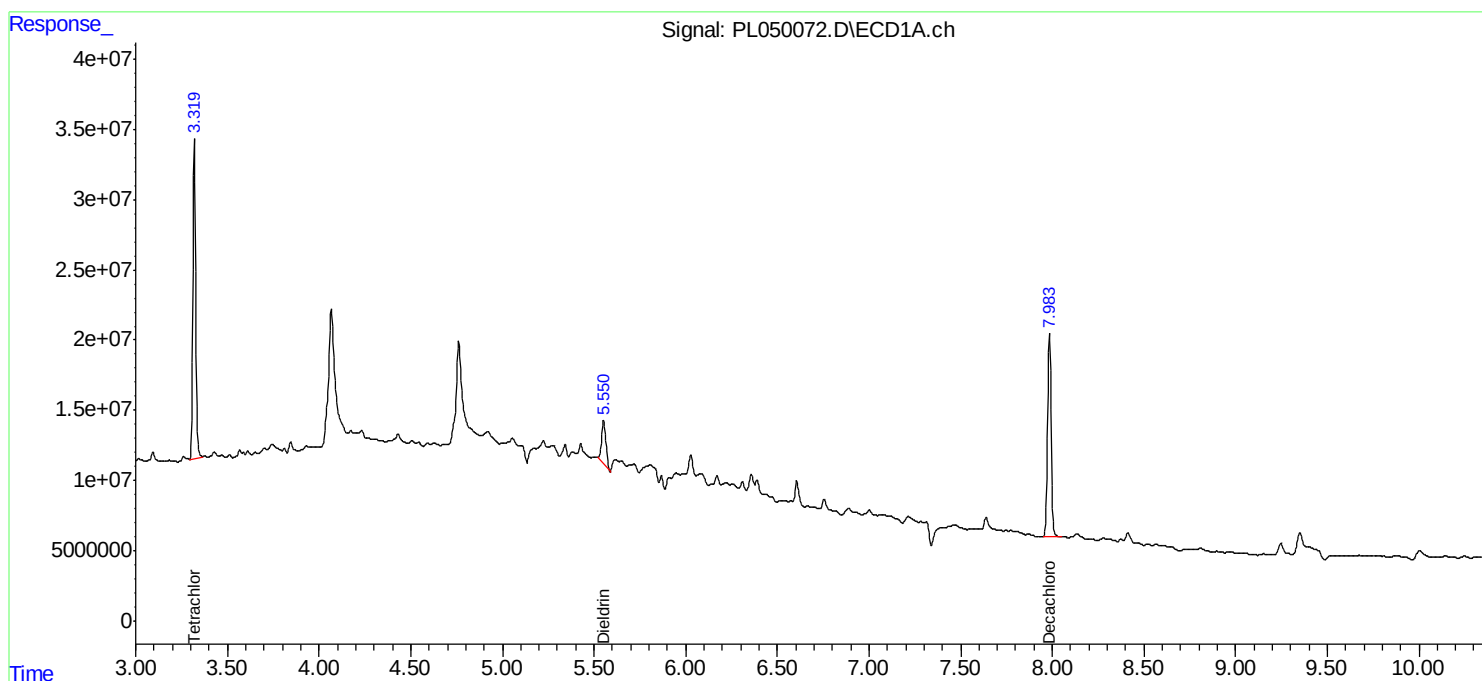

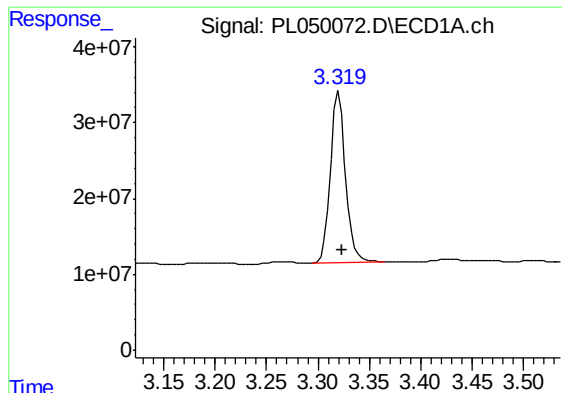


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 229991642
Conc: 20.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW147-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:09:56 PM

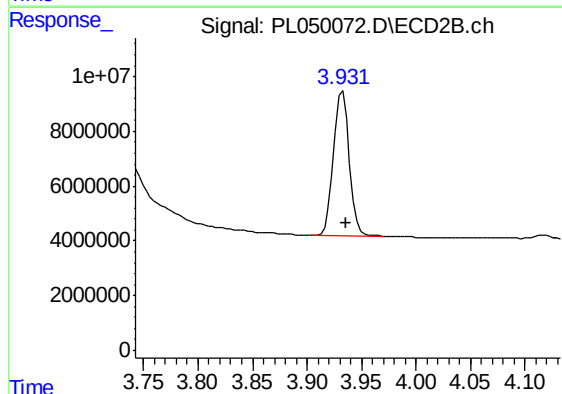


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 53371000
Conc: 17.43 ng/ml

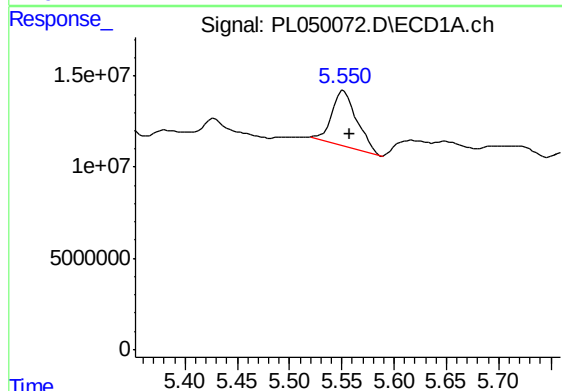


#13 Dieldrin

R.T.: 5.552 min
Delta R.T.: -0.006 min
Response: 49709968
Conc: 2.98 ng/ml

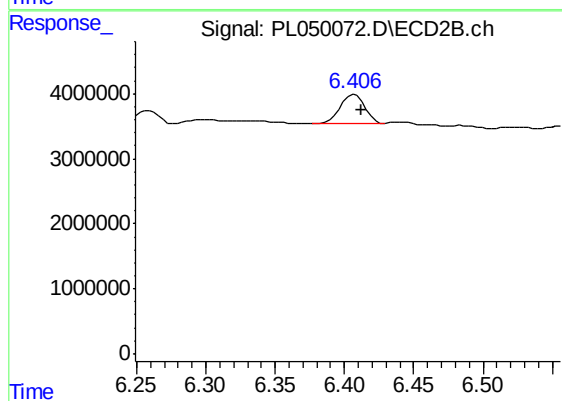

#13 Dieldrin

R.T.: 6.406 min
Delta R.T.: -0.006 min
Response: 5401473
Conc: 1.52 ng/ml m

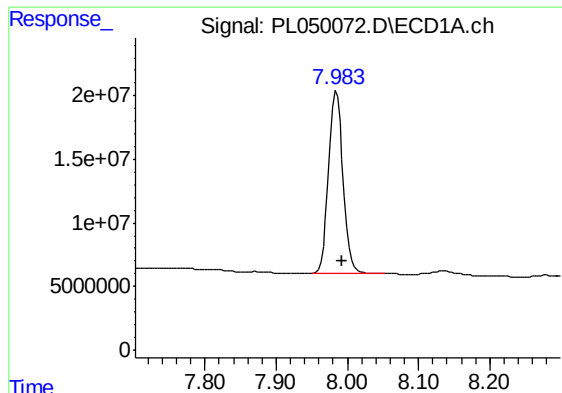


#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 202175284
Conc: 15.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW147-062419

Manual Integrations
APPROVED

Ankita
7/2/2019 1:09:56 PM

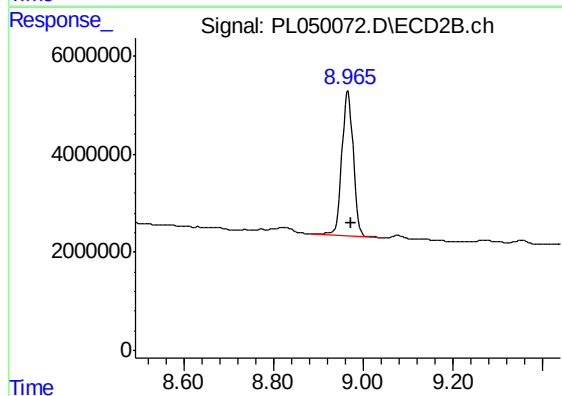

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 52725441
Conc: 15.71 ng/ml