

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 13:49
 Operator : SM\AJ
 Sample : K3560-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-009-SW143-062419

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:12:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:26:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	163.6E6	43234612	14.509	14.121
28)	SA Decachlor...	7.986	8.966	167.1E6	42970944	13.152	12.800
Target Compounds							
12)	B 4,4'-DDE	5.426	6.259	22746435	4589469	1.365m	1.323m
17)	MA 4,4'-DDT	6.172	7.047	13218017	4068538	0.996m	1.389m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 13:49
Operator : SM\AJ
Sample : K3560-06
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-009-SW143-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:12:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:26:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

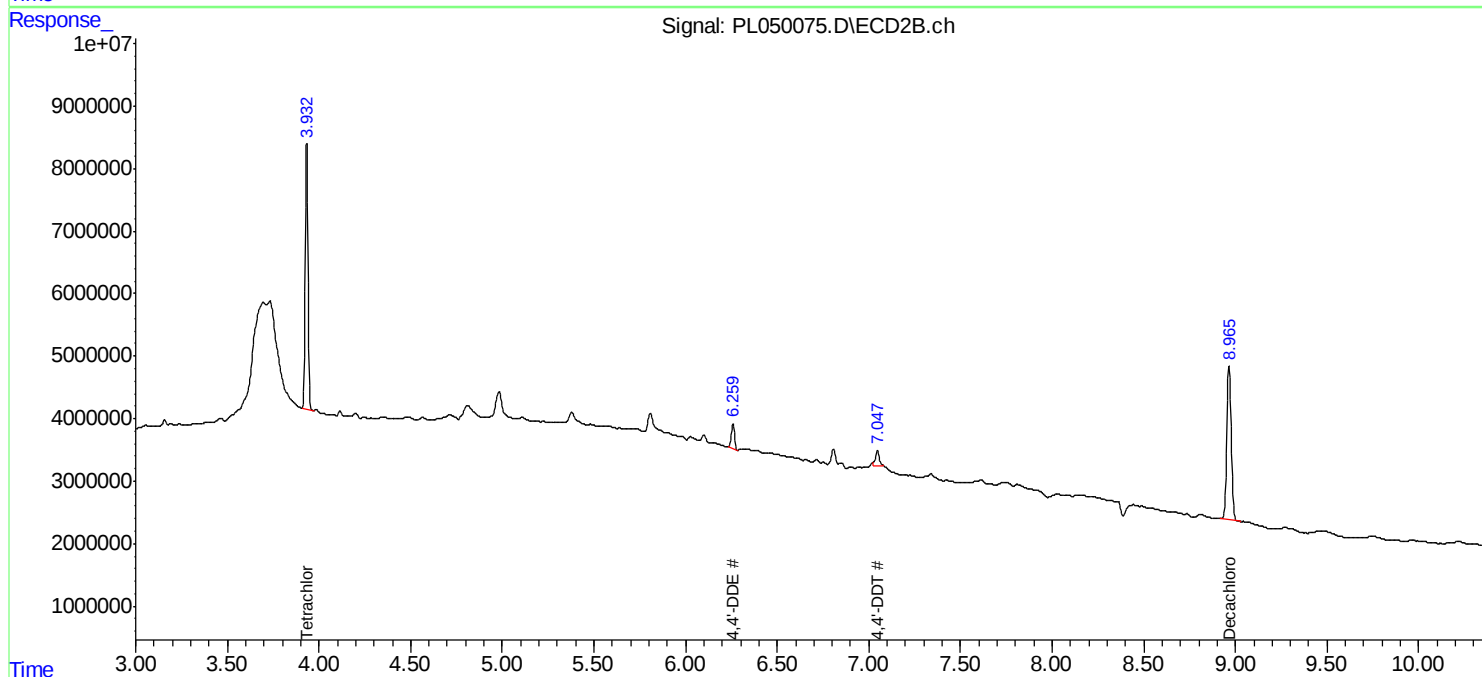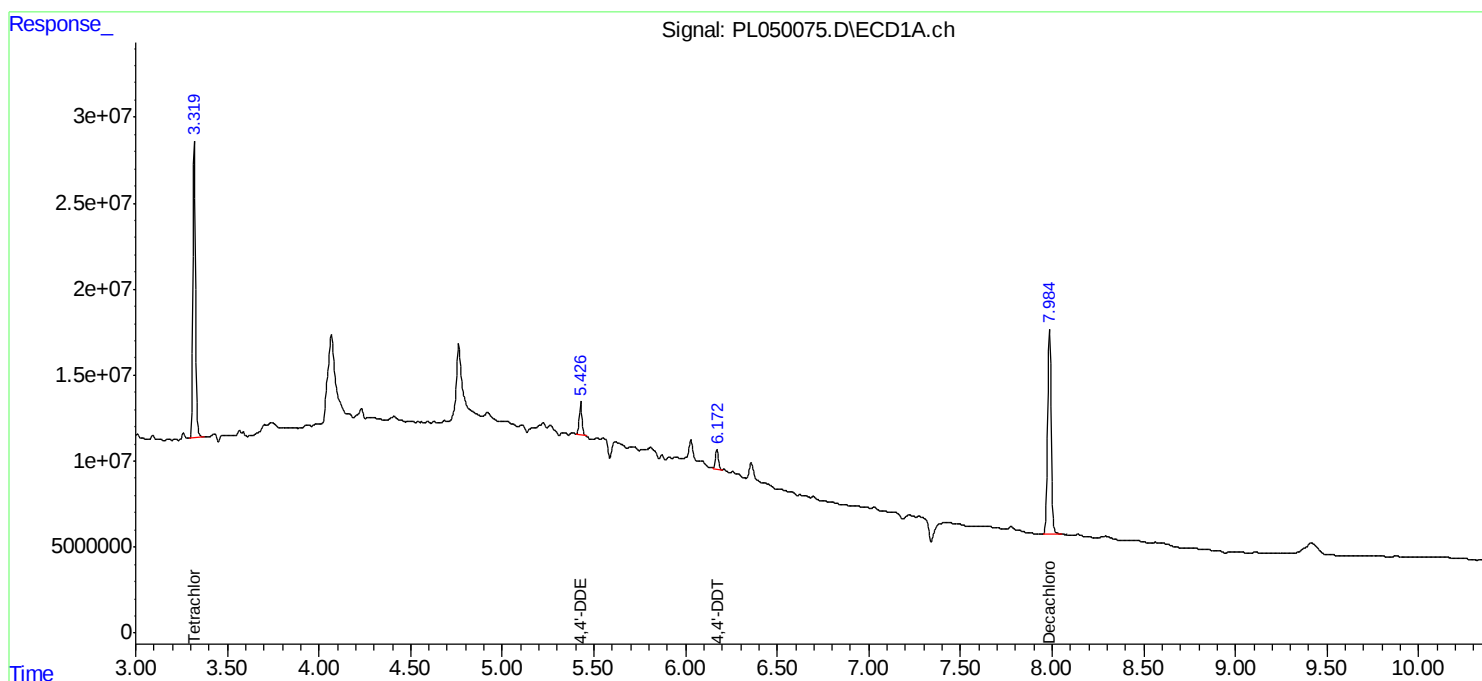

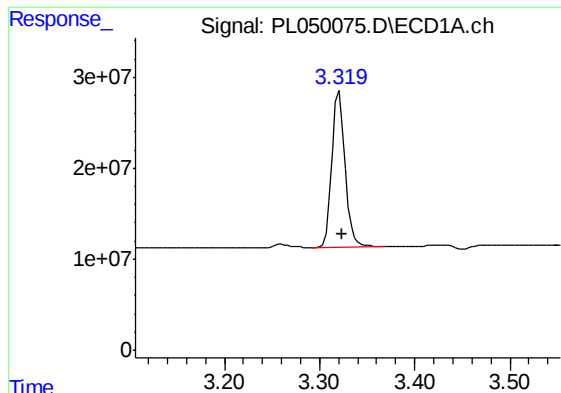


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 163627607
Conc: 14.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW143-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:12:16 PM

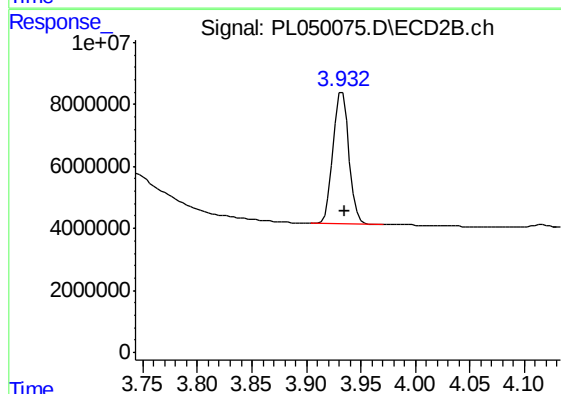


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 43234612
Conc: 14.12 ng/ml

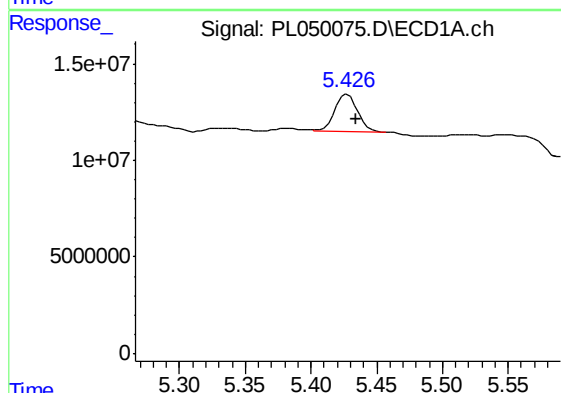


#12 4,4'-DDE

R.T.: 5.426 min
Delta R.T.: -0.008 min
Response: 22746435
Conc: 1.37 ng/ml m

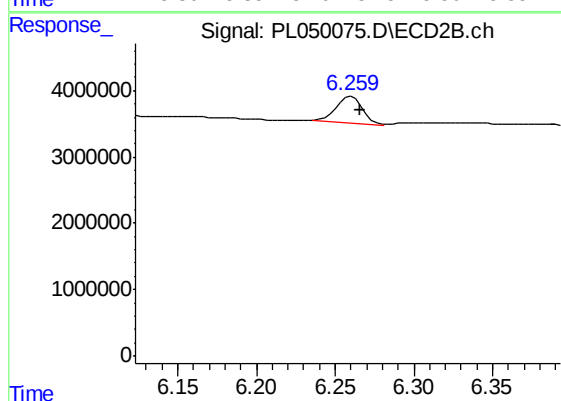

#12 4,4'-DDE

R.T.: 6.259 min
Delta R.T.: -0.007 min
Response: 4589469
Conc: 1.32 ng/ml m

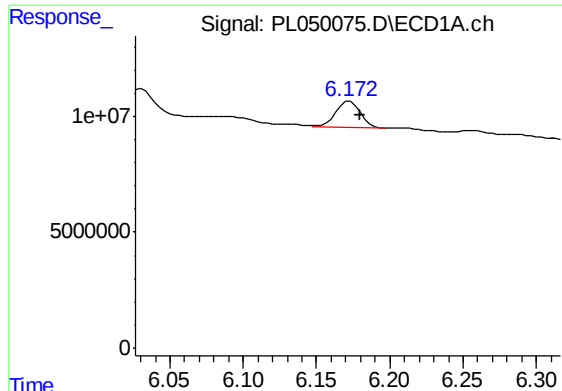


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: -0.008 min
Response: 13218017
Conc: 1.00 ng/ml m

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW143-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:12:16 PM

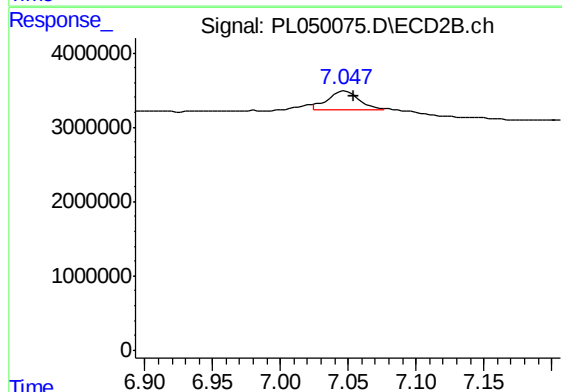


#17 4,4'-DDT

R.T.: 7.047 min
Delta R.T.: -0.007 min
Response: 4068538
Conc: 1.39 ng/ml m

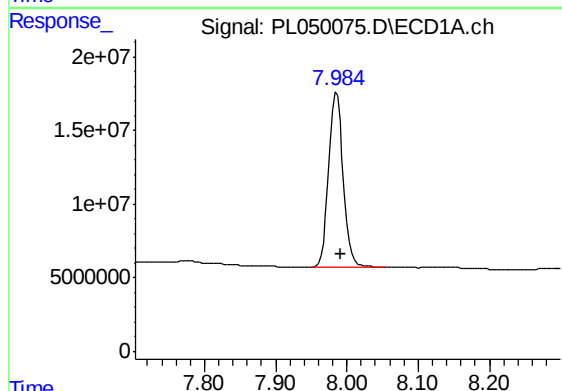

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.007 min
Response: 167109783
Conc: 13.15 ng/ml

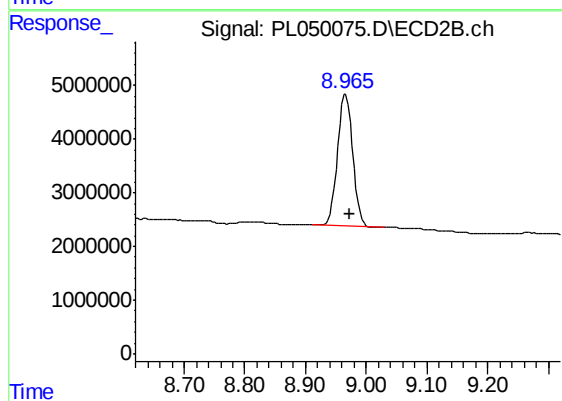

#28 Decachlorobiphenyl

R.T.: 8.966 min
Delta R.T.: -0.007 min
Response: 42970944
Conc: 12.80 ng/ml