

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 14:03
 Operator : SM\AJ
 Sample : K3560-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-009-SW137-062419

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:10:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:26:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.320	3.933	238.7E6	54653721	21.165	17.850
28)	SA Decachlor...	7.985	8.965	213.3E6	56136938	16.784	16.722m
Target Compounds							
12)	B 4,4'-DDE	5.428	6.260	101.0E6	16092218	6.065	4.637
17)	MA 4,4'-DDT	6.172	7.048	34578441	8376454	2.605	2.860m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 14:03
Operator : SM\AJ
Sample : K3560-07
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:26:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

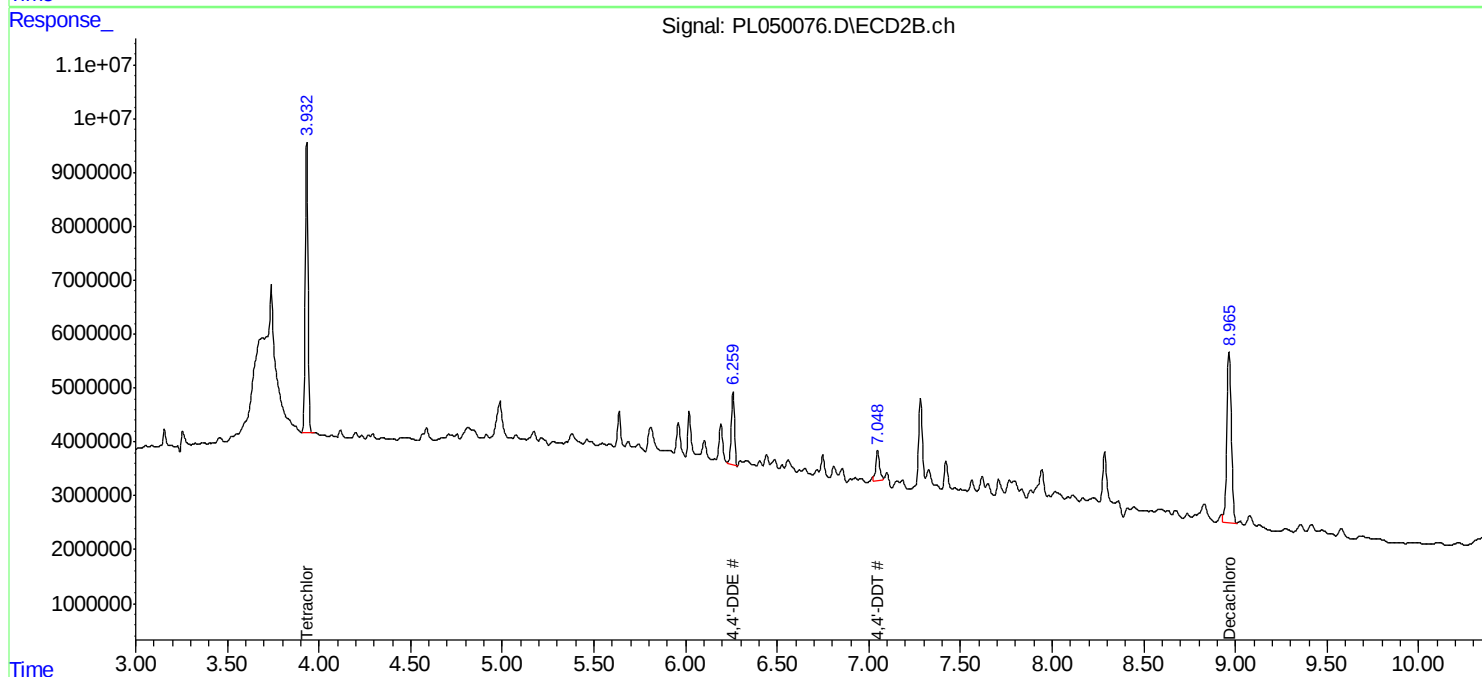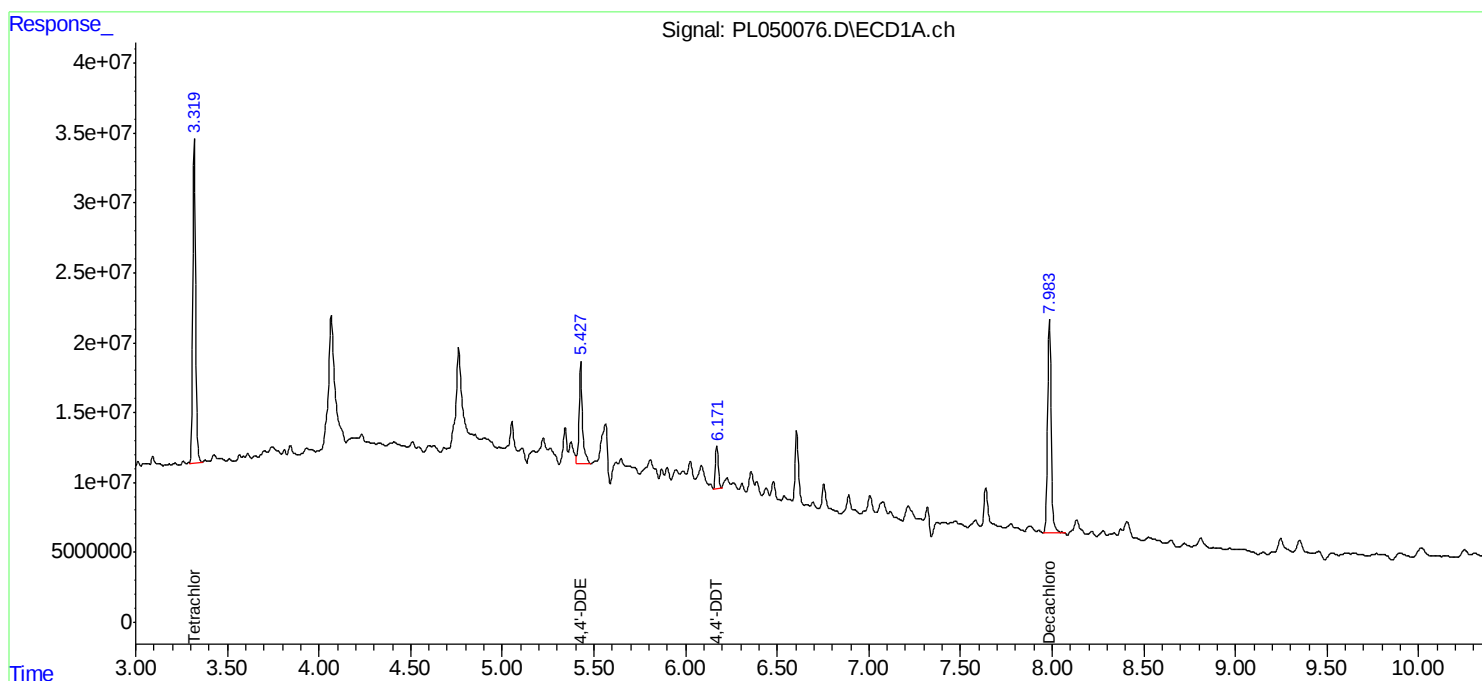

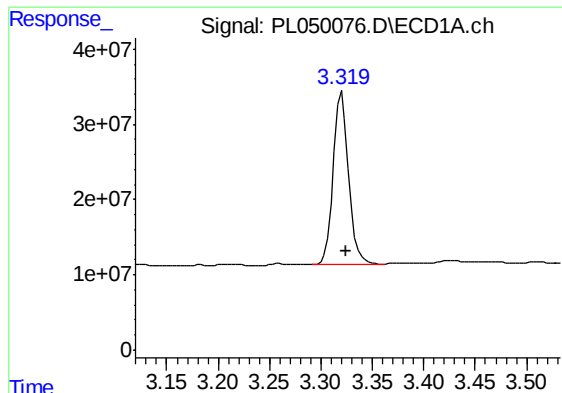


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.004 min
Response: 238688256
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:02 PM

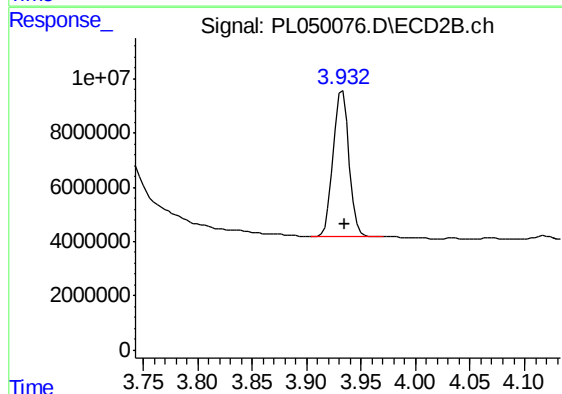


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 54653721
Conc: 17.85 ng/ml

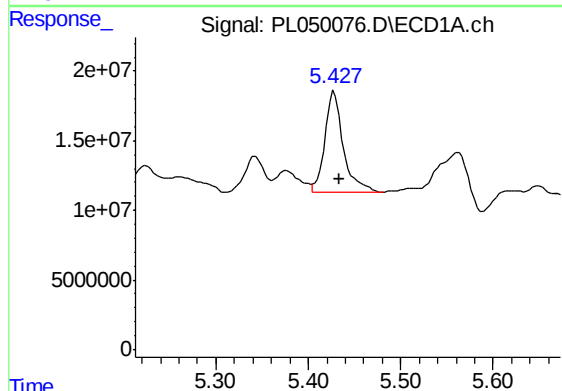


#12 4,4'-DDE

R.T.: 5.428 min
Delta R.T.: -0.006 min
Response: 101031016
Conc: 6.06 ng/ml

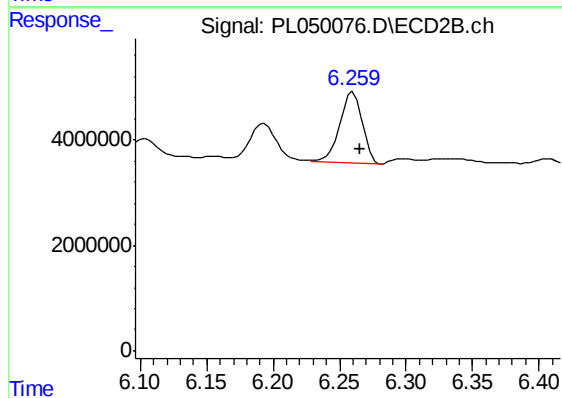

#12 4,4'-DDE

R.T.: 6.260 min
Delta R.T.: -0.005 min
Response: 16092218
Conc: 4.64 ng/ml

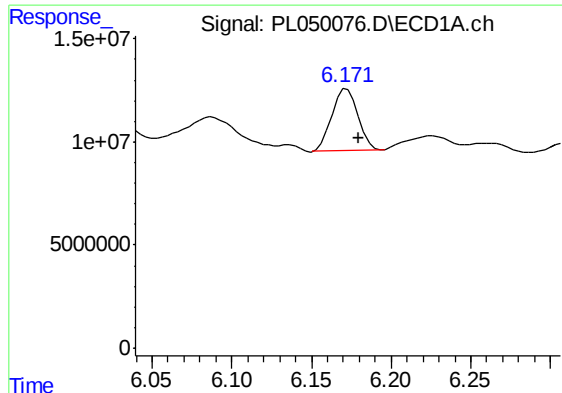


#17 4,4'-DDT

R.T.: 6.172 min
Delta R.T.: -0.007 min
Response: 34578441
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-009-SW137-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:02 PM

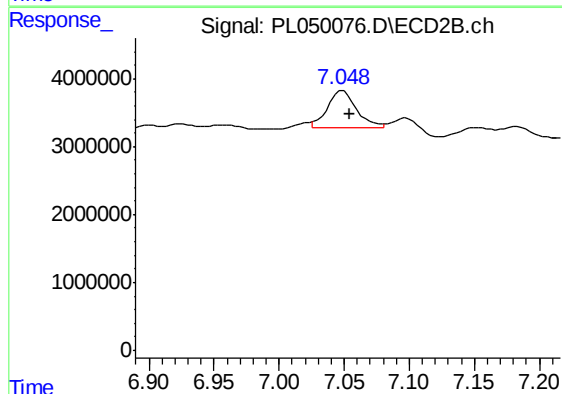


#17 4,4'-DDT

R.T.: 7.048 min
Delta R.T.: -0.006 min
Response: 8376454
Conc: 2.86 ng/ml m

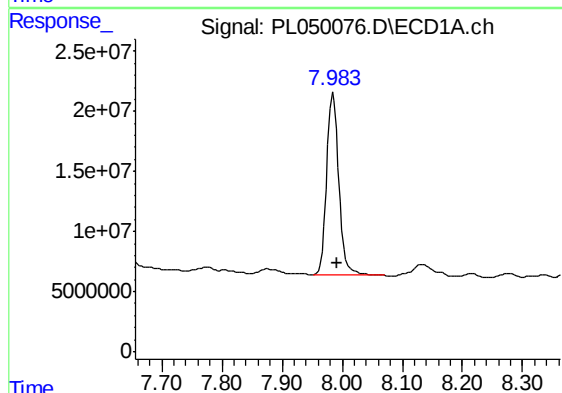

#28 Decachlorobiphenyl

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 213262192
Conc: 16.78 ng/ml

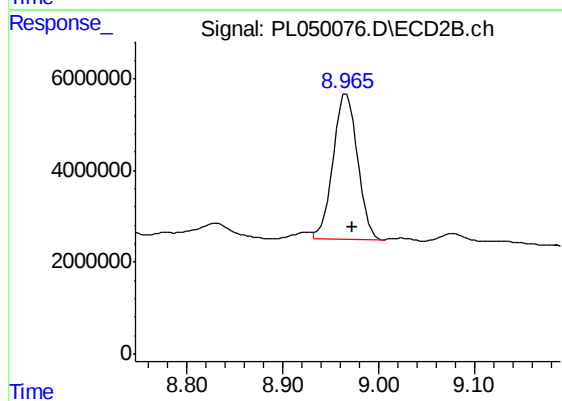

#28 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: -0.008 min
Response: 56136938
Conc: 16.72 ng/ml m