

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
 Data File : PL050088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2019 17:00
 Operator : SM\AJ
 Sample : K3560-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-009-B223-062419

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:10:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:28:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 02:23:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.322	3.933	174.4E6	46280595	15.461	15.116
28) SA Decachlor...	7.986	8.967	196.6E6	51922863	15.475	15.467
Target Compounds						
12) B 4,4'-DDE	5.431	6.259	27154174	5102956	1.630	1.471m
17) MA 4,4'-DDT	6.173	7.048	19254589	6454448	1.450m	2.204m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070119\
Data File : PL050088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2019 17:00
Operator : SM\AJ
Sample : K3560-15
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-009-B223-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:28:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062019.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 02:23:20 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

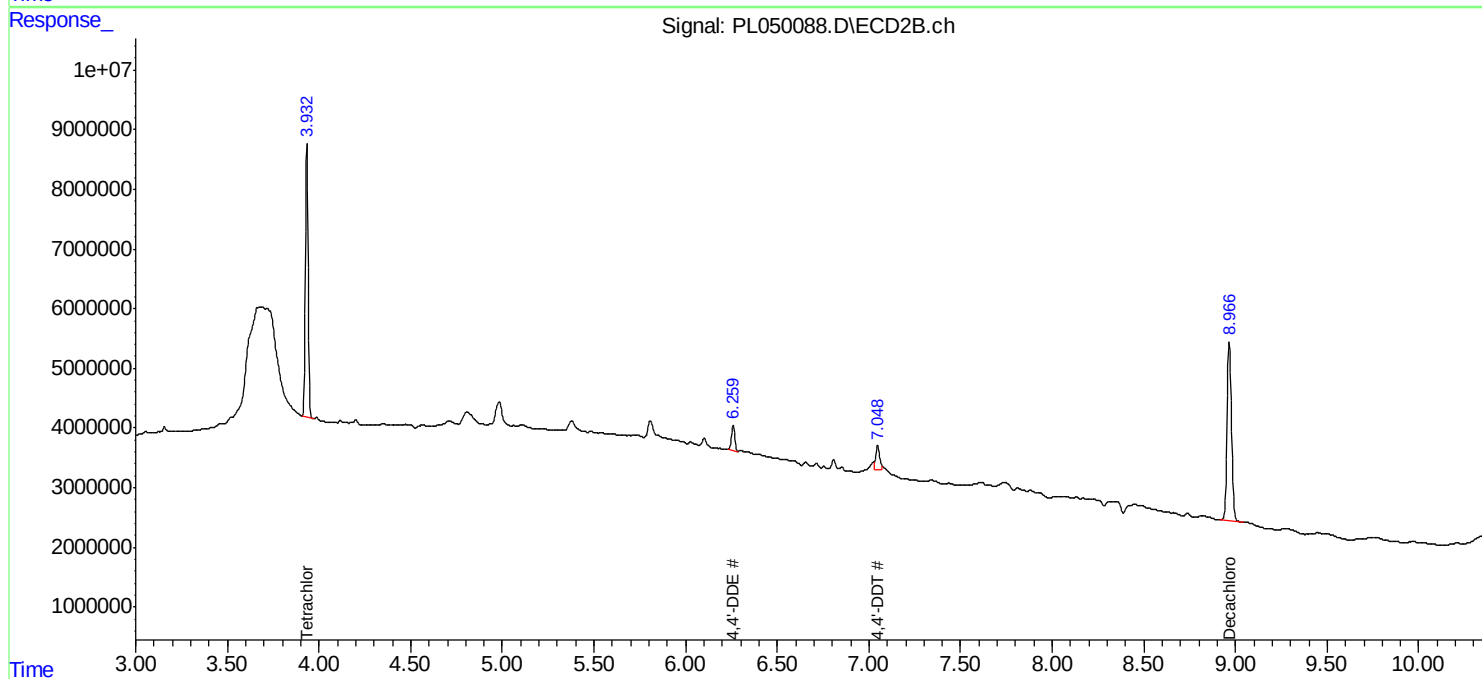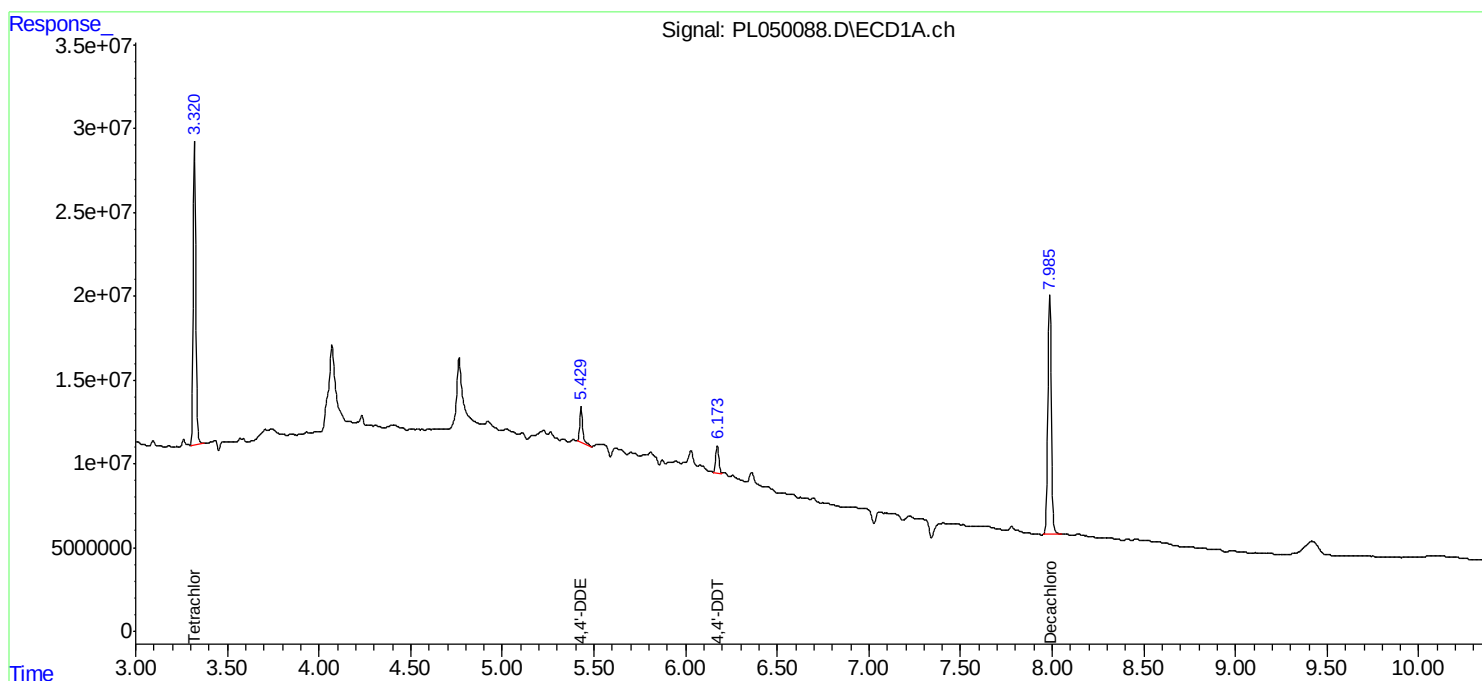

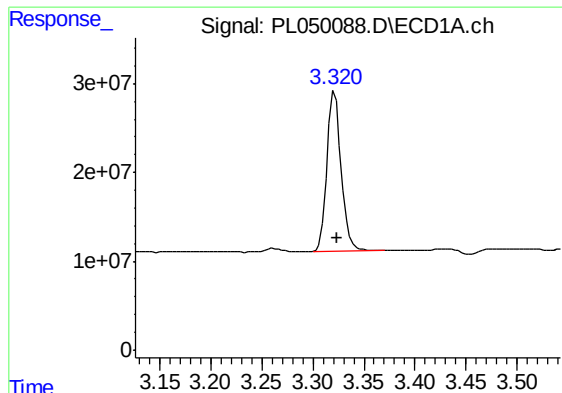


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: -0.002 min
Response: 174364956
Conc: 15.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-009-B223-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:15 PM

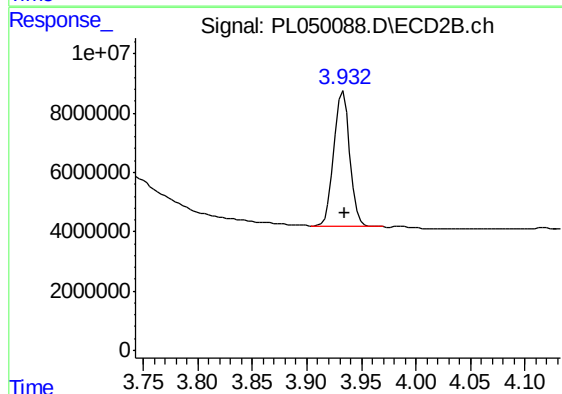


#1 Tetrachloro-m-xylene

R.T.: 3.933 min
Delta R.T.: -0.002 min
Response: 46280595
Conc: 15.12 ng/ml

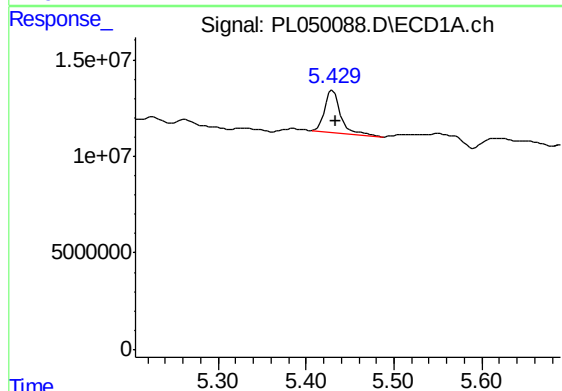


#12 4,4'-DDE

R.T.: 5.431 min
Delta R.T.: -0.004 min
Response: 27154174
Conc: 1.63 ng/ml

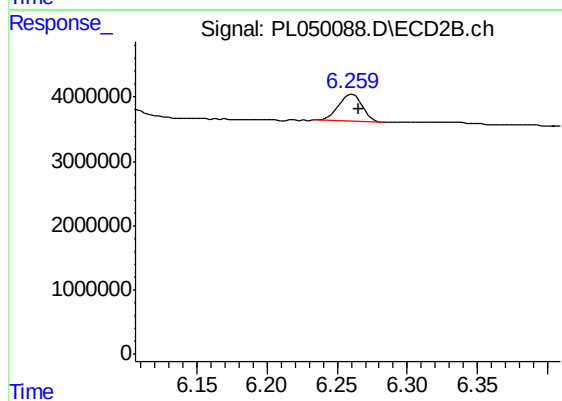

#12 4,4'-DDE

R.T.: 6.259 min
Delta R.T.: -0.006 min
Response: 5102956
Conc: 1.47 ng/ml m

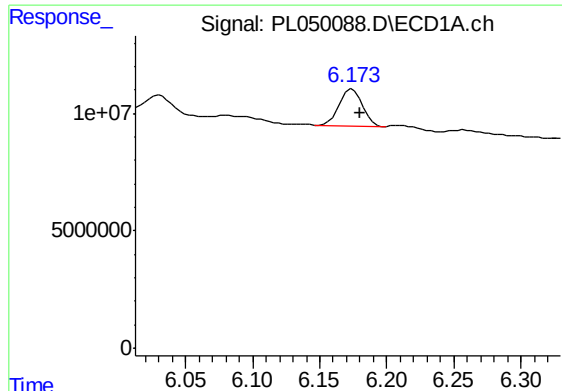


#17 4,4'-DDT

R.T.: 6.173 min
Delta R.T.: -0.007 min
Response: 19254589
Conc: 1.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PST-009-B223-062419


Manual Integrations
APPROVED

Ankita
7/2/2019 1:10:15 PM

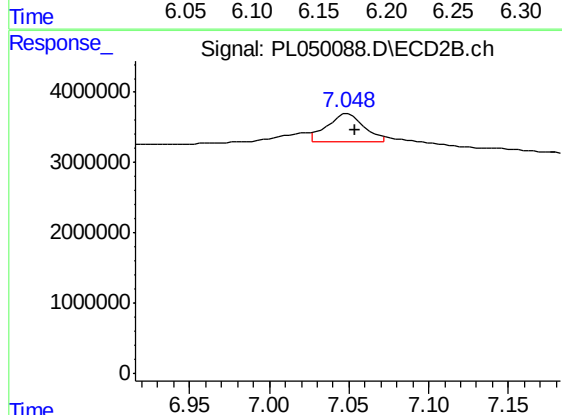


#17 4,4'-DDT

R.T.: 7.048 min
Delta R.T.: -0.006 min
Response: 6454448
Conc: 2.20 ng/ml m

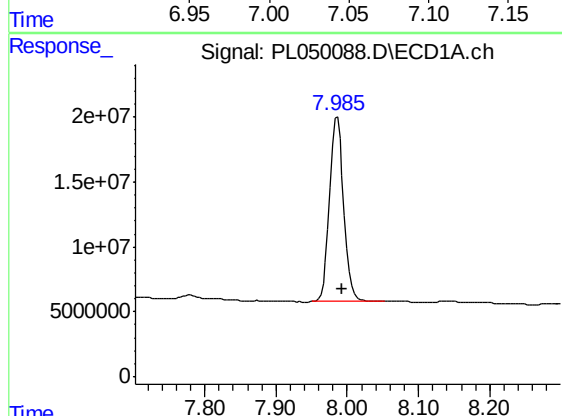

#28 Decachlorobiphenyl

R.T.: 7.986 min
Delta R.T.: -0.006 min
Response: 196625525
Conc: 15.47 ng/ml

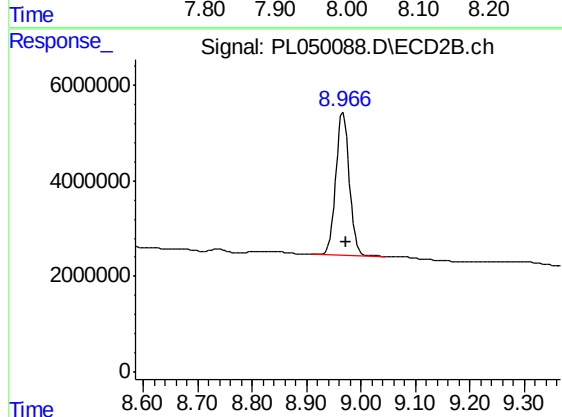

#28 Decachlorobiphenyl

R.T.: 8.967 min
Delta R.T.: -0.006 min
Response: 51922863
Conc: 15.47 ng/ml