

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
 Data File : PL059627.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 08:22
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 04:04:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	4.475	0	16527	N.D. 0.004 #
8) B	Heptachlo...	0.000	5.950	0	117101	N.D. 0.048 #
11) B	alpha-Chl...	0.000	6.262	0	1479086	N.D. 0.500 #
13) MA	Dieldrin	5.810f	6.591	273679	459393	0.171 0.163
14) MA	Endrin	0.000	6.787	0	11705937	N.D. 4.760 #
16) A	4,4'-DDD	6.208	0.000	6033960	0	4.520 N.D. #
17) MA	4,4'-DDT	0.000	7.200	0	101834	N.D. 0.045 #
20) A	Methoxychlor	6.998	0.000	354945	0	0.464 N.D. #
22)	Mirex	7.406f	0.000	2257446	0	1.739 N.D. #
24)	Chlordane-2	4.912	0.000	190955	0	3.669 N.D. #
26)	Chlordane-4	0.000	6.262	0	1479086	N.D. 3.284 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
Data File : PL059627.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 08:22
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 04:04:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

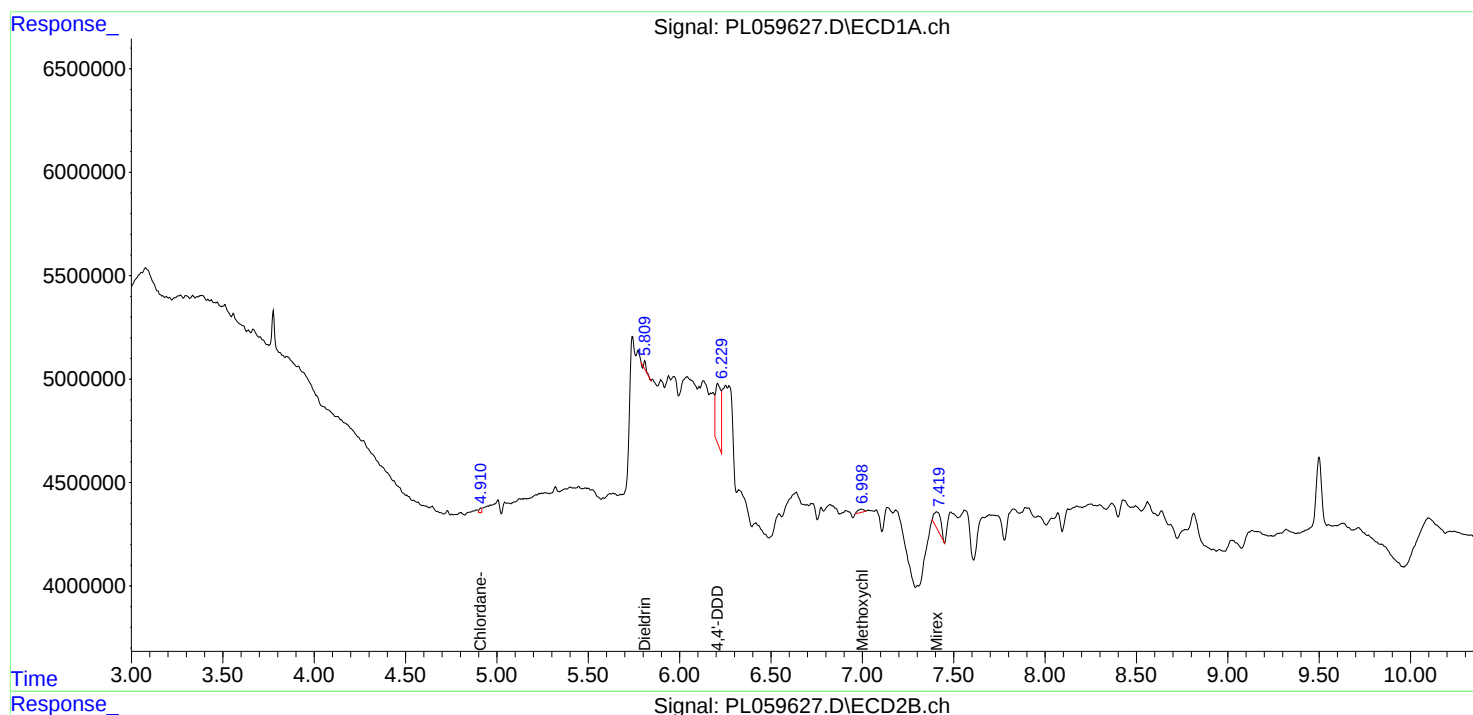


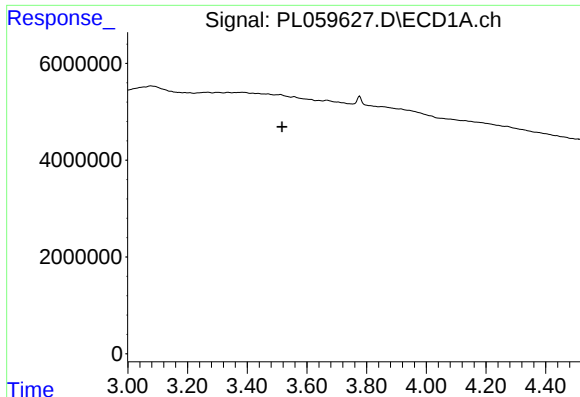

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

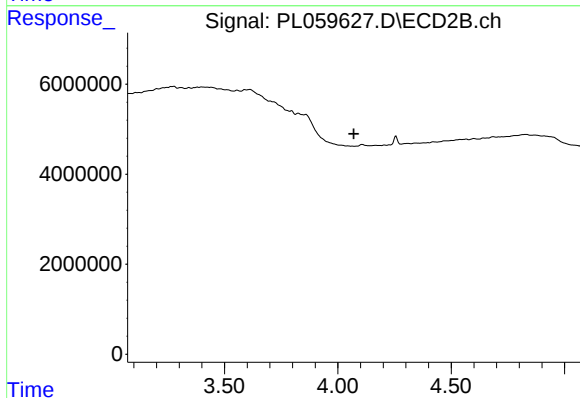


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.071 min
Response: 0
Conc: N.D.

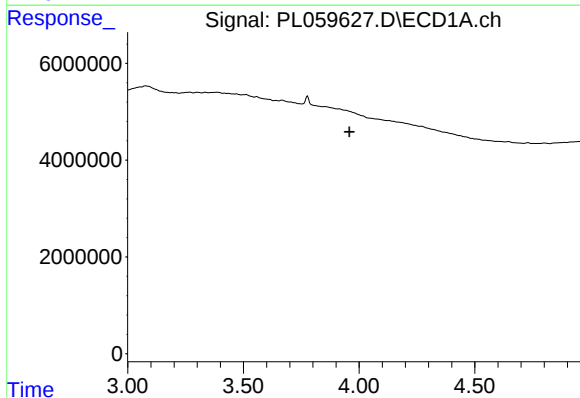


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.958 min
Response: 0
Conc: N.D.

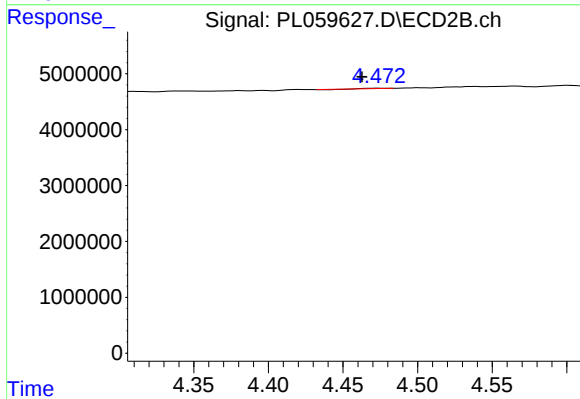

#2 alpha-BHC


R.T.: 4.475 min
Delta R.T.: 0.013 min
Response: 16527
Conc: 0.00 ng/ml

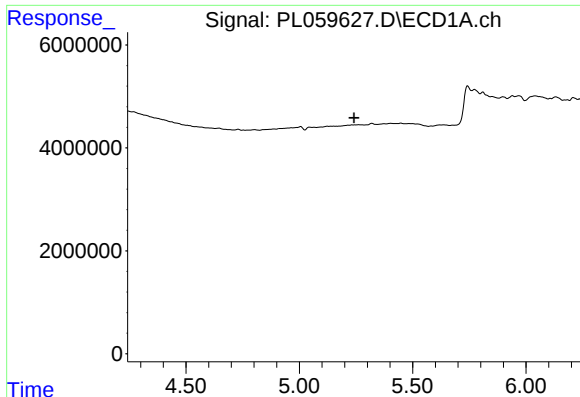

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

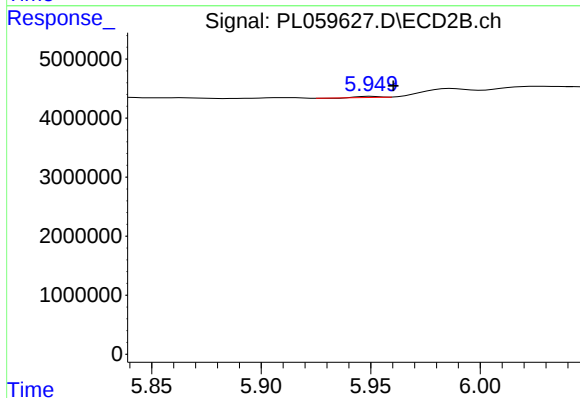


#8 Heptachlor epoxide

R.T.: 5.950 min
Delta R.T.: -0.010 min
Response: 117101
Conc: 0.05 ng/ml

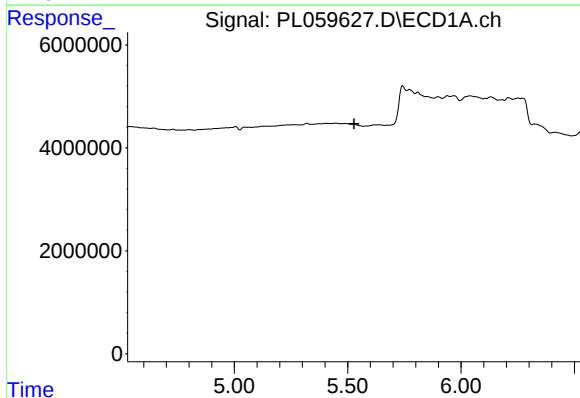


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.528 min
Response: 0
Conc: N.D.

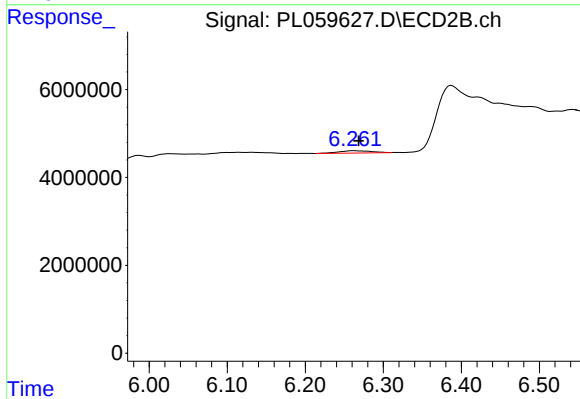

#11 alpha-Chlordane


R.T.: 6.262 min
Delta R.T.: -0.006 min
Response: 1479086
Conc: 0.50 ng/ml

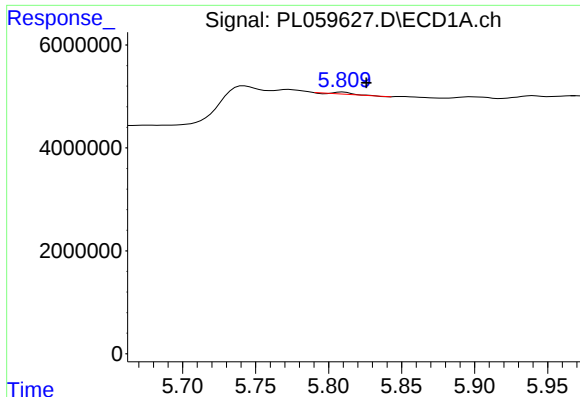

#13 Dieldrin


R.T.: 5.810 min
Delta R.T.: -0.016 min
Response: 273679
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

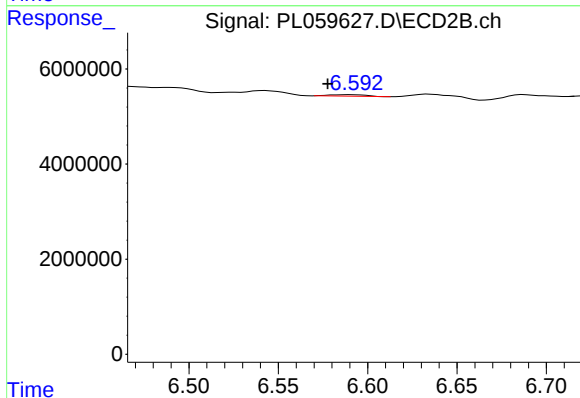


#13 Dieldrin

R.T.: 6.591 min
Delta R.T.: 0.013 min
Response: 459393
Conc: 0.16 ng/ml

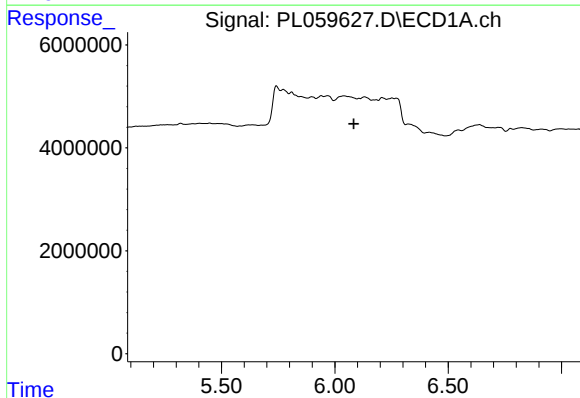


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.083 min
Response: 0
Conc: N.D.

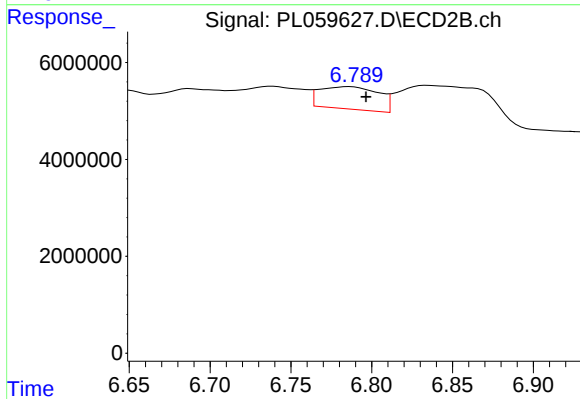

#14 Endrin


R.T.: 6.787 min
Delta R.T.: -0.010 min
Response: 11705937
Conc: 4.76 ng/ml

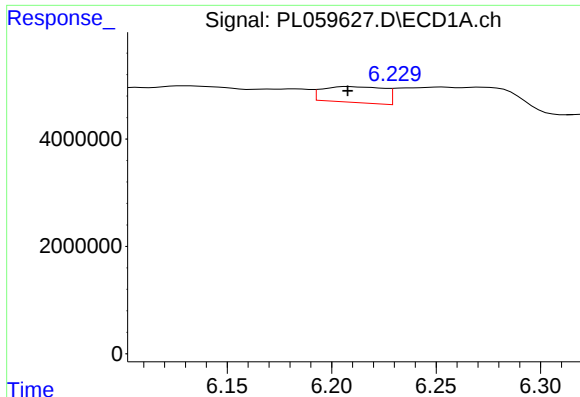

#16 4,4'-DDD


R.T.: 6.208 min
Delta R.T.: 0.000 min
Response: 6033960
Conc: 4.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

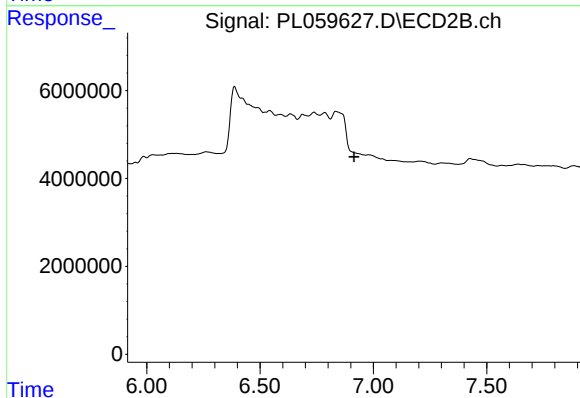


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

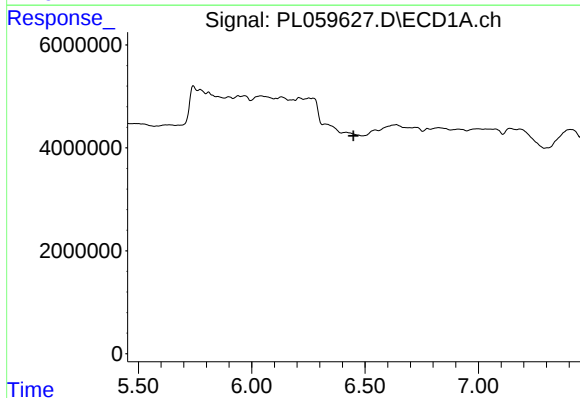


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.449 min
Response: 0
Conc: N.D.

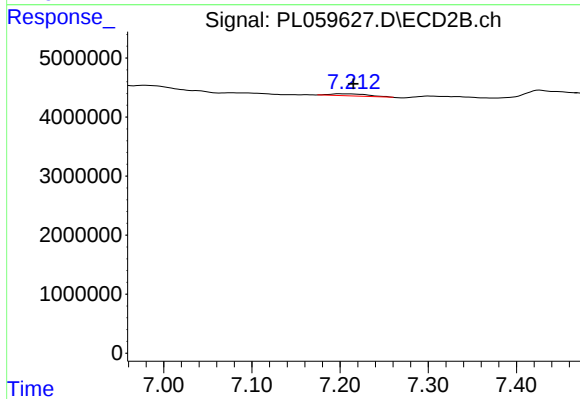

#17 4,4'-DDT


R.T.: 7.200 min
Delta R.T.: -0.015 min
Response: 101834
Conc: 0.05 ng/ml

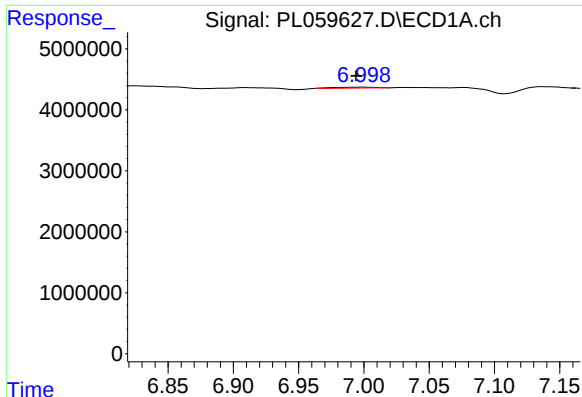

#20 Methoxychlor


R.T.: 6.998 min
Delta R.T.: 0.004 min
Response: 354945
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

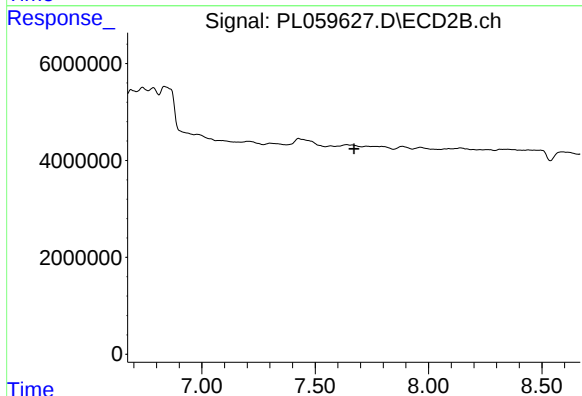


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.672 min
Response: 0
Conc: N.D.

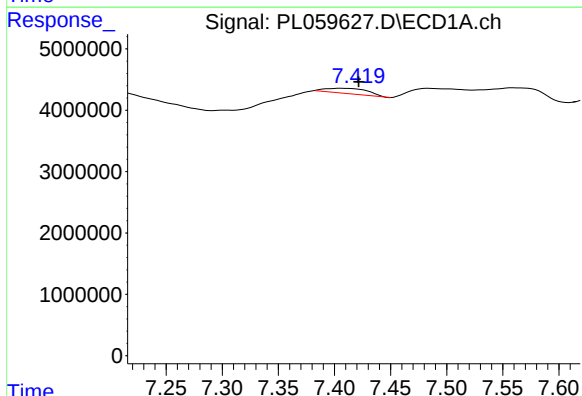


#22 Mirex

R.T.: 7.406 min
Delta R.T.: -0.015 min
Response: 2257446
Conc: 1.74 ng/ml

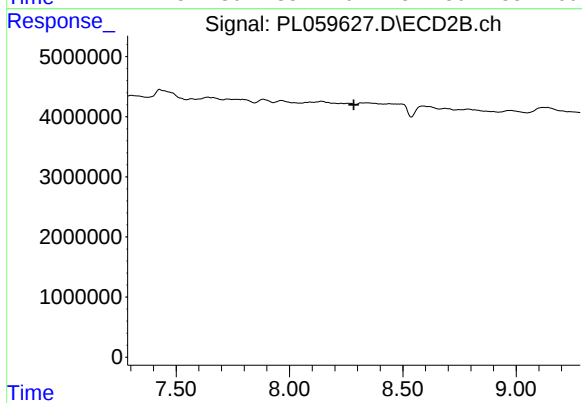

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

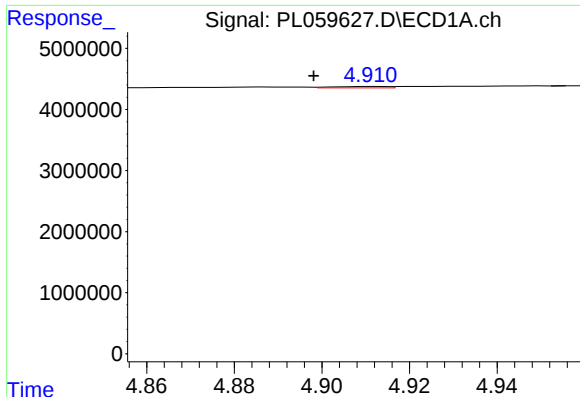

#24 Chlordane-2


R.T.: 4.912 min
Delta R.T.: 0.014 min
Response: 190955
Conc: 3.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

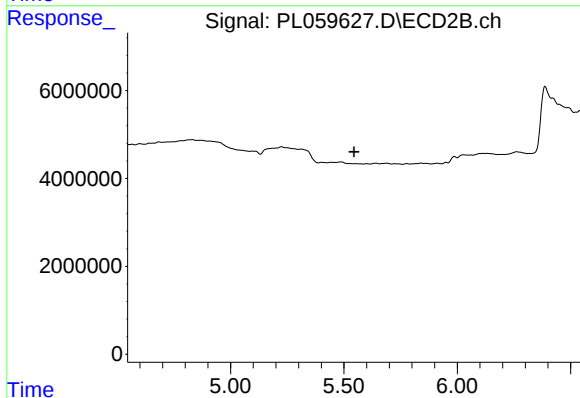


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.544 min
Response: 0
Conc: N.D.

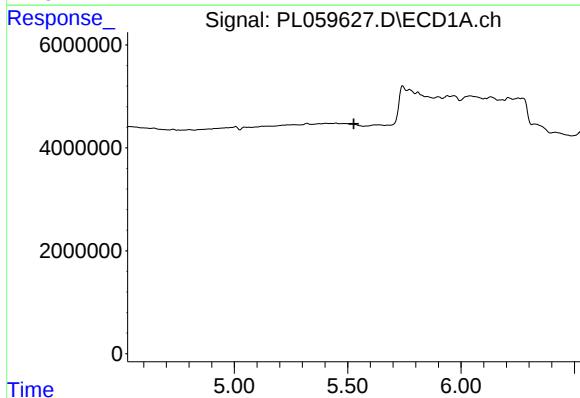


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.527 min
Response: 0
Conc: N.D.

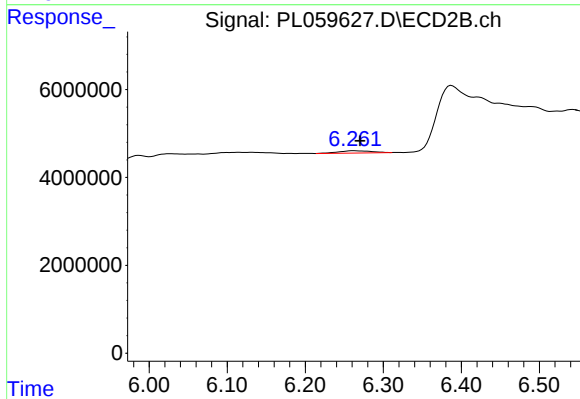

#26 Chlordane-4


R.T.: 6.262 min
Delta R.T.: -0.008 min
Response: 1479086
Conc: 3.28 ng/ml

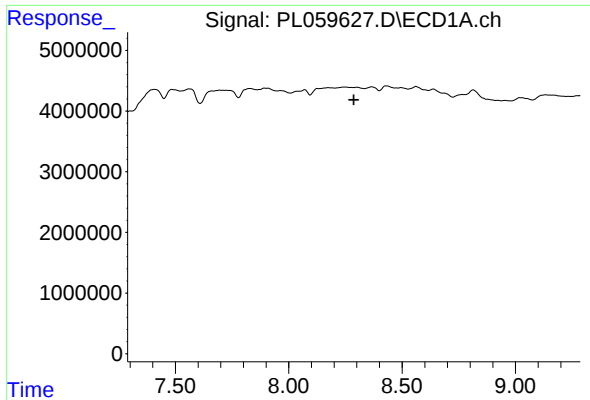

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

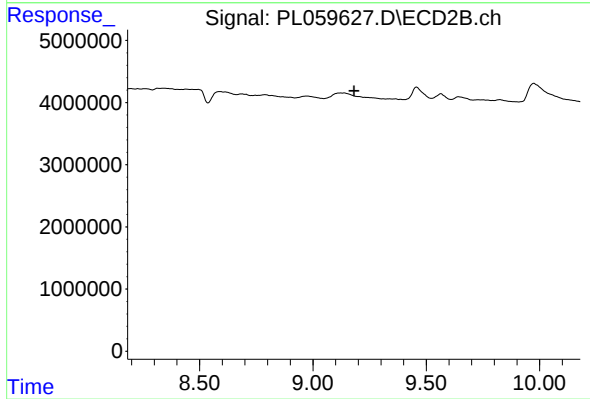

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.182 min
Response: 0
Conc: N.D.