

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
 Data File : PL059651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 14:07
 Operator : AJ\MA
 Sample : PB129895BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 04:09:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.521	4.071	34968248	51936692	19.469	19.529
28)	SA Decachlor...	8.291	9.184	31847895	43595611	20.745	20.056
Target Compounds							
4)	MA Heptachlor	0.000	5.263	0	3959735	N.D.	1.130 #
6)	B beta-BHC	4.462f	0.000	620796	0	0.662	N.D. #
9)	A Endosulfan I	0.000	6.304f	0	270691	N.D.	0.100 #
15)	B Endosulfa...	6.357	7.007	197726	1348060	0.130	0.525 #
16)	A 4,4'-DDD	6.210	0.000	344949	0	0.258	N.D. #
18)	B Endrin al...	0.000	7.113f	0	114243	N.D.	0.052 #
20)	A Methoxychlor	7.022f	0.000	41933	0	0.055	N.D. #
22)	Mirex	7.406f	8.306f	68386	58191	0.053	0.030 #
27)	Chlordane-5	6.357	7.072	197726	818016	3.849	9.400 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
Data File : PL059651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 14:07
Operator : AJ\MA
Sample : PB129895BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 04:09:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

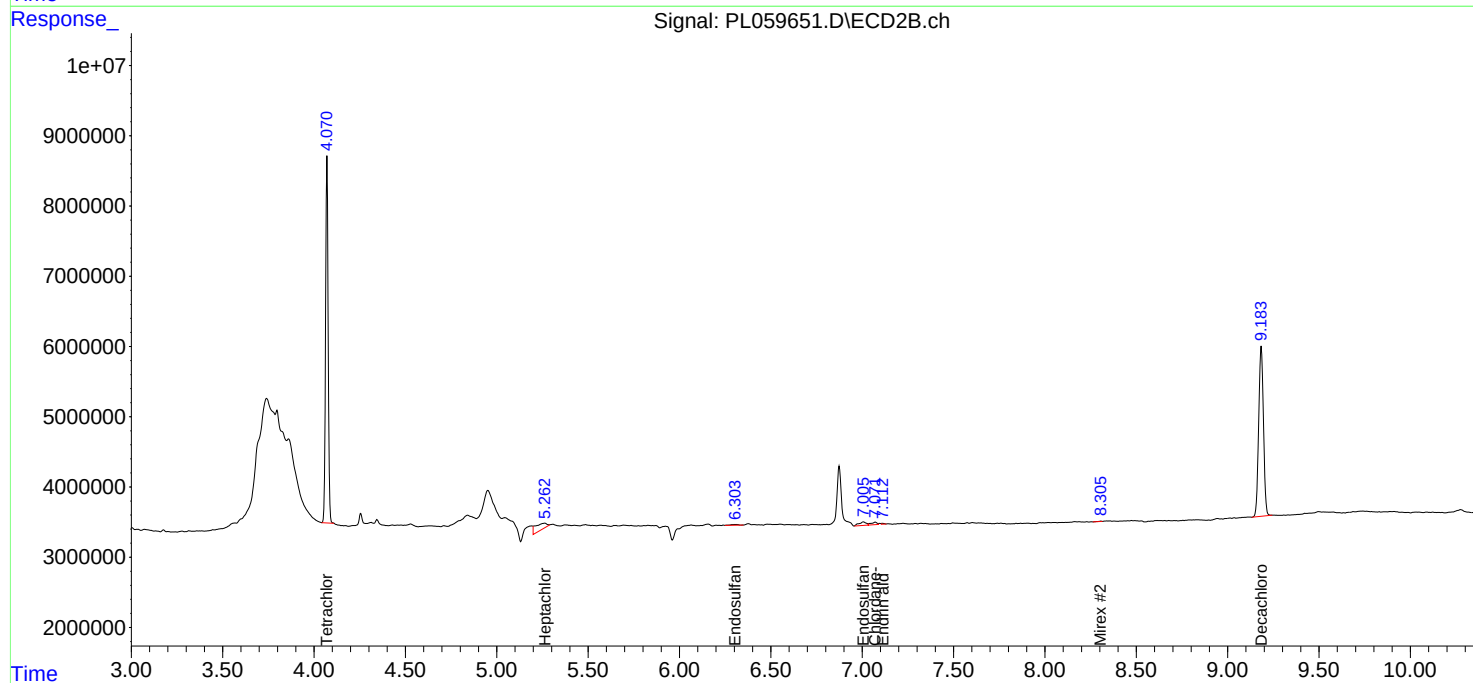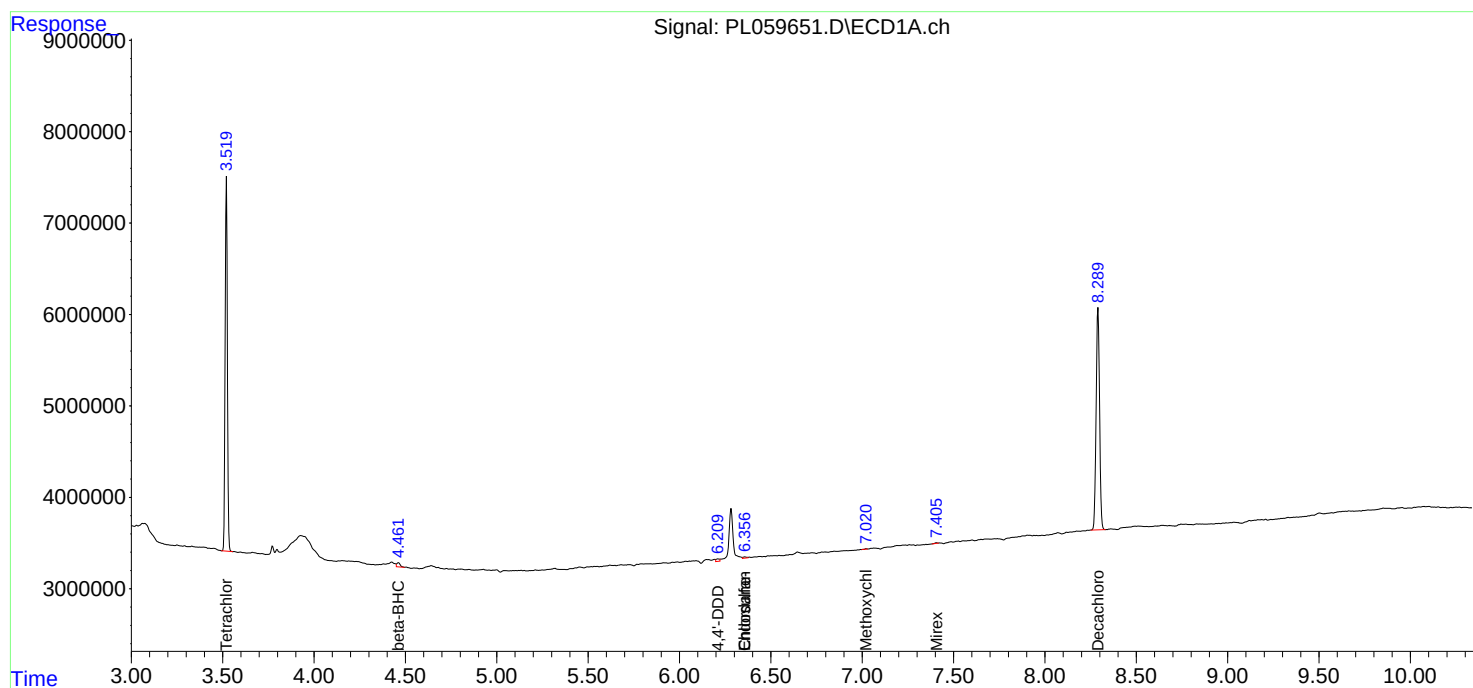


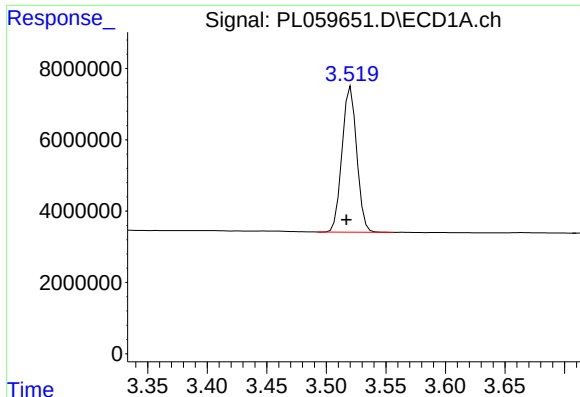

#1 Tetrachloro-m-xylene


R.T.: 3.521 min
Delta R.T.: 0.004 min
Response: 34968248
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

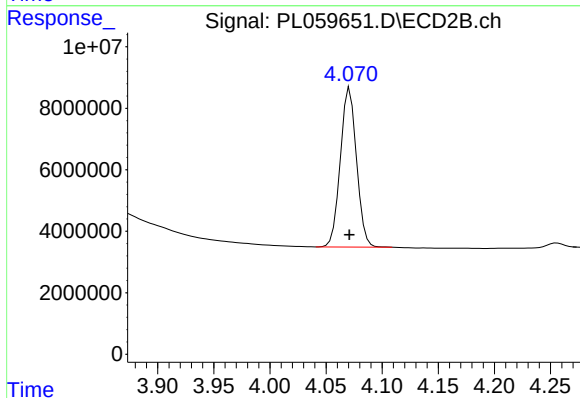


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 51936692
Conc: 19.53 ng/ml

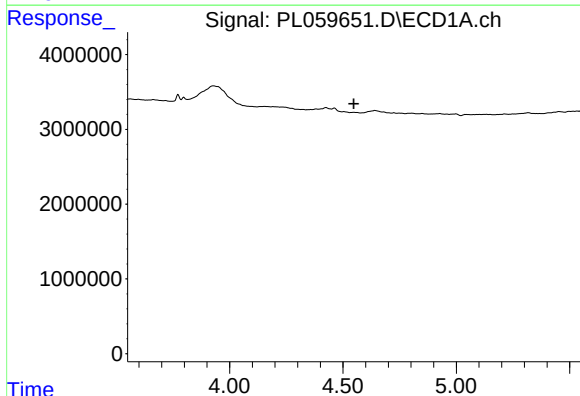


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.548 min
Response: 0
Conc: N.D.

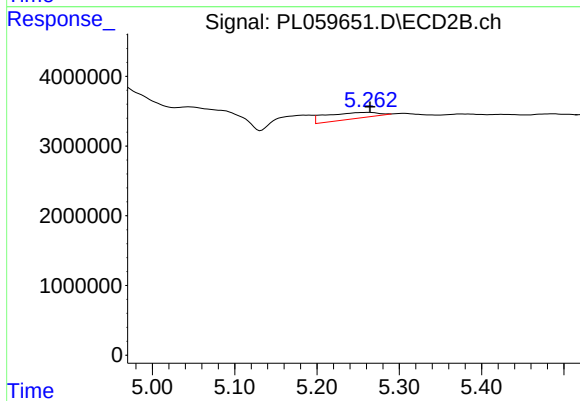

#4 Heptachlor


R.T.: 5.263 min
Delta R.T.: -0.002 min
Response: 3959735
Conc: 1.13 ng/ml

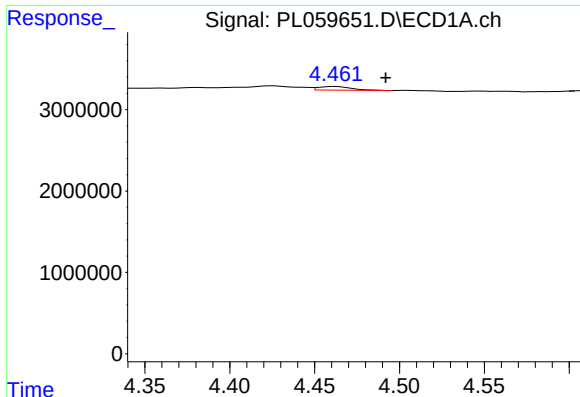

#6 beta-BHC


R.T.: 4.462 min
Delta R.T.: -0.030 min
Response: 620796
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

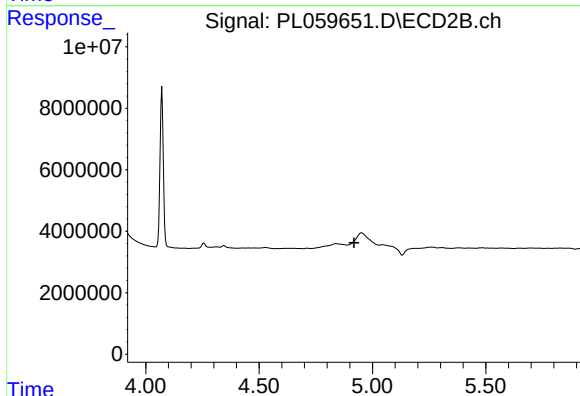


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.919 min
Response: 0
Conc: N.D.

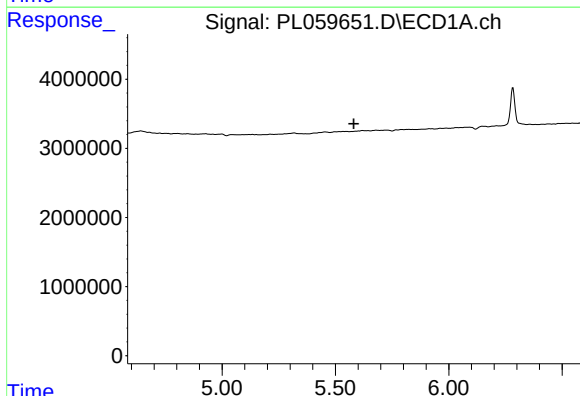


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

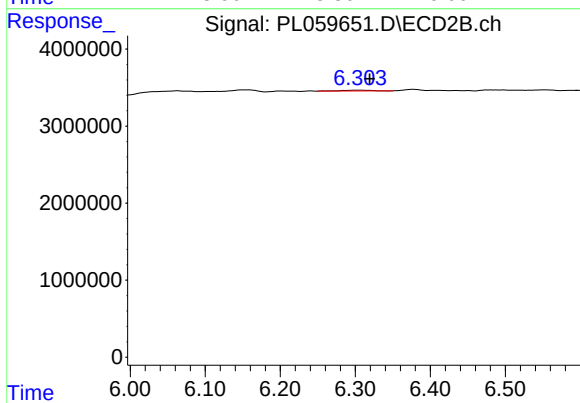

#9 Endosulfan I


R.T.: 6.304 min
Delta R.T.: -0.015 min
Response: 270691
Conc: 0.10 ng/ml

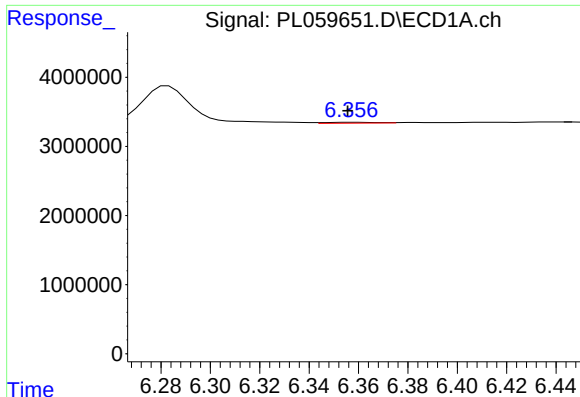

#15 Endosulfan II


R.T.: 6.357 min
Delta R.T.: 0.002 min
Response: 197726
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

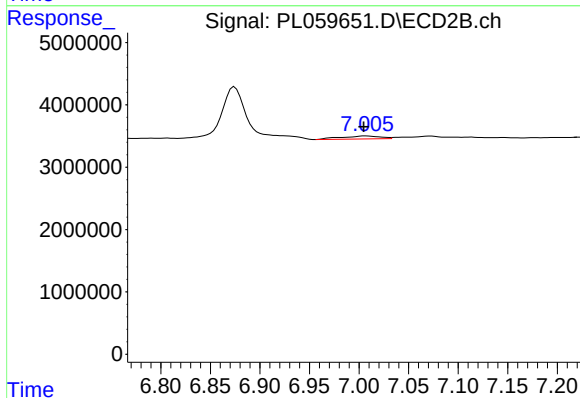


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.002 min
Response: 1348060
Conc: 0.52 ng/ml

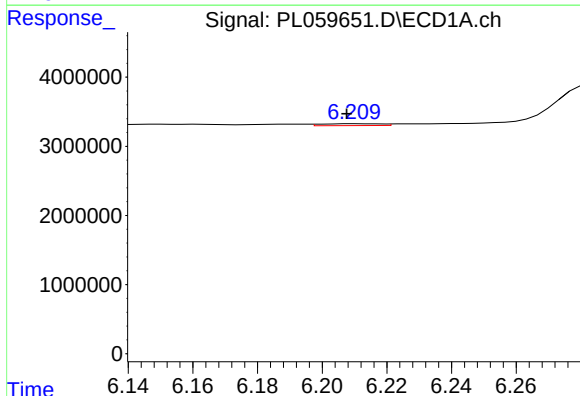


#16 4,4'-DDD

R.T.: 6.210 min
Delta R.T.: 0.003 min
Response: 344949
Conc: 0.26 ng/ml

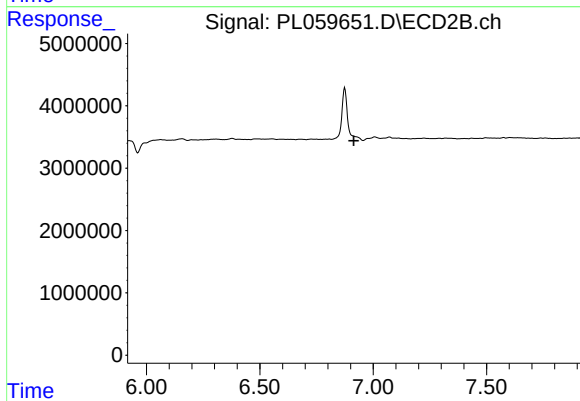

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

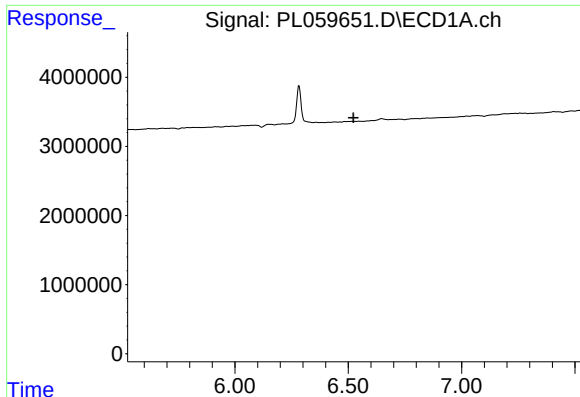

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

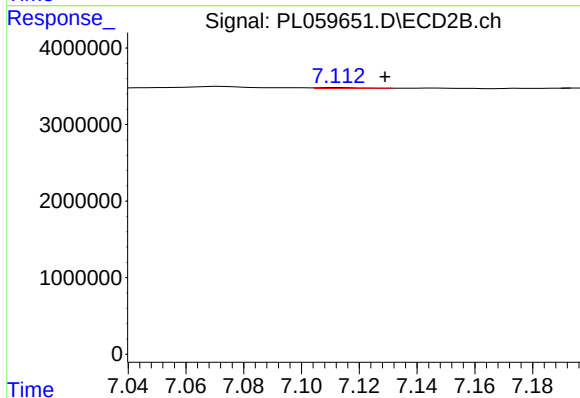


#18 Endrin aldehyde

R.T.: 7.113 min
Delta R.T.: -0.016 min
Response: 114243
Conc: 0.05 ng/ml

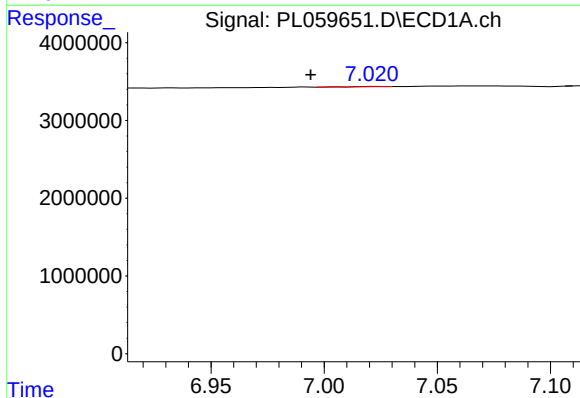


#20 Methoxychlor

R.T.: 7.022 min
Delta R.T.: 0.028 min
Response: 41933
Conc: 0.05 ng/ml

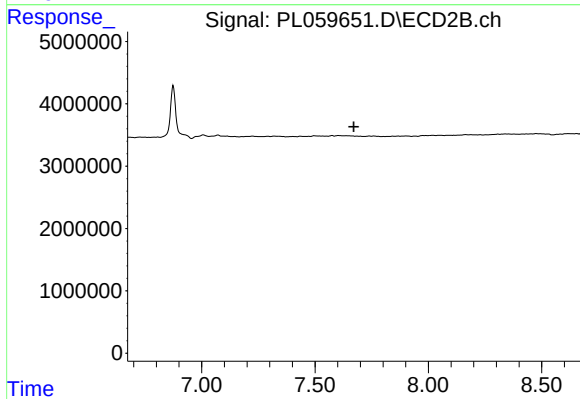

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.672 min
Response: 0
Conc: N.D.

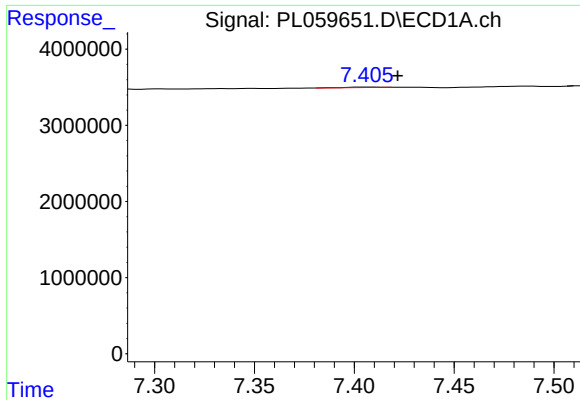

#22 Mirex


R.T.: 7.406 min
Delta R.T.: -0.015 min
Response: 68386
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

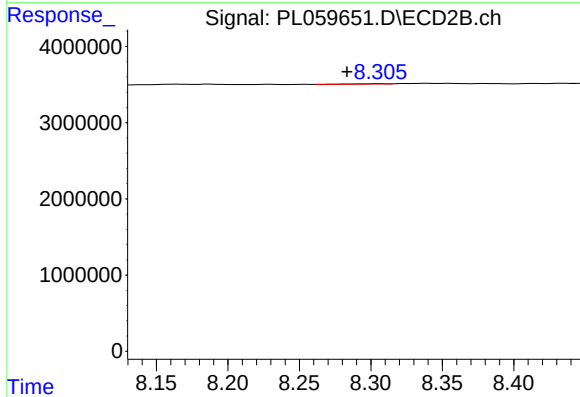


#22 Mirex

R.T.: 8.306 min
Delta R.T.: 0.023 min
Response: 58191
Conc: 0.03 ng/ml

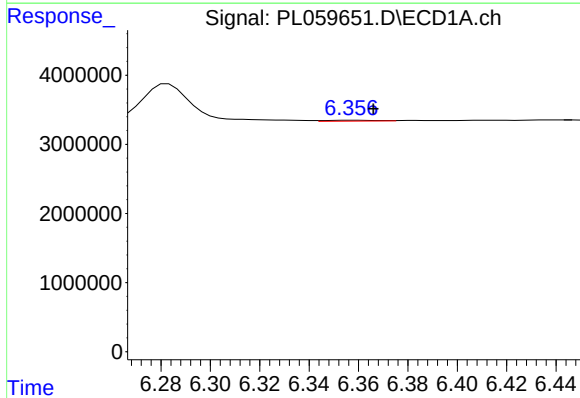


#27 Chlordane-5

R.T.: 6.357 min
Delta R.T.: -0.009 min
Response: 197726
Conc: 3.85 ng/ml

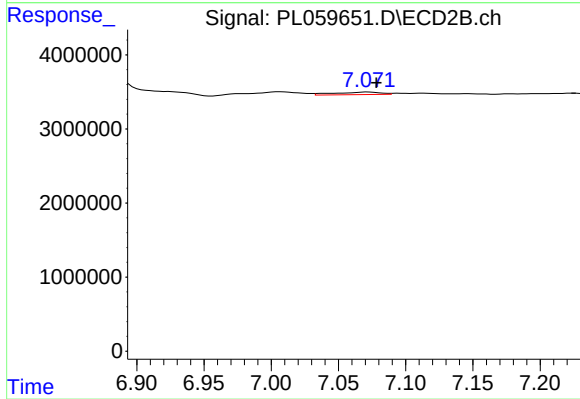

#27 Chlordane-5


R.T.: 7.072 min
Delta R.T.: -0.006 min
Response: 818016
Conc: 9.40 ng/ml

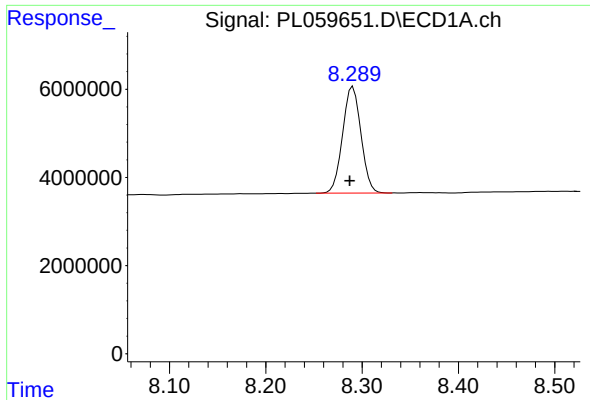

#28 Decachlorobiphenyl

R.T.: 8.291 min
Delta R.T.: 0.003 min
Response: 31847895
Conc: 20.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

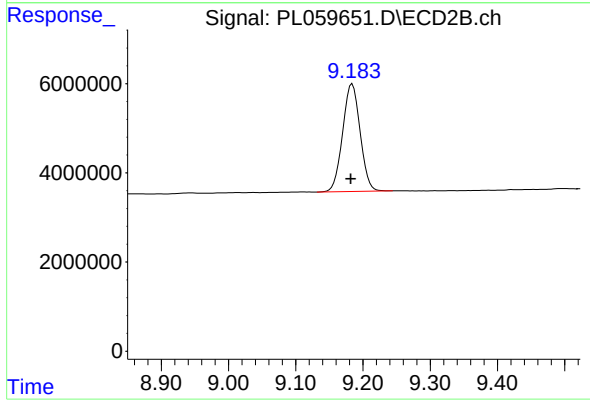

#28 Decachlorobiphenyl

R.T.: 9.184 min
Delta R.T.: 0.002 min
Response: 43595611
Conc: 20.06 ng/ml