

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
 Data File : PL059679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2020 20:41
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 04:18:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.071	49024419	69324312	27.296	26.067
28)	SA Decachlor...	8.286	9.183	34934438	50797583	22.755	23.370
Target Compounds							
2)	A alpha-BHC	3.963	0.000	1377825	0	0.536	N.D. #
4)	MA Heptachlor	0.000	5.264	0	1916351	N.D.	0.547 #
8)	B Heptachlo...	0.000	5.950	0	2061321	N.D.	0.848 #
9)	A Endosulfan I	0.000	6.317	0	66517	N.D.	0.025 #
14)	MA Endrin	6.083	0.000	277698	0	0.188	N.D. #
15)	B Endosulfa...	0.000	7.010	0	1040228	N.D.	0.405 #
17)	MA 4,4'-DDT	0.000	7.217	0	504777	N.D.	0.223 #
19)	B Endosulfa...	0.000	7.343	0	29102	N.D.	0.012 #
22)	Mirex	7.441f	8.305f	187823	569353	0.145	0.298 #
23)	Chlordane-1	4.422f	0.000	1096012	0	21.031	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070120\
Data File : PL059679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2020 20:41
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 04:18:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

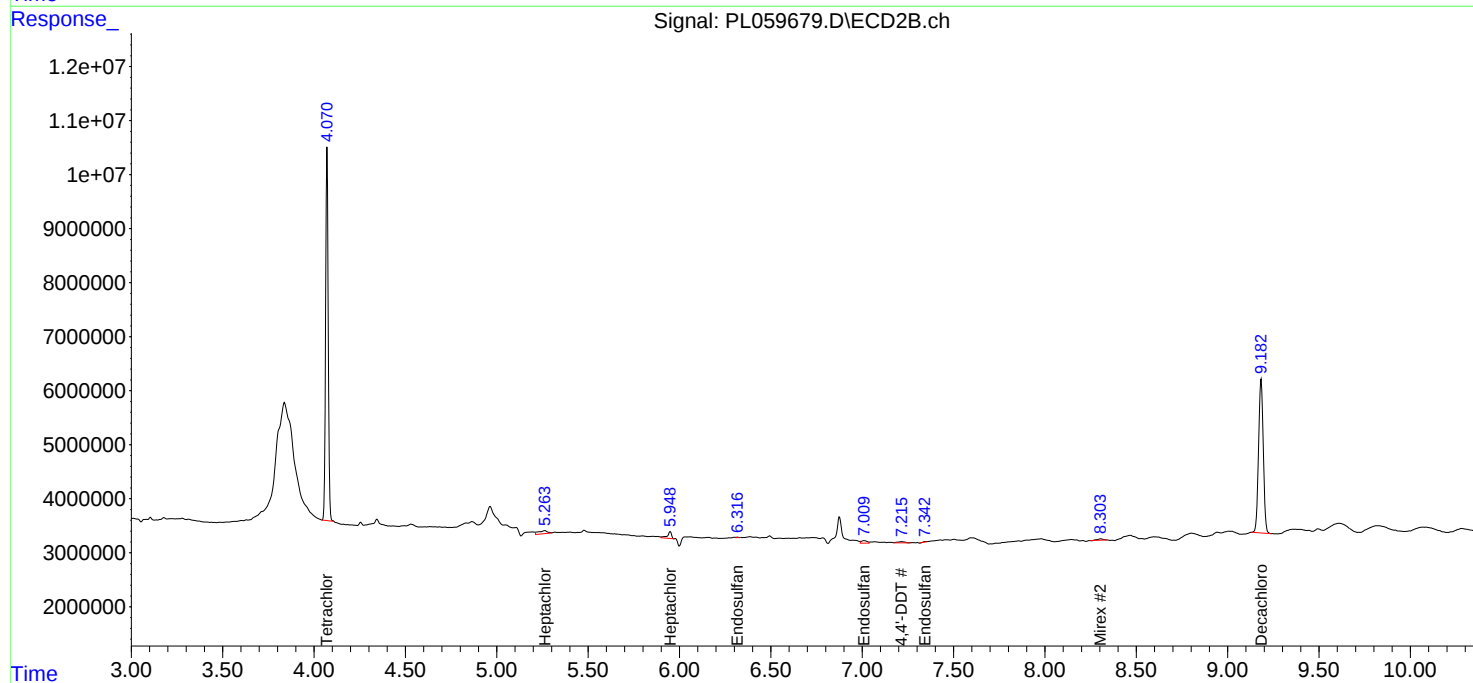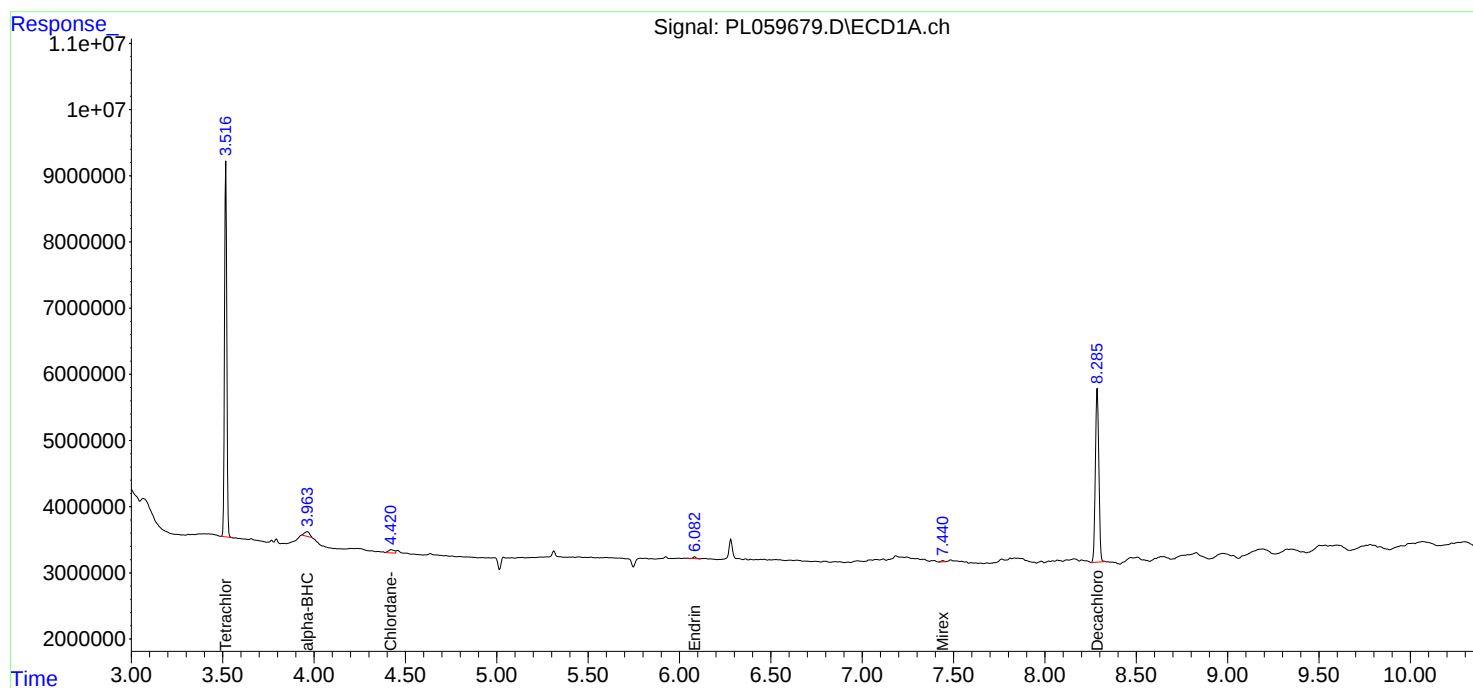


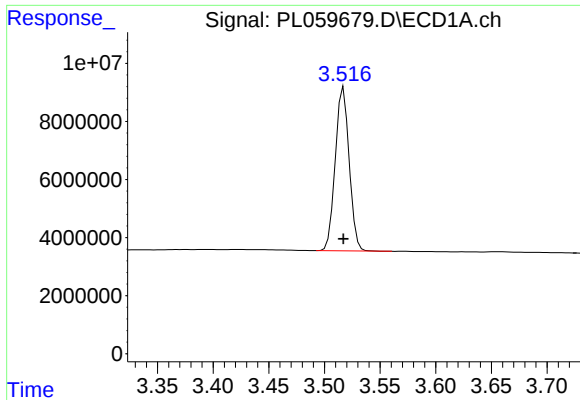

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 49024419
Conc: 27.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

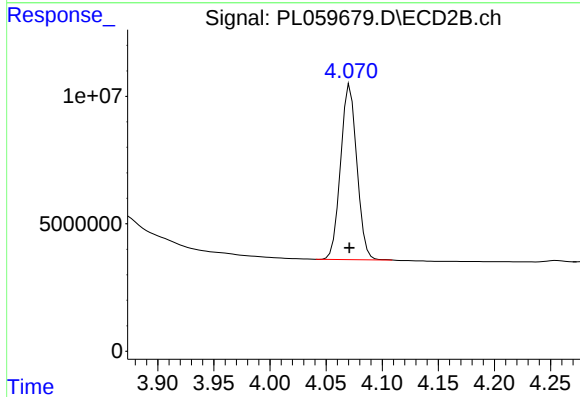


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 69324312
Conc: 26.07 ng/ml

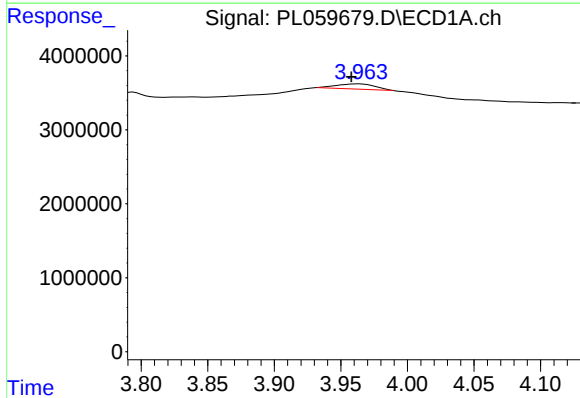


#2 alpha-BHC

R.T.: 3.963 min
Delta R.T.: 0.006 min
Response: 1377825
Conc: 0.54 ng/ml

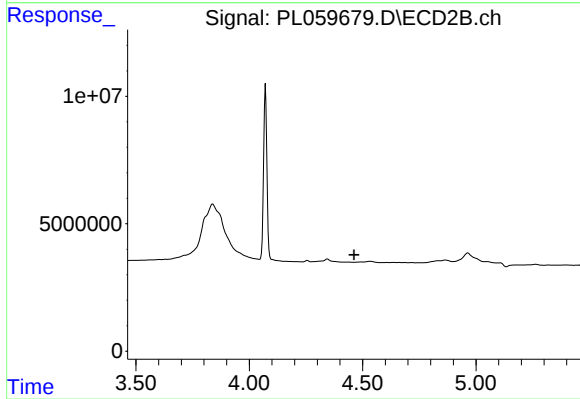

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.463 min
Response: 0
Conc: N.D.

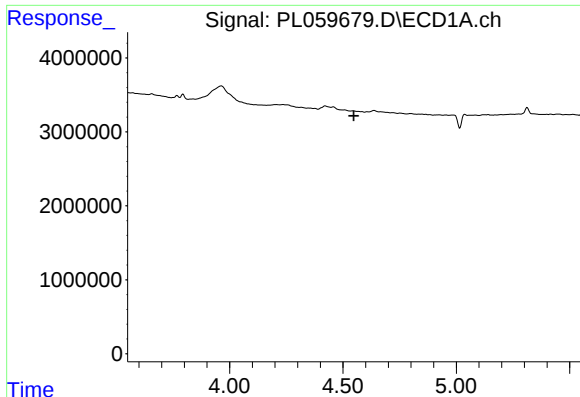

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

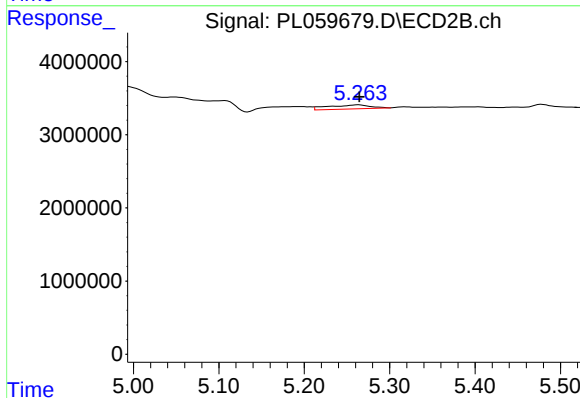


#4 Heptachlor

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 1916351
Conc: 0.55 ng/ml

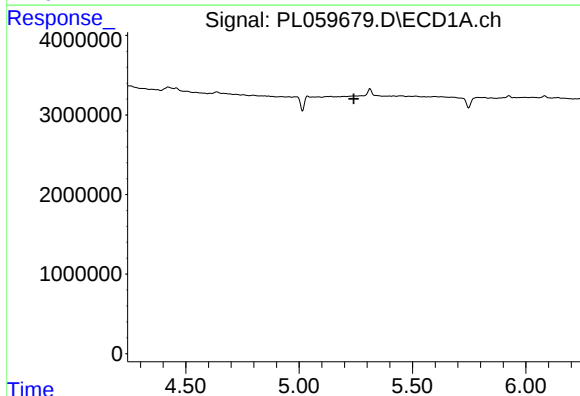


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

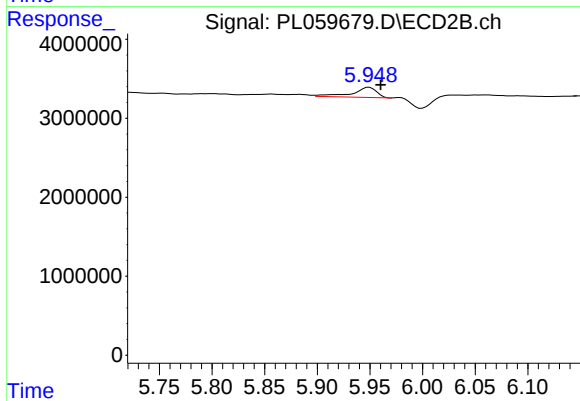

#8 Heptachlor epoxide


R.T.: 5.950 min
Delta R.T.: -0.011 min
Response: 2061321
Conc: 0.85 ng/ml

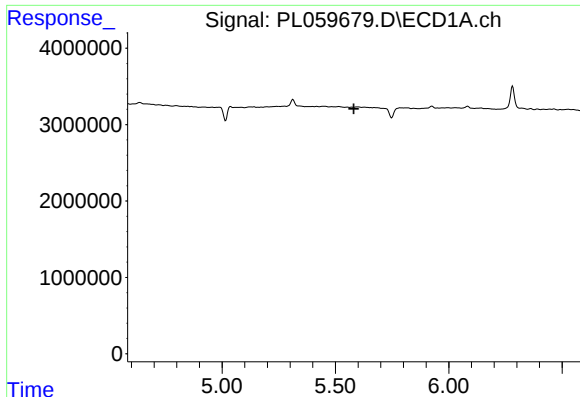

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

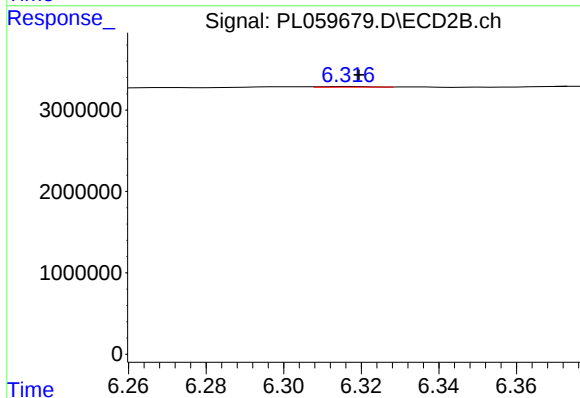


#9 Endosulfan I

R.T.: 6.317 min
Delta R.T.: -0.002 min
Response: 66517
Conc: 0.02 ng/ml

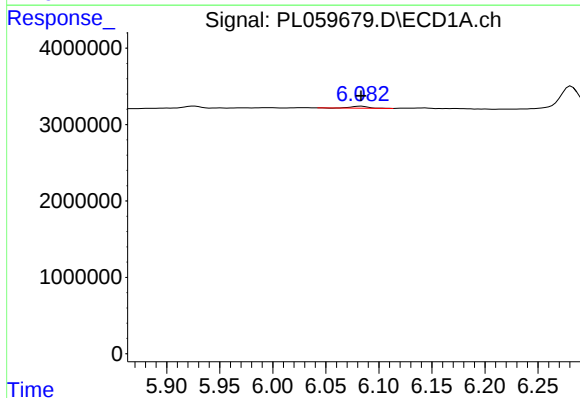


#14 Endrin

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 277698
Conc: 0.19 ng/ml

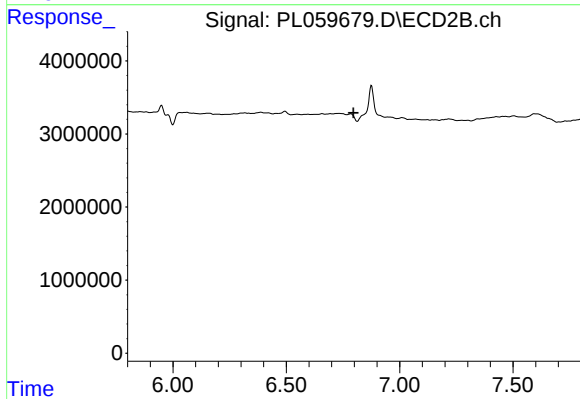

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.797 min
Response: 0
Conc: N.D.

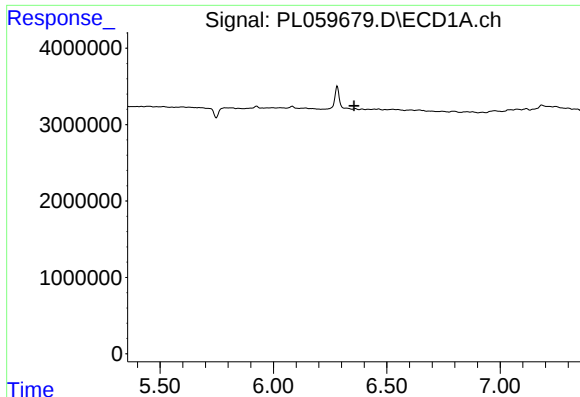

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.356 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

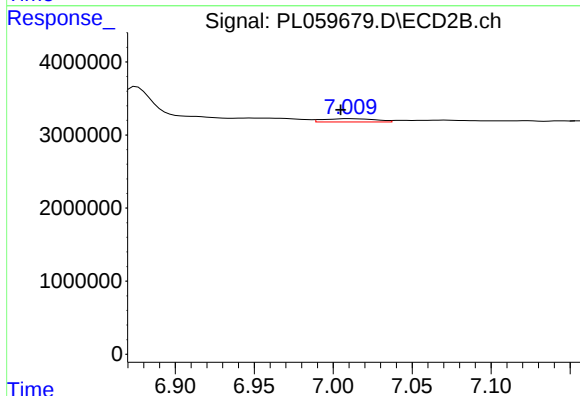


#15 Endosulfan II

R.T.: 7.010 min
Delta R.T.: 0.006 min
Response: 1040228
Conc: 0.40 ng/ml

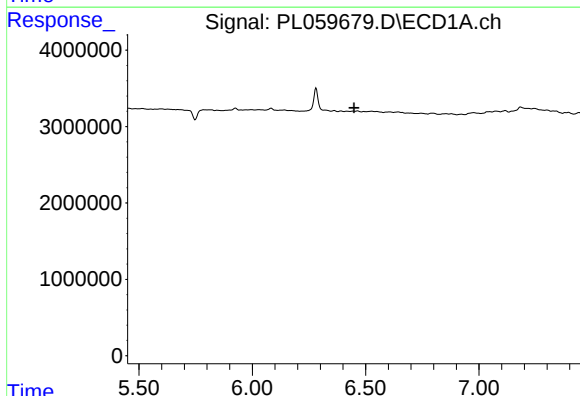


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.449 min
Response: 0
Conc: N.D.

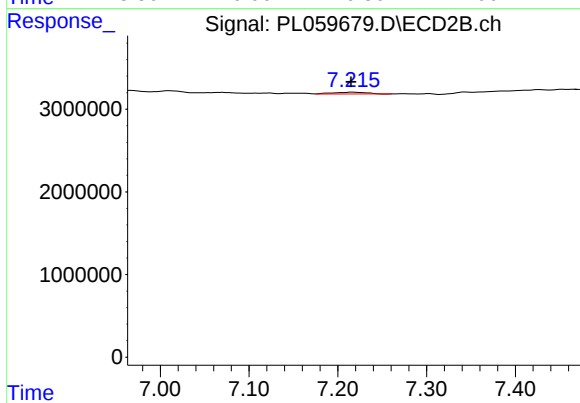

#17 4,4'-DDT


R.T.: 7.217 min
Delta R.T.: 0.002 min
Response: 504777
Conc: 0.22 ng/ml

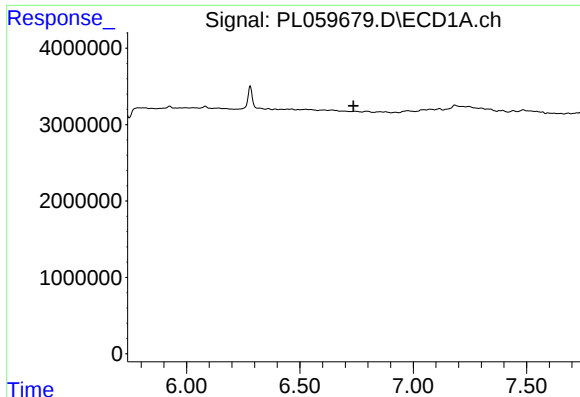

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

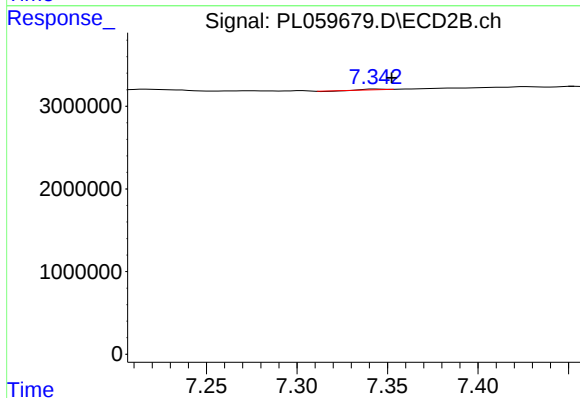


#19 Endosulfan Sulfate

R.T.: 7.343 min
Delta R.T.: -0.009 min
Response: 29102
Conc: 0.01 ng/ml

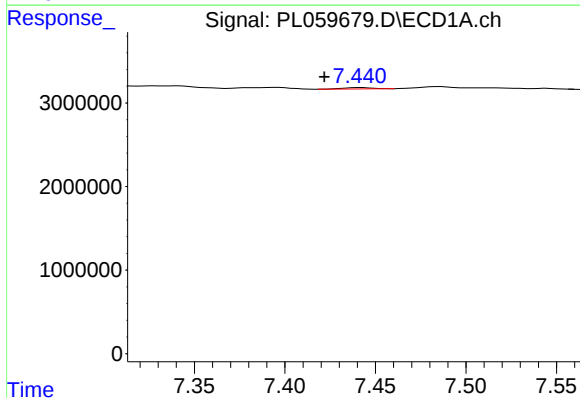


#22 Mirex

R.T.: 7.441 min
Delta R.T.: 0.020 min
Response: 187823
Conc: 0.14 ng/ml

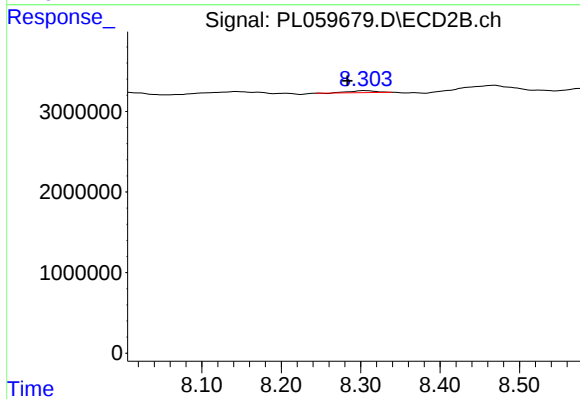

#22 Mirex


R.T.: 8.305 min
Delta R.T.: 0.021 min
Response: 569353
Conc: 0.30 ng/ml

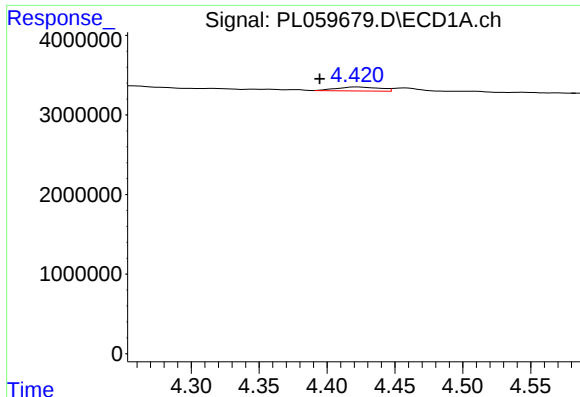

#23 Chlordane-1


R.T.: 4.422 min
Delta R.T.: 0.027 min
Response: 1096012
Conc: 21.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

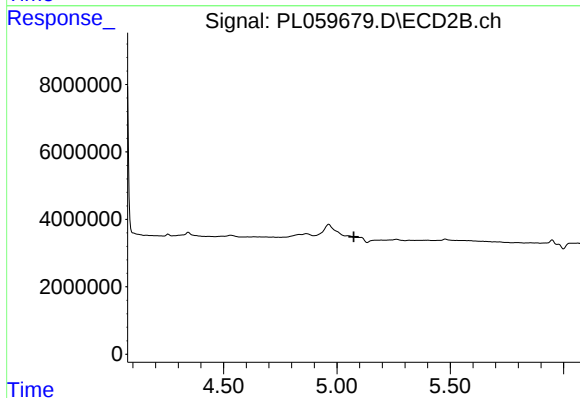


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

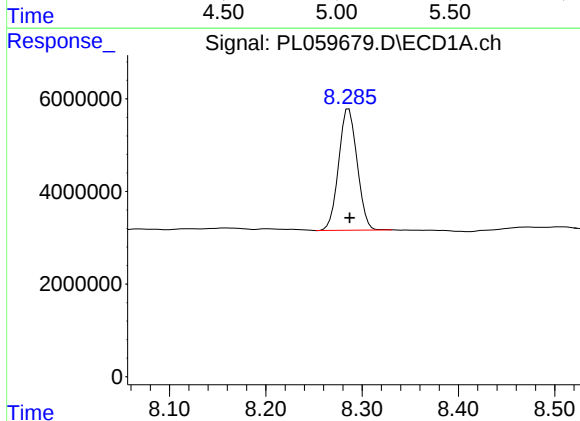

#28 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 34934438
Conc: 22.76 ng/ml

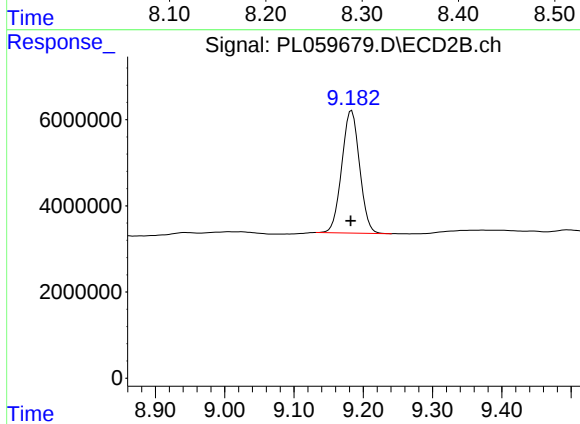

#28 Decachlorobiphenyl

R.T.: 9.183 min
Delta R.T.: 0.001 min
Response: 50797583
Conc: 23.37 ng/ml