

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070124\
 Data File : PL090419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2024 16:34
 Operator : AR\AJ
 Sample : P3135-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-628-COMP-01

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 07/02/2024
 Supervised By :Ankita Jodhani 07/02/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 01:51:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 25 11:05:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.789	31379144	22587379	13.826m	14.280
2) SA Decachlor...	9.057	7.932	23080598	22122056	14.966	14.830

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070124\
Data File : PL090419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2024 16:34
Operator : AR\AJ
Sample : P3135-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-628-COMP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/02/2024
Supervised By : Ankita Jodhani 07/02/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 01:51:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL062424.M
Quant Title : GC Extractables
QLast Update : Tue Jun 25 11:05:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

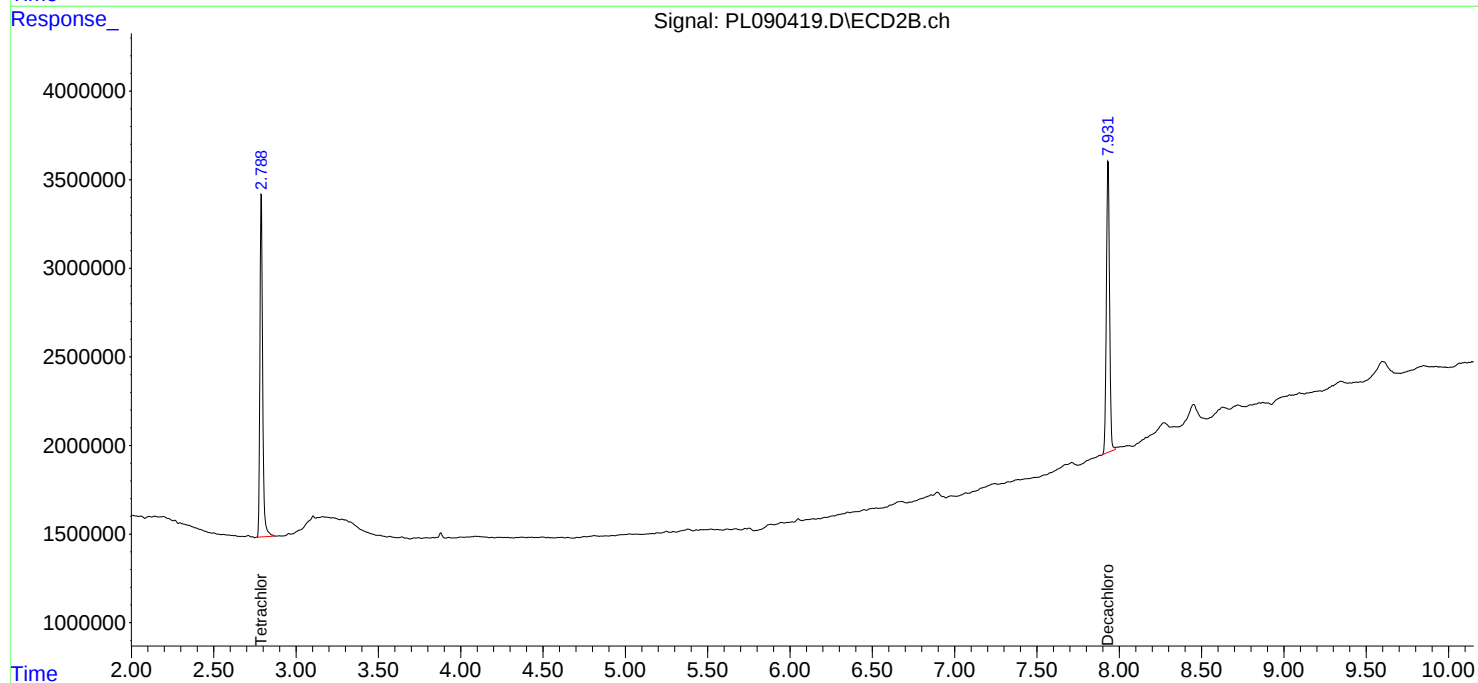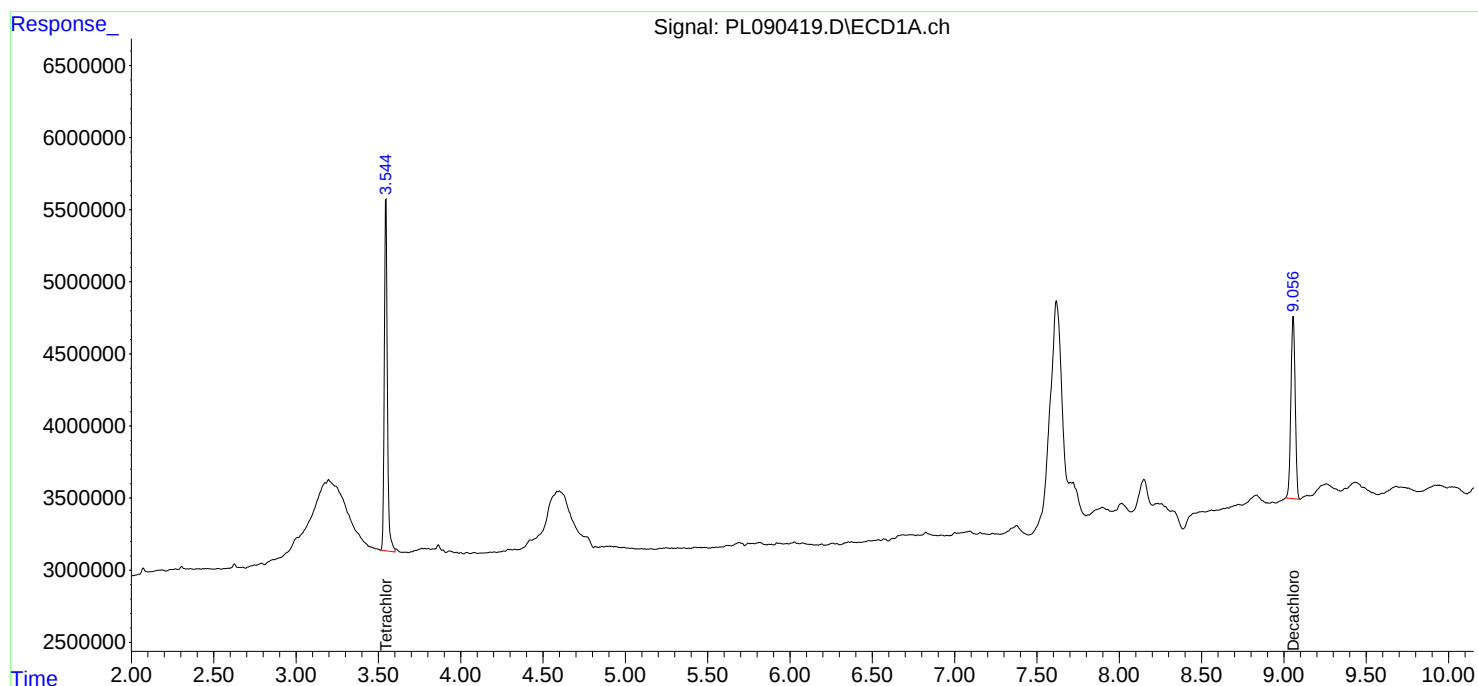

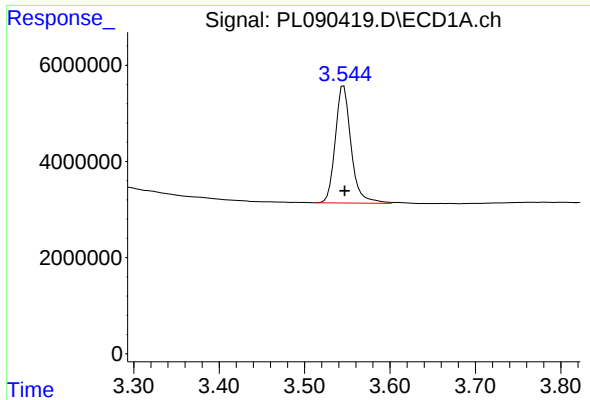


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.003 min
Response: 31379144
Conc: 13.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-628-COMP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/02/2024
Supervised By :Ankita Jodhani 07/02/2024

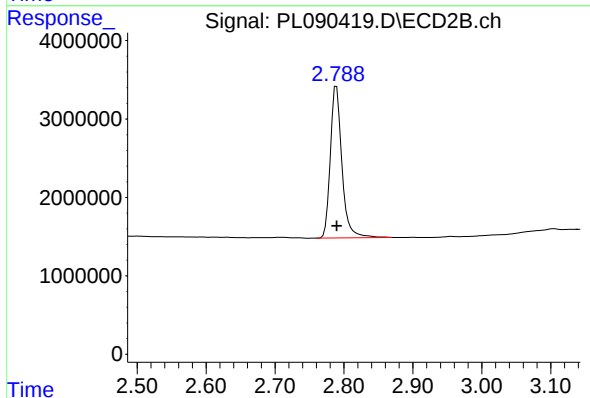


#1 Tetrachloro-m-xylene

R.T.: 2.789 min
Delta R.T.: 0.000 min
Response: 22587379
Conc: 14.28 ng/ml

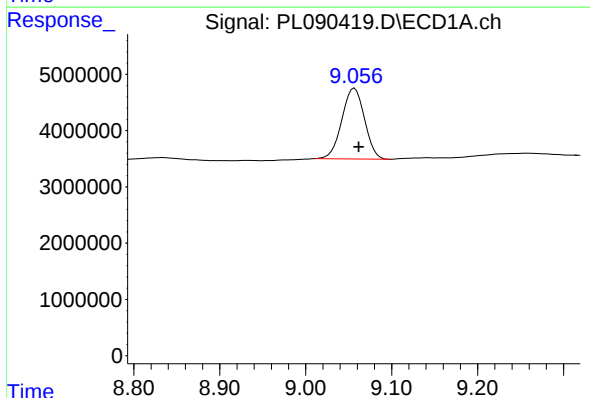

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: -0.005 min
Response: 23080598
Conc: 14.97 ng/ml

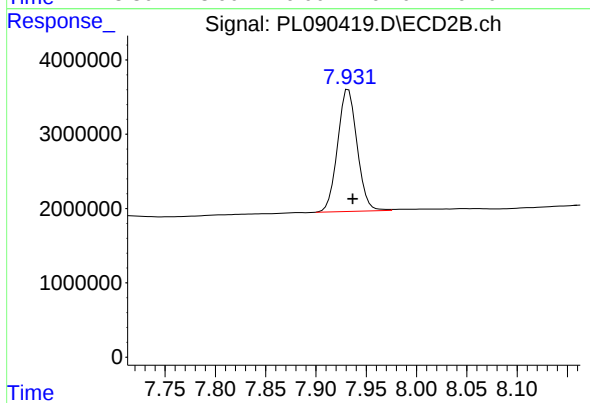

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.004 min
Response: 22122056
Conc: 14.83 ng/ml