

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070218\
 Data File : PL037617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 21:14
 Operator : UA\AJ
 Sample : J3252-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:09:28 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.334	3.936	148.2E6	46269767	18.731	16.724
28)	SA Decachlor...	8.012	8.947	114.5E6	36817890	18.972	18.558
Target Compounds							
4)	MA Heptachlor	0.000	5.112	0	11781941	N.D.	3.409 #
5)	MB Aldrin	4.569	0.000	6853389	0	0.673	N.D. #
8)	B Heptachlo...	5.074f	5.842f	8603286	5758114	0.918	2.020 #
10)	B gamma-Chl...	0.000	6.030	0	10163430	N.D.	3.609 #
11)	B alpha-Chl...	0.000	6.030f	0	10163430	N.D.	3.531 #
15)	B Endosulfa...	6.134	0.000	393257	0	0.053	N.D. #
17)	MA 4,4'-DDT	0.000	6.978f	0	6687894	N.D.	3.157 #
18)	B Endrin al...	0.000	6.978f	0	6687894	N.D.	3.324 #
25)	Chlordane-3	0.000	6.030	0	10163430	N.D.	25.988 #
26)	Chlordane-4	0.000	6.030	0	10163430	N.D.	21.209 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070218\
Data File : PL037617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 21:14
Operator : UA\AJ
Sample : J3252-06
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:09:28 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

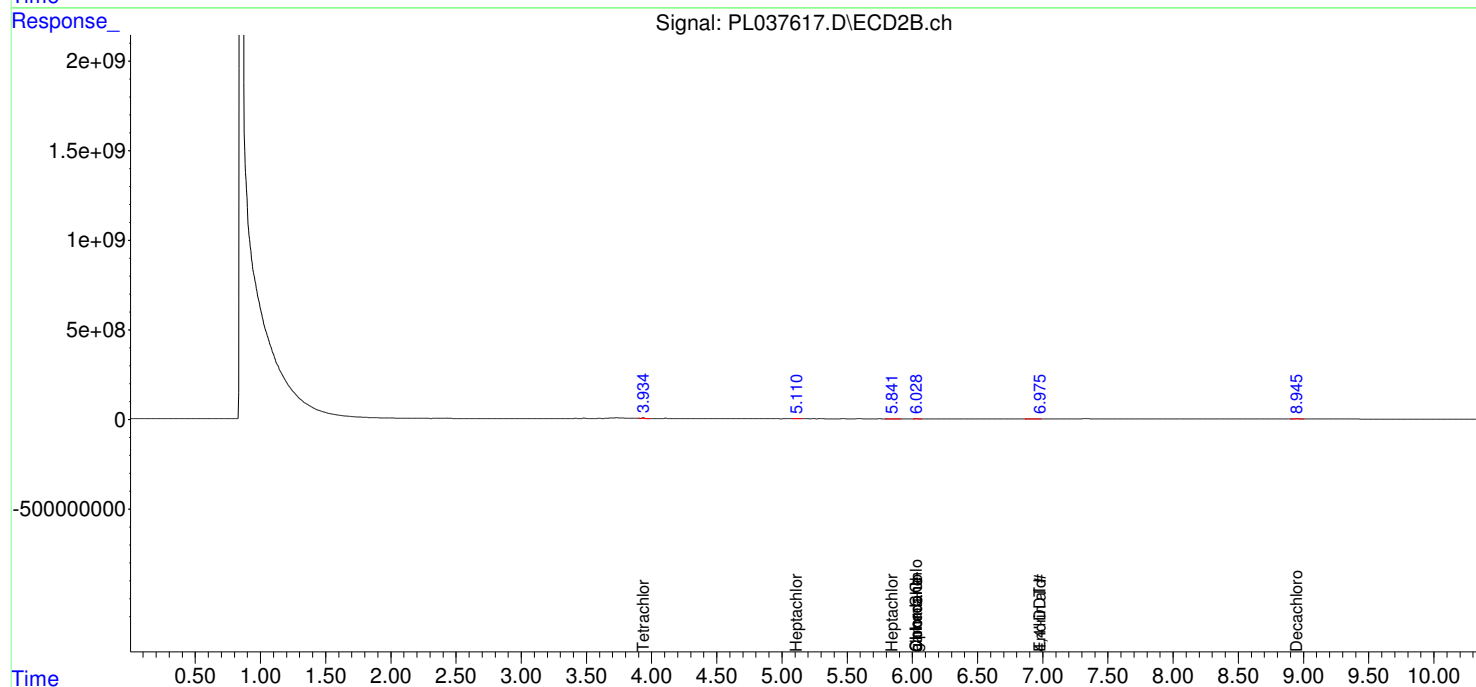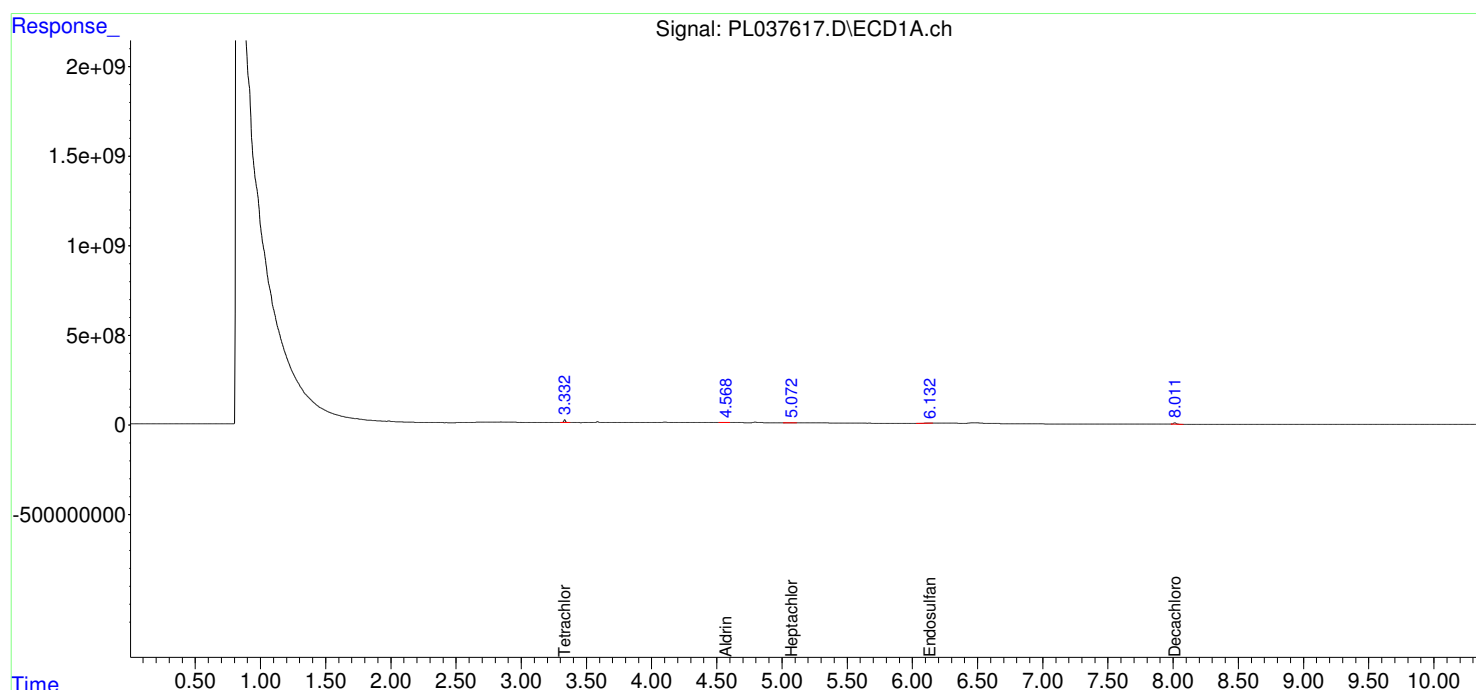


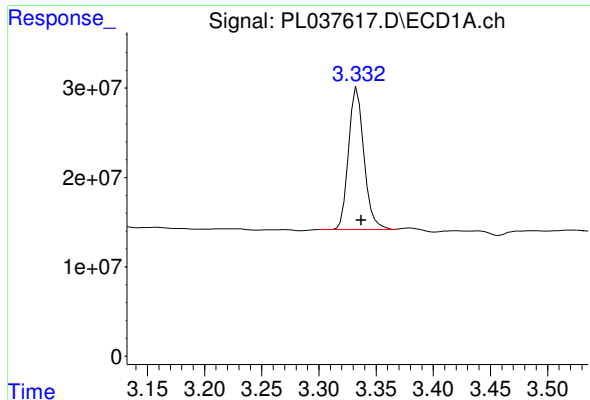

#1 Tetrachloro-m-xylene


R.T.: 3.334 min
Delta R.T.: -0.003 min
Response: 148170064
Conc: 18.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

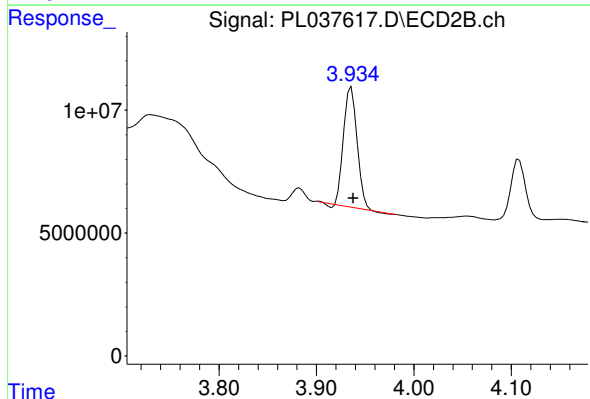


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.002 min
Response: 46269767
Conc: 16.72 ng/ml

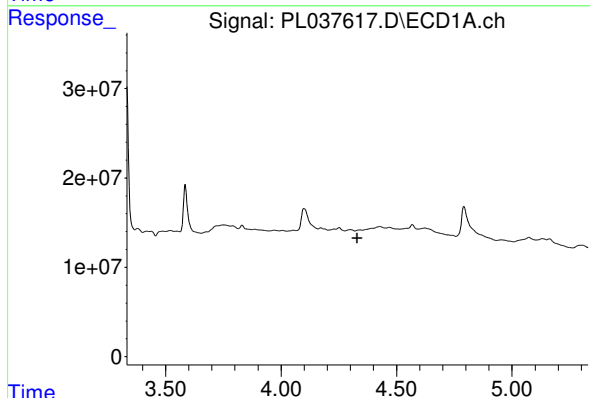


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.330 min
Response: 0
Conc: N.D.

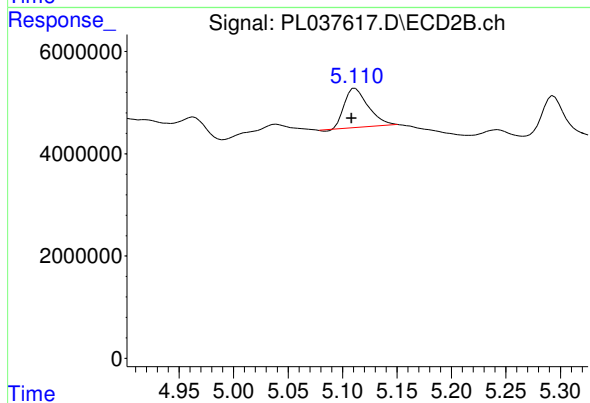

#4 Heptachlor


R.T.: 5.112 min
Delta R.T.: 0.003 min
Response: 11781941
Conc: 3.41 ng/ml

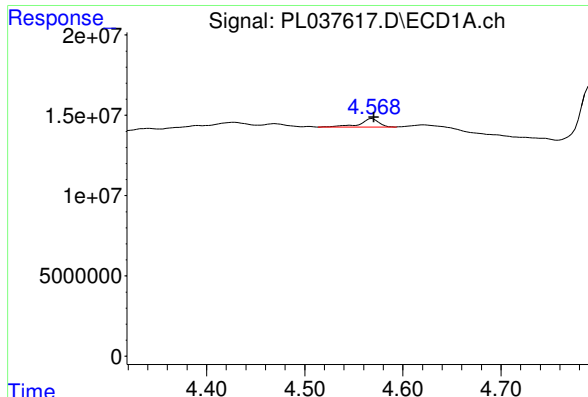

#5 Aldrin


R.T.: 4.569 min
Delta R.T.: -0.002 min
Response: 6853389
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

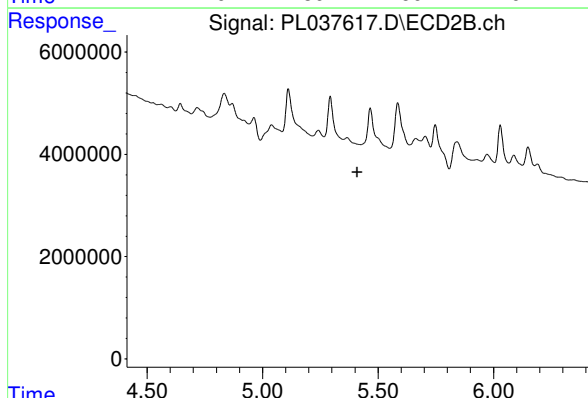


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.411 min
Response: 0
Conc: N.D.

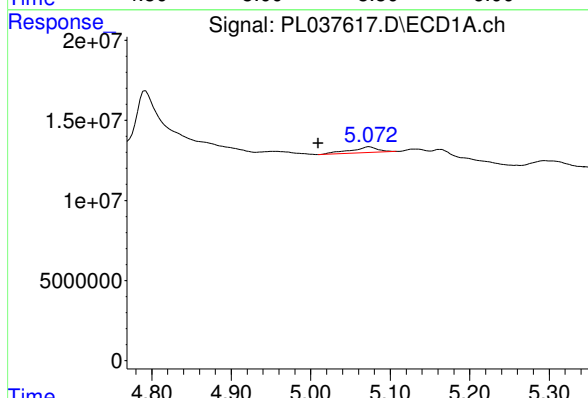


#8 Heptachlor epoxide

R.T.: 5.074 min
Delta R.T.: 0.005 min
Response: 8603286
Conc: 0.92 ng/ml

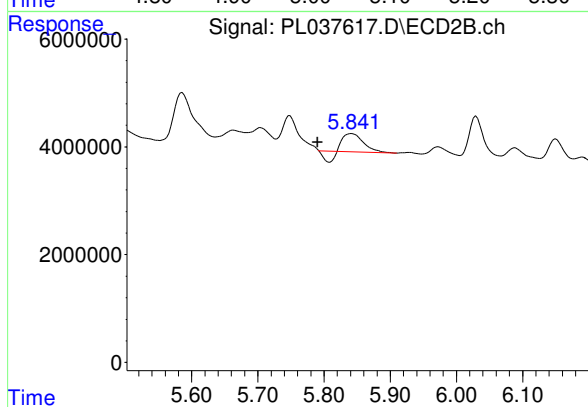

#8 Heptachlor epoxide


R.T.: 5.842 min
Delta R.T.: 0.002 min
Response: 5758114
Conc: 2.02 ng/ml

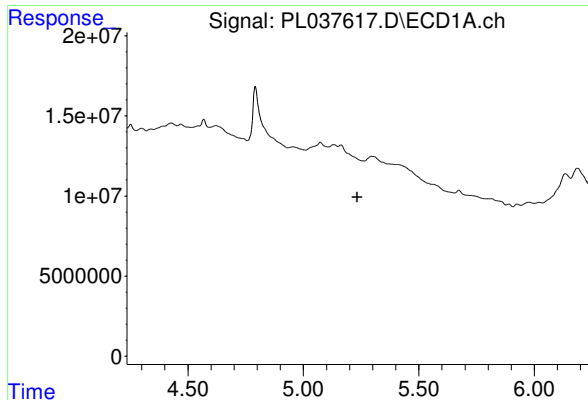

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.233 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

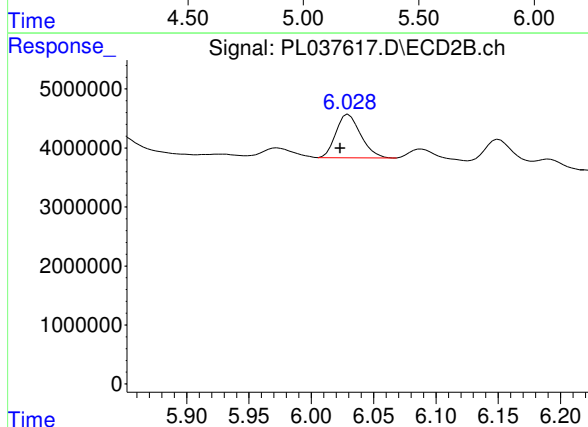


#10 gamma-Chlordane

R.T.: 6.030 min
Delta R.T.: 0.007 min
Response: 10163430
Conc: 3.61 ng/ml

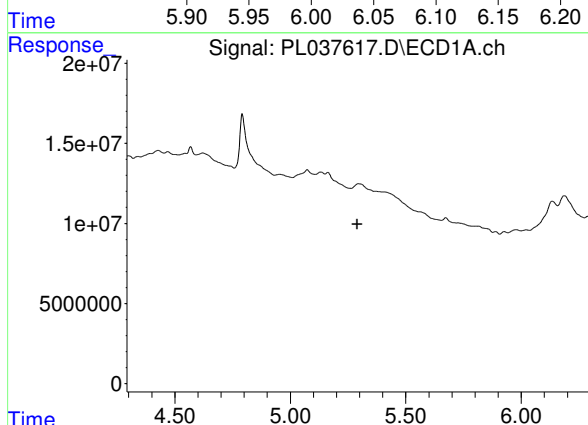


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

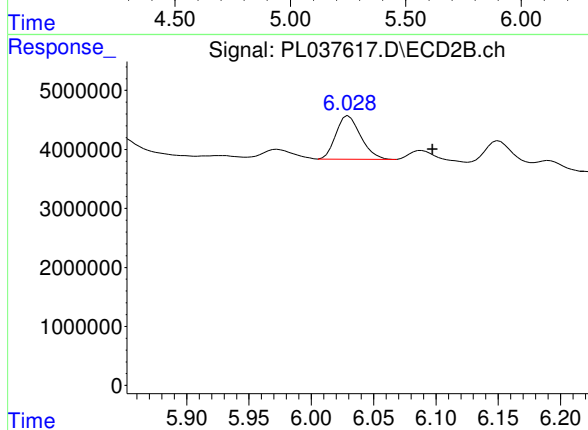

#11 alpha-Chlordane


R.T.: 6.030 min
Delta R.T.: -0.067 min
Response: 10163430
Conc: 3.53 ng/ml

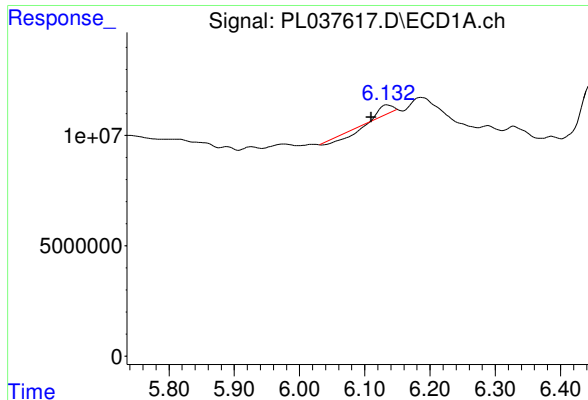

#15 Endosulfan II


R.T.: 6.134 min
Delta R.T.: 0.024 min
Response: 393257
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

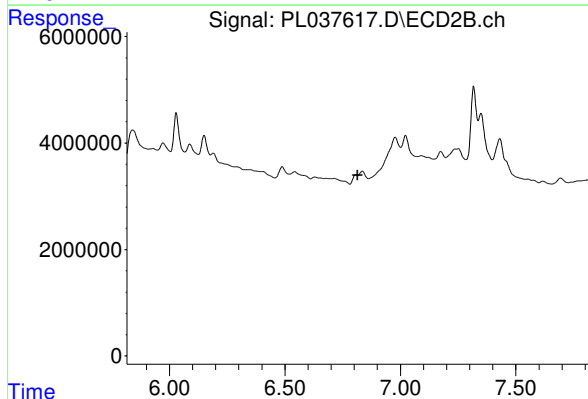


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.814 min
Response: 0
Conc: N.D.

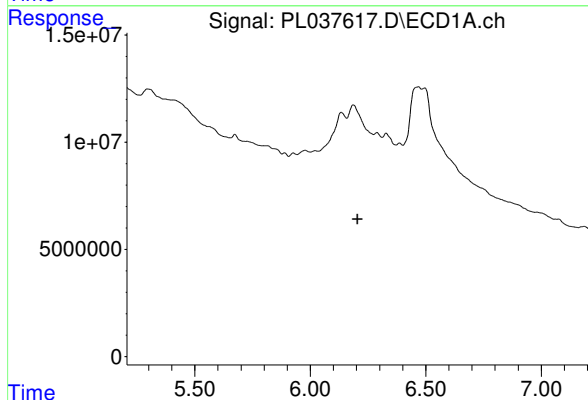


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

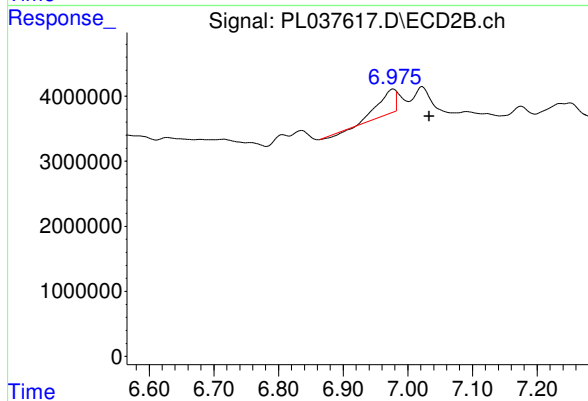

#17 4,4'-DDT


R.T.: 6.978 min
Delta R.T.: -0.055 min
Response: 6687894
Conc: 3.16 ng/ml

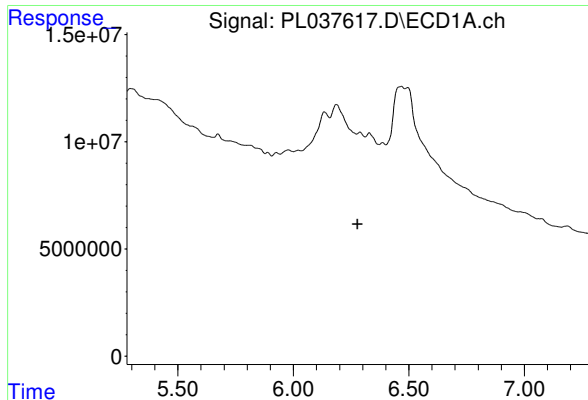

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

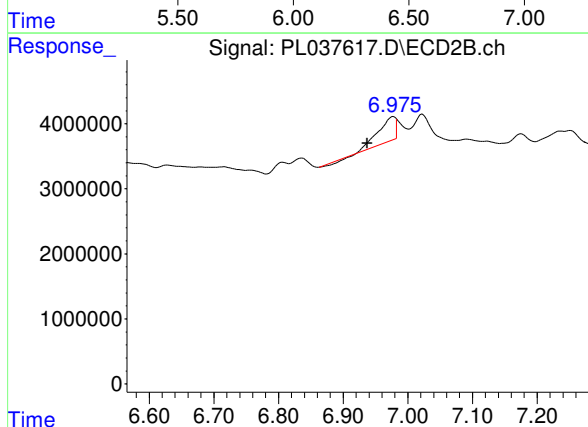


#18 Endrin aldehyde

R.T.: 6.978 min
Delta R.T.: 0.041 min
Response: 6687894
Conc: 3.32 ng/ml

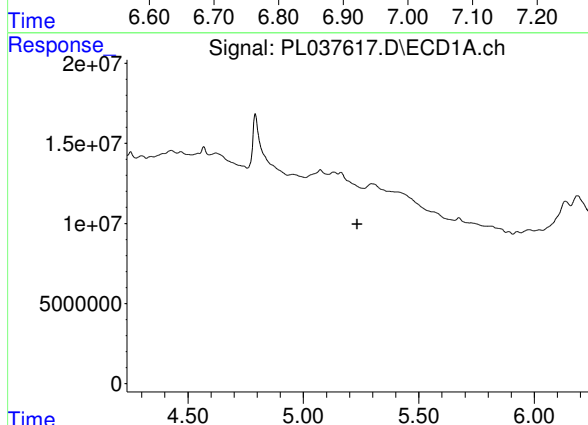


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.232 min
Response: 0
Conc: N.D.

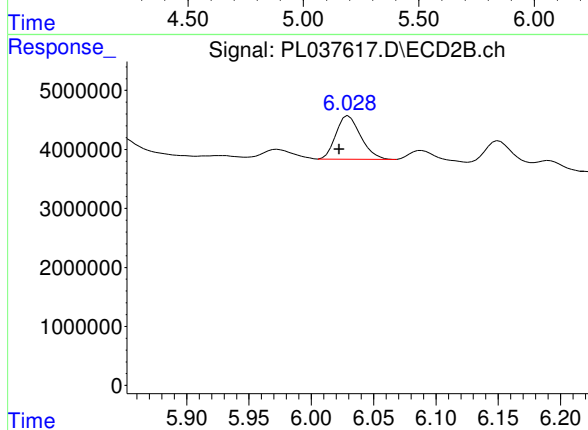

#25 Chlordane-3


R.T.: 6.030 min
Delta R.T.: 0.008 min
Response: 10163430
Conc: 25.99 ng/ml

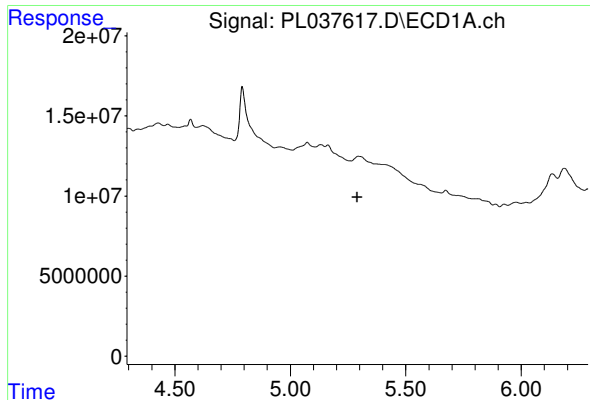

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

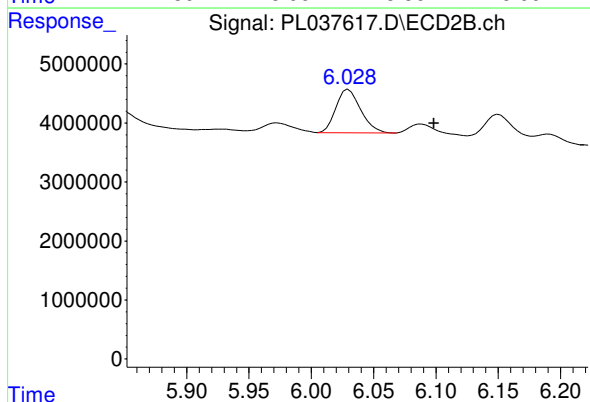


#26 Chlordane-4

R.T.: 6.030 min
Delta R.T.: -0.008 min
Response: 10163430
Conc: 21.21 ng/ml

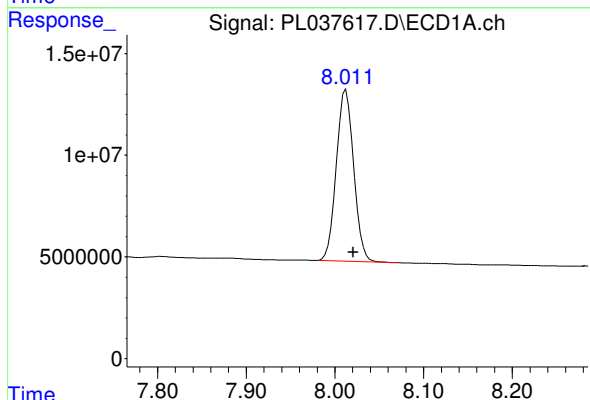

#28 Decachlorobiphenyl

R.T.: 8.012 min
Delta R.T.: -0.008 min
Response: 114478297
Conc: 18.97 ng/ml

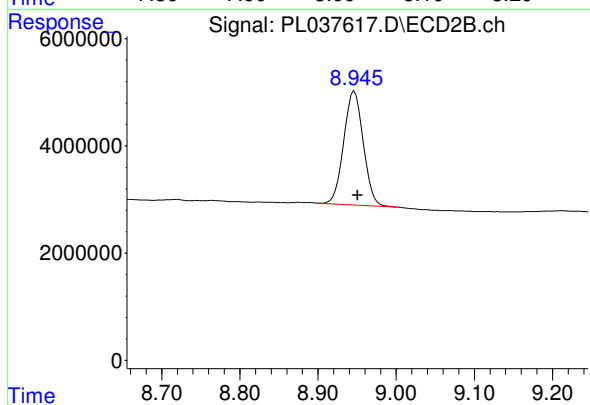

#28 Decachlorobiphenyl

R.T.: 8.947 min
Delta R.T.: -0.004 min
Response: 36817890
Conc: 18.56 ng/ml