

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 12:28
 Operator : AJ\MA
 Sample : PB129923BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 14:36:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.524	4.071	37424765	54106821	20.837	20.345
28)	SA Decachlor...	8.297	9.187	32616297	45576277	21.245	20.968
Target Compounds							
8)	B Heptachlo...	5.263f	0.000	50625	0	0.031	N.D. #
9)	A Endosulfan I	0.000	6.300f	0	1672816	N.D.	0.620 #
11)	B alpha-Chl...	5.518	0.000	278828	0	0.170	N.D. #
14)	MA Endrin	0.000	6.789	0	32707398	N.D.	13.299 #
15)	B Endosulfa...	0.000	6.985f	0	5297902	N.D.	2.062 #
16)	A 4,4'-DDD	6.212	0.000	12192945	0	9.134	N.D. #
17)	MA 4,4'-DDT	6.432f	7.203	96853	792554	0.076	0.350 #
22)	Mirex	7.412	0.000	711387	0	0.548	N.D. #
26)	Chlordane-4	5.518	6.300f	278828	1672816	2.333	3.714 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 12:28
Operator : AJ\MA
Sample : PB129923BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 14:36:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

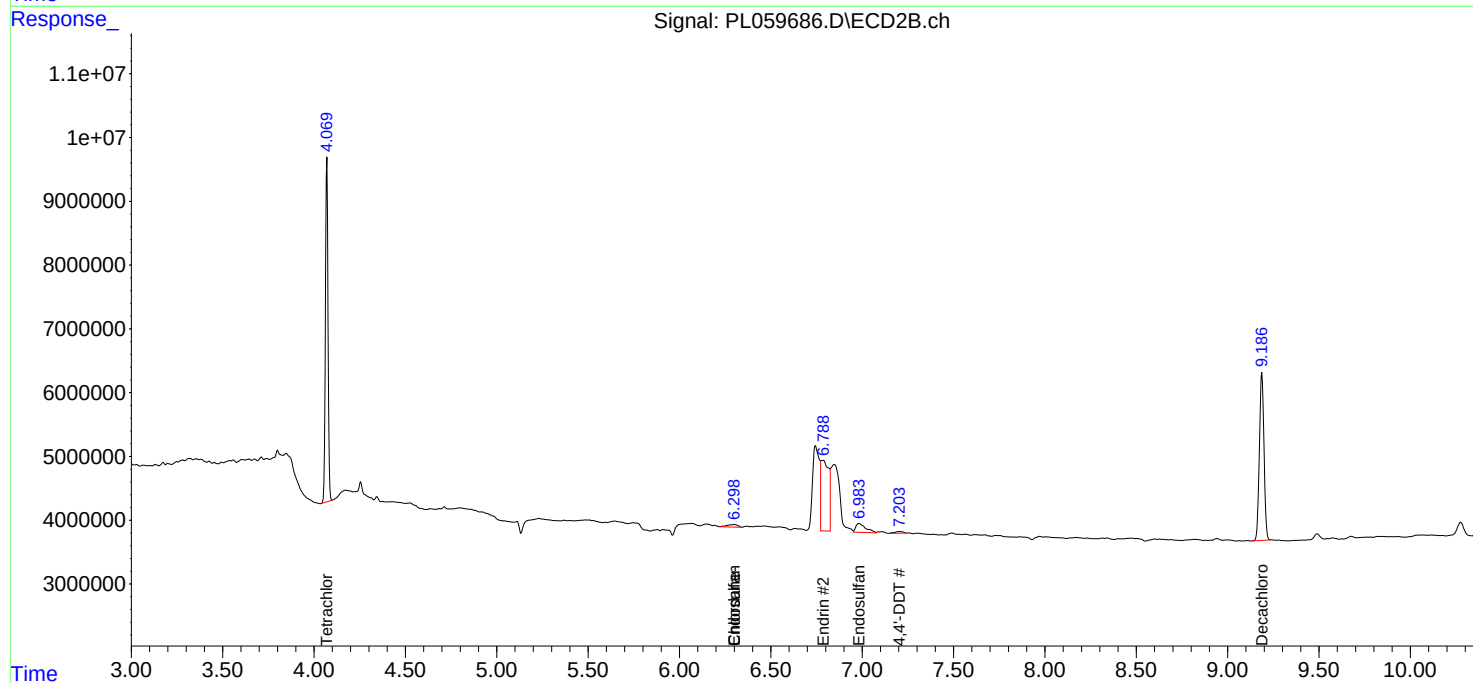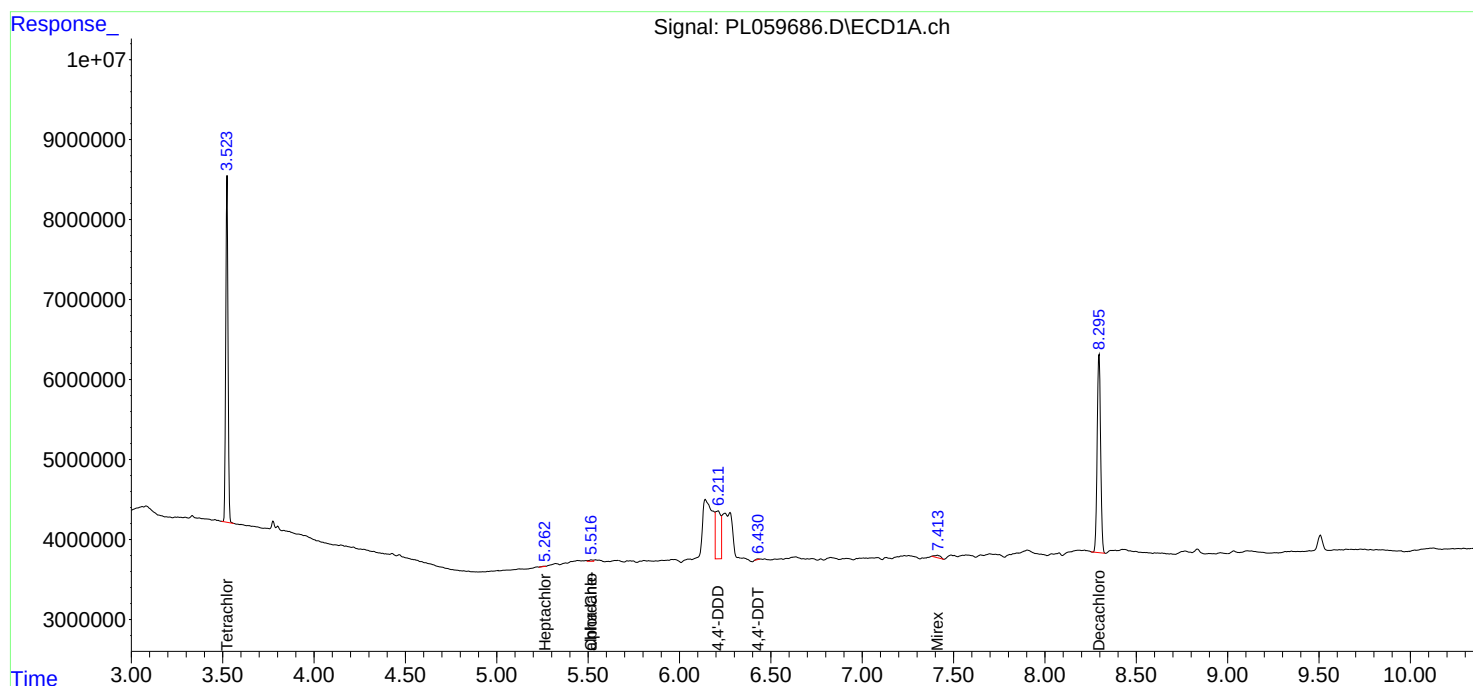


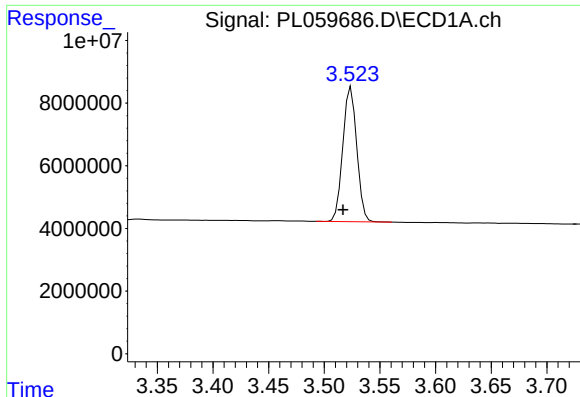

#1 Tetrachloro-m-xylene


R.T.: 3.524 min
Delta R.T.: 0.007 min
Response: 37424765
Conc: 20.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

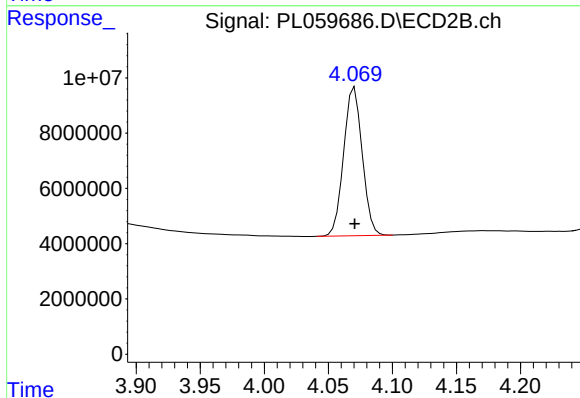


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 54106821
Conc: 20.35 ng/ml

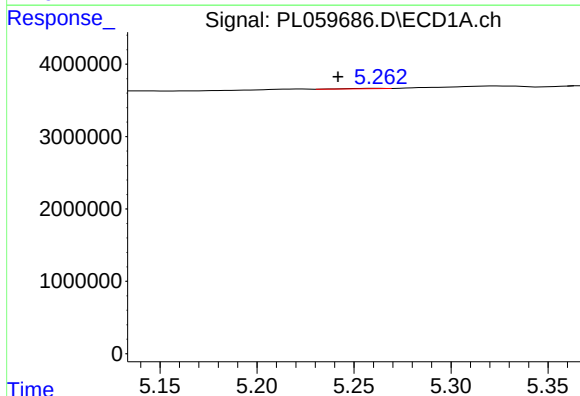


#8 Heptachlor epoxide

R.T.: 5.263 min
Delta R.T.: 0.021 min
Response: 50625
Conc: 0.03 ng/ml

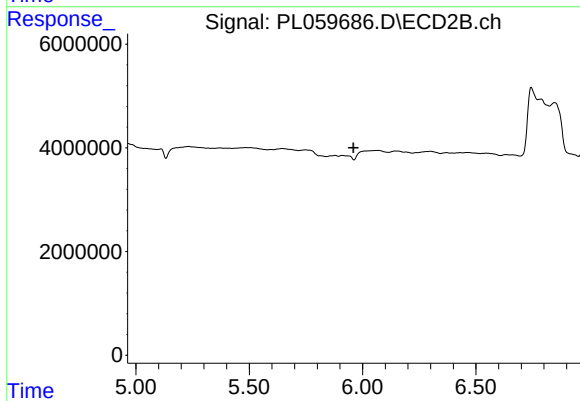

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.960 min
Response: 0
Conc: N.D.

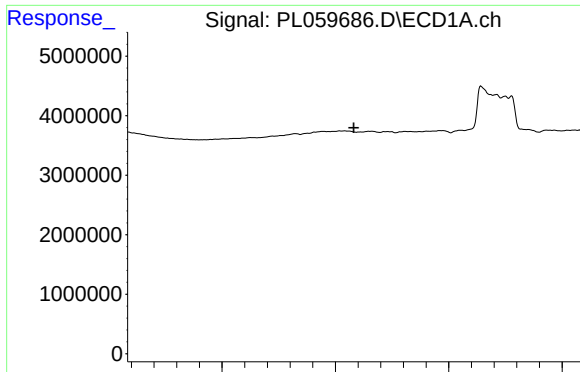

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

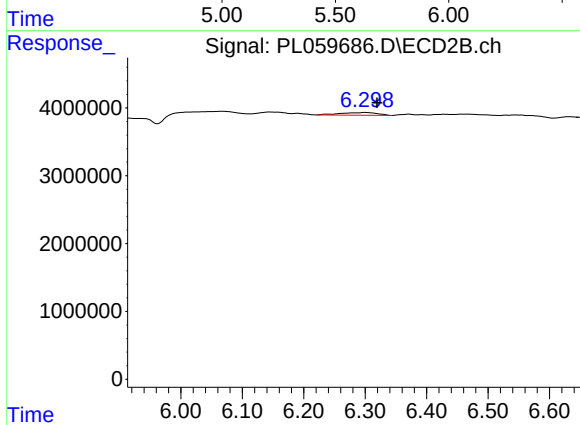


#9 Endosulfan I

R.T.: 6.300 min
Delta R.T.: -0.020 min
Response: 1672816
Conc: 0.62 ng/ml

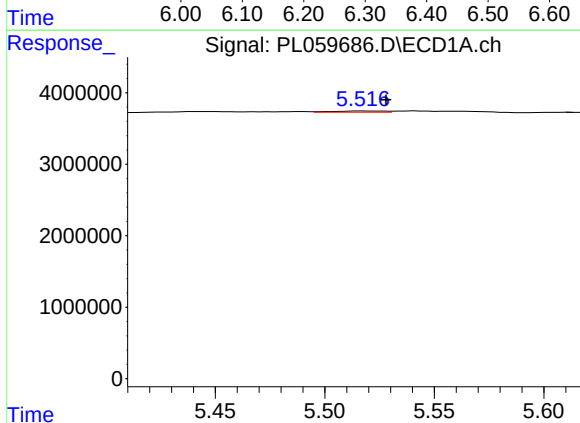


#11 alpha-Chlordane

R.T.: 5.518 min
Delta R.T.: -0.010 min
Response: 278828
Conc: 0.17 ng/ml

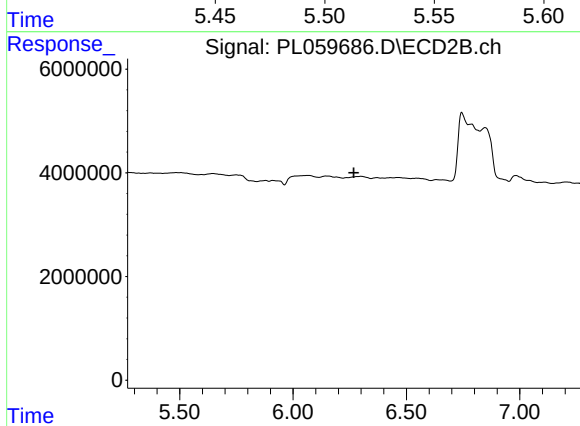

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.269 min
Response: 0
Conc: N.D.

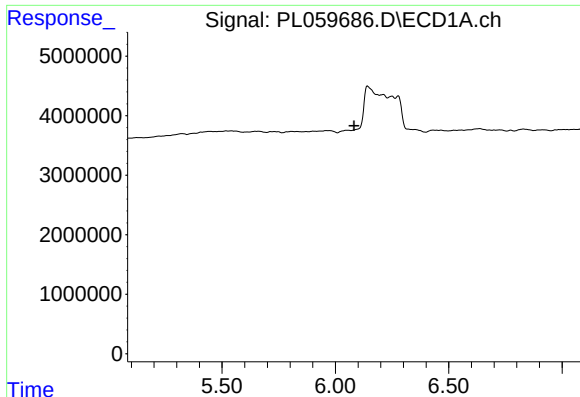

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

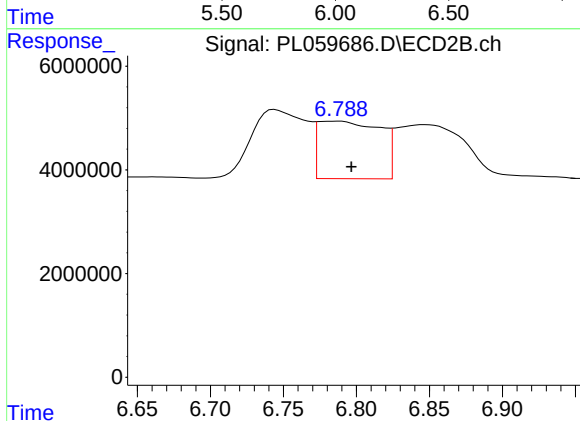


#14 Endrin

R.T.: 6.789 min
Delta R.T.: -0.008 min
Response: 32707398
Conc: 13.30 ng/ml

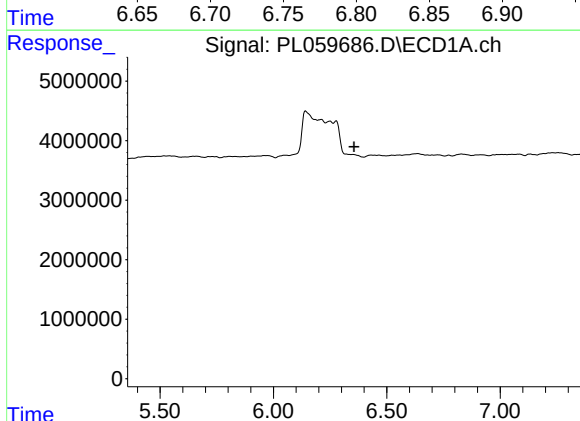


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.356 min
Response: 0
Conc: N.D.

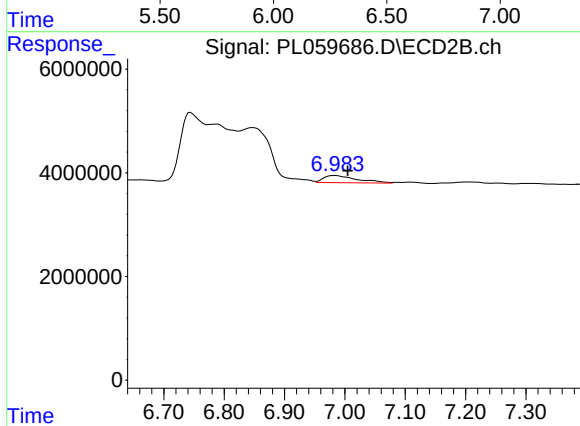

#15 Endosulfan II


R.T.: 6.985 min
Delta R.T.: -0.020 min
Response: 5297902
Conc: 2.06 ng/ml

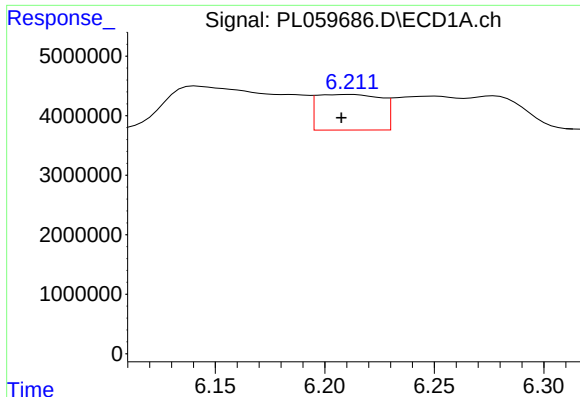

#16 4,4'-DDD


R.T.: 6.212 min
Delta R.T.: 0.004 min
Response: 12192945
Conc: 9.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

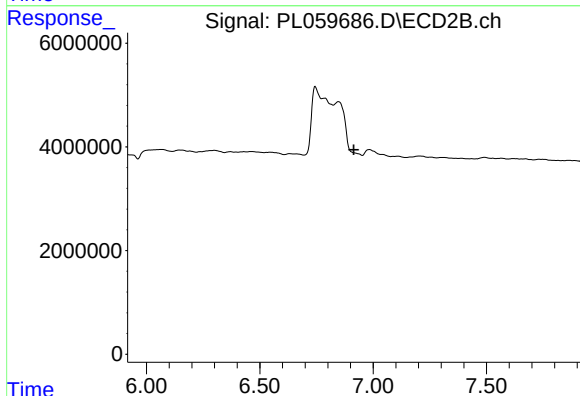


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

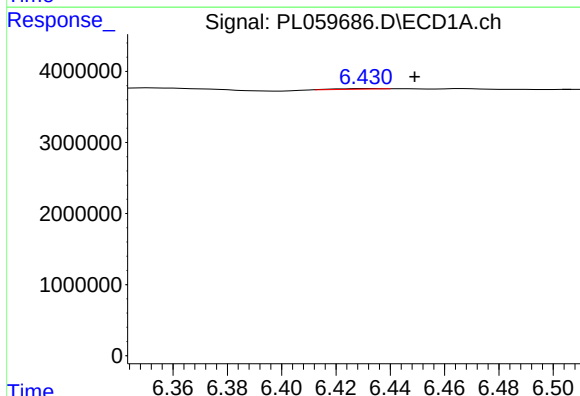


#17 4,4'-DDT

R.T.: 6.432 min
Delta R.T.: -0.017 min
Response: 96853
Conc: 0.08 ng/ml

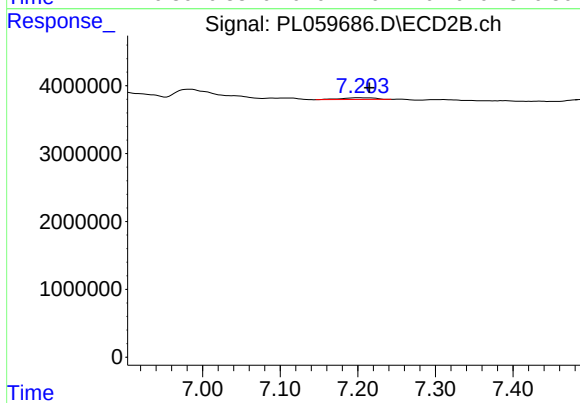

#17 4,4'-DDT


R.T.: 7.203 min
Delta R.T.: -0.012 min
Response: 792554
Conc: 0.35 ng/ml

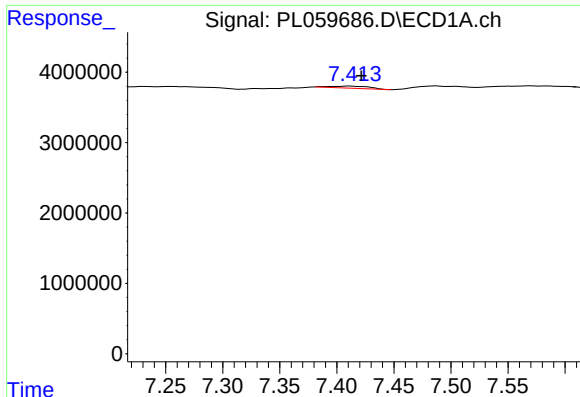

#22 Mirex


R.T.: 7.412 min
Delta R.T.: -0.010 min
Response: 711387
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

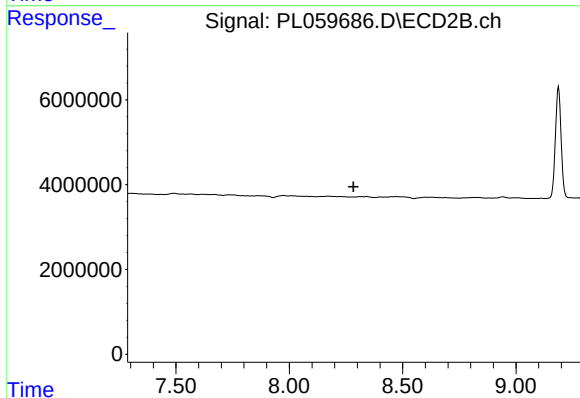


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 8.283 min
Response: 0
Conc: N.D.

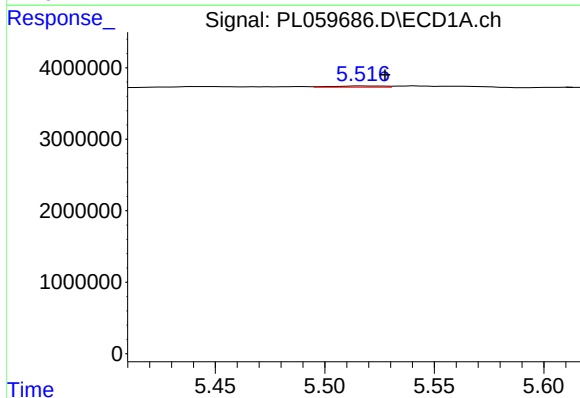


#26 Chlordane-4

R.T.: 5.518 min
Delta R.T.: -0.010 min
Response: 278828
Conc: 2.33 ng/ml

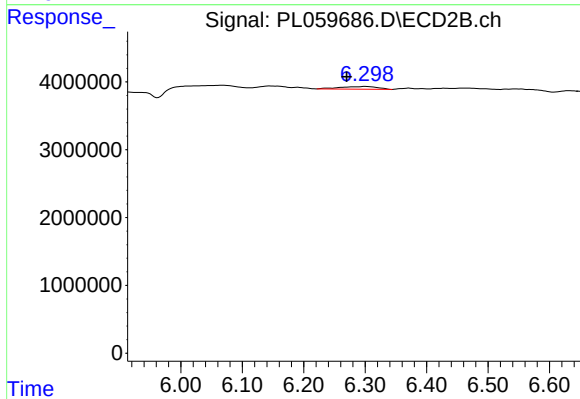

#26 Chlordane-4


R.T.: 6.300 min
Delta R.T.: 0.030 min
Response: 1672816
Conc: 3.71 ng/ml

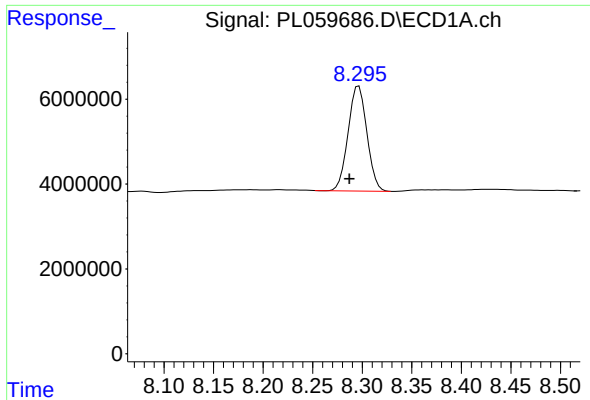

#28 Decachlorobiphenyl

R.T.: 8.297 min
Delta R.T.: 0.009 min
Response: 32616297
Conc: 21.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

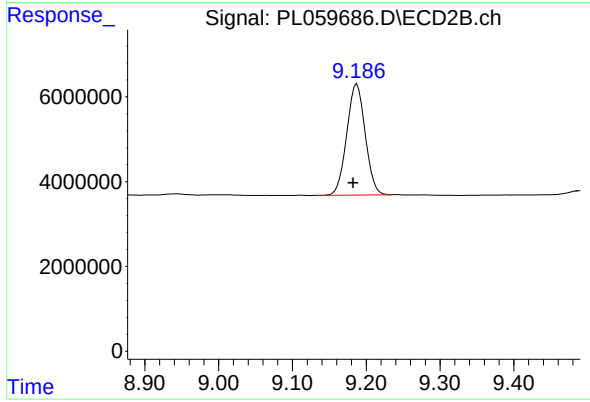

#28 Decachlorobiphenyl

R.T.: 9.187 min
Delta R.T.: 0.005 min
Response: 45576277
Conc: 20.97 ng/ml