

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059717.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 20:00
 Operator : AJ\MA
 Sample : PB129943TB
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:03:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.518	4.072	35823861	52409071	19.946	19.707
28)	SA Decachlor...	8.288	9.185	29638380	40807980	19.306	18.774
Target Compounds							
2)	A alpha-BHC	3.965	0.000	1027149	0	0.399	N.D. #
4)	MA Heptachlor	0.000	5.263	0	1712730	N.D.	0.489 #
7)	B delta-BHC	0.000	5.110f	0	2310132	N.D.	0.790 #
15)	B Endosulfa...	6.363	7.007	91425	558132	0.060	0.217 #
16)	A 4,4'-DDD	6.227f	0.000	397060	0	0.297	N.D. #
19)	B Endosulfa...	0.000	7.381f	0	404979	N.D.	0.169 #
22)	Mirex	0.000	8.312f	0	47172	N.D.	0.025 #
23)	Chlordane-1	4.422f	0.000	941925	0	18.074	N.D. #
27)	Chlordane-5	6.363	0.000	91425	0	1.780	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059717.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 20:00
Operator : AJ\MA
Sample : PB129943TB
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:03:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

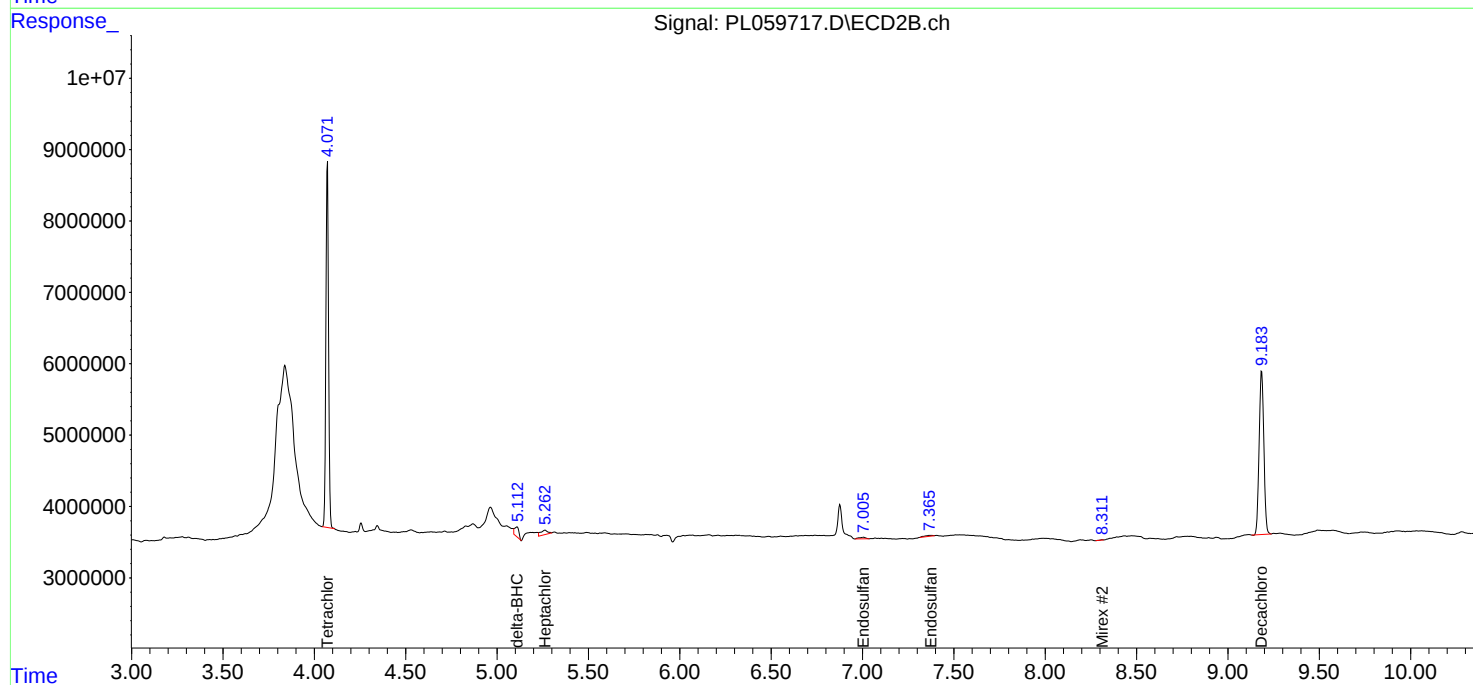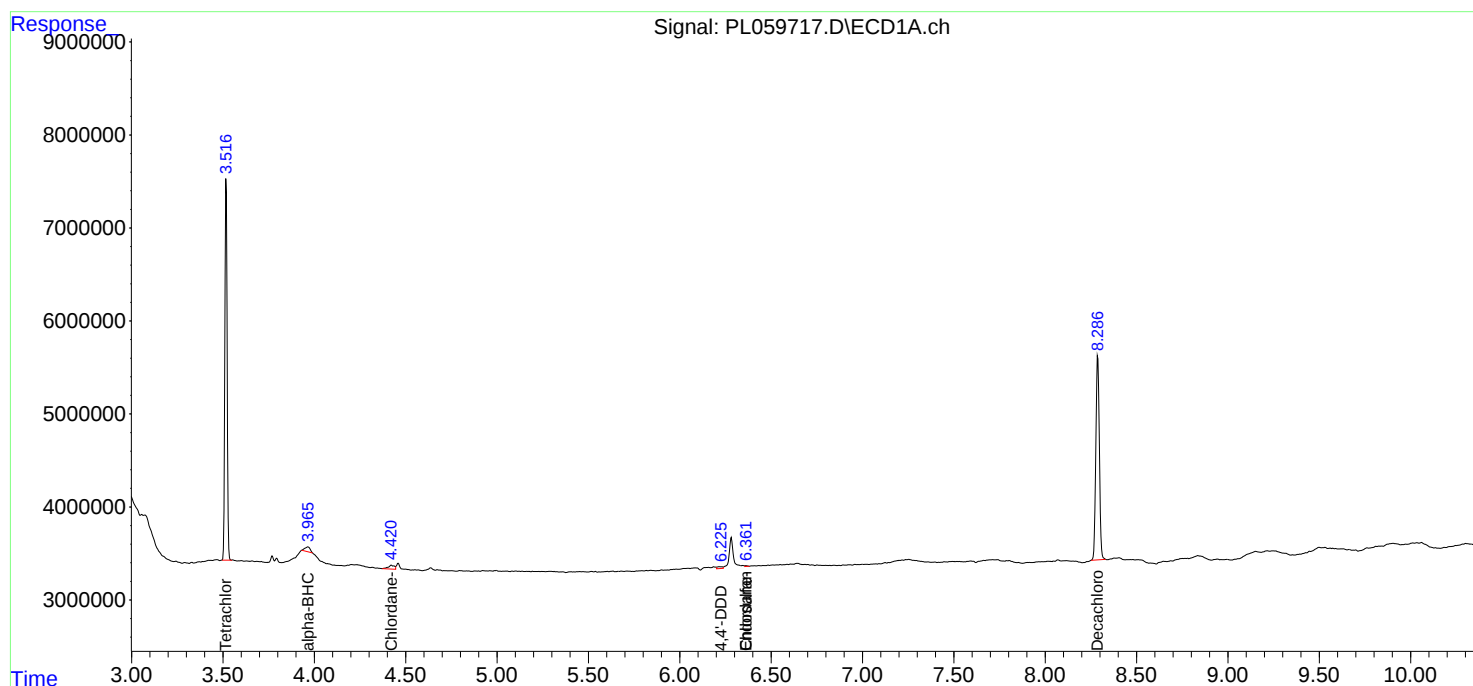


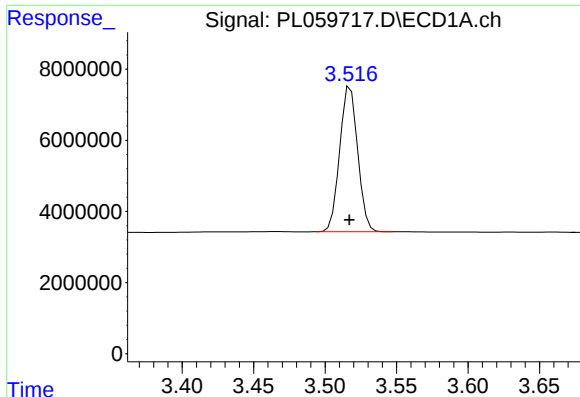

#1 Tetrachloro-m-xylene


R.T.: 3.518 min
Delta R.T.: 0.000 min
Response: 35823861
Conc: 19.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

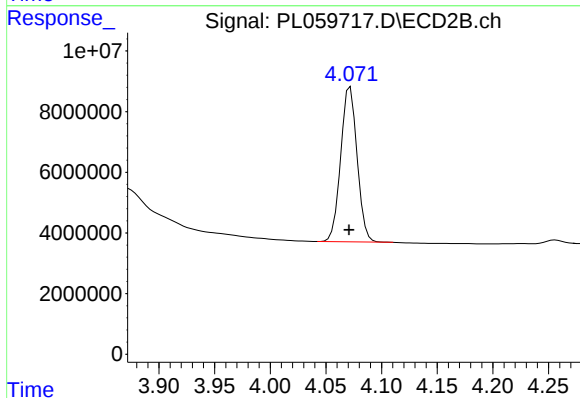


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.001 min
Response: 52409071
Conc: 19.71 ng/ml

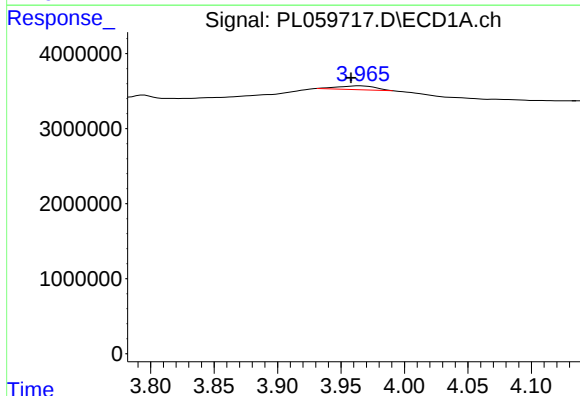


#2 alpha-BHC

R.T.: 3.965 min
Delta R.T.: 0.007 min
Response: 1027149
Conc: 0.40 ng/ml

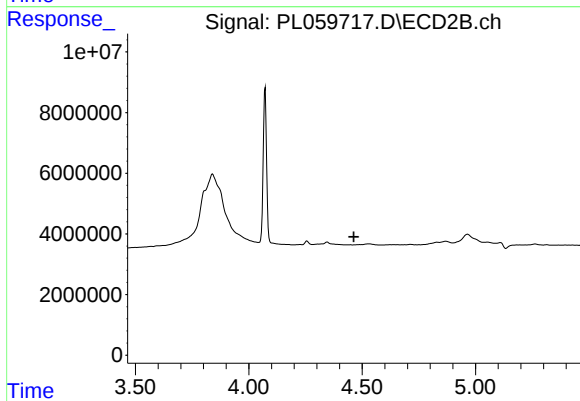

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

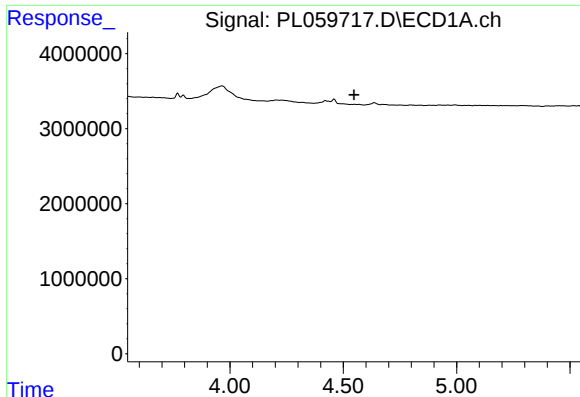

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

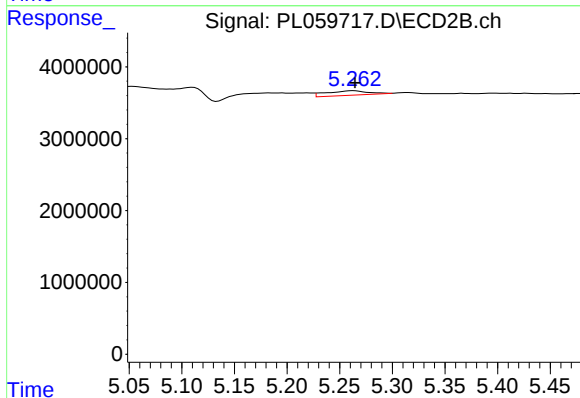


#4 Heptachlor

R.T.: 5.263 min
Delta R.T.: -0.001 min
Response: 1712730
Conc: 0.49 ng/ml

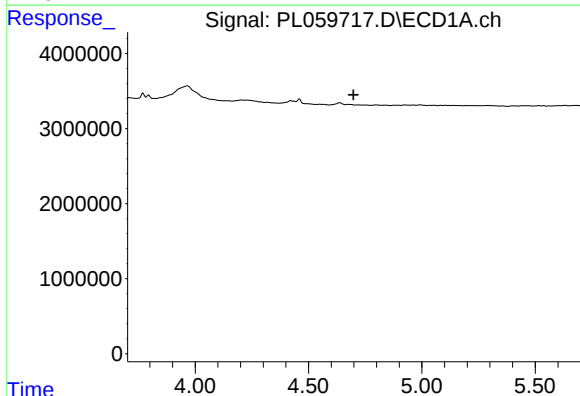


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.699 min
Response: 0
Conc: N.D.

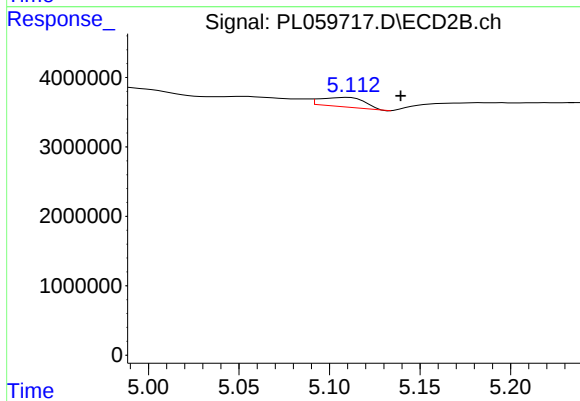

#7 delta-BHC


R.T.: 5.110 min
Delta R.T.: -0.029 min
Response: 2310132
Conc: 0.79 ng/ml

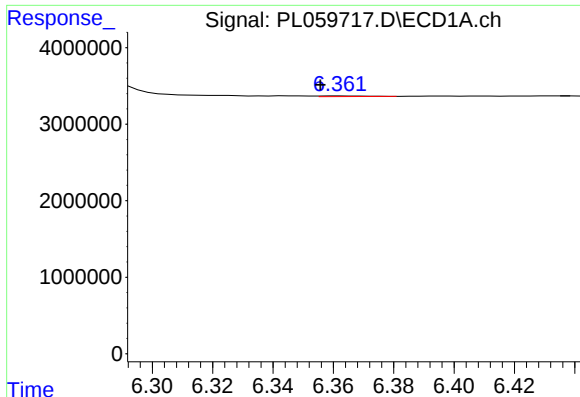

#15 Endosulfan II


R.T.: 6.363 min
Delta R.T.: 0.007 min
Response: 91425
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

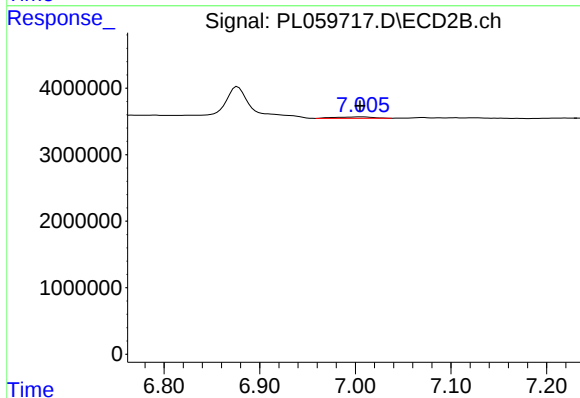


#15 Endosulfan II

R.T.: 7.007 min
Delta R.T.: 0.002 min
Response: 558132
Conc: 0.22 ng/ml

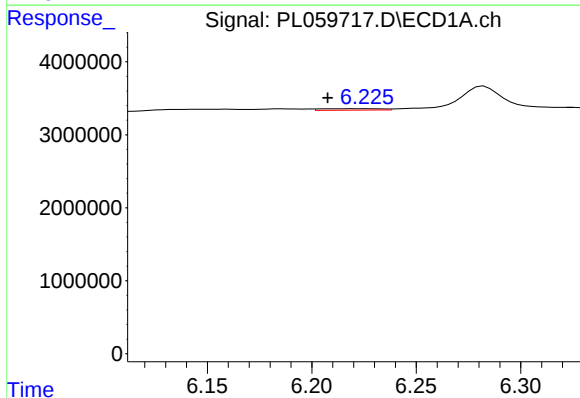


#16 4,4'-DDD

R.T.: 6.227 min
Delta R.T.: 0.019 min
Response: 397060
Conc: 0.30 ng/ml

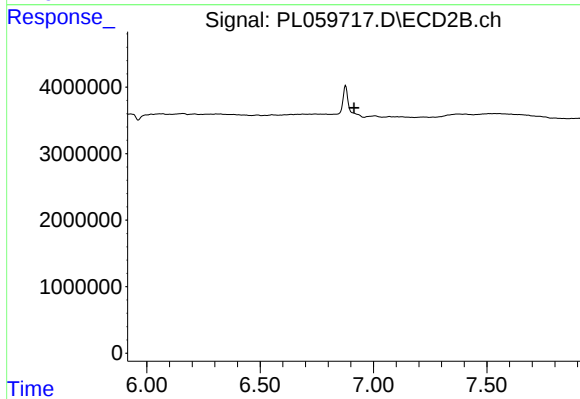

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

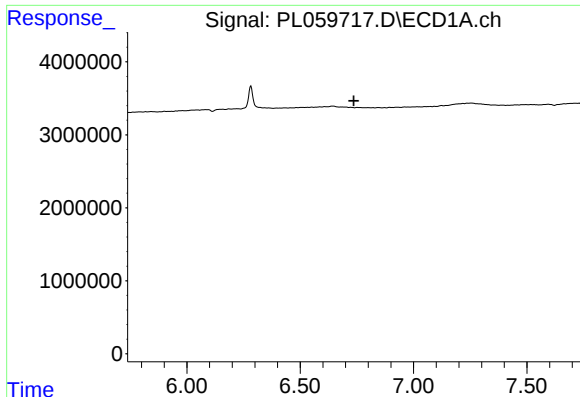

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.737 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

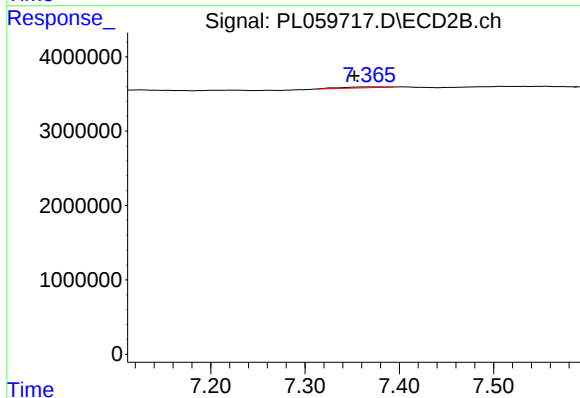


#19 Endosulfan Sulfate

R.T.: 7.381 min
Delta R.T.: 0.029 min
Response: 404979
Conc: 0.17 ng/ml

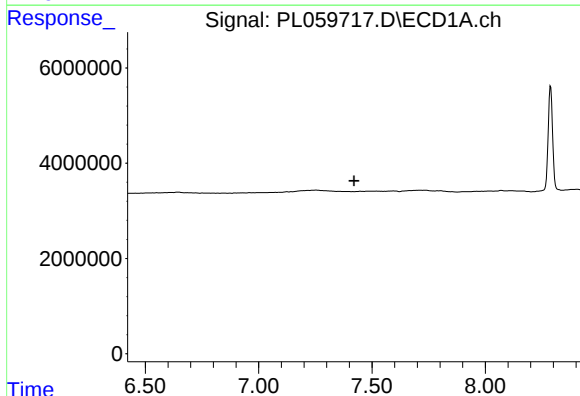


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.

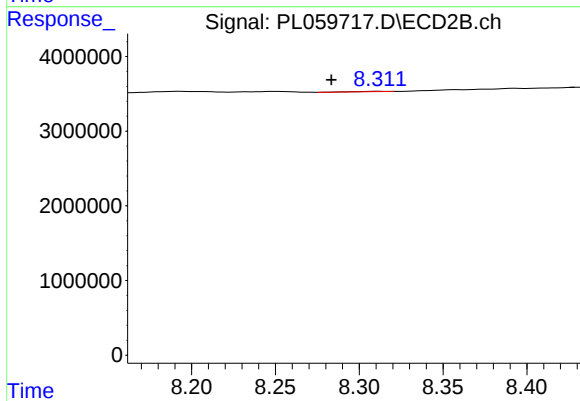

#22 Mirex


R.T.: 8.312 min
Delta R.T.: 0.029 min
Response: 47172
Conc: 0.02 ng/ml

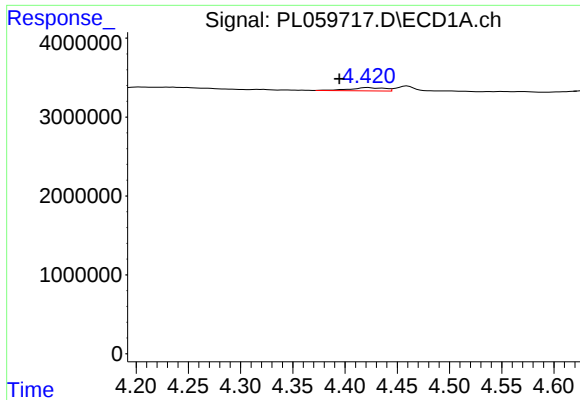

#23 Chlordane-1


R.T.: 4.422 min
Delta R.T.: 0.027 min
Response: 941925
Conc: 18.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

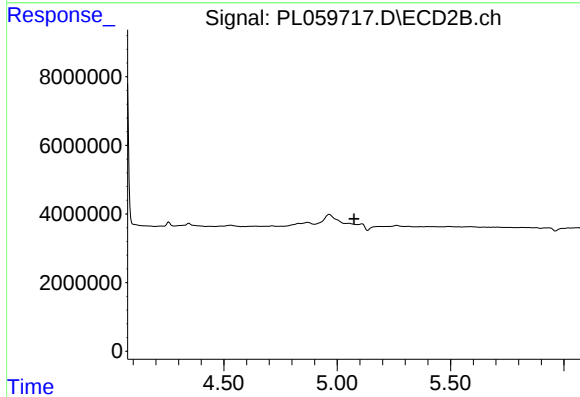


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

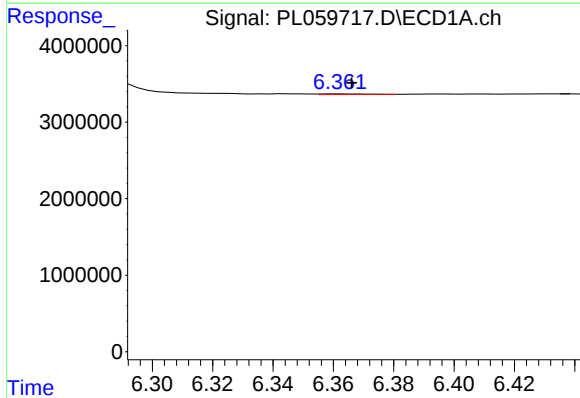


#27 Chlordane-5

R.T.: 6.363 min
Delta R.T.: -0.003 min
Response: 91425
Conc: 1.78 ng/ml

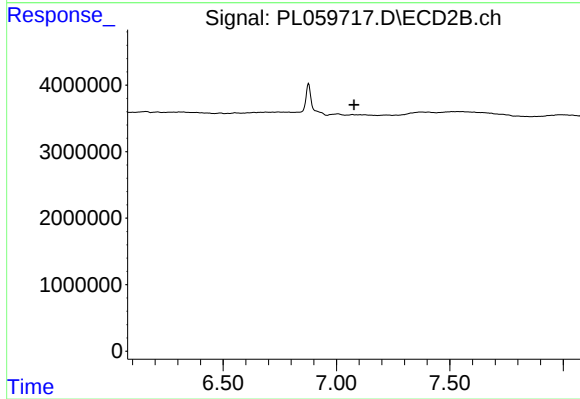

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.078 min
Response: 0
Conc: N.D.

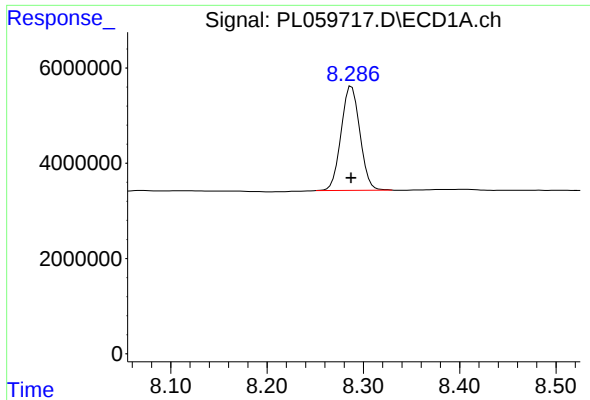

#28 Decachlorobiphenyl

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 29638380
Conc: 19.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

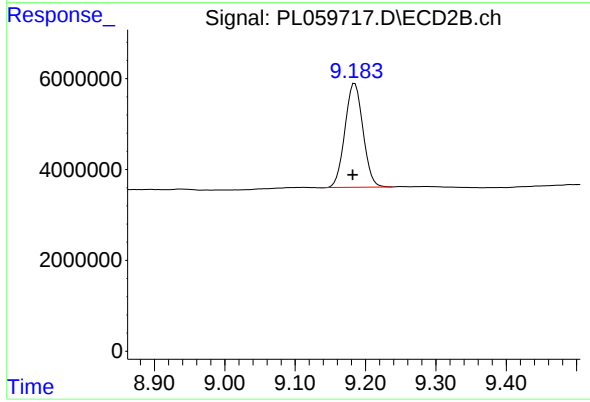

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 40807980
Conc: 18.77 ng/ml