

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059721.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 20:57
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:04:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.517	4.072	34284351	50106334	19.089	18.841
28)	SA Decachlor...	8.287	9.185	26929529	38862680	17.541	17.879
Target Compounds							
2)	A alpha-BHC	3.966	0.000	1244322	0	0.484	N.D. #
4)	MA Heptachlor	0.000	5.265	0	636769	N.D.	0.182 #
8)	B Heptachlo...	0.000	5.953	0	15459789	N.D.	6.362 #
14)	MA Endrin	6.084	0.000	528626	0	0.358	N.D. #
15)	B Endosulfa...	6.342	7.010	181688	5857440	0.120	2.280 #
17)	MA 4,4'-DDT	0.000	7.221	0	814753	N.D.	0.360 #
18)	B Endrin al...	6.527	7.122	46274	3917697	0.037	1.768 #
23)	Chlordane-1	4.422f	0.000	515578	0	9.893	N.D. #
27)	Chlordane-5	6.342f	7.085	181688	4195280	3.537	48.210 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059721.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 20:57
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:04:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

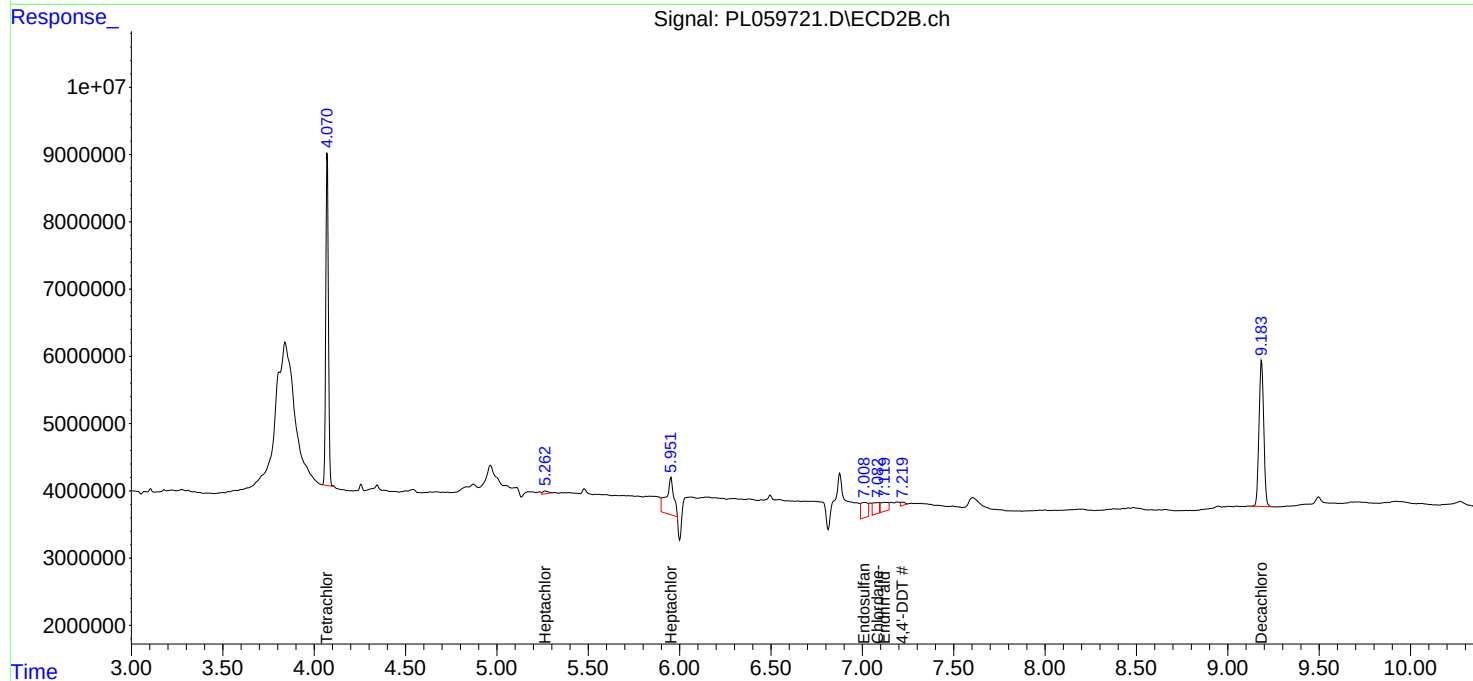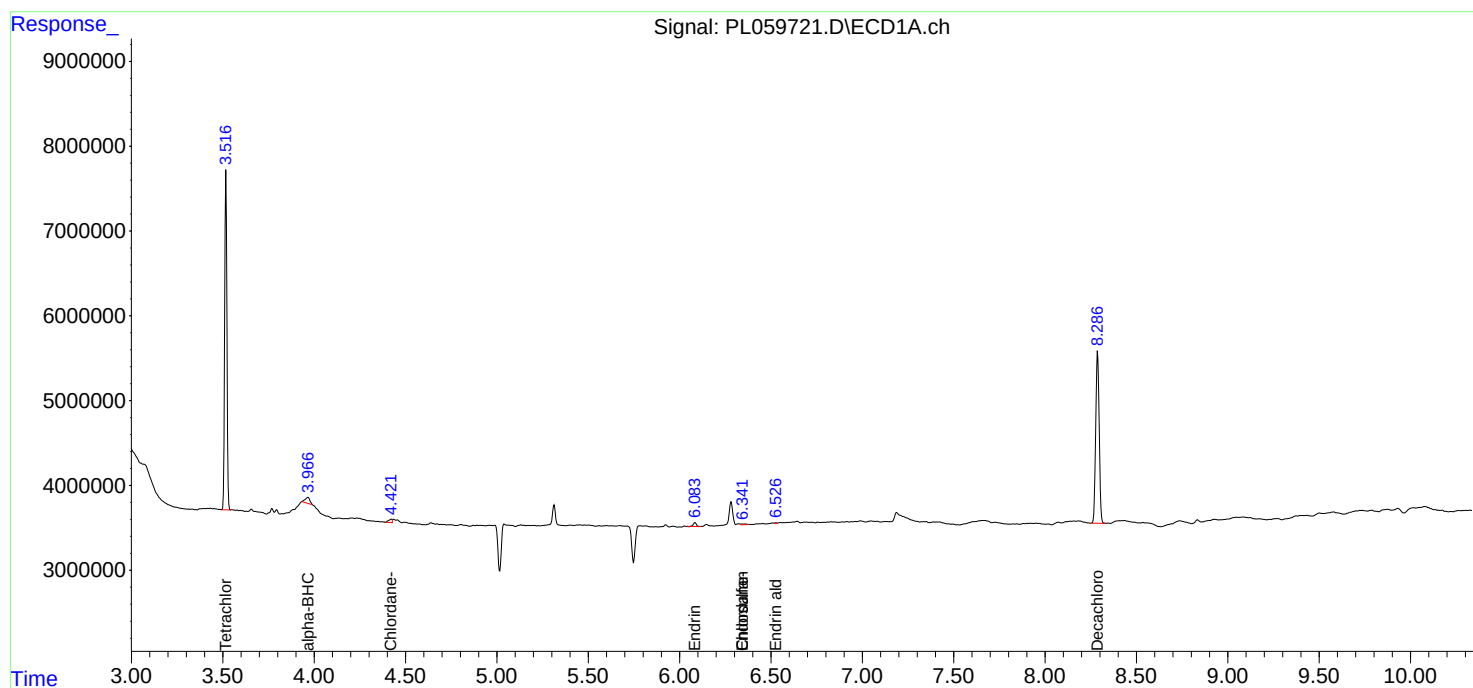


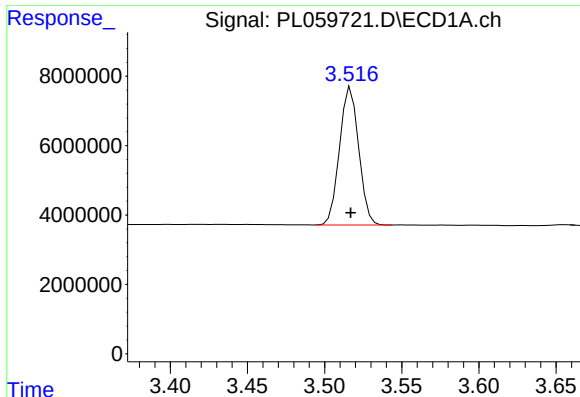

#1 Tetrachloro-m-xylene


R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 34284351
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

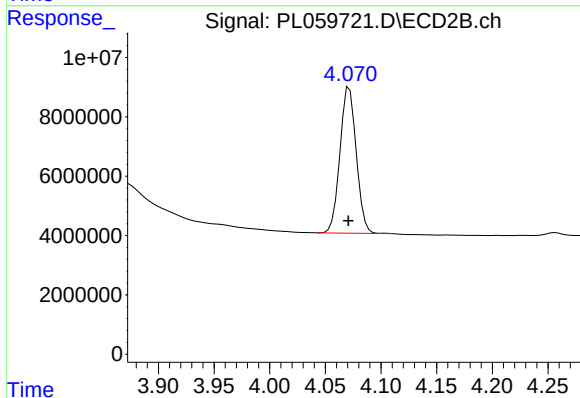


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 50106334
Conc: 18.84 ng/ml

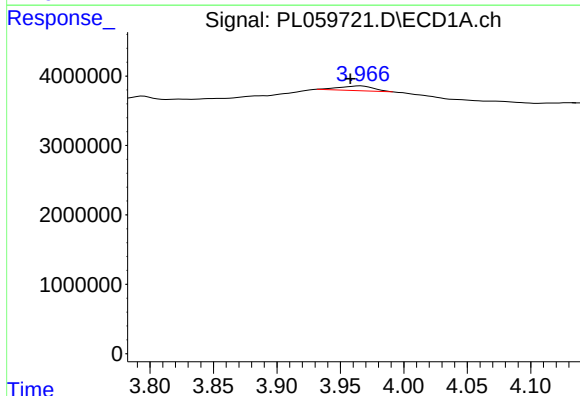


#2 alpha-BHC

R.T.: 3.966 min
Delta R.T.: 0.009 min
Response: 1244322
Conc: 0.48 ng/ml

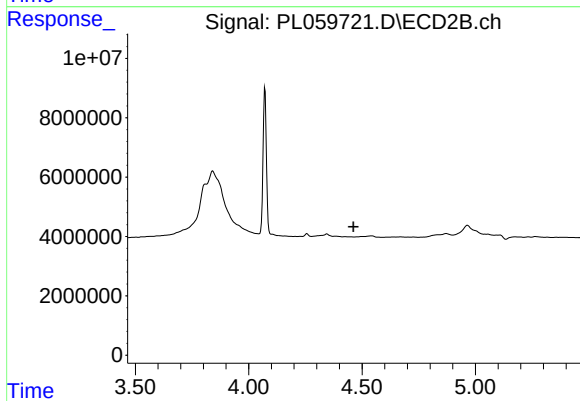

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.463 min
Response: 0
Conc: N.D.

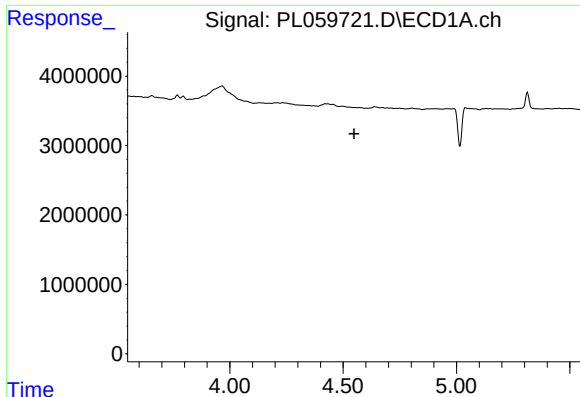

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

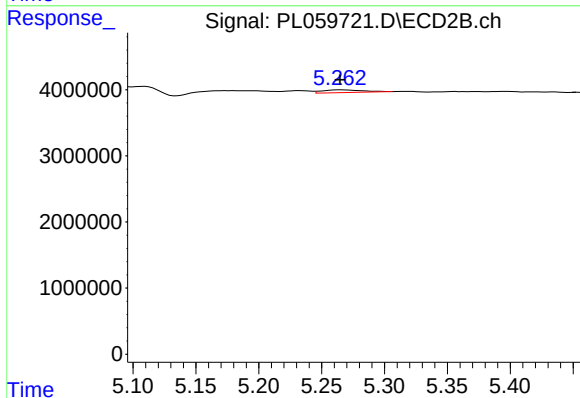


#4 Heptachlor

R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 636769
Conc: 0.18 ng/ml

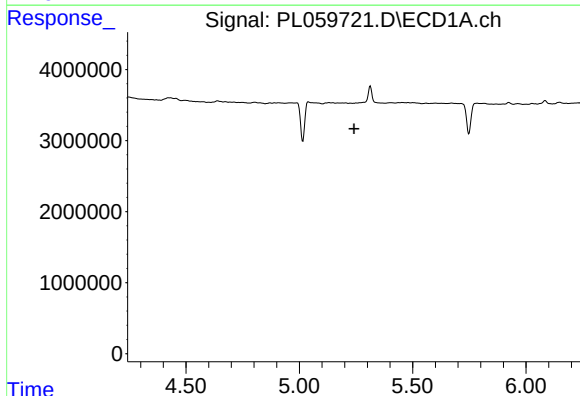


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.242 min
Response: 0
Conc: N.D.

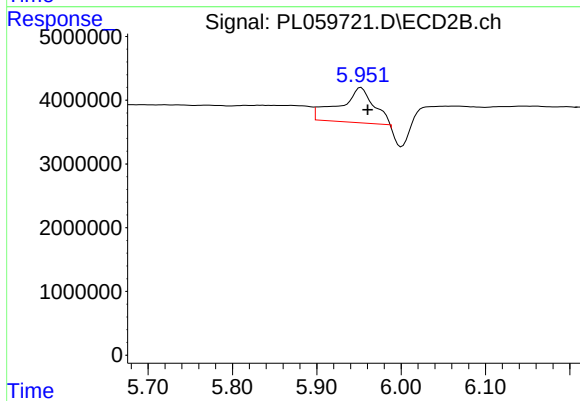

#8 Heptachlor epoxide


R.T.: 5.953 min
Delta R.T.: -0.008 min
Response: 15459789
Conc: 6.36 ng/ml

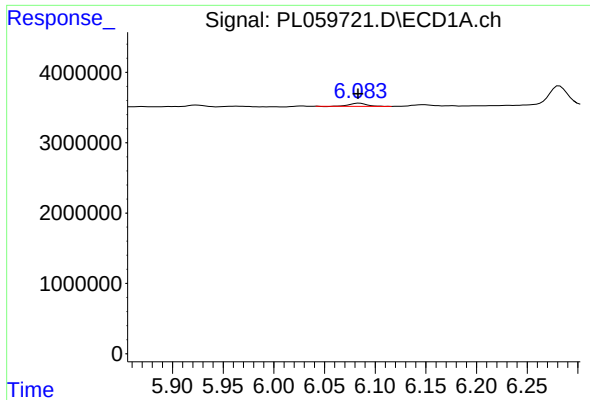

#14 Endrin


R.T.: 6.084 min
Delta R.T.: 0.001 min
Response: 528626
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

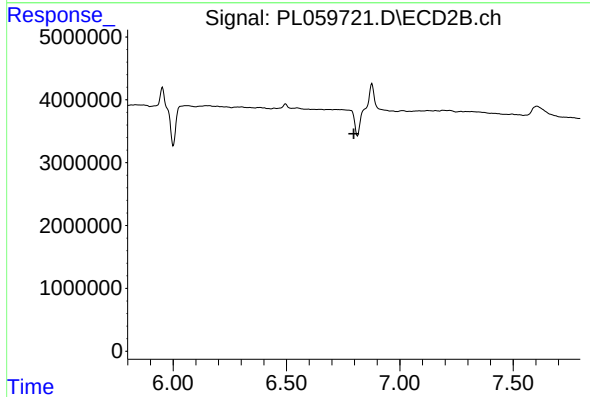


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.797 min
Response: 0
Conc: N.D.

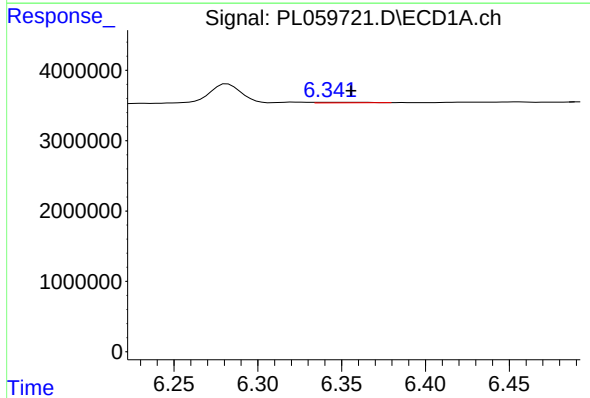


#15 Endosulfan II

R.T.: 6.342 min
Delta R.T.: -0.013 min
Response: 181688
Conc: 0.12 ng/ml

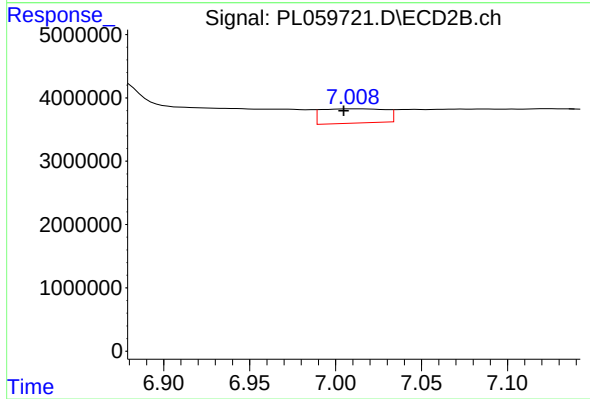

#15 Endosulfan II


R.T.: 7.010 min
Delta R.T.: 0.005 min
Response: 5857440
Conc: 2.28 ng/ml

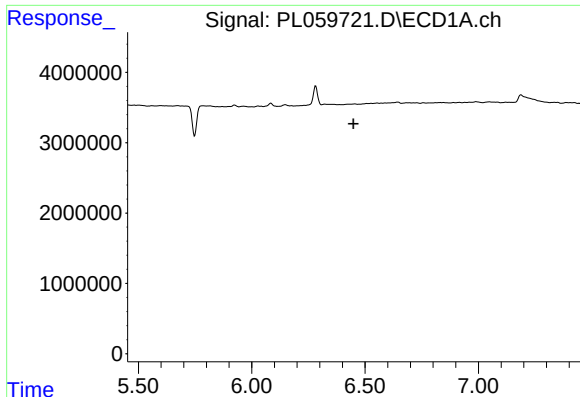

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

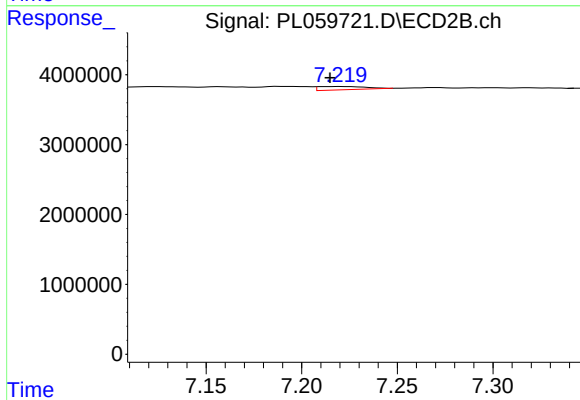


#17 4,4'-DDT

R.T.: 7.221 min
Delta R.T.: 0.006 min
Response: 814753
Conc: 0.36 ng/ml

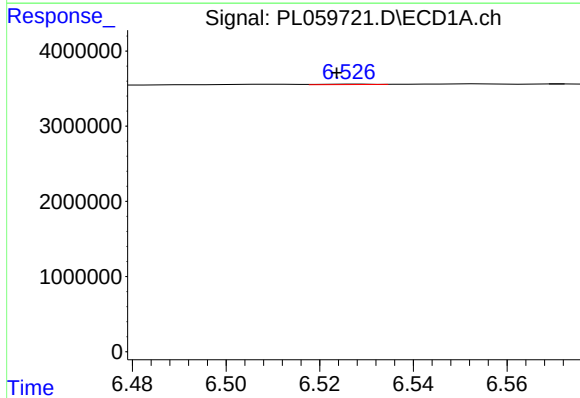


#18 Endrin aldehyde

R.T.: 6.527 min
Delta R.T.: 0.004 min
Response: 46274
Conc: 0.04 ng/ml

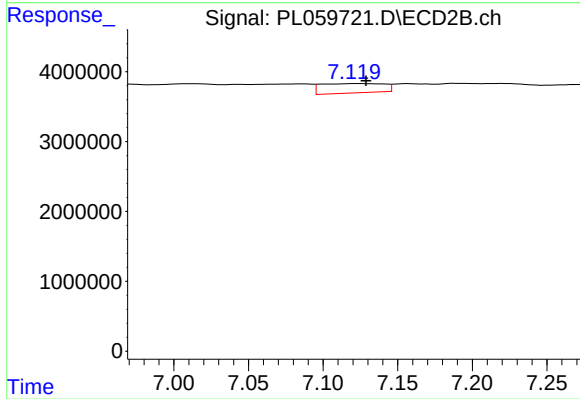

#18 Endrin aldehyde


R.T.: 7.122 min
Delta R.T.: -0.007 min
Response: 3917697
Conc: 1.77 ng/ml

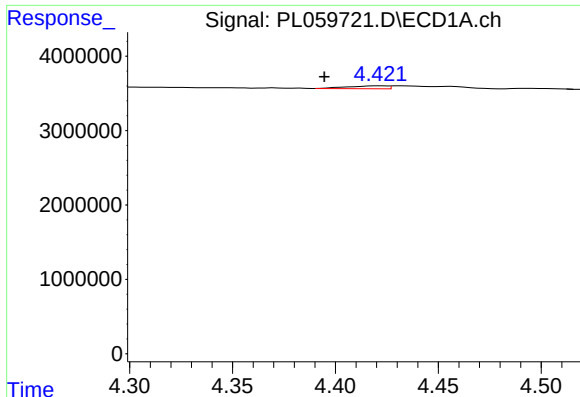

#23 Chlordane-1


R.T.: 4.422 min
Delta R.T.: 0.027 min
Response: 515578
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

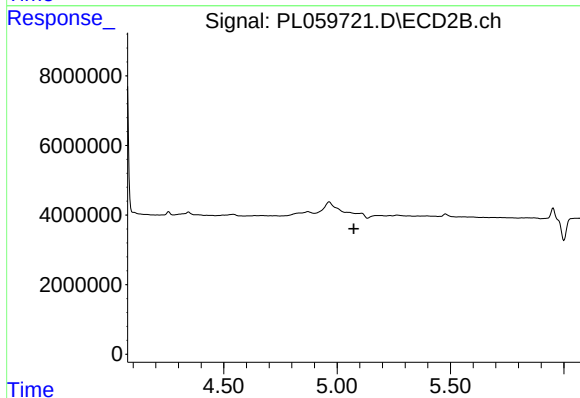


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

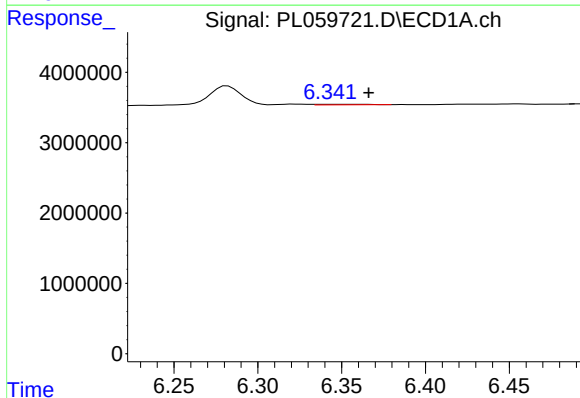


#27 Chlordane-5

R.T.: 6.342 min
Delta R.T.: -0.024 min
Response: 181688
Conc: 3.54 ng/ml

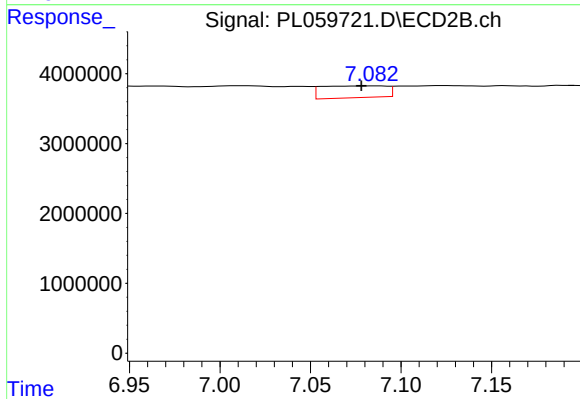

#27 Chlordane-5


R.T.: 7.085 min
Delta R.T.: 0.007 min
Response: 4195280
Conc: 48.21 ng/ml

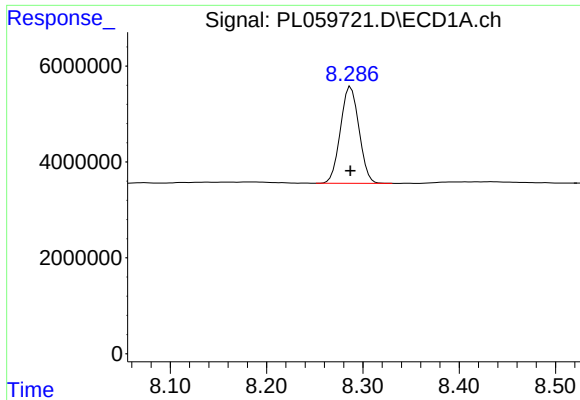

#28 Decachlorobiphenyl

R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 26929529
Conc: 17.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

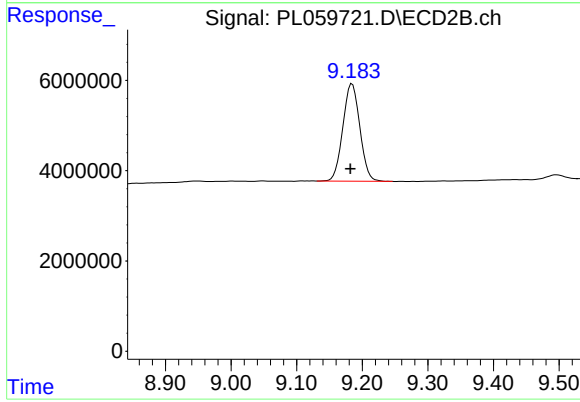

#28 Decachlorobiphenyl

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 38862680
Conc: 17.88 ng/ml