

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 15:04
 Operator : AJ\MA
 Sample : L3172-21
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP8-SS

Manual Integrations
 APPROVED

Ankita
 7/6/2020 2:14:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 16:30:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.516	4.070	38893884	57302067	21.655	21.547
28)	SA Decachlor...	8.286	9.182	28374817	41344703	18.483	19.021
Target Compounds							
12)	B 4,4'-DDE	5.691	6.422	858103	1286980	0.572	0.482m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 15:04
Operator : AJ\MA
Sample : L3172-21
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP8-SS


Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 16:30:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

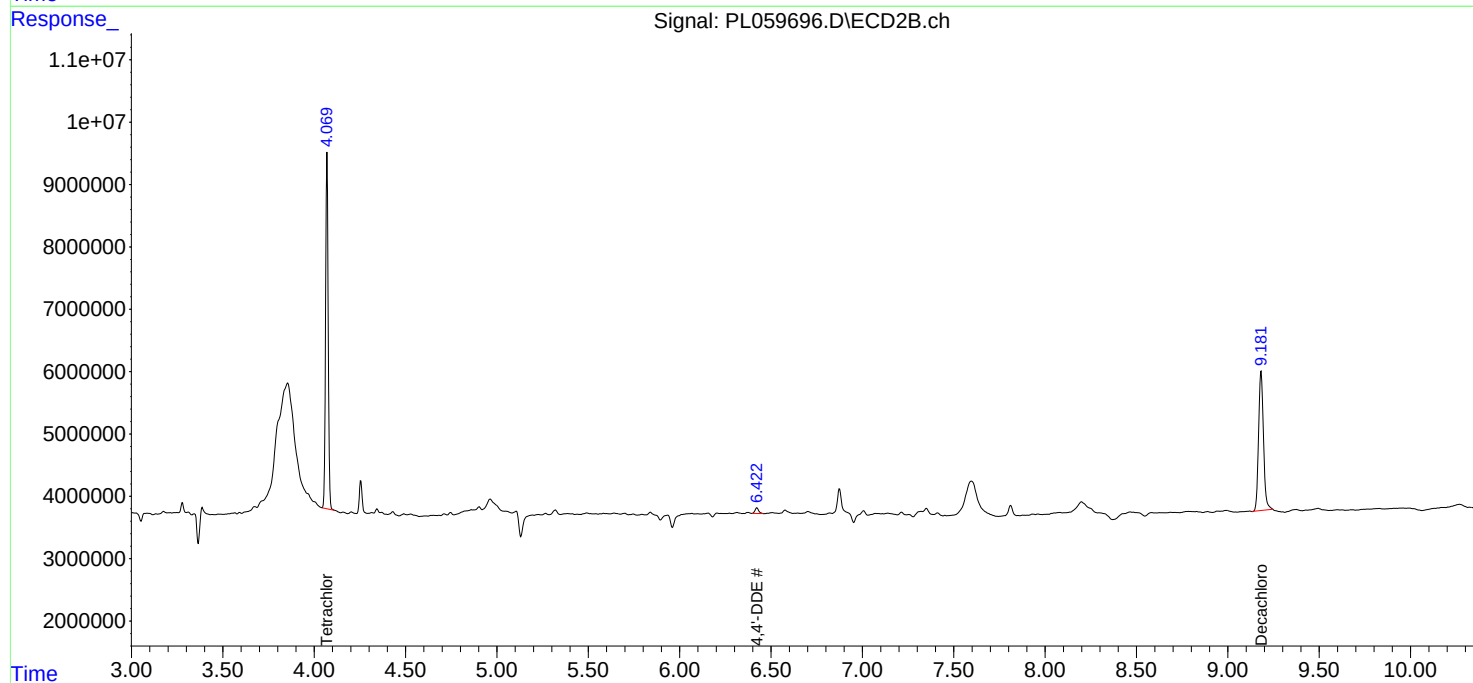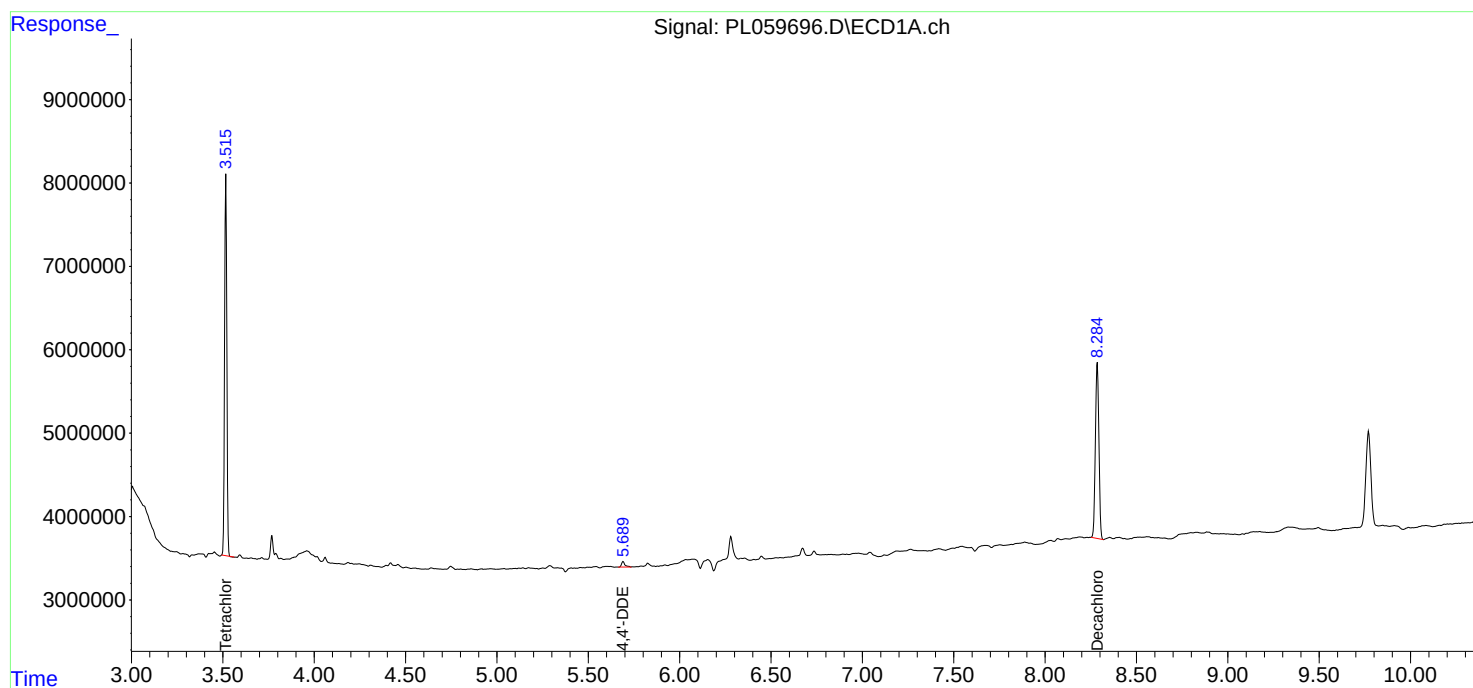

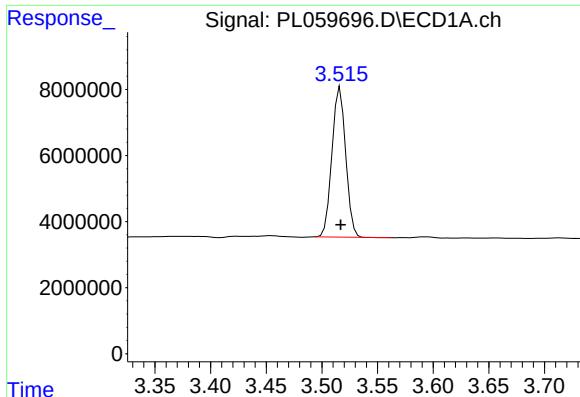


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 38893884
Conc: 21.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP8-SS


Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:14 PM

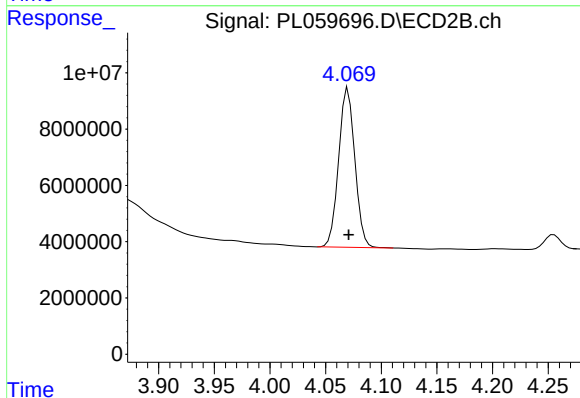


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 57302067
Conc: 21.55 ng/ml

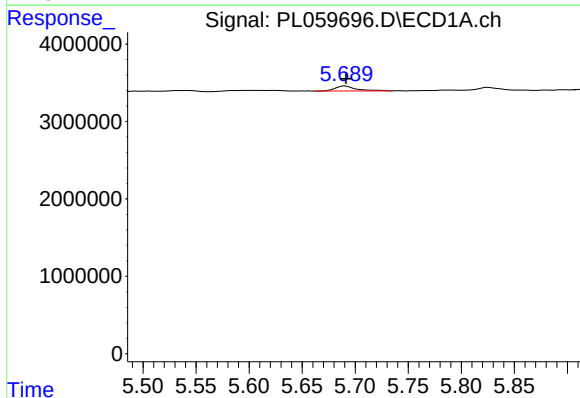


#12 4,4'-DDE

R.T.: 5.691 min
Delta R.T.: 0.000 min
Response: 858103
Conc: 0.57 ng/ml

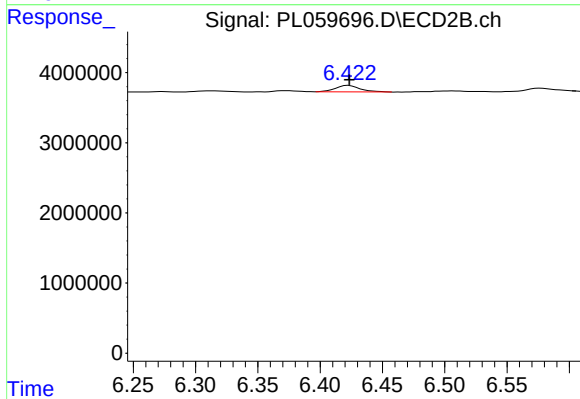

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: -0.002 min
Response: 1286980
Conc: 0.48 ng/ml m

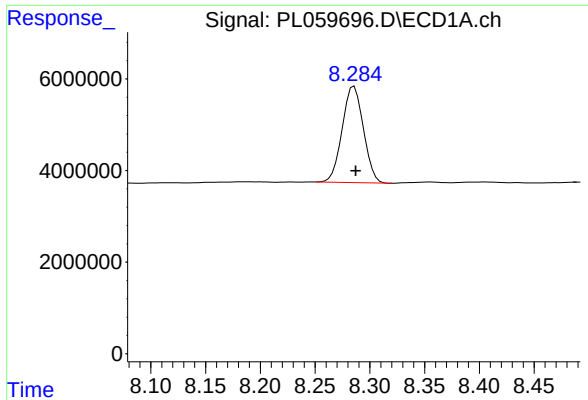

#28 Decachlorobiphenyl

R.T.: 8.286 min

Delta R.T.: -0.001 min


Response: 28374817

Conc: 18.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP8-SS

Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:14 PM

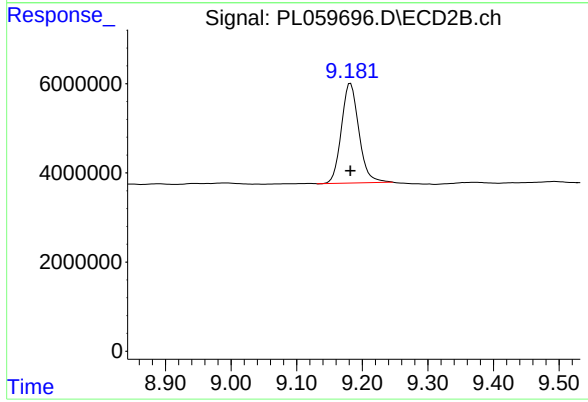

#28 Decachlorobiphenyl

R.T.: 9.182 min

Delta R.T.: 0.000 min

Response: 41344703

Conc: 19.02 ng/ml