

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 15:18
 Operator : AJ\MA
 Sample : L3172-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP1-SS

Manual Integrations
 APPROVED

Ankita
 7/6/2020 2:14:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 16:30:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.516	4.071	37114950	54099669	20.665	20.343
28)	SA Decachlor...	8.286	9.182	29458636	41118003	19.189	18.917
Target Compounds							
12)	B 4,4'-DDE	5.690	6.423	12003551	20574089	8.007	7.712
13)	MA Dieldrin	5.825	6.577	2987620	4931554	1.871	1.750
17)	MA 4,4'-DDT	6.449	7.213	3981039	7665275	3.136	3.389m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 15:18
Operator : AJ\MA
Sample : L3172-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP1-SS


Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 16:30:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

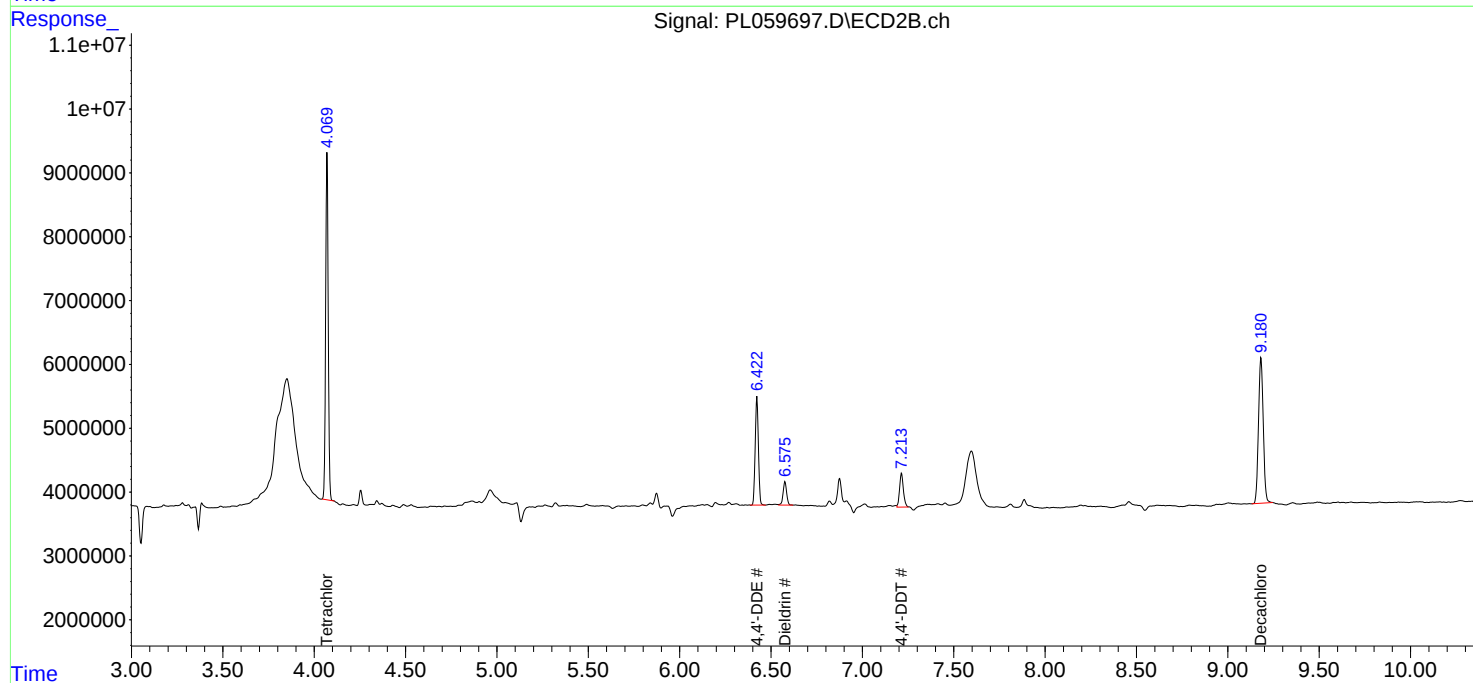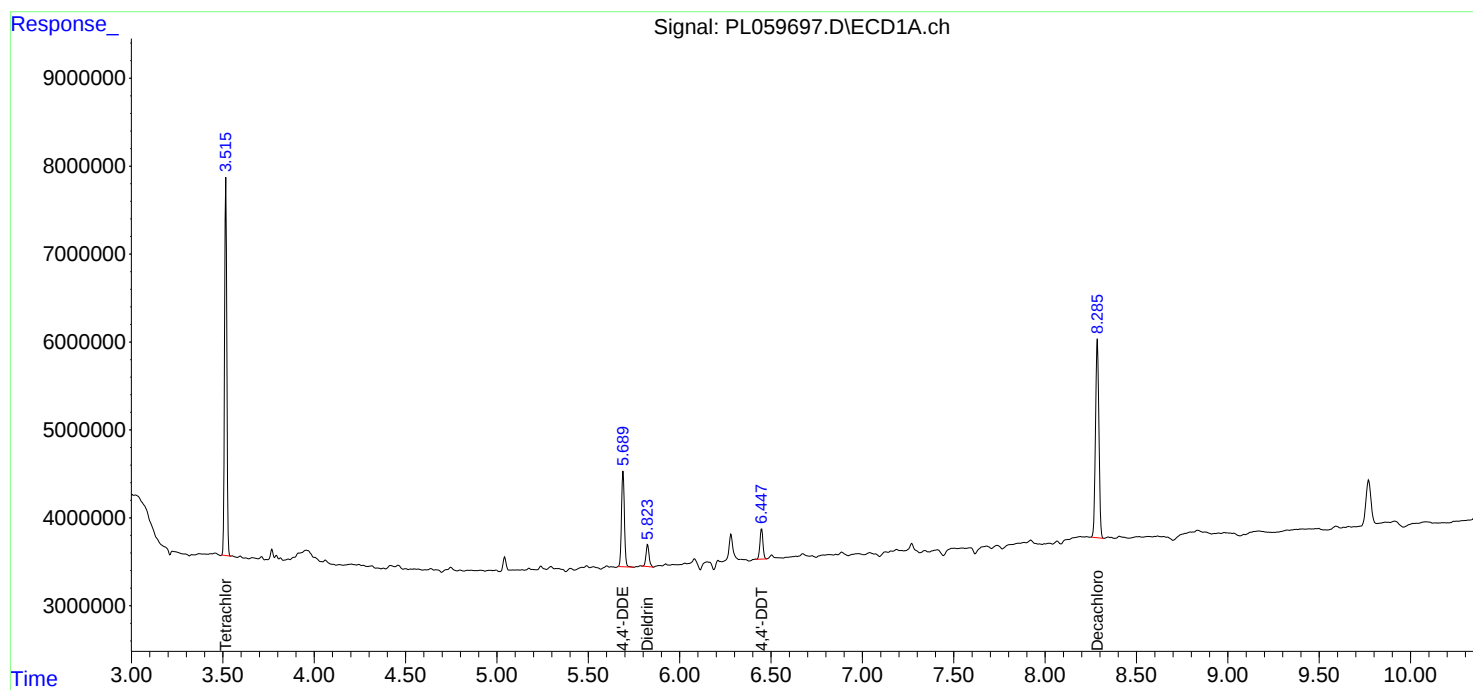

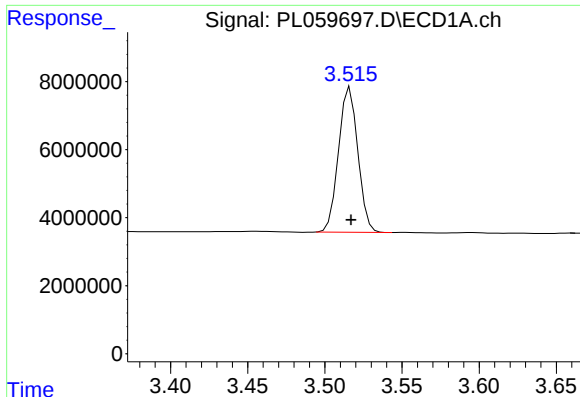


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 37114950
Conc: 20.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-SS


Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:16 PM

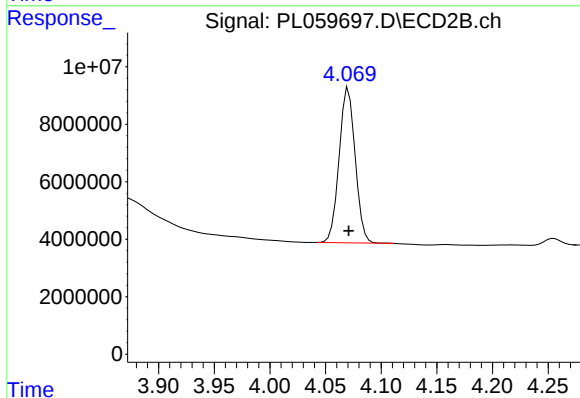


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: 0.000 min
Response: 54099669
Conc: 20.34 ng/ml

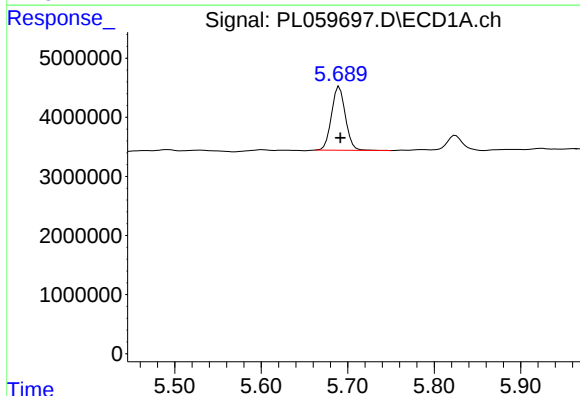


#12 4,4'-DDE

R.T.: 5.690 min
Delta R.T.: 0.000 min
Response: 12003551
Conc: 8.01 ng/ml

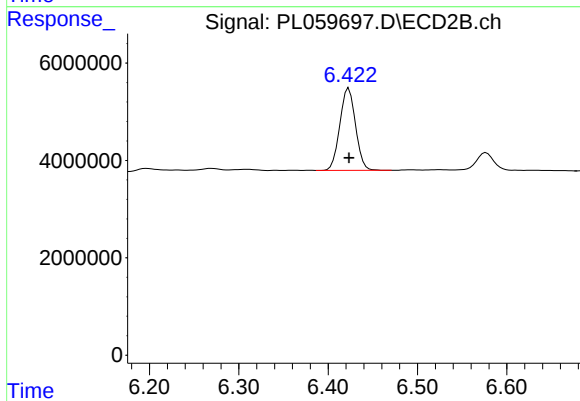

#12 4,4'-DDE

R.T.: 6.423 min
Delta R.T.: 0.000 min
Response: 20574089
Conc: 7.71 ng/ml

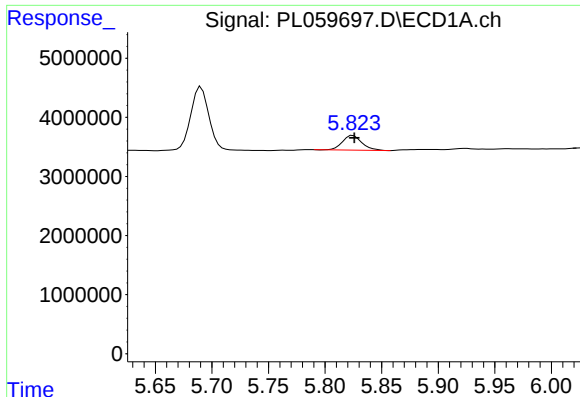


#13 Dieldrin

R.T.: 5.825 min
Delta R.T.: -0.001 min
Response: 2987620
Conc: 1.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-SS


Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:16 PM

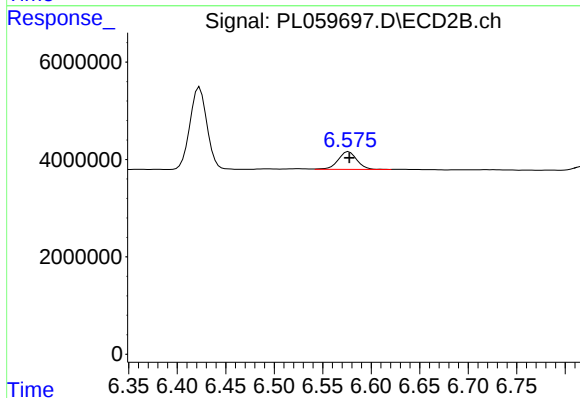


#13 Dieldrin

R.T.: 6.577 min
Delta R.T.: 0.000 min
Response: 4931554
Conc: 1.75 ng/ml

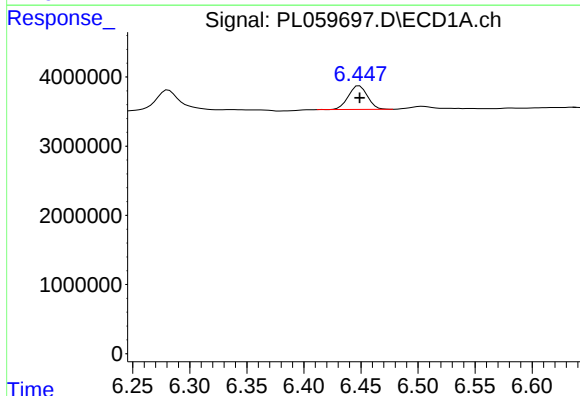


#17 4,4'-DDT

R.T.: 6.449 min
Delta R.T.: 0.000 min
Response: 3981039
Conc: 3.14 ng/ml

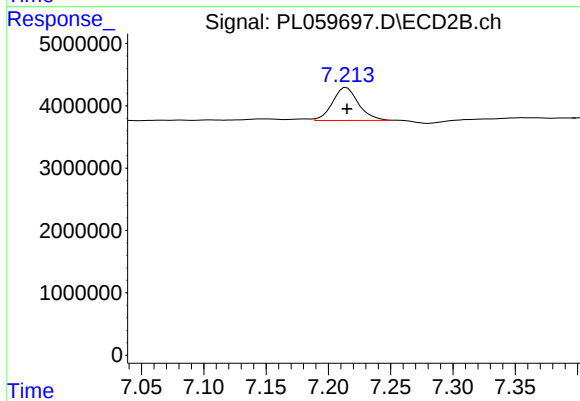

#17 4,4'-DDT

R.T.: 7.213 min
Delta R.T.: -0.002 min
Response: 7665275
Conc: 3.39 ng/ml m

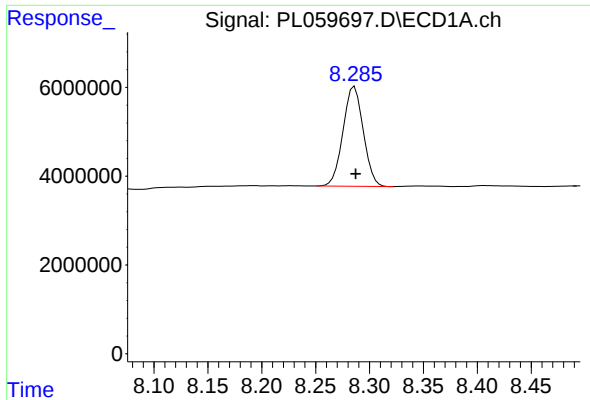


#28 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: -0.001 min
Response: 29458636
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP1-SS

Manual Integrations
APPROVED

Ankita
7/6/2020 2:14:16 PM

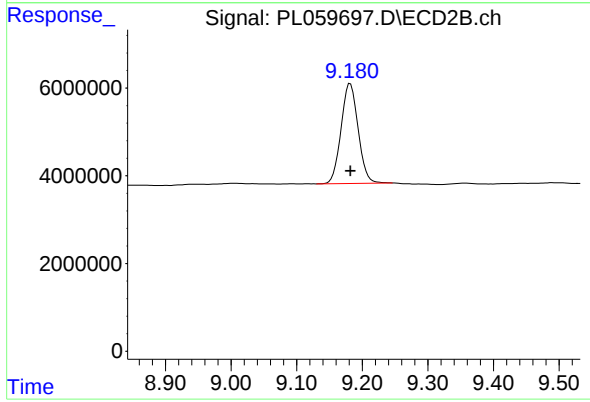

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 41118003
Conc: 18.92 ng/ml