

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
 Data File : PL059700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2020 16:00
 Operator : AJ\MA
 Sample : L3172-23
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP9-SS

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 16:31:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 01 01:23:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Ankita

7/6/2020 2:14:23 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.516	4.070	40785654	59935497	22.708	22.537
28) SA Decachlor...	8.286	9.182	32163843	44461239	20.951	20.455
Target Compounds						
12) B 4,4'-DDE	5.690	6.422	1424648	1918362	0.950	0.719
17) MA 4,4'-DDT	6.448	7.213	891032	1380632	0.702	0.610m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070220\
Data File : PL059700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2020 16:00
Operator : AJ\MA
Sample : L3172-23
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP9-SS



Manual Integrations
APPROVED


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 16:31:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL063020.M
Quant Title : GC Extractables
QLast Update : Wed Jul 01 01:23:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Ankita

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

7/6/2020 2:14:23 PM

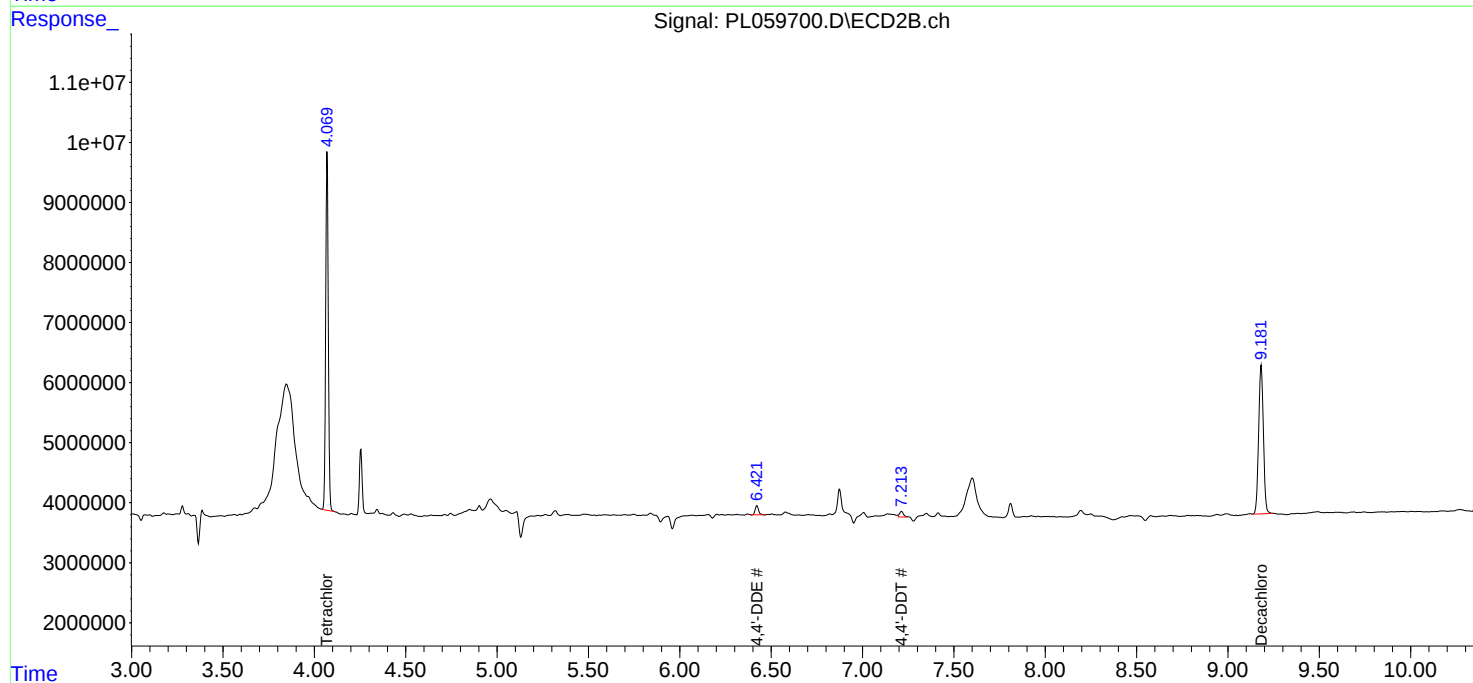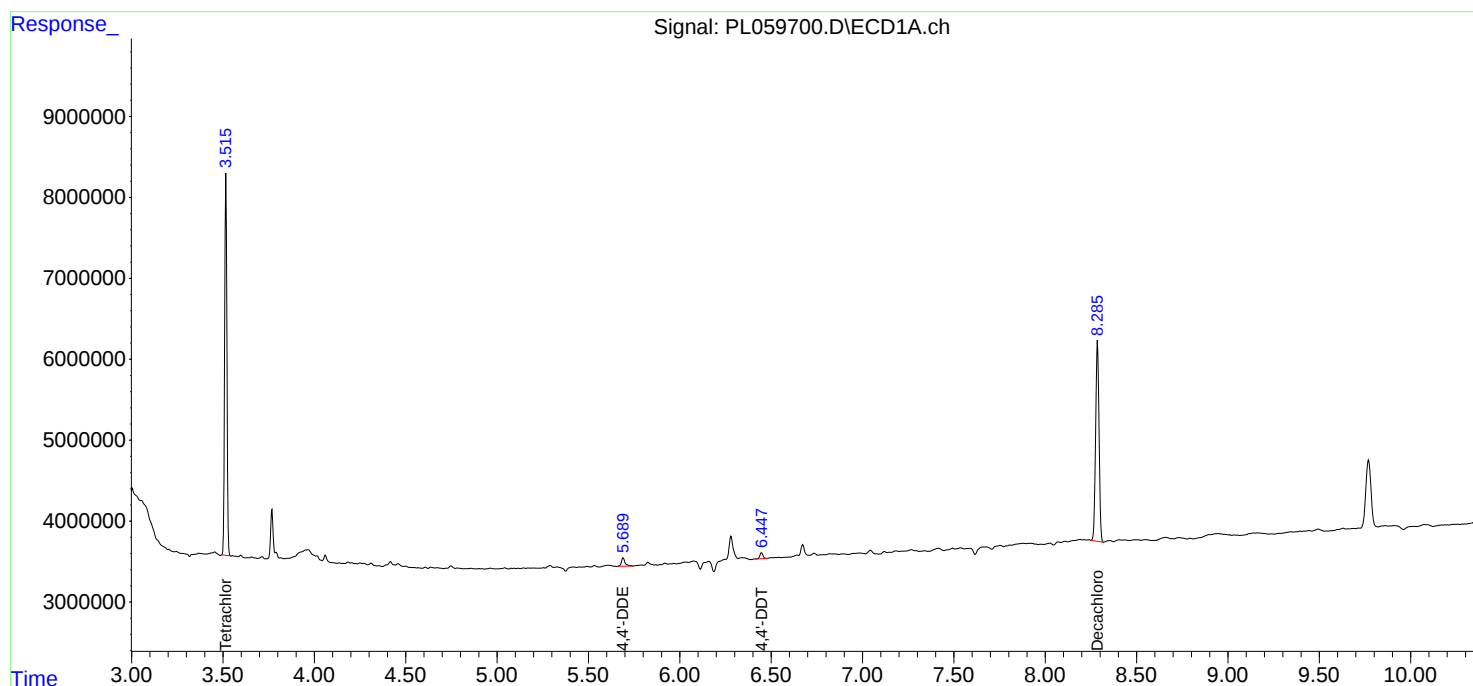

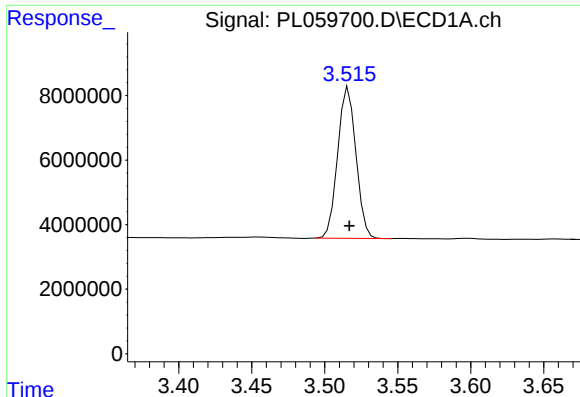


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 40785654
Conc: 22.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP9-SS

Manual Integrations
APPROVED

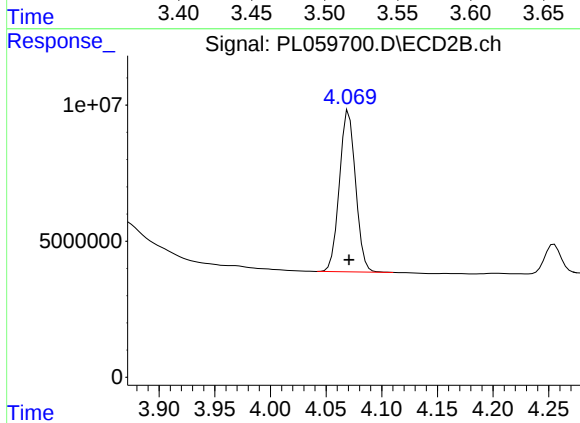


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: 0.000 min
Response: 59935497
Conc: 22.54 ng/ml


Ankita

7/6/2020 2:14:23 PM

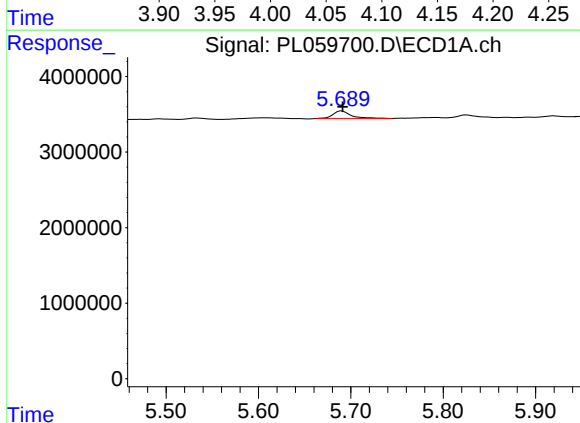


#12 4,4'-DDE

R.T.: 5.690 min
Delta R.T.: -0.001 min
Response: 1424648
Conc: 0.95 ng/ml

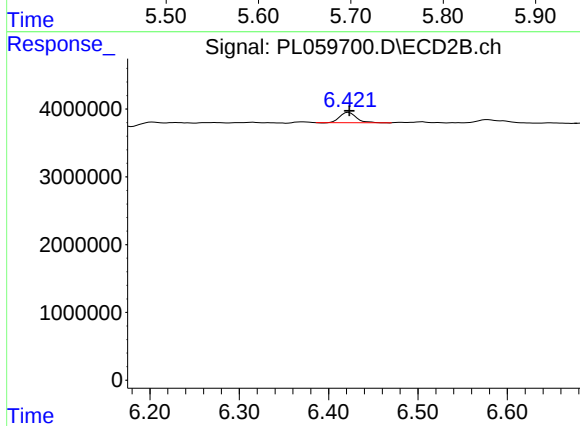

#12 4,4'-DDE

R.T.: 6.422 min
Delta R.T.: 0.000 min
Response: 1918362
Conc: 0.72 ng/ml

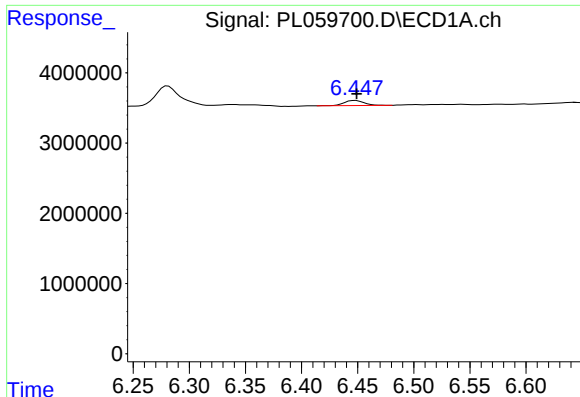


#17 4,4'-DDT

R.T.: 6.448 min
Delta R.T.: 0.000 min
Response: 891032
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP9-SS

Manual Integrations
APPROVED

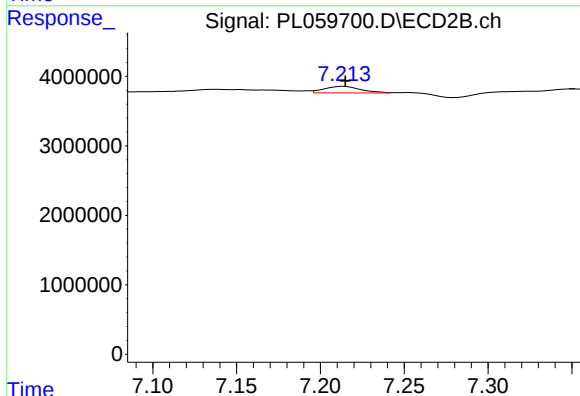


#17 4,4'-DDT

R.T.: 7.213 min
Delta R.T.: -0.002 min
Response: 1380632
Conc: 0.61 ng/ml m


Ankita

7/6/2020 2:14:23 PM

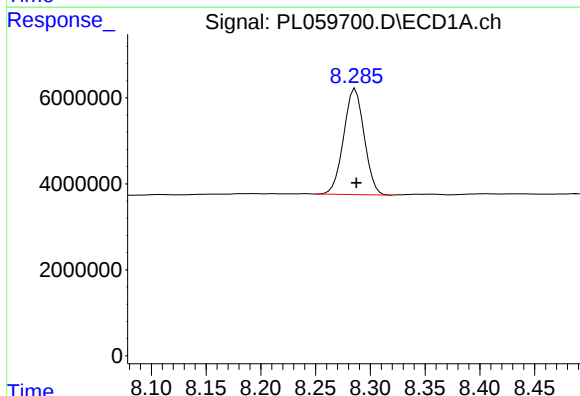

#28 Decachlorobiphenyl

R.T.: 8.286 min
Delta R.T.: 0.000 min
Response: 32163843
Conc: 20.95 ng/ml

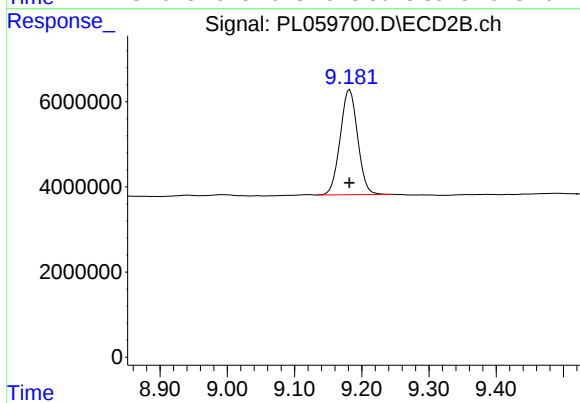

#28 Decachlorobiphenyl

R.T.: 9.182 min
Delta R.T.: 0.000 min
Response: 44461239
Conc: 20.45 ng/ml