

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
 Data File : PL067927.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2021 10:41
 Operator : AR\AJ
 Sample : M2900-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VB16208

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:09:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.475	5.527	9855354	18001452	17.926	19.095
28)	SA Decachlor...	10.217	11.424	12301777	16639905	17.359	16.706
Target Compounds							
2)	A alpha-BHC	5.182	0.000	639508	0	0.869	N.D. #
6)	B beta-BHC	0.000	6.742f	0	207149	N.D.	0.381 #
11)	B alpha-Chl...	7.250	0.000	250617	0	0.342	N.D. #
14)	MA Endrin	7.892	0.000	438456	0	0.669	N.D. #
15)	B Endosulfa...	8.175f	9.178f	240428	294963	0.390	0.370
19)	B Endosulfa...	8.586f	0.000	311905	0	0.491	N.D. #
21)	B Endrin ke...	9.099f	10.045f	170955	79700	0.225	0.088 #
26)	Chlordane-4	7.250	0.000	250617	0	3.429	N.D. #
27)	Chlordane-5	8.175f	0.000	240428	0	10.989	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
Data File : PL067927.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2021 10:41
Operator : AR\AJ
Sample : M2900-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VB16208

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:09:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

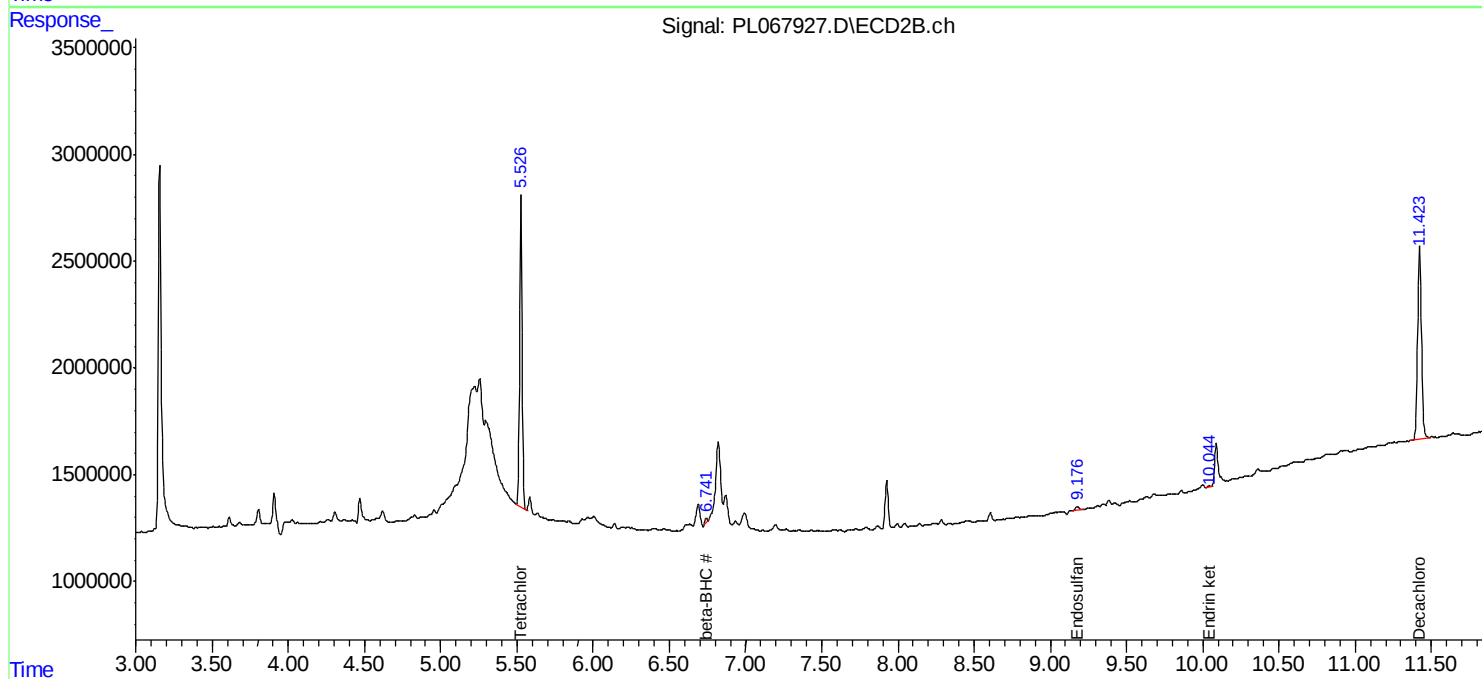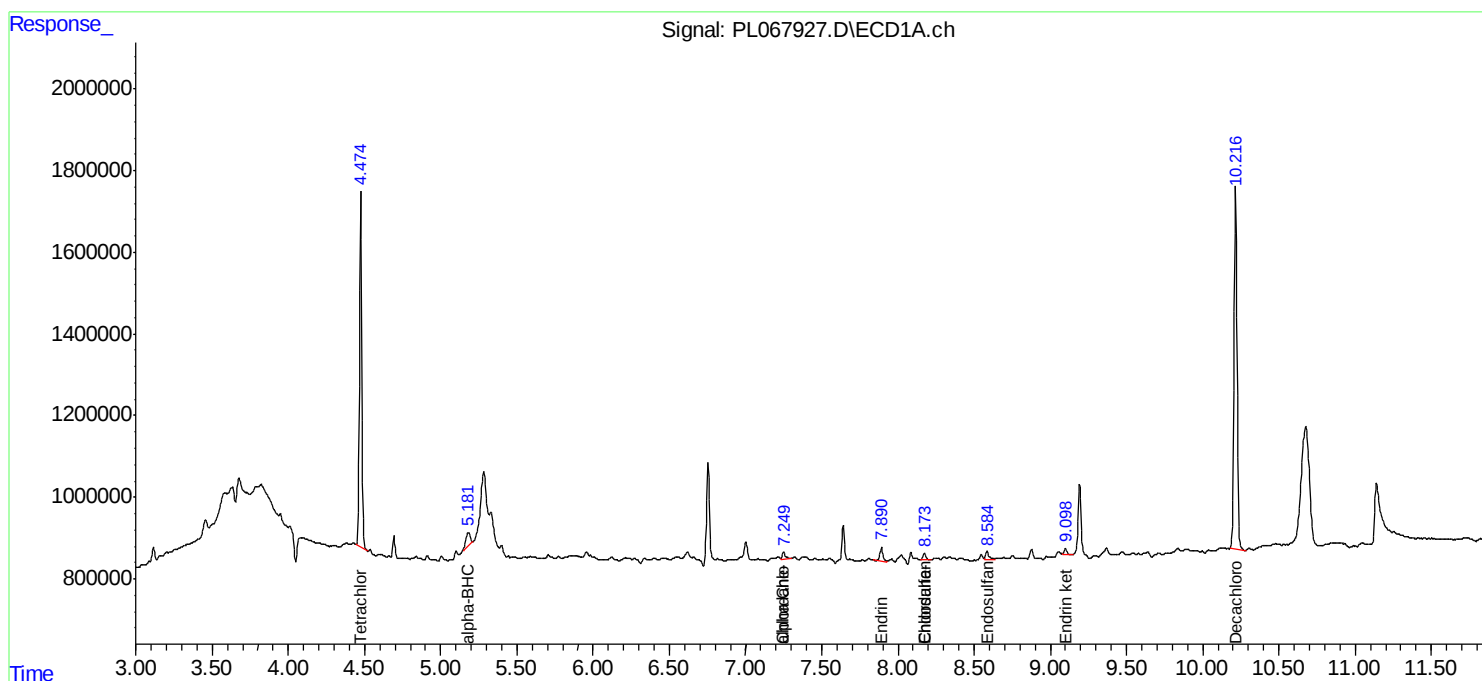


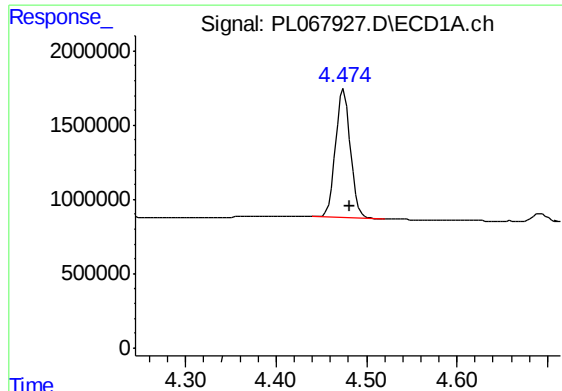

#1 Tetrachloro-m-xylene


R.T.: 4.475 min
Delta R.T.: -0.006 min
Response: 9855354
Conc: 17.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16208

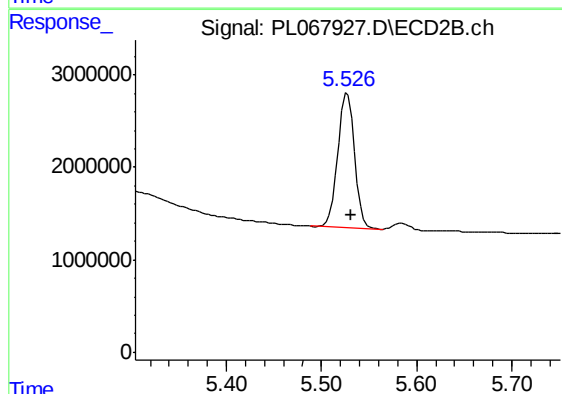


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 18001452
Conc: 19.09 ng/ml

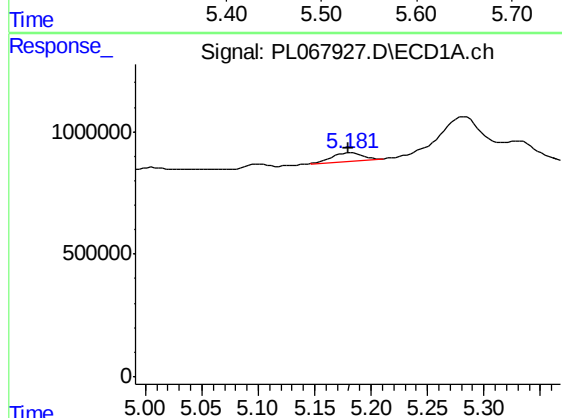


#2 alpha-BHC

R.T.: 5.182 min
Delta R.T.: 0.002 min
Response: 639508
Conc: 0.87 ng/ml

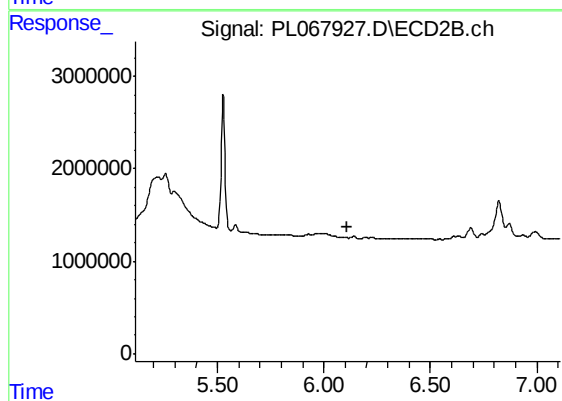

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

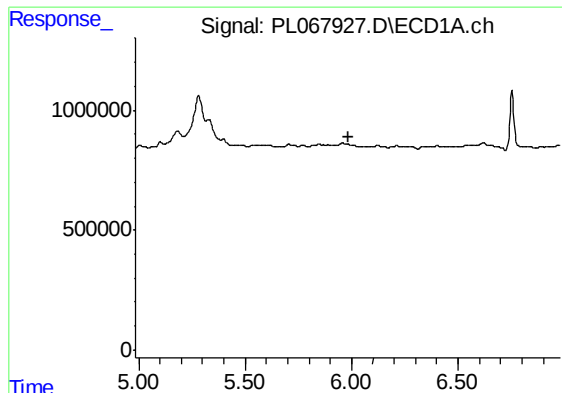

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 5.983 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
VB16208

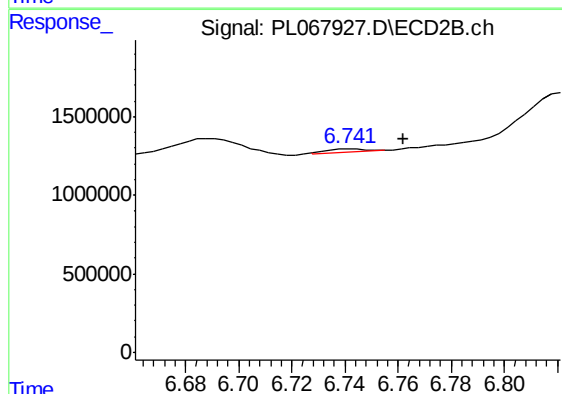


#6 beta-BHC

R.T.: 6.742 min
Delta R.T.: -0.020 min
Response: 207149
Conc: 0.38 ng/ml

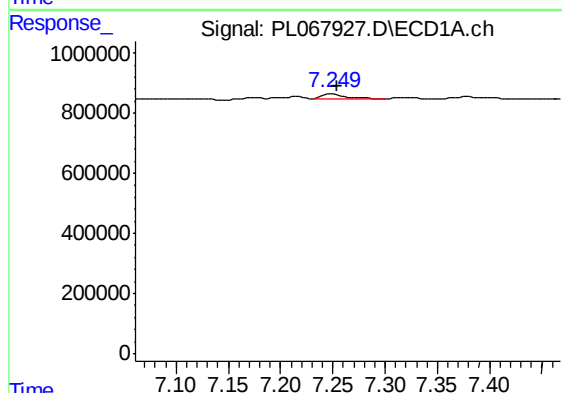


#11 alpha-Chlordane

R.T.: 7.250 min
Delta R.T.: -0.004 min
Response: 250617
Conc: 0.34 ng/ml

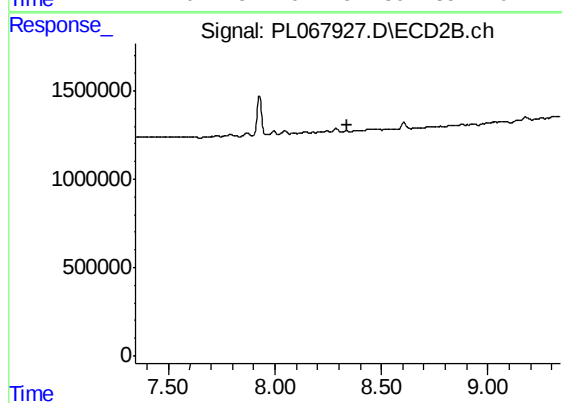

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.342 min
Response: 0
Conc: N.D.

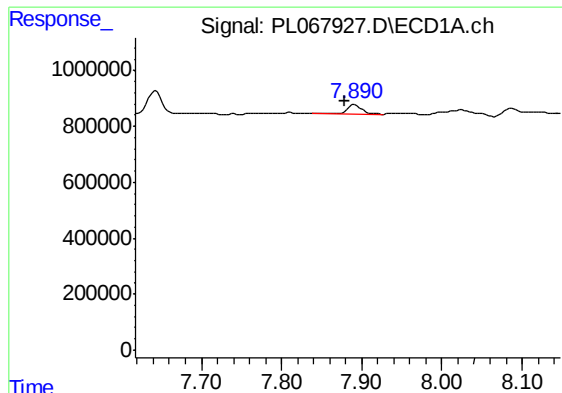

#14 Endrin


R.T.: 7.892 min
Delta R.T.: 0.013 min
Response: 438456
Conc: 0.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16208

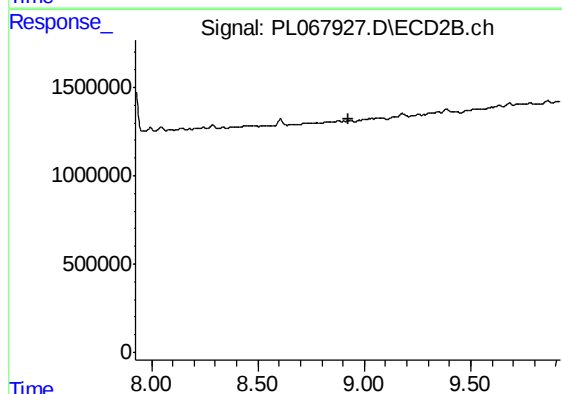


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

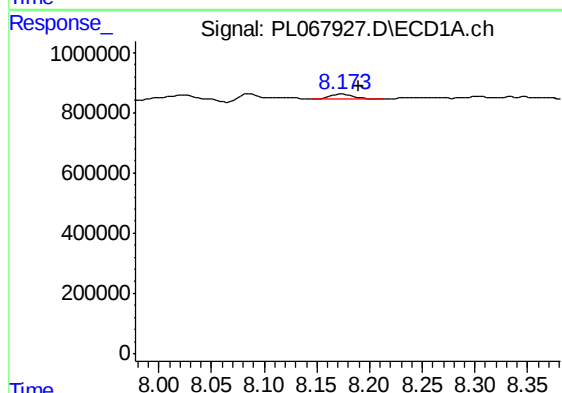


#15 Endosulfan II

R.T.: 8.175 min
Delta R.T.: -0.015 min
Response: 240428
Conc: 0.39 ng/ml

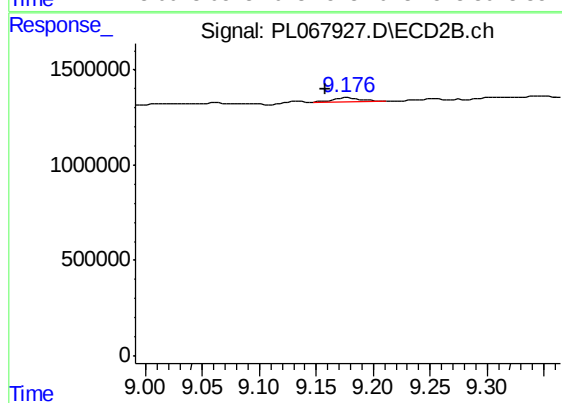

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 294963
Conc: 0.37 ng/ml

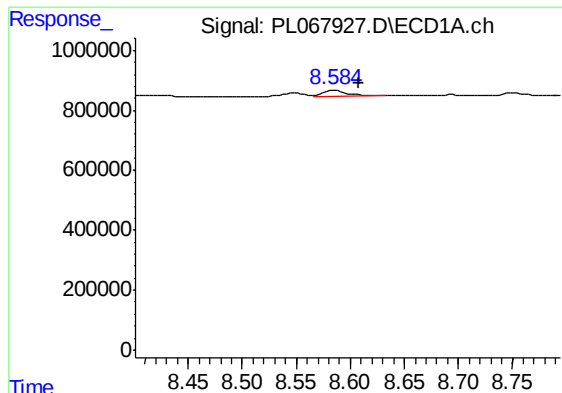

#19 Endosulfan Sulfate


R.T.: 8.586 min
Delta R.T.: -0.023 min
Response: 311905
Conc: 0.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16208

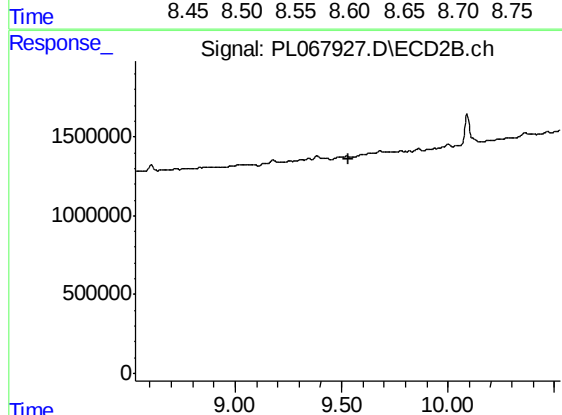


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 9.530 min
Response: 0
Conc: N.D.

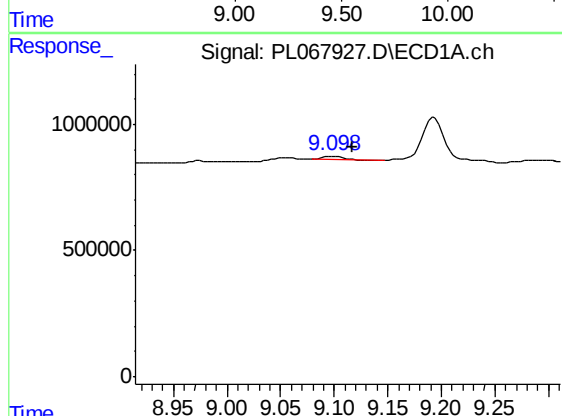


#21 Endrin ketone

R.T.: 9.099 min
Delta R.T.: -0.018 min
Response: 170955
Conc: 0.22 ng/ml

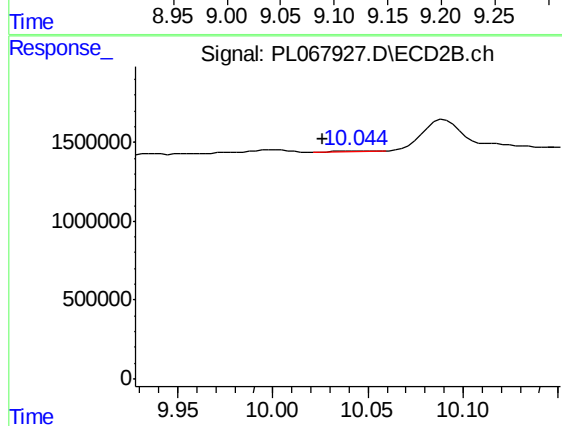

#21 Endrin ketone


R.T.: 10.045 min
Delta R.T.: 0.019 min
Response: 79700
Conc: 0.09 ng/ml

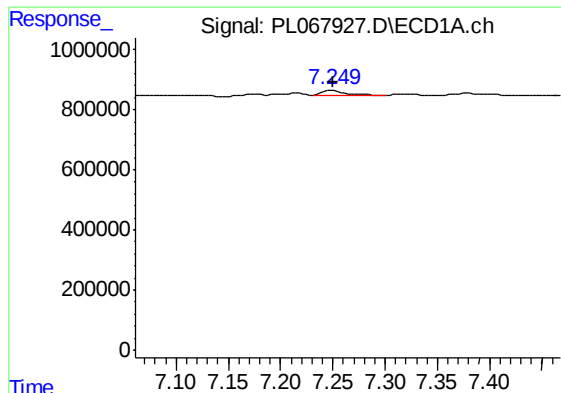

#26 Chlordane-4


R.T.: 7.250 min
Delta R.T.: 0.000 min
Response: 250617
Conc: 3.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16208

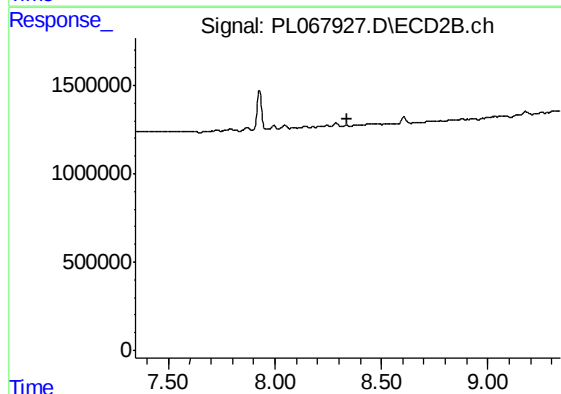


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.341 min
Response: 0
Conc: N.D.

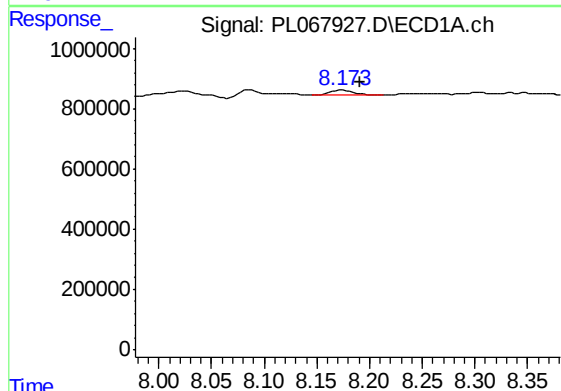


#27 Chlordane-5

R.T.: 8.175 min
Delta R.T.: -0.016 min
Response: 240428
Conc: 10.99 ng/ml

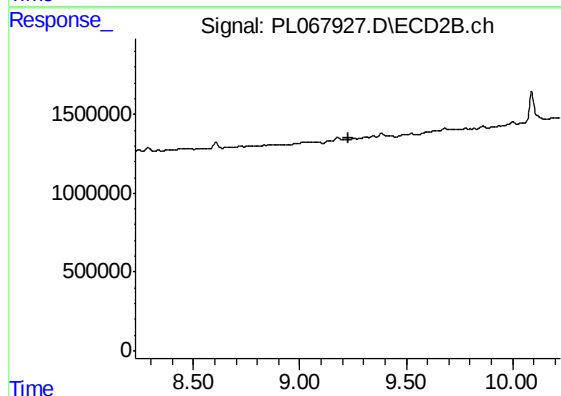

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

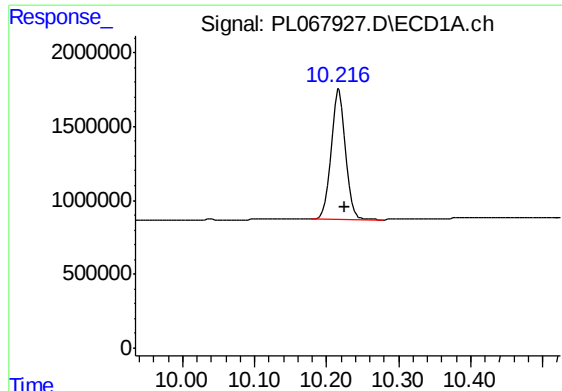

#28 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.007 min
Response: 12301777
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16208

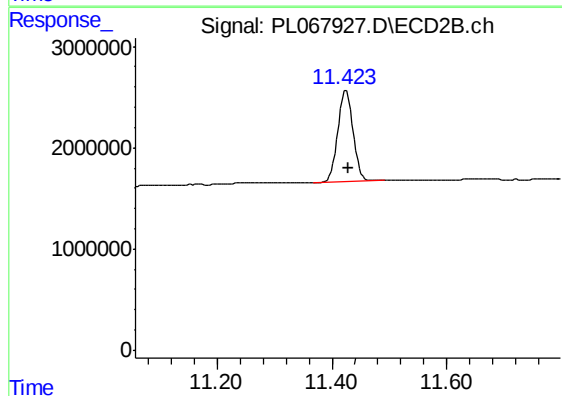

#28 Decachlorobiphenyl

R.T.: 11.424 min
Delta R.T.: -0.005 min
Response: 16639905
Conc: 16.71 ng/ml