

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
 Data File : PL067943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2021 17:16
 Operator : AR\AJ
 Sample : M2902-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-CROPSEY-AQUEOUS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:16:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	4.476	5.527	635144	1297689	1.155	1.377
28) SA	Decachlor...	10.216	11.425	895770	861518	1.264	0.865 #
Target Compounds							
3) MA	gamma-BHC...	5.611	0.000	1073623	0	1.433	N.D. #
8) B	Heptachlo...	6.932f	0.000	540649	0	0.773	N.D. #
10) B	gamma-Chl...	0.000	8.279f	0	2059365	N.D.	2.040 #
14) MA	Endrin	7.893f	0.000	1432628	0	2.185	N.D. #
15) B	Endosulfa...	8.173f	9.178f	897855	273465	1.458	0.343 #
25)	Chlordane-3	0.000	8.279f	0	2059365	N.D.	15.387 #
27)	Chlordane-5	8.173f	0.000	897855	0	41.037	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
Data File : PL067943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2021 17:16
Operator : AR\AJ
Sample : M2902-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:16:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

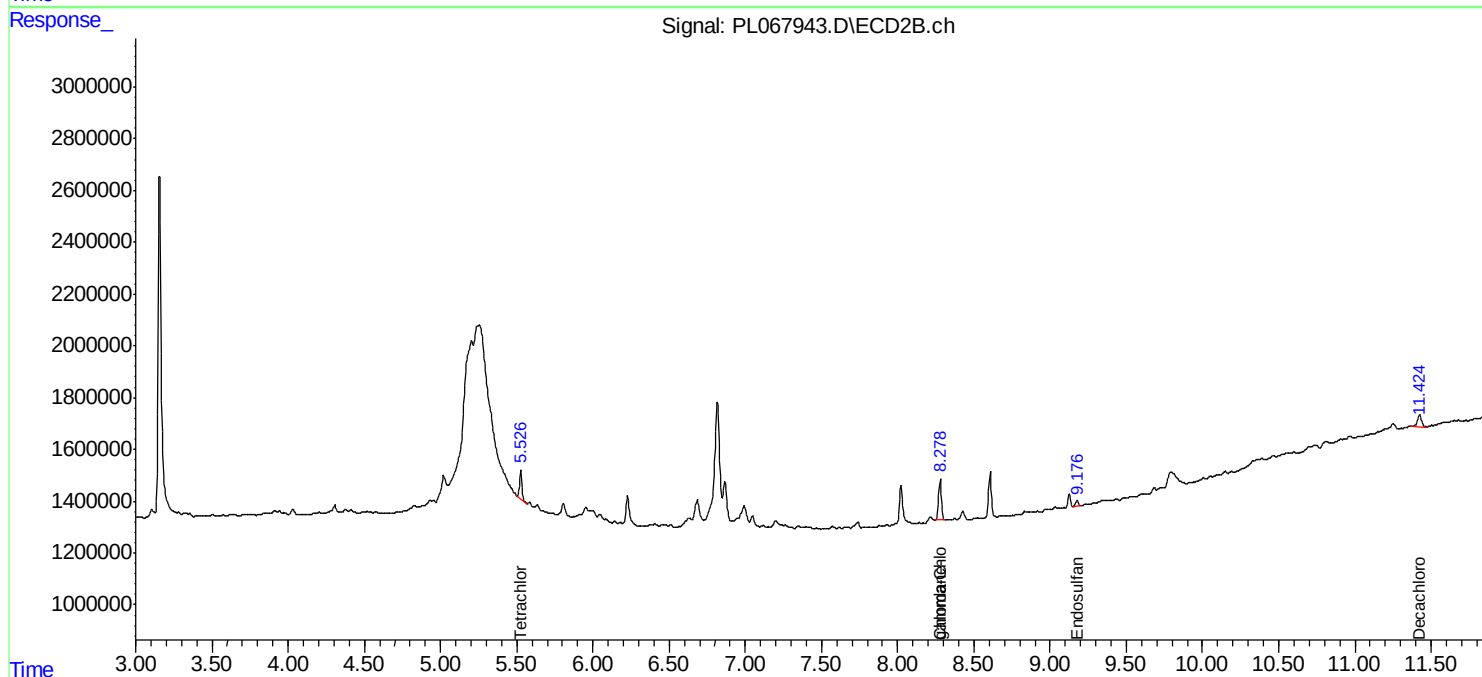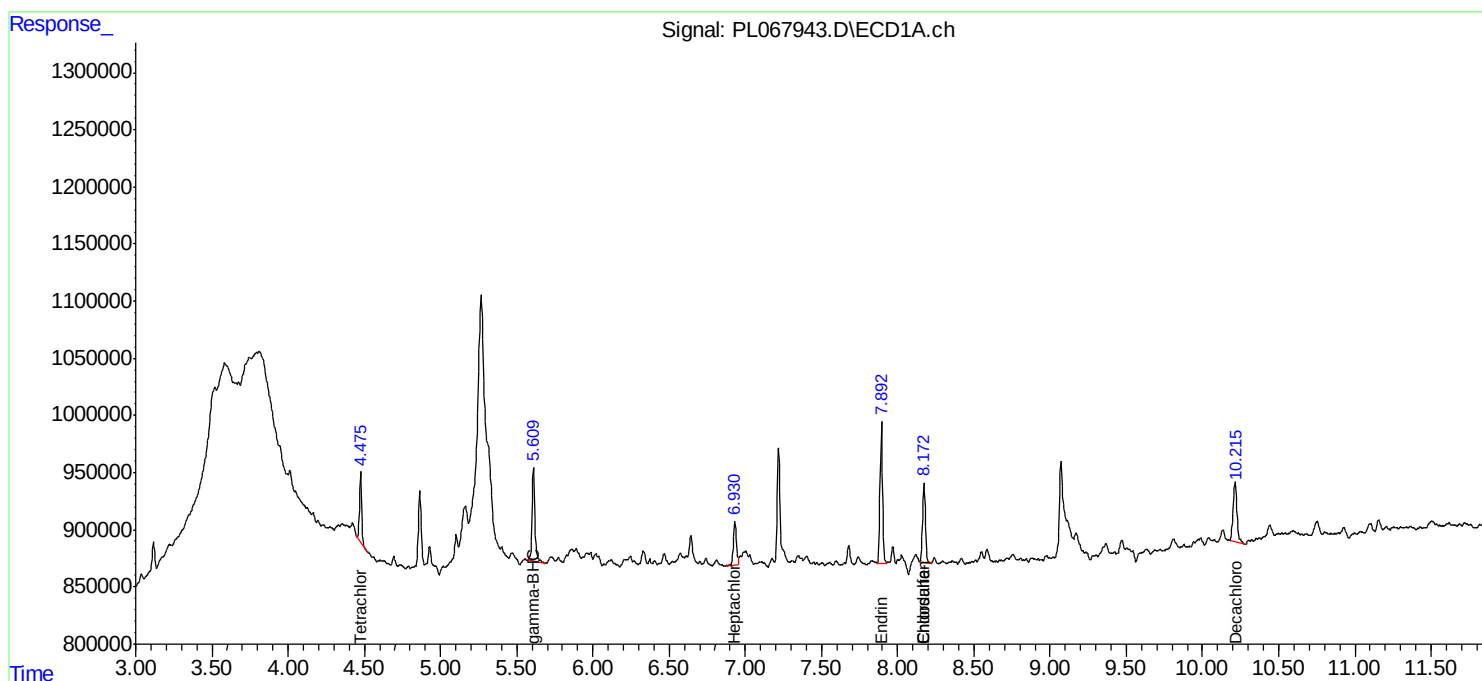


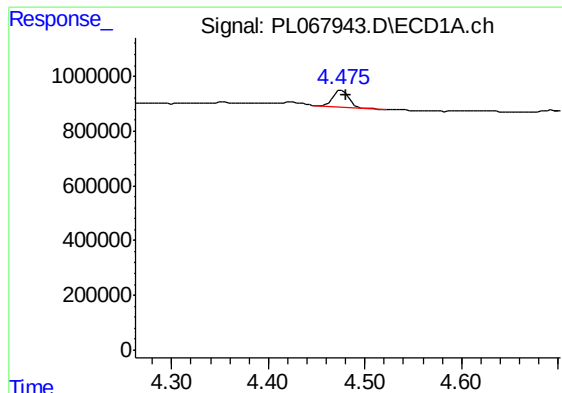

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 635144
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

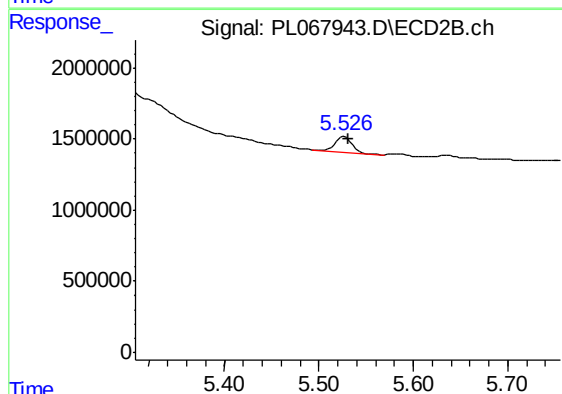


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 1297689
Conc: 1.38 ng/ml

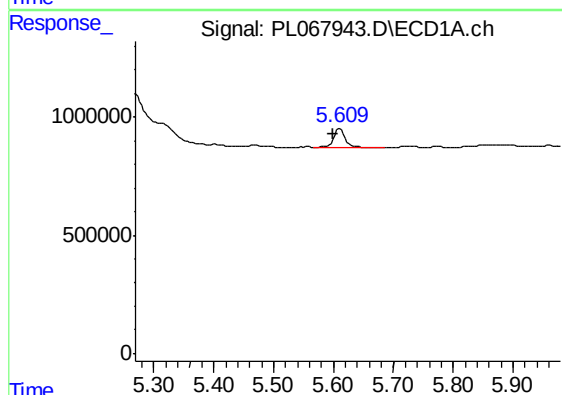


#3 gamma-BHC (Lindane)

R.T.: 5.611 min
Delta R.T.: 0.010 min
Response: 1073623
Conc: 1.43 ng/ml

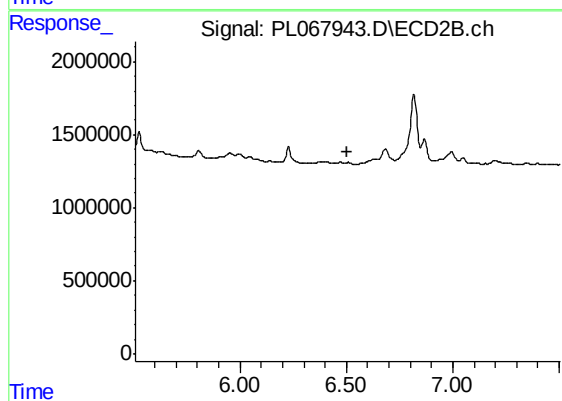

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

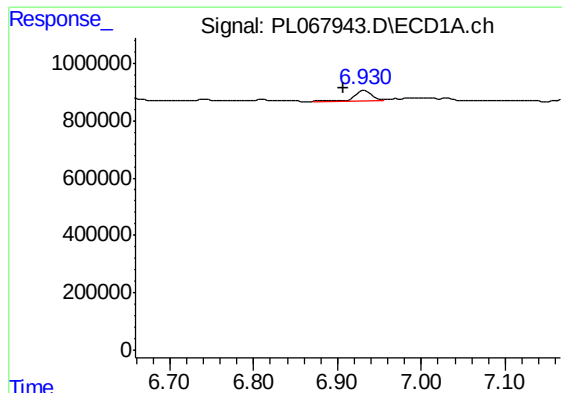

#8 Heptachlor epoxide


R.T.: 6.932 min
Delta R.T.: 0.024 min
Response: 540649
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

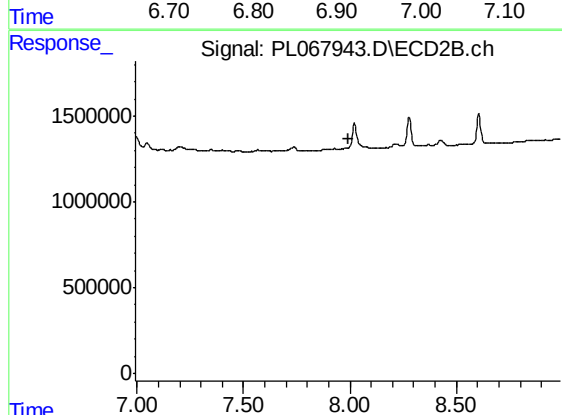


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.991 min
Response: 0
Conc: N.D.

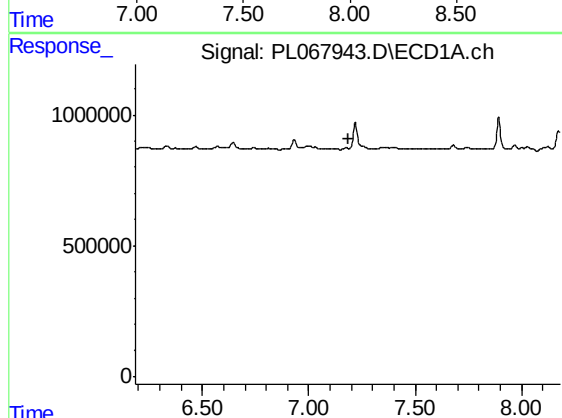


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

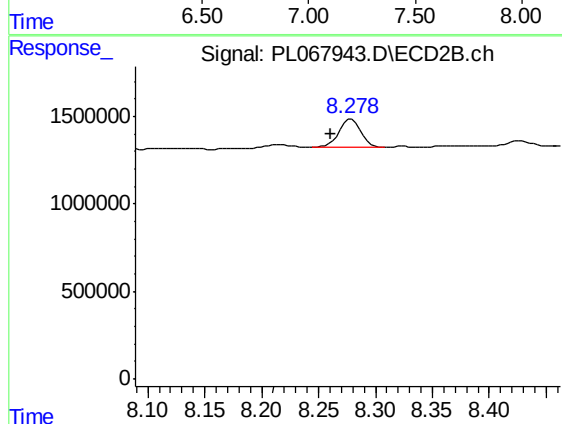

#10 gamma-Chlordane


R.T.: 8.279 min
Delta R.T.: 0.018 min
Response: 2059365
Conc: 2.04 ng/ml

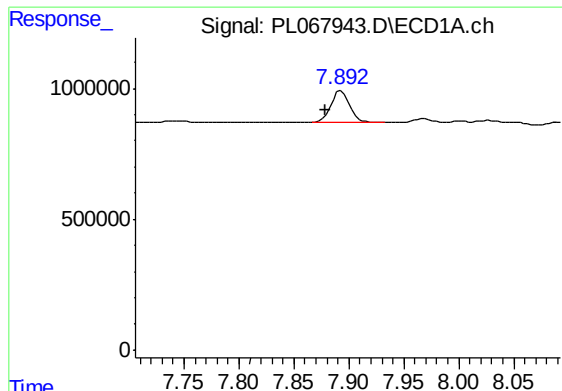

#14 Endrin


R.T.: 7.893 min
Delta R.T.: 0.015 min
Response: 1432628
Conc: 2.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

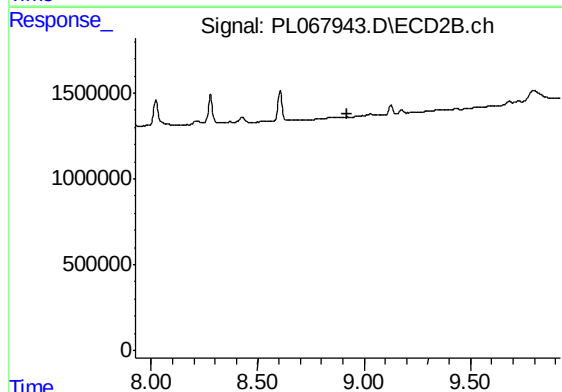


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.924 min
Response: 0
Conc: N.D.

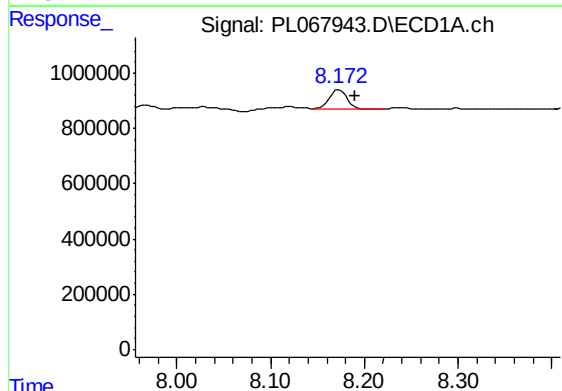


#15 Endosulfan II

R.T.: 8.173 min
Delta R.T.: -0.017 min
Response: 897855
Conc: 1.46 ng/ml

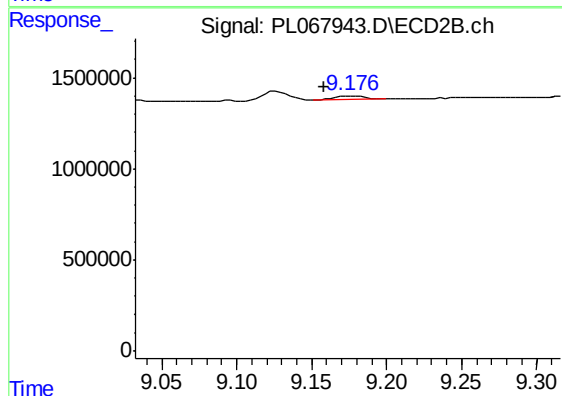

#15 Endosulfan II


R.T.: 9.178 min
Delta R.T.: 0.019 min
Response: 273465
Conc: 0.34 ng/ml

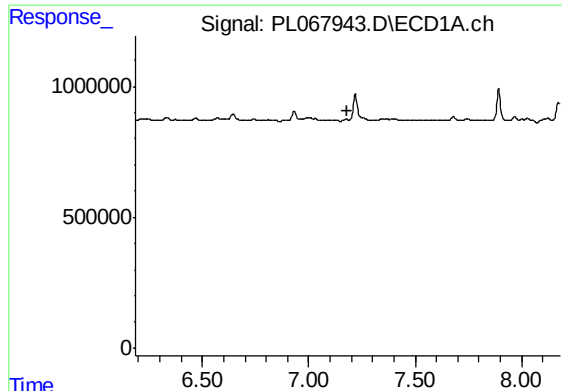

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

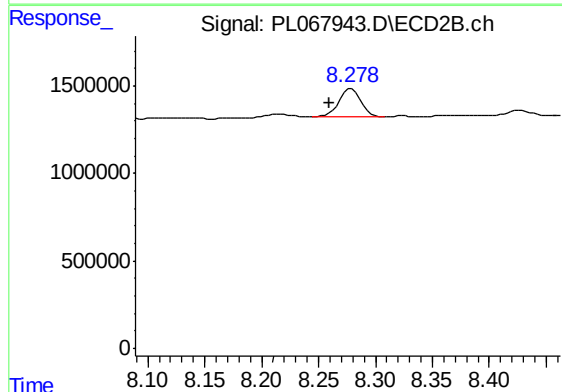


#25 Chlordane-3

R.T.: 8.279 min
Delta R.T.: 0.020 min
Response: 2059365
Conc: 15.39 ng/ml

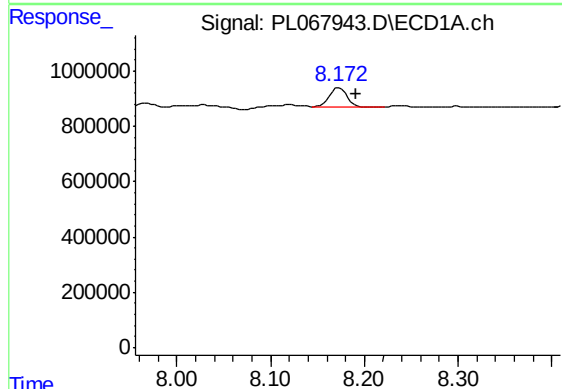


#27 Chlordane-5

R.T.: 8.173 min
Delta R.T.: -0.018 min
Response: 897855
Conc: 41.04 ng/ml

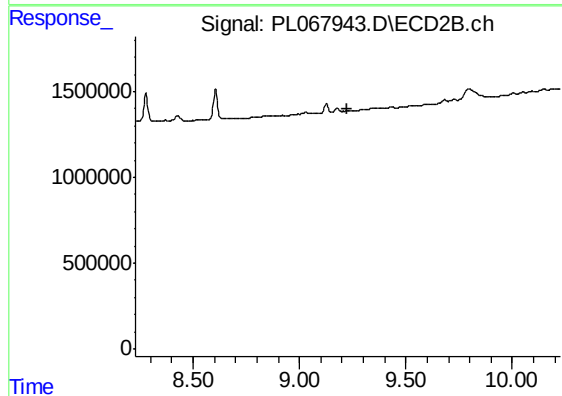

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

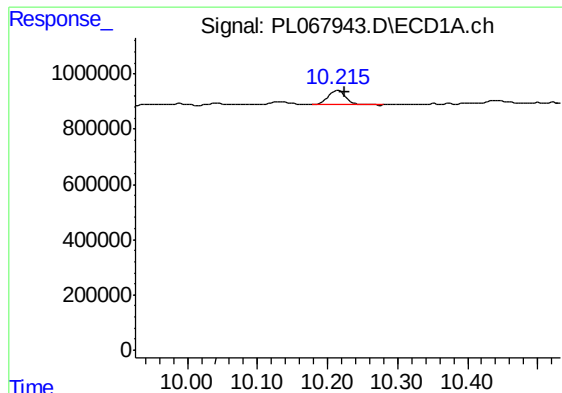

#28 Decachlorobiphenyl

R.T.: 10.216 min
Delta R.T.: -0.008 min
Response: 895770
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-CROPSEY-AQUEOUS

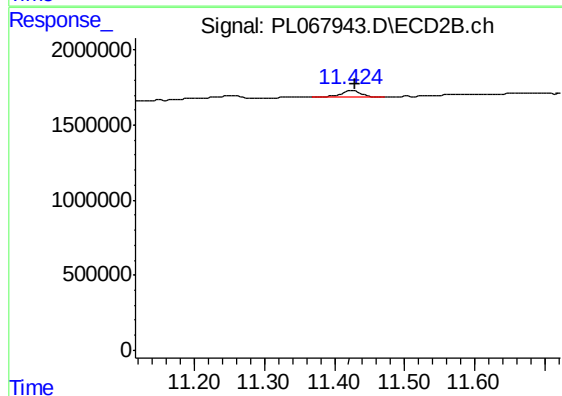

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 861518
Conc: 0.86 ng/ml