

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
 Data File : PL067947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2021 18:22
 Operator : AR\AJ
 Sample : M2904-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:17:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	5.528	6944949	12946110	12.632	13.733
28)	SA Decachlor...	10.219	11.425	9306428	13794328	13.132	13.849
Target Compounds							
13)	MA Dieldrin	0.000	8.704f	0	576337	N.D.	0.635 #
21)	B Endrin ke...	0.000	10.049f	0	91453	N.D.	0.101 #
23)	Chlordane-1	5.777f	0.000	554536	0	29.972	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
Data File : PL067947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2021 18:22
Operator : AR\AJ
Sample : M2904-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:17:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

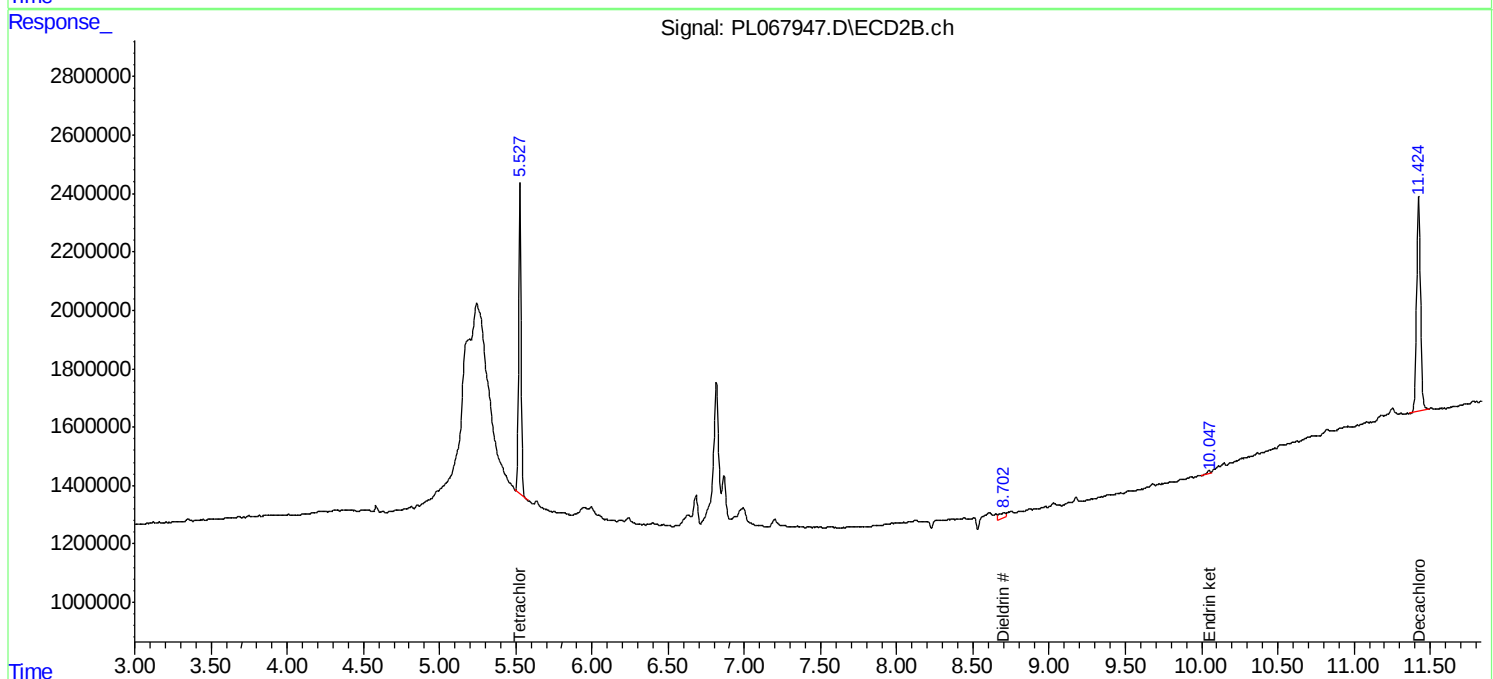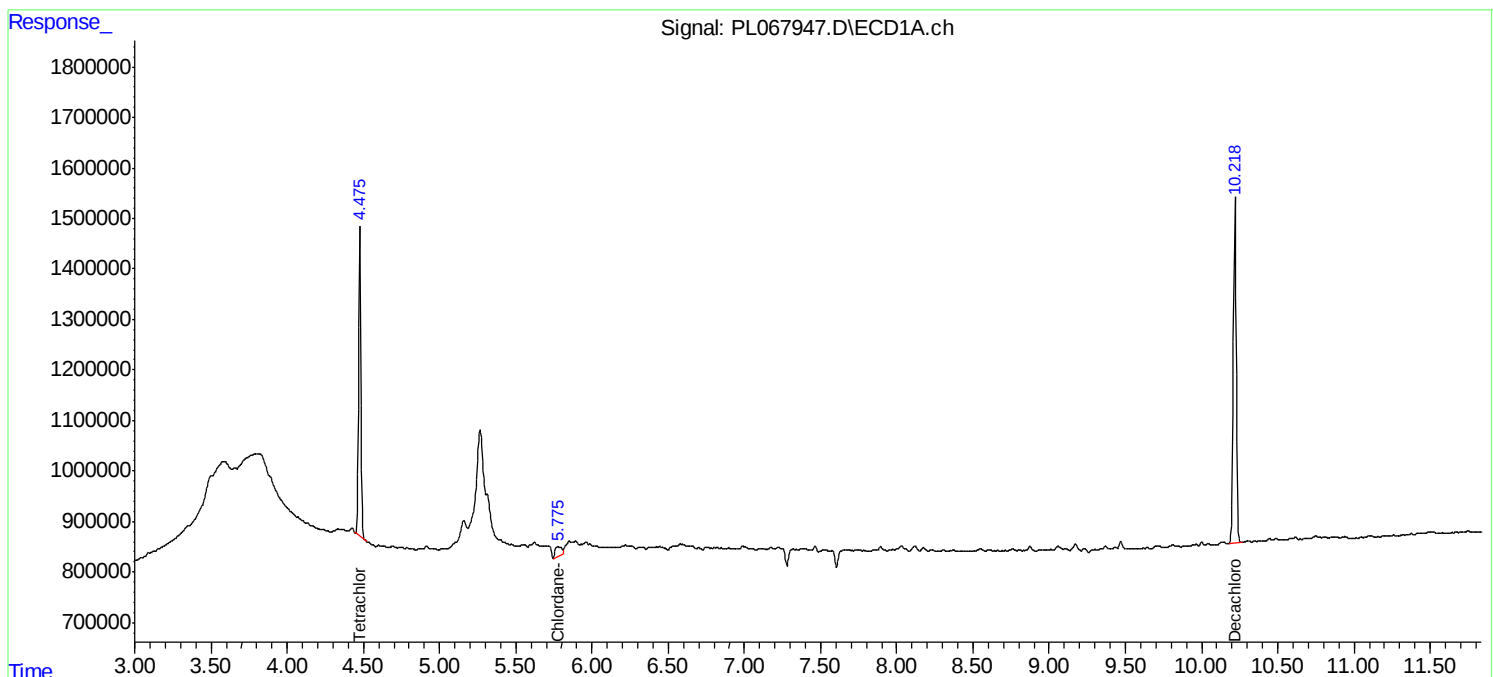


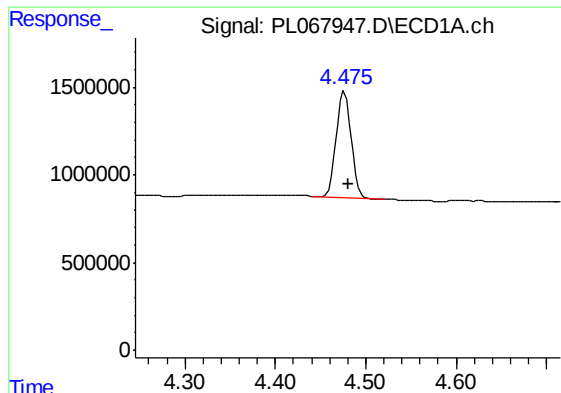

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 6944949
Conc: 12.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

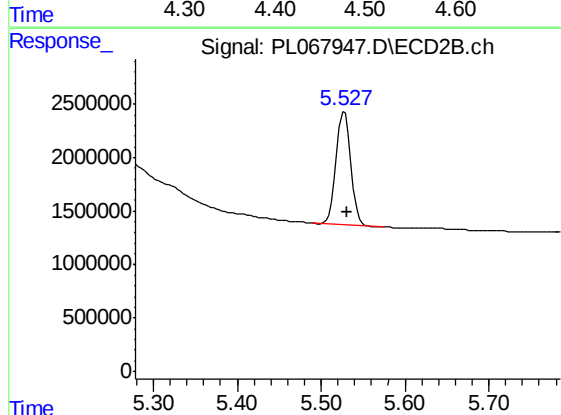


#1 Tetrachloro-m-xylene

R.T.: 5.528 min
Delta R.T.: -0.003 min
Response: 12946110
Conc: 13.73 ng/ml

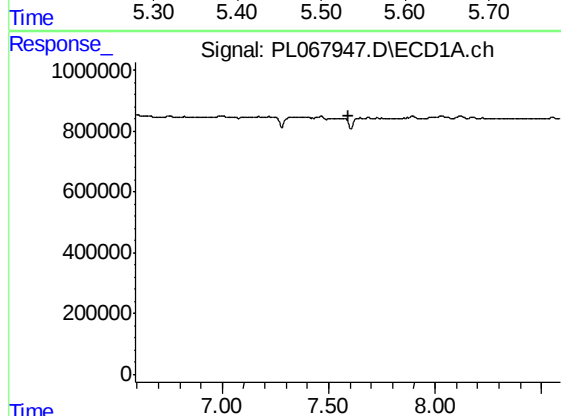


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

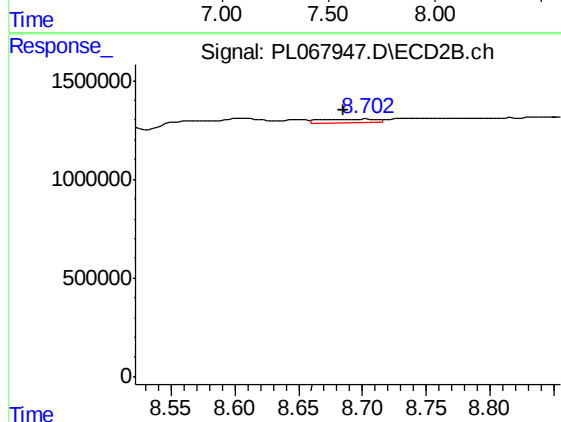

#13 Dieldrin


R.T.: 8.704 min
Delta R.T.: 0.019 min
Response: 576337
Conc: 0.63 ng/ml

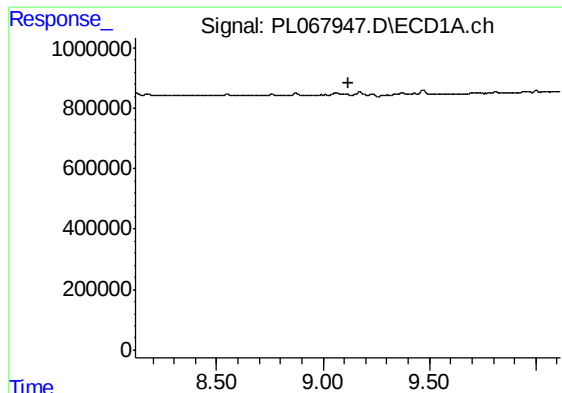

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

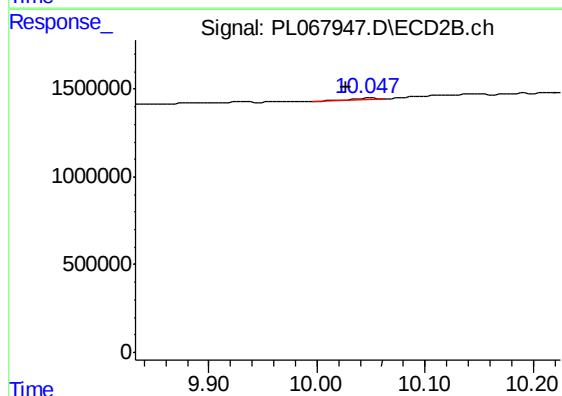


#21 Endrin ketone

R.T.: 10.049 min
Delta R.T.: 0.023 min
Response: 91453
Conc: 0.10 ng/ml

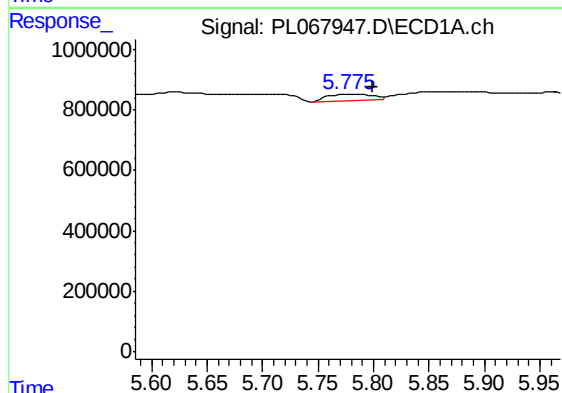


#23 Chlordane-1

R.T.: 5.777 min
Delta R.T.: -0.023 min
Response: 554536
Conc: 29.97 ng/ml

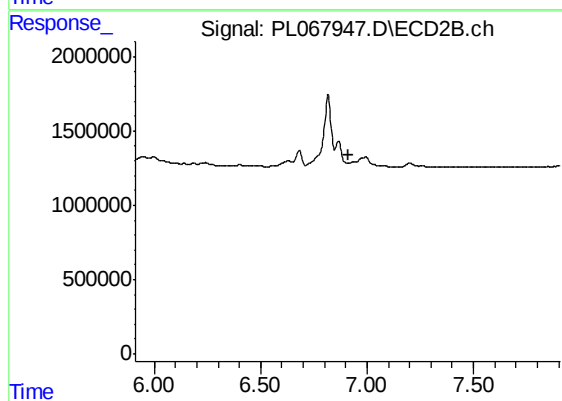

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

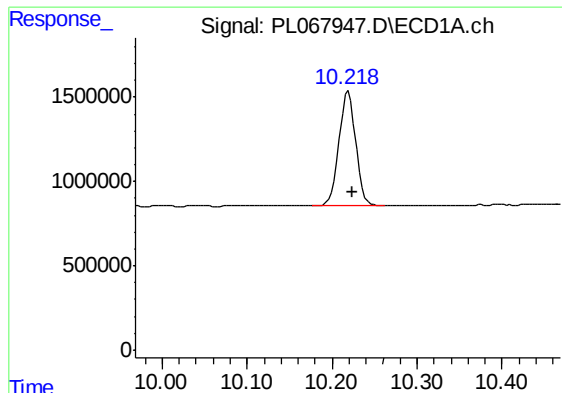

#28 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: -0.005 min
Response: 9306428
Conc: 13.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

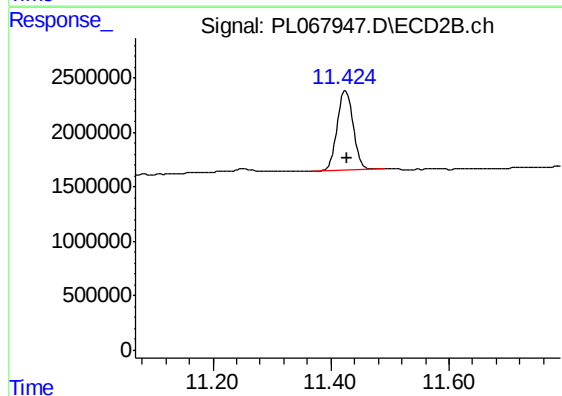

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.004 min
Response: 13794328
Conc: 13.85 ng/ml