

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
 Data File : PL067948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2021 18:38
 Operator : AR\AJ
 Sample : M2904-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 02:17:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 11 02:00:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.476	5.527	6495319	12195175	11.814	12.936
28)	SA Decachlor...	10.217	11.425	8308660	12220393	11.724	12.269
Target Compounds							
2)	A alpha-BHC	5.163f	0.000	185289	0	0.252	N.D. #
9)	A Endosulfan I	7.310	0.000	485177	0	0.722	N.D. #
10)	B gamma-Chl...	0.000	8.255	0	11779	N.D.	0.012 #
11)	B alpha-Chl...	0.000	8.339	0	261515	N.D.	0.259 #
12)	B 4,4'-DDE	7.466	0.000	233961	0	0.352	N.D. #
13)	MA Dieldrin	0.000	8.688	0	287391	N.D.	0.316 #
21)	B Endrin ke...	0.000	10.048f	0	148136	N.D.	0.163 #
23)	Chlordane-1	5.792	0.000	382602	0	20.679	N.D. #
25)	Chlordane-3	0.000	8.255	0	11779	N.D.	0.088 #
26)	Chlordane-4	0.000	8.339	0	261515	N.D.	1.613 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070221\
Data File : PL067948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2021 18:38
Operator : AR\AJ
Sample : M2904-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 02:17:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL061021.M
Quant Title : GC Extractables
QLast Update : Fri Jun 11 02:00:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

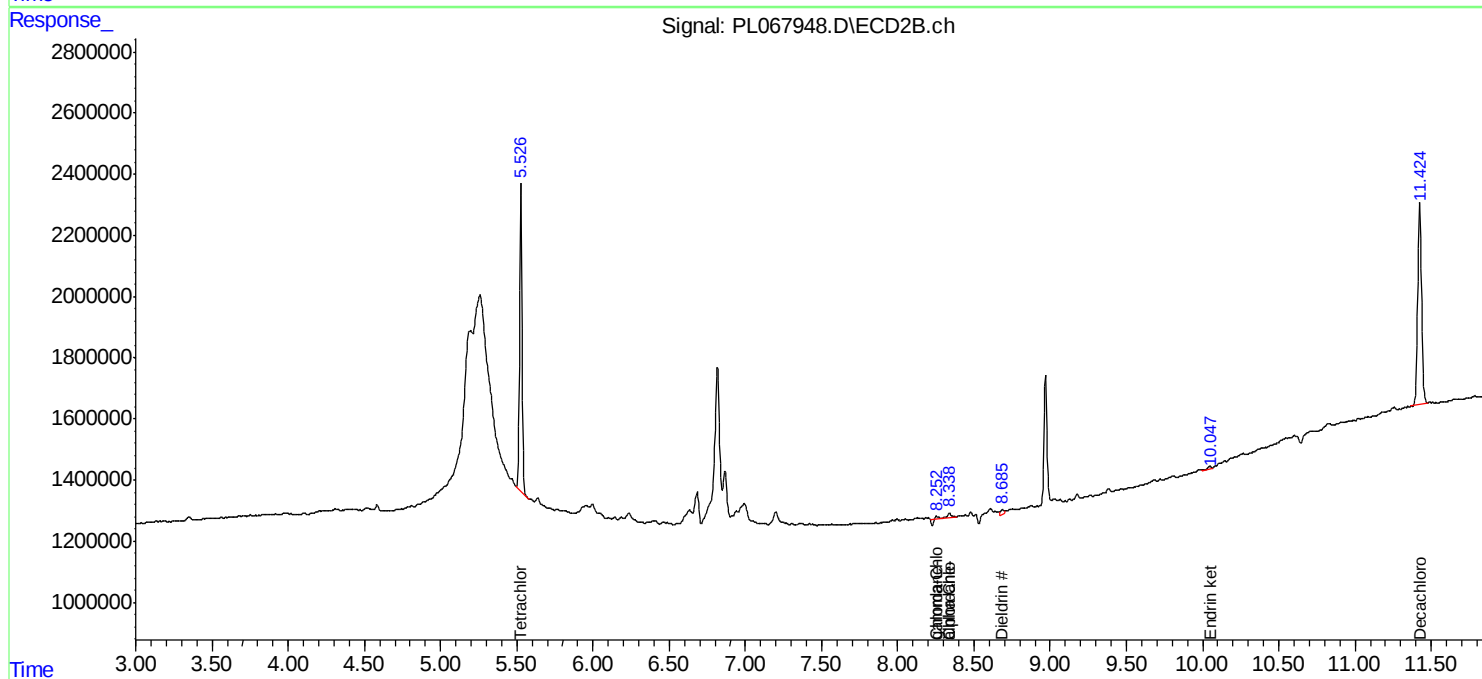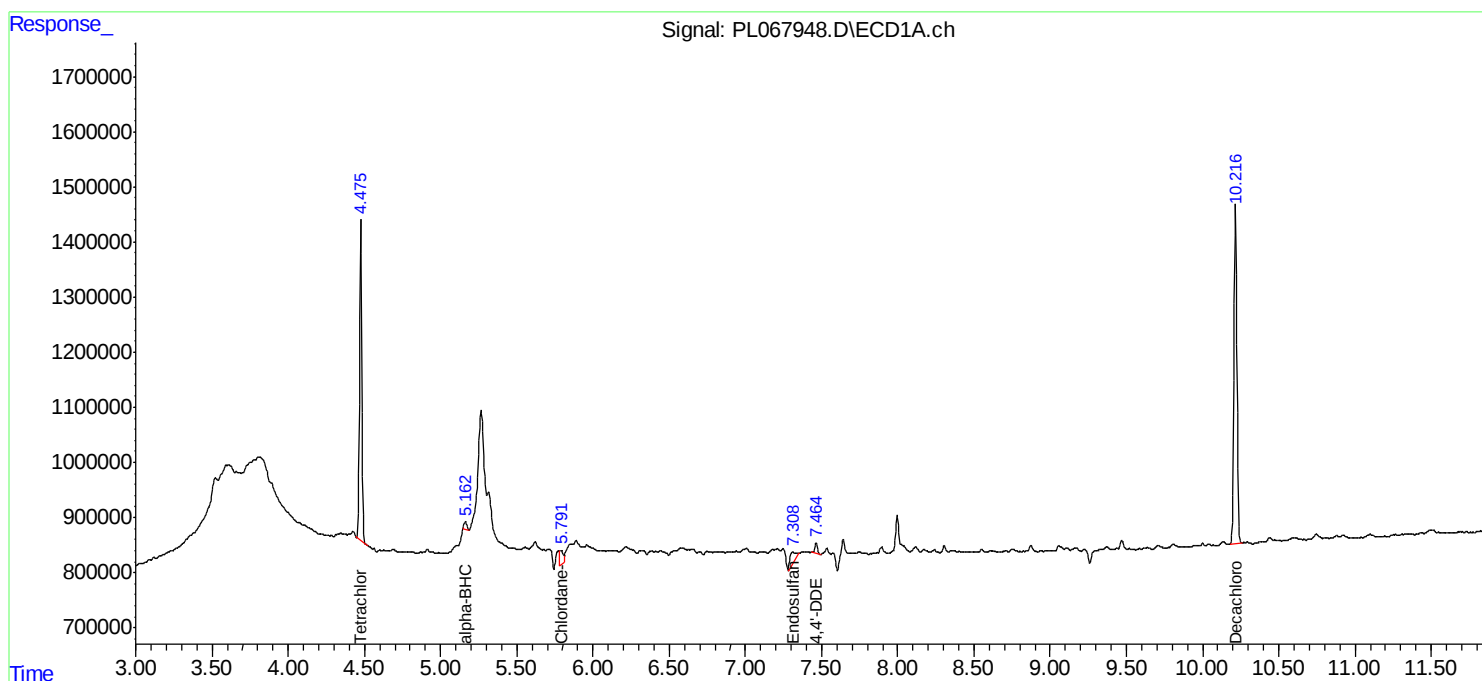


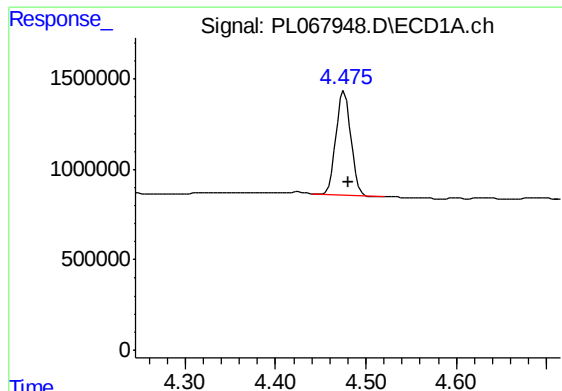

#1 Tetrachloro-m-xylene


R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 6495319
Conc: 11.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

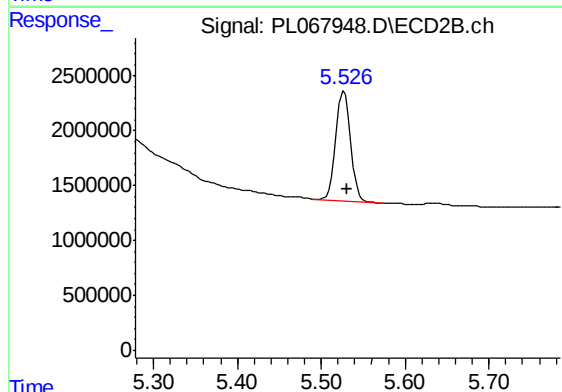


#1 Tetrachloro-m-xylene

R.T.: 5.527 min
Delta R.T.: -0.004 min
Response: 12195175
Conc: 12.94 ng/ml

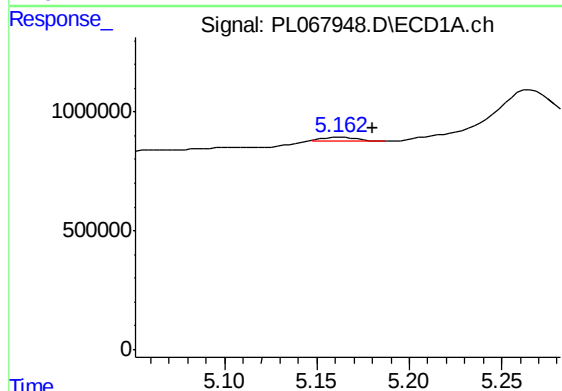


#2 alpha-BHC

R.T.: 5.163 min
Delta R.T.: -0.018 min
Response: 185289
Conc: 0.25 ng/ml

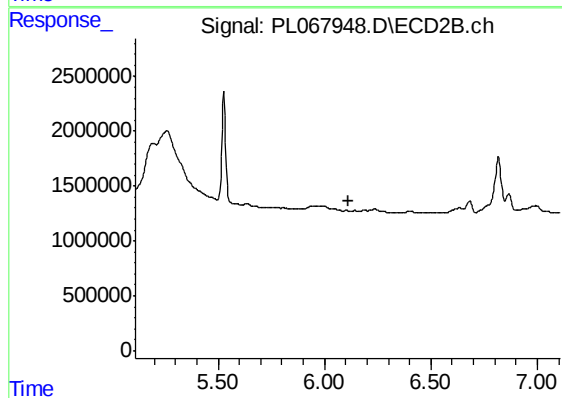

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.112 min
Response: 0
Conc: N.D.

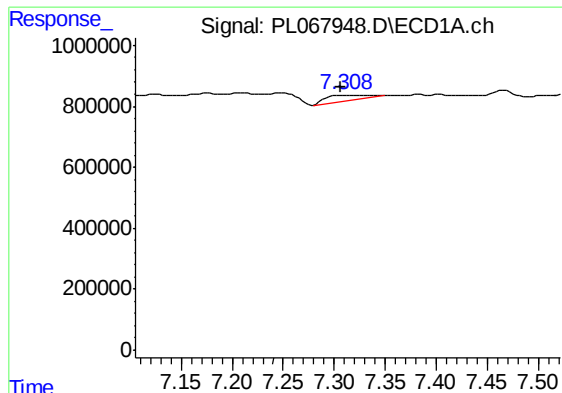

#9 Endosulfan I


R.T.: 7.310 min
Delta R.T.: 0.003 min
Response: 485177
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

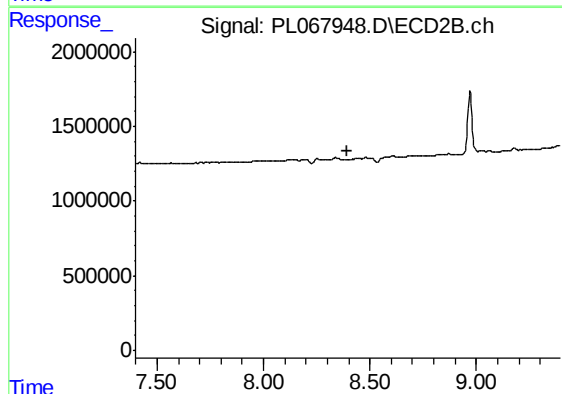


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.397 min
Response: 0
Conc: N.D.

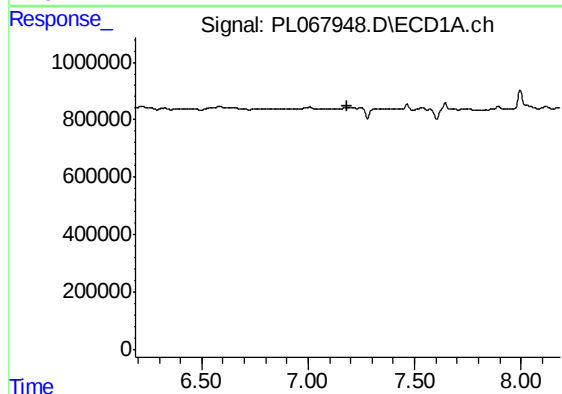


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

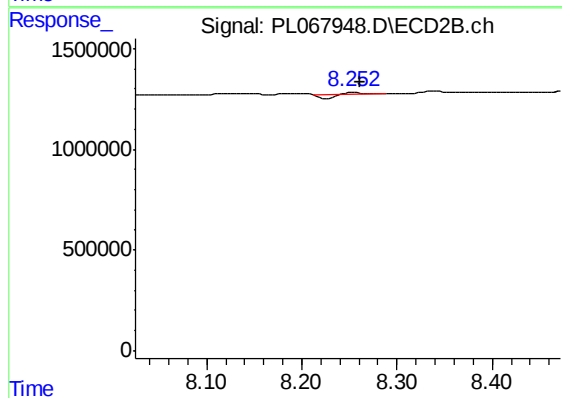

#10 gamma-Chlordane


R.T.: 8.255 min
Delta R.T.: -0.007 min
Response: 11779
Conc: 0.01 ng/ml

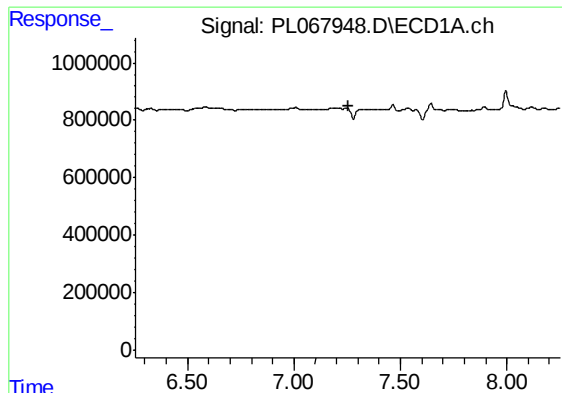

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

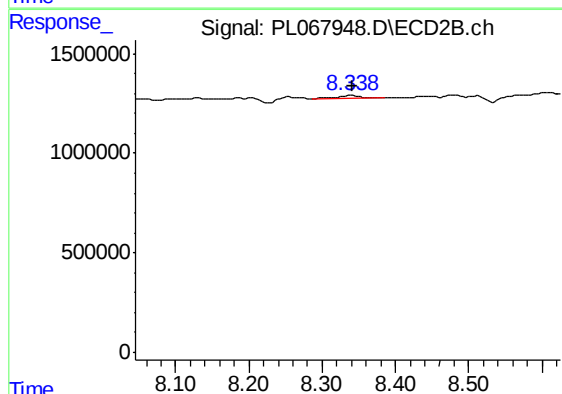


#11 alpha-Chlordane

R.T.: 8.339 min
Delta R.T.: -0.003 min
Response: 261515
Conc: 0.26 ng/ml

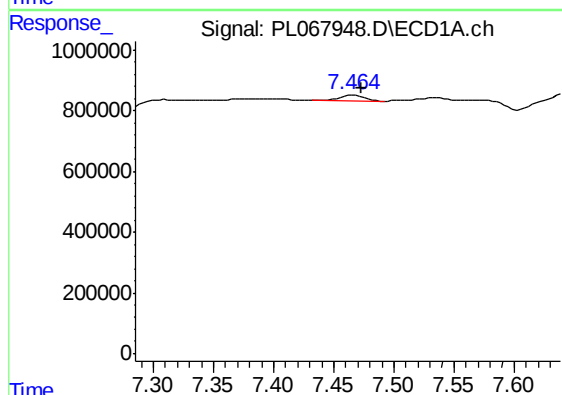


#12 4,4'-DDE

R.T.: 7.466 min
Delta R.T.: -0.007 min
Response: 233961
Conc: 0.35 ng/ml

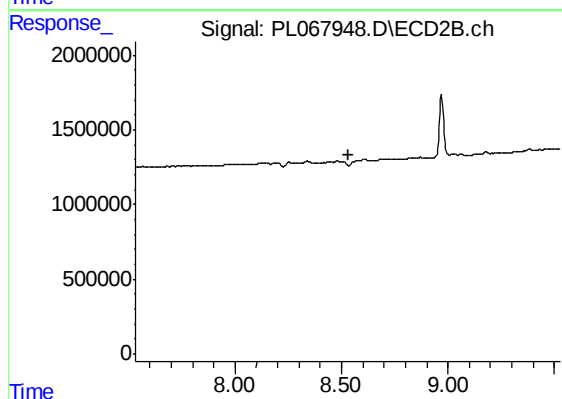

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 8.530 min
Response: 0
Conc: N.D.

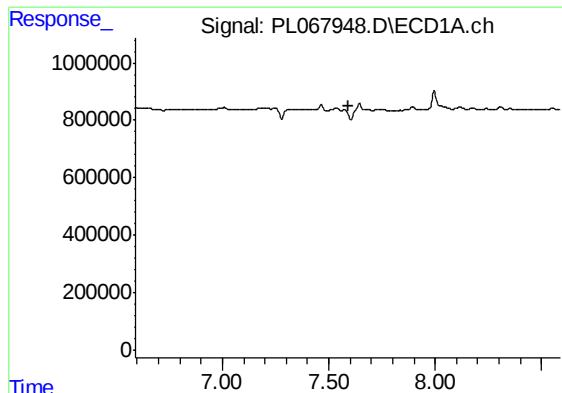

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 7.592 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

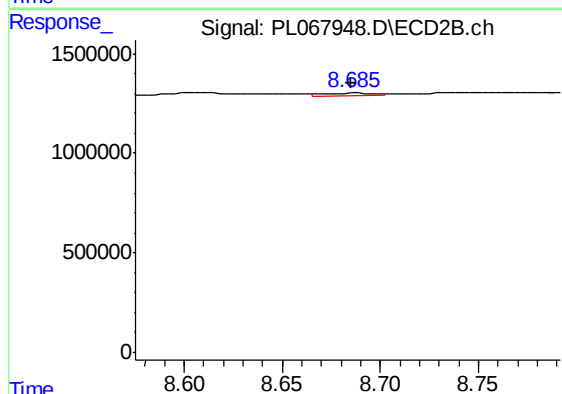


#13 Dielldrin

R.T.: 8.688 min
Delta R.T.: 0.002 min
Response: 287391
Conc: 0.32 ng/ml

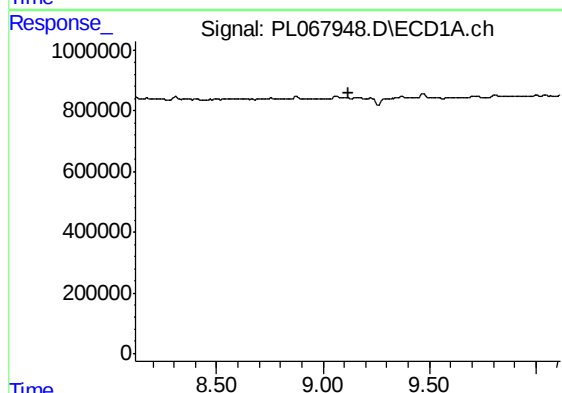


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.118 min
Response: 0
Conc: N.D.

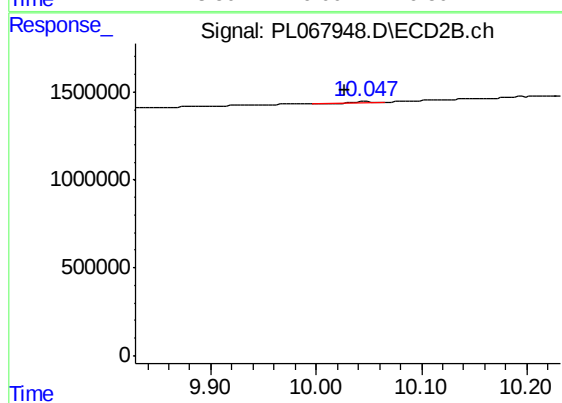

#21 Endrin ketone


R.T.: 10.048 min
Delta R.T.: 0.022 min
Response: 148136
Conc: 0.16 ng/ml

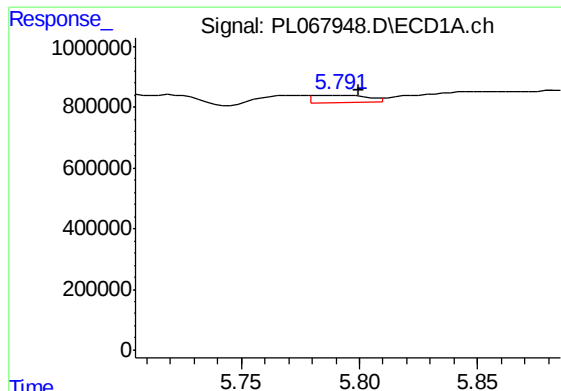

#23 Chlordane-1


R.T.: 5.792 min
Delta R.T.: -0.007 min
Response: 382602
Conc: 20.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

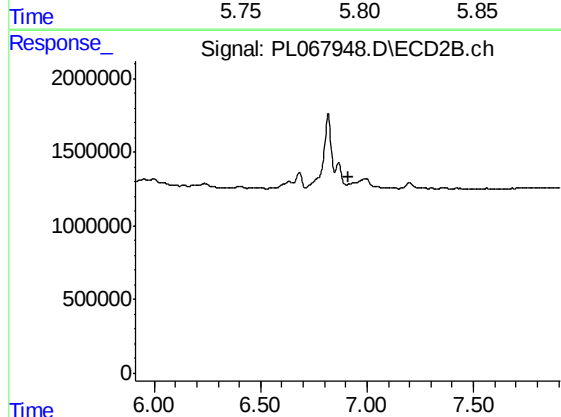


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

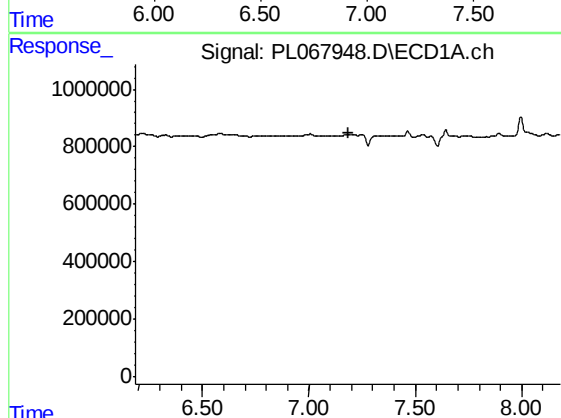


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.184 min
Response: 0
Conc: N.D.

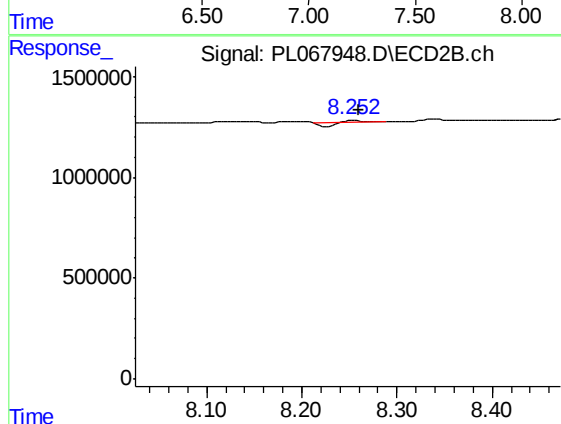

#25 Chlordane-3


R.T.: 8.255 min
Delta R.T.: -0.005 min
Response: 11779
Conc: 0.09 ng/ml

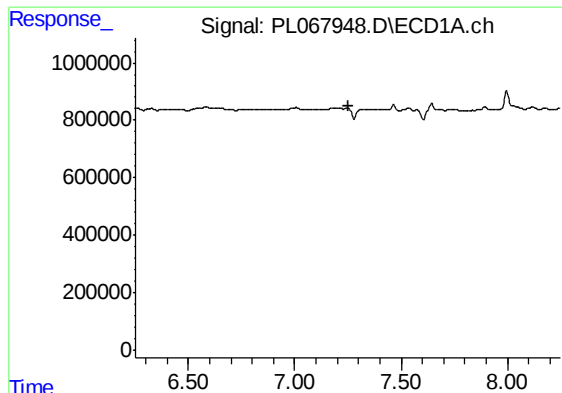

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

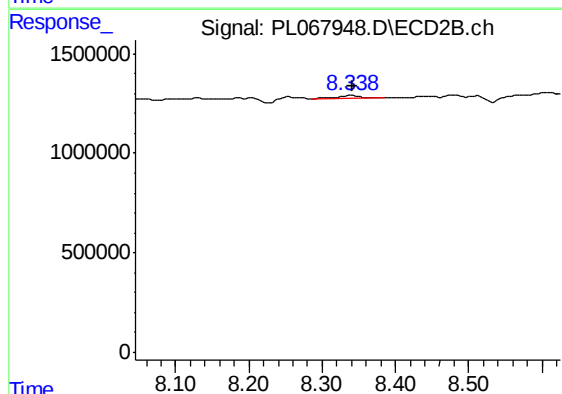


#26 Chlordane-4

R.T.: 8.339 min
Delta R.T.: -0.002 min
Response: 261515
Conc: 1.61 ng/ml

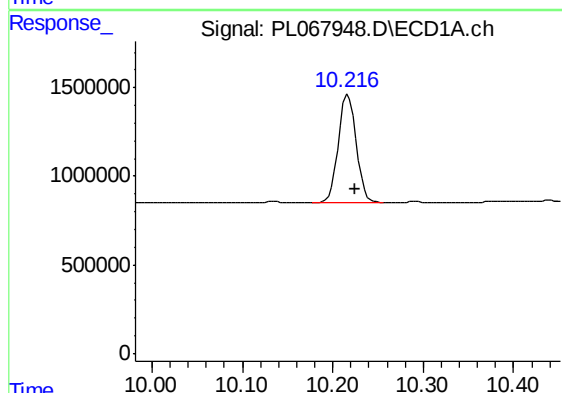

#28 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: -0.007 min
Response: 8308660
Conc: 11.72 ng/ml

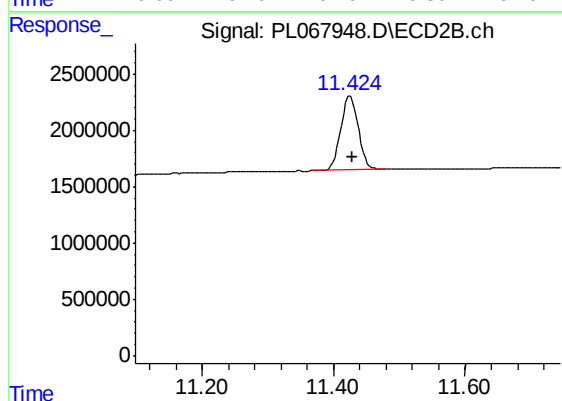

#28 Decachlorobiphenyl

R.T.: 11.425 min
Delta R.T.: -0.003 min
Response: 12220393
Conc: 12.27 ng/ml